
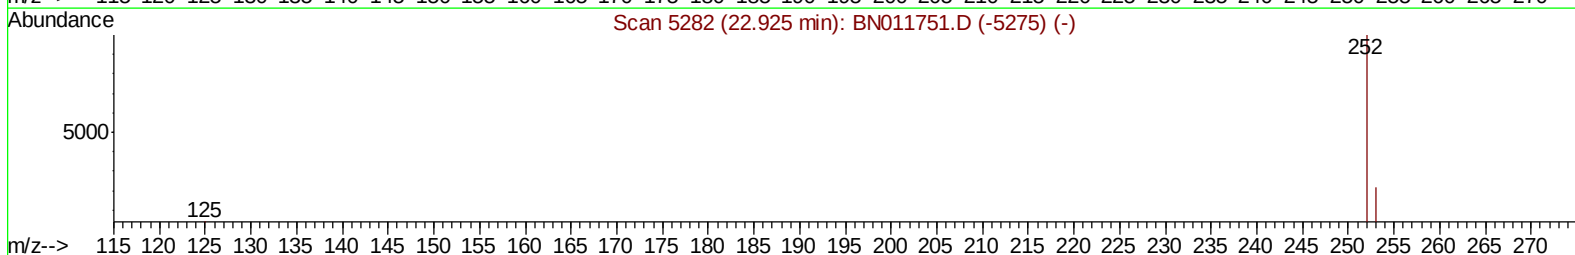
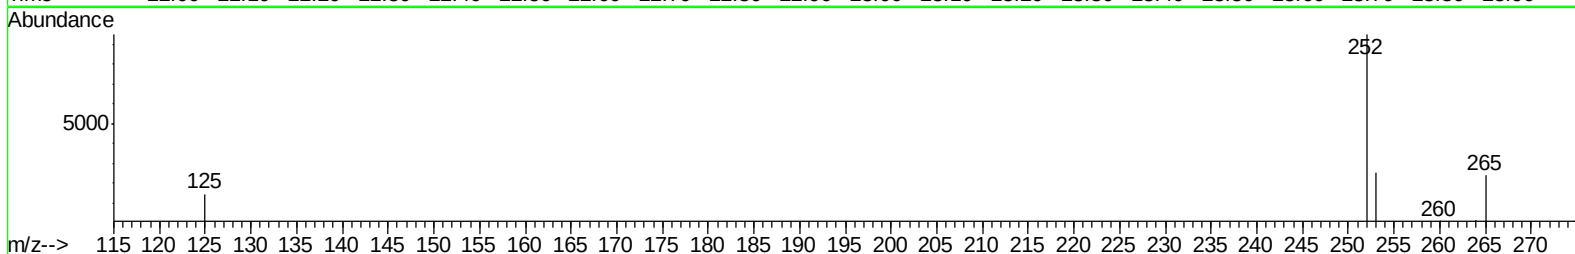


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090820\
Data File : BN011754.D
Acq On : 09 Sep 2020 02:08
Operator : CG/JU
Sample : L3843-05
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Sep 09 07:34:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN090820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 09 07:05:35 2020
Response via : Initial Calibration

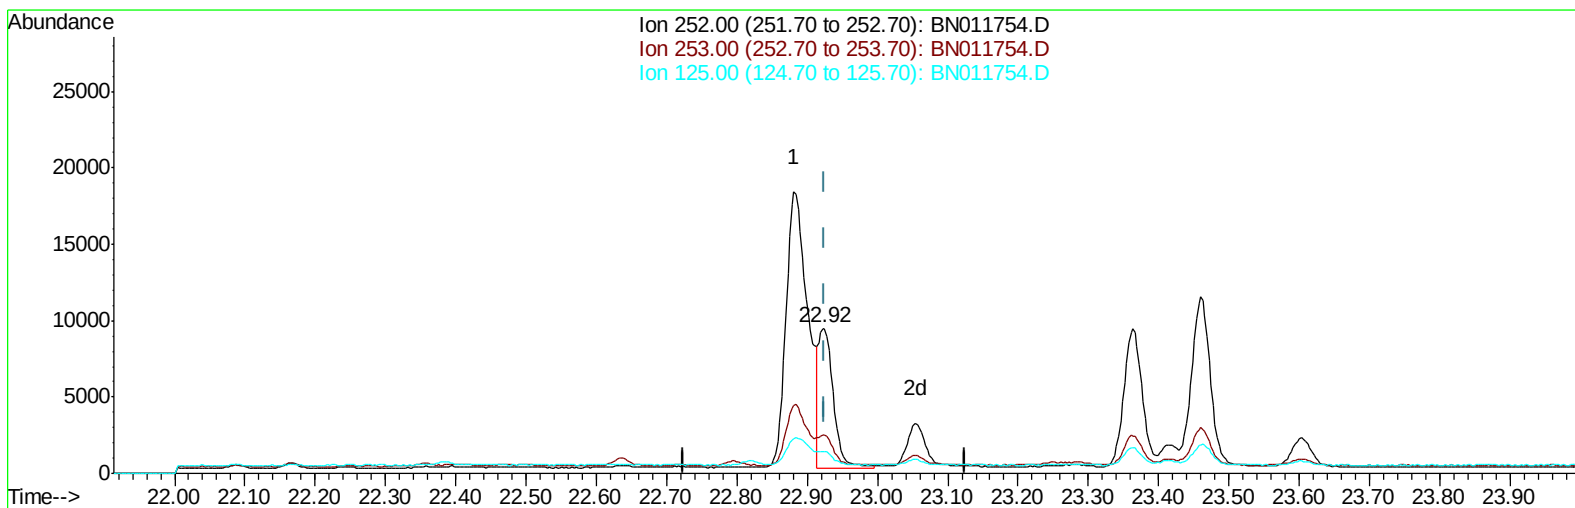

TIC: BN011754.D

(22) Benzo(k)fluoranthene

22.922min (-0.003) 0.30ng/ul m

response 13332

Ion	Exp%	Act%
252.00	100	100
253.00	25.90	26.43
125.00	12.10	15.23#
0.00	0.00	0.00