
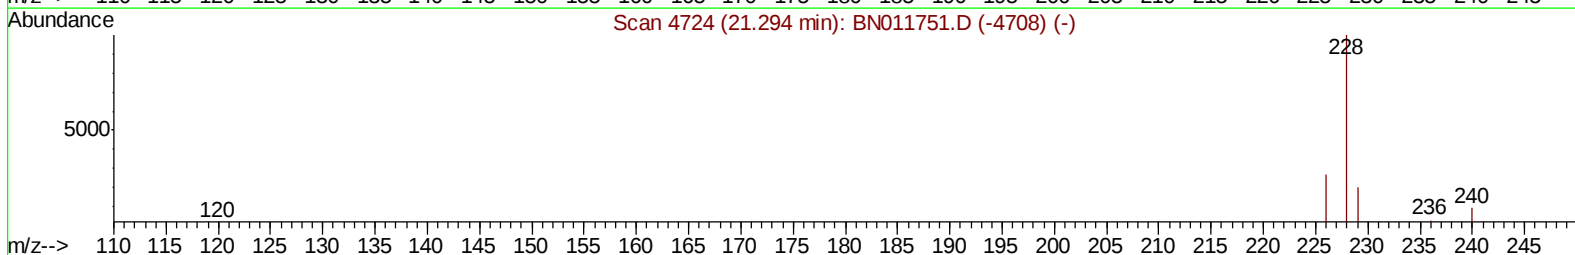
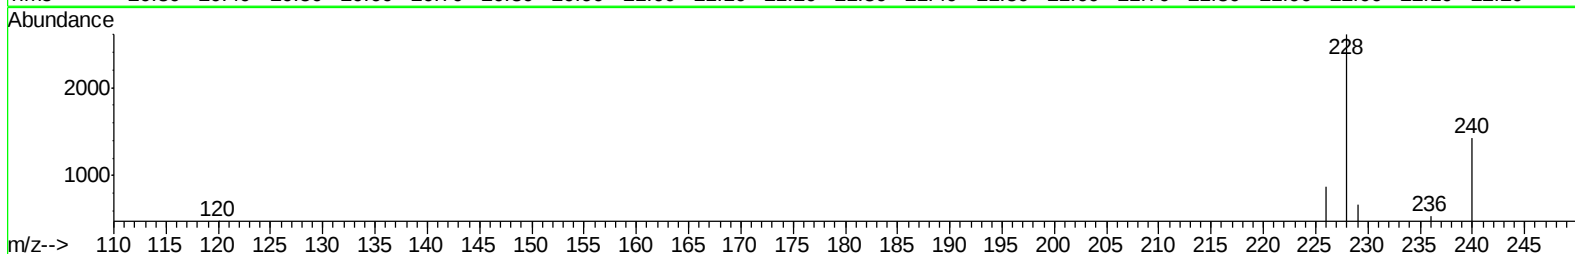


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090820\
Data File : BN011755.D
Acq On : 09 Sep 2020 02:45
Operator : CG/JU
Sample : L3843-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Sep 09 07:37:54 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN090820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 09 07:05:35 2020
Response via : Initial Calibration

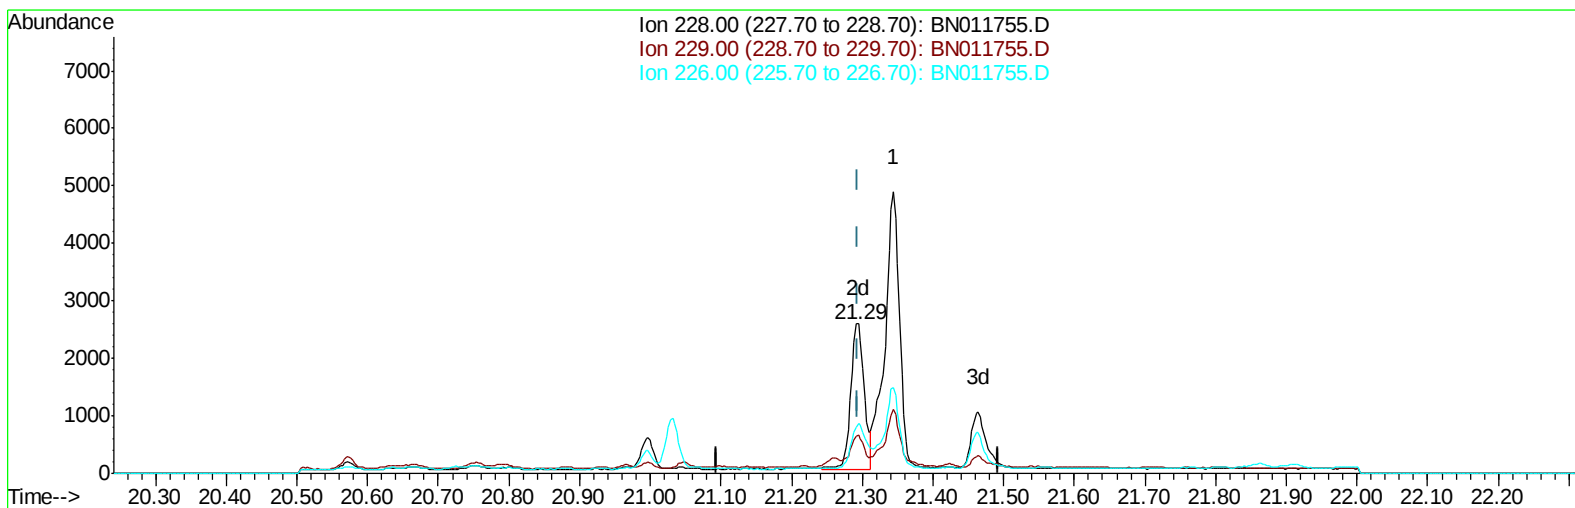

TIC: BN011755.D

(18) Benzo(a)anthracene

21.294min (+0.000) 0.10ng/ul m

response 3397

Ion	Exp%	Act%
228.00	100	100
229.00	19.90	25.88#
226.00	27.40	33.37#
0.00	0.00	0.00