
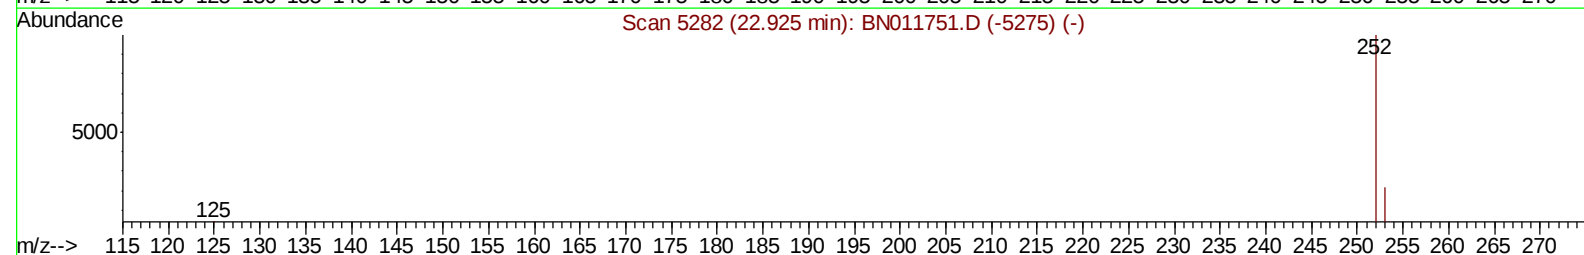
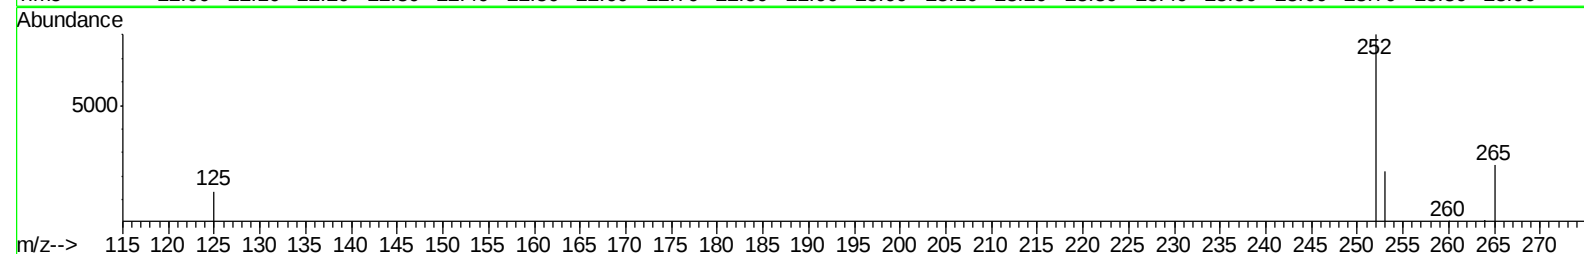


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090820\
 Data File : BN011756.D
 Acq On : 09 Sep 2020 03:21
 Operator : CG/JU
 Sample : L3843-07
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Quant Time: Sep 09 07:40:07 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN090820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 09 07:05:35 2020
 Response via : Initial Calibration

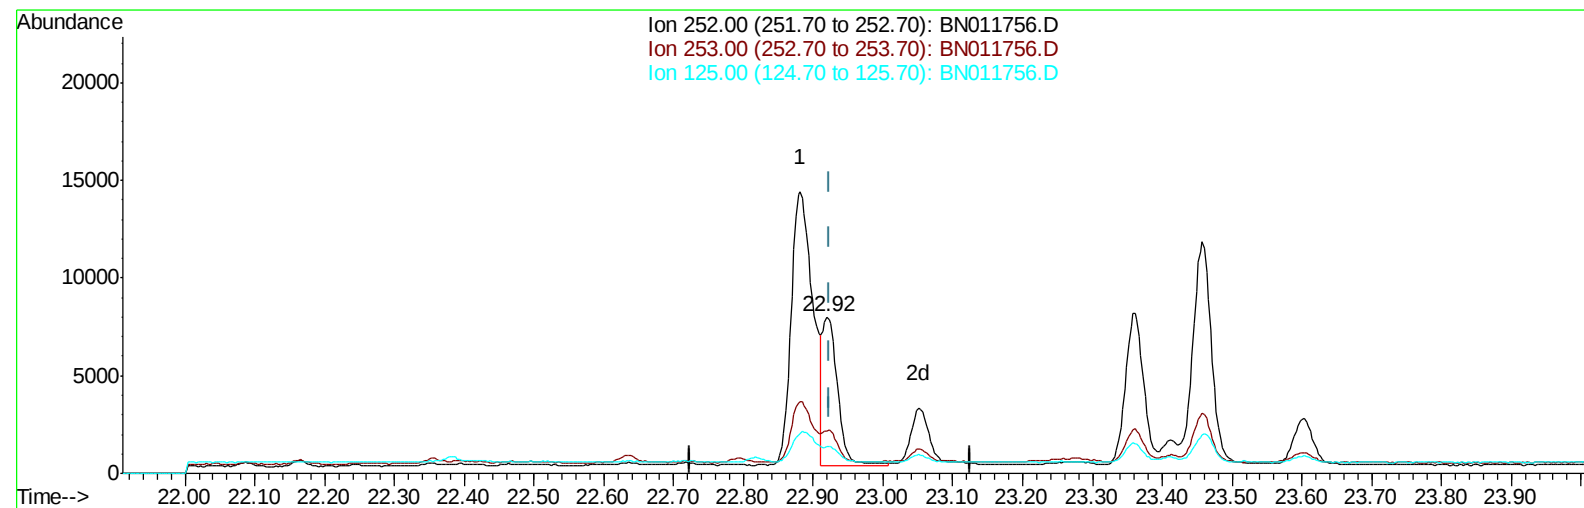

TIC: BN011756.D

(22) Benzo(k)fluoranthene

22.919min (-0.006) 0.24ng/ul m

response 11247

Ion	Exp%	Act%
252.00	100	100
253.00	25.90	27.24
125.00	12.10	16.91#
0.00	0.00	0.00