
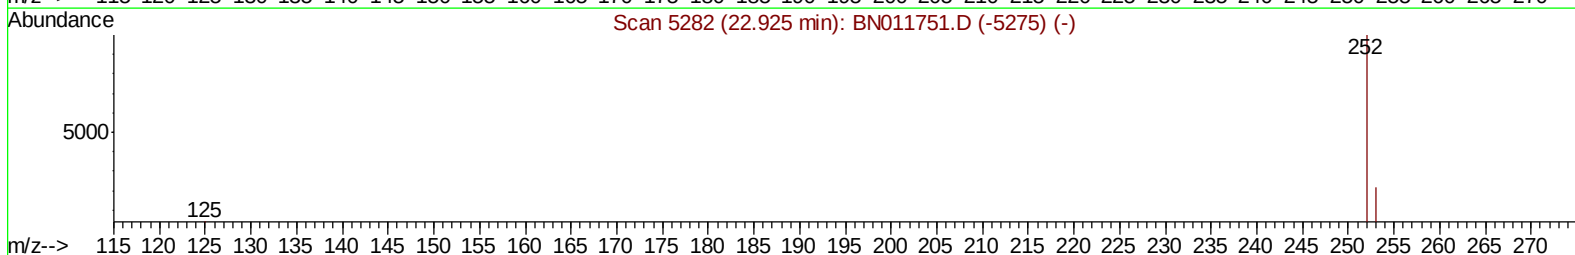
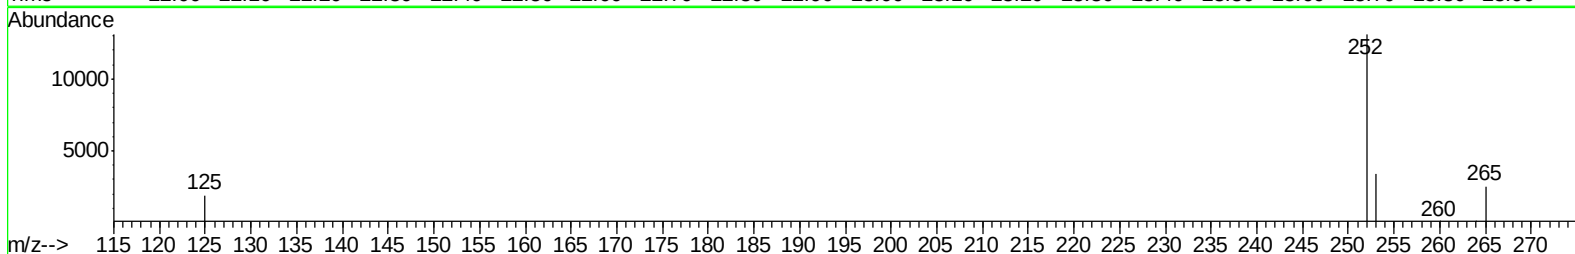


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090820\
Data File : BN011757.D
Acq On : 09 Sep 2020 03:57
Operator : CG/JU
Sample : L3843-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Sep 09 07:42:07 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN090820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 09 07:05:35 2020
Response via : Initial Calibration

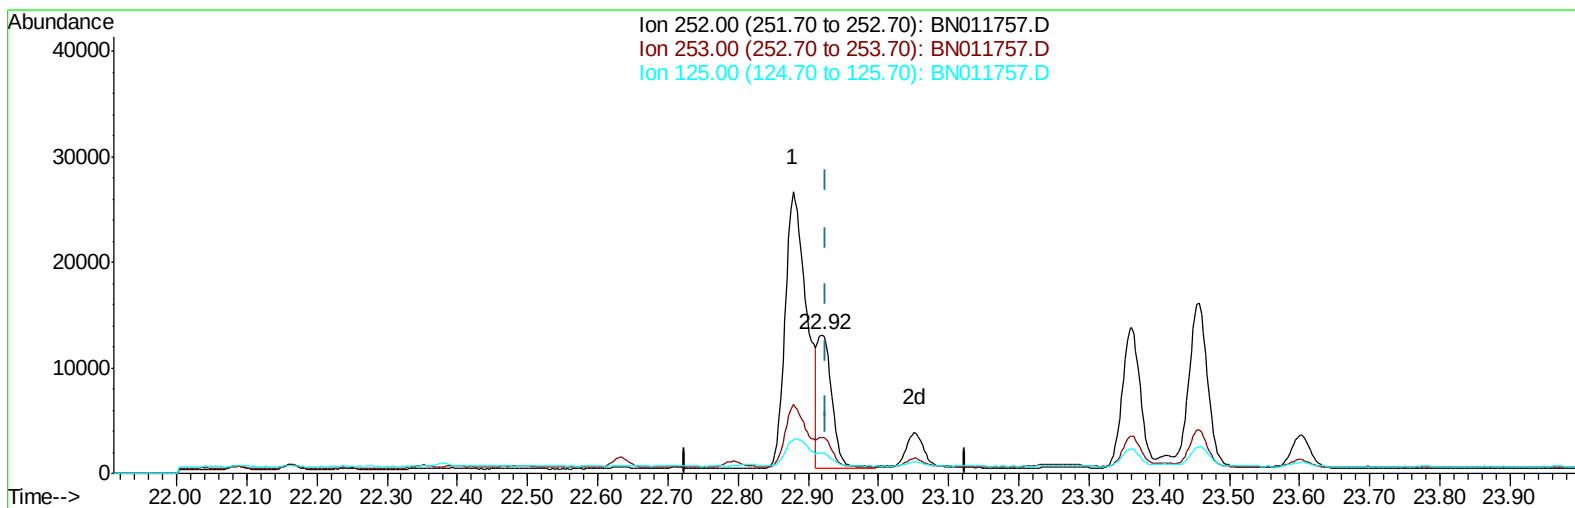

TIC: BN011757.D

(22) Benzo(k)fluoranthene

22.919min (-0.006) 0.38ng/ul m

response 18134

Ion	Exp%	Act%
252.00	100	100
253.00	25.90	26.10
125.00	12.10	14.65#
0.00	0.00	0.00