
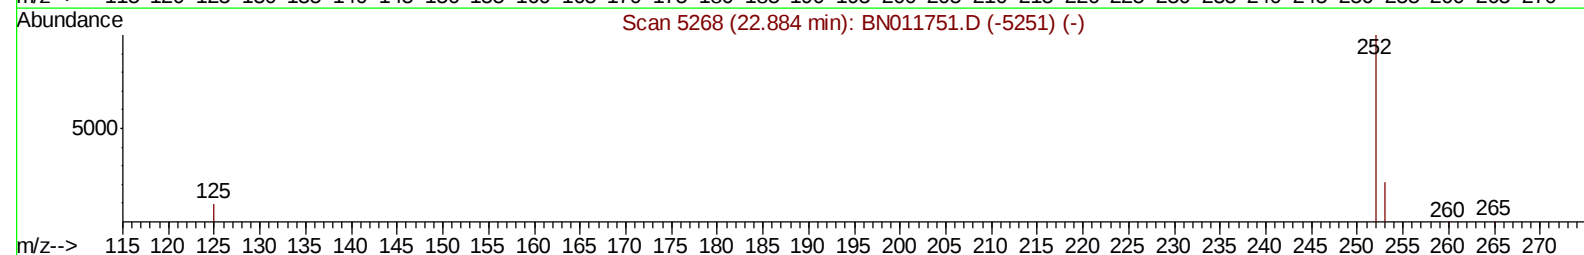
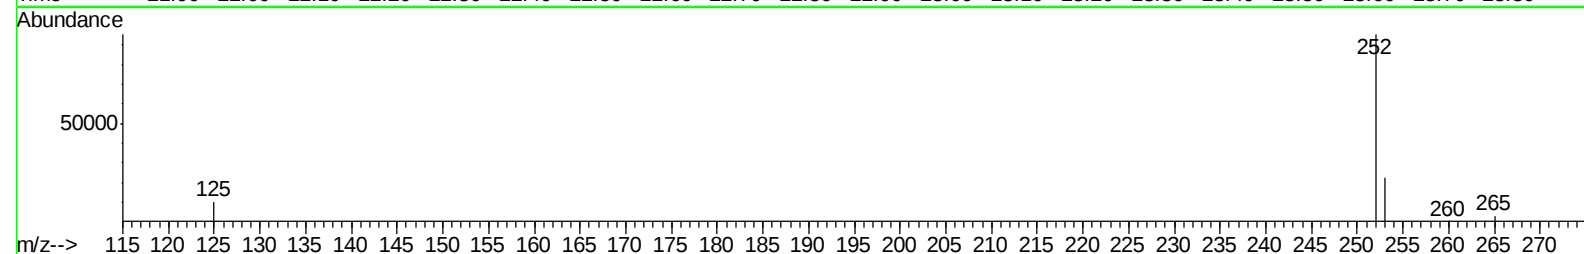


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090820\
Data File : BN011758.D
Acq On : 09 Sep 2020 04:33
Operator : CG/JU
Sample : L3843-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Quant Time: Sep 09 07:44:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN090820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 09 07:05:35 2020
Response via : Initial Calibration

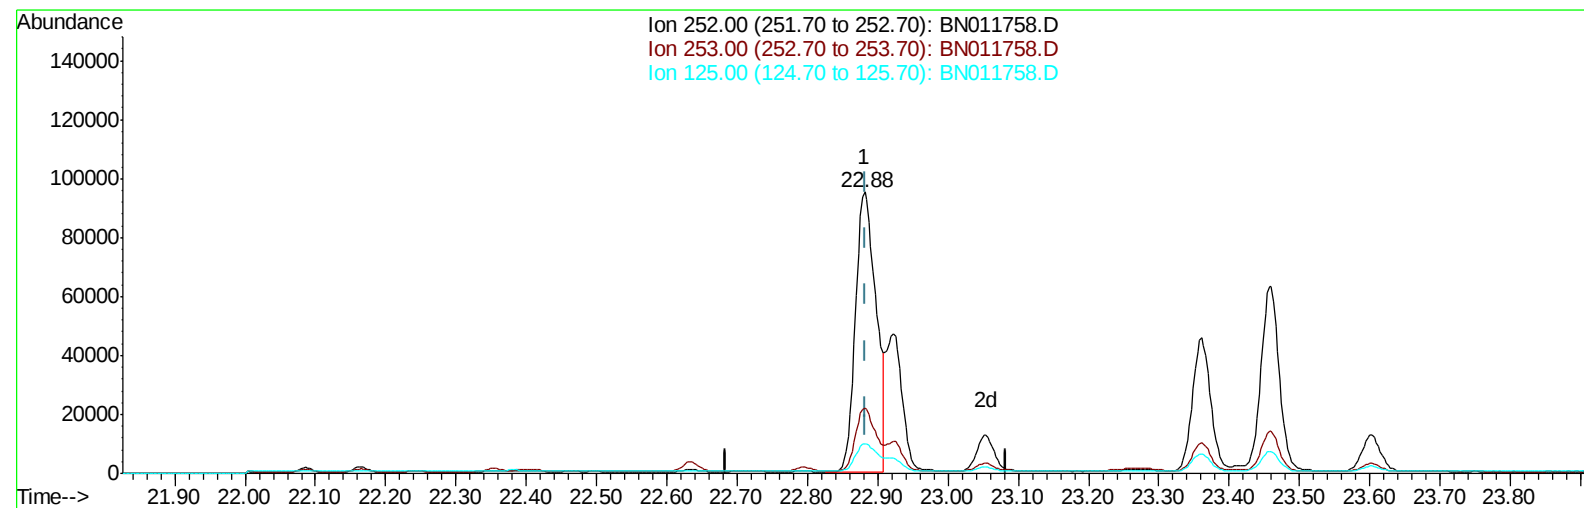

TIC: BN011758.D

(21) Benzo(b)fluoranthene

22.881min (-0.003) 3.76ng/ul m

response 192402

Ion	Exp%	Act%
252.00	100	100
253.00	25.30	23.11
125.00	11.80	10.57
0.00	0.00	0.00