


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090820\
Data File : BN011748.D
Acq On : 08 Sep 2020 21:55
Operator : CG/JU
Sample : L3840-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE3

Manual Integrations
APPROVED

Sohil
9/9/2020 3:46:28 PM

Quant Time: Sep 09 06:59:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN090820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 09 06:29:50 2020
Response via : Initial Calibration

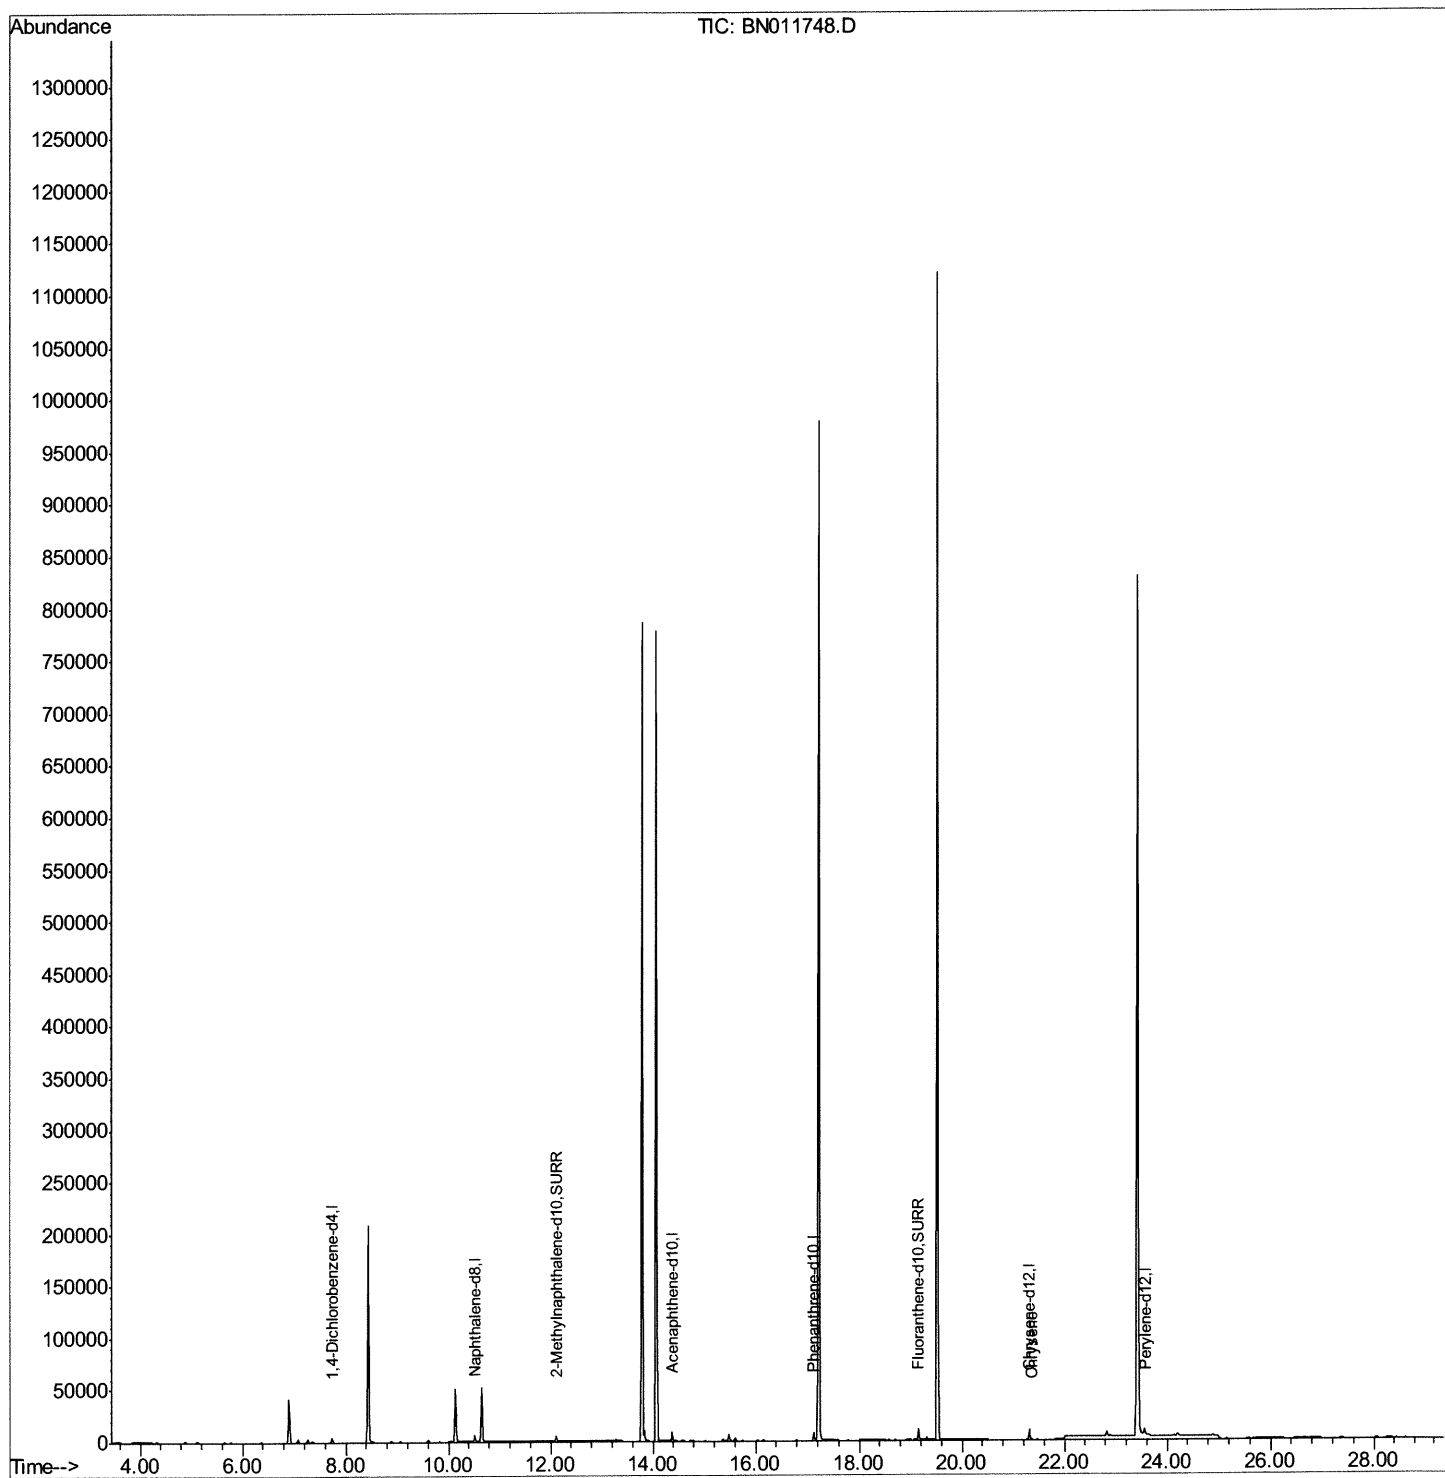

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090820\
 Data File : BN011748.D
 Acq On : 08 Sep 2020 21:55
 Operator : CG/JU
 Sample : L3840-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 C0AE3

Manual Integrations
APPROVED

Sohil
 9/9/2020 3:46:28 PM

Quant Time: Sep 09 06:37:27 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN090820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 09 06:29:50 2020
 Response via : Initial Calibration

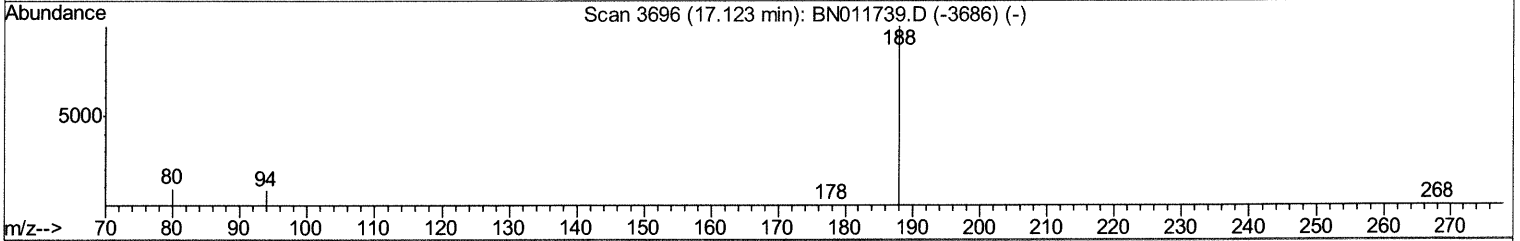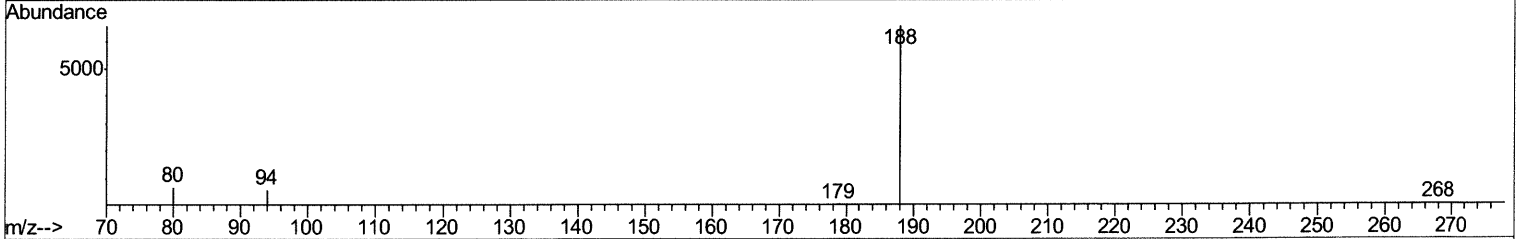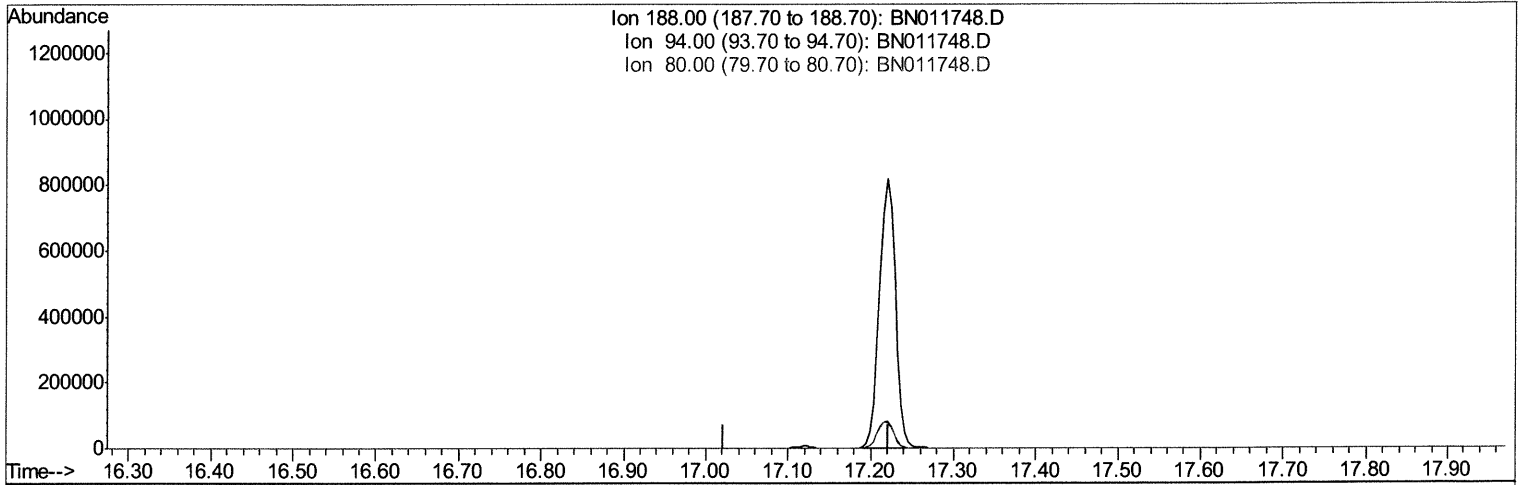

TIC: BN011748.D

(10) Phenanthrene-d10 (I)
 17.122min (-17.122) 0.00ng/ul
 response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	8.40	0.00#
80.00	9.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090820\
Data File : BN011748.D
Acq On : 08 Sep 2020 21:55
Operator : CG/JU
Sample : L3840-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE3

Manual Integrations
APPROVED

Sohil
9/9/2020 3:46:28 PM

Quant Time: Sep 09 06:37:27 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN090820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 09 06:29:50 2020
Response via : Initial Calibration

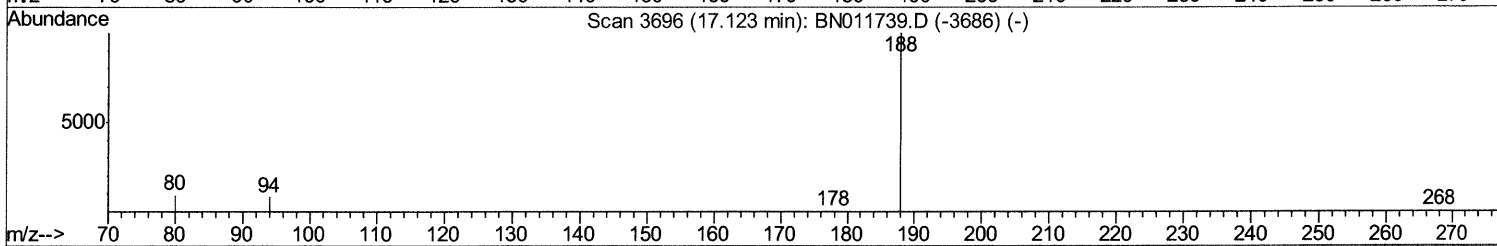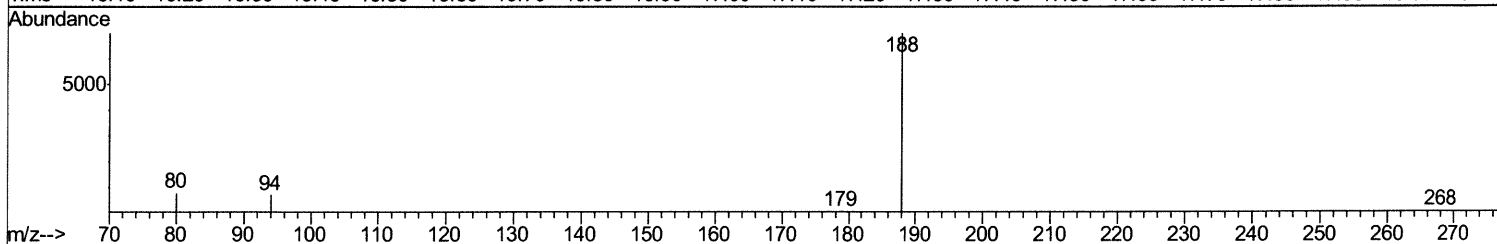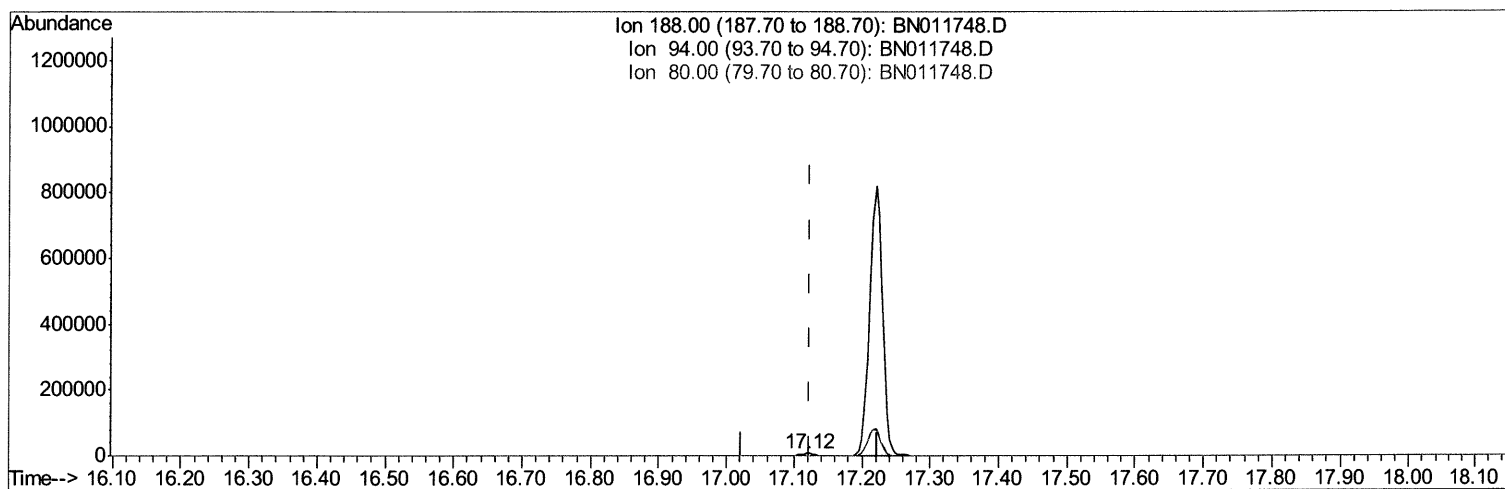

TIC: BN011748.D

(10) Phenanthrene-d10 (I)

17.119min (-0.004) 0.40ng/ul m

09/09/20 JU

response 9362

Ion	Exp%	Act%
188.00	100	100
94.00	8.40	9.88
80.00	9.90	10.92
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN090820\
 Data File : BN011748.D
 Acq On : 08 Sep 2020 21:55
 Operator : CG/JU
 Sample : L3840-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE3

Manual Integrations
 APPROVED

Sohil
 9/9/2020 3:46:28 PM

Quant Time: Sep 09 06:59:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN090820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 09 06:29:50 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	1954	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	7667	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.38	164	4622	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.12	188	9362m>	0.40	ng/ul>	0.00
16) Chrysene-d12	21.31	240	8200	0.40	ng/ul	0.00
20) Perylene-d12	23.56	264	8729	0.40	ng/ul	0.00

09/09/2020 JV

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev (Min)
4) 2-Methylnaphthalene-d10	12.11	152	5884	0.49	ng/ul	0.00
14) Fluoranthene-d10	19.15	212	12018	0.49	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
19) Chrysene	21.34	228	1066	0.030	ng/ul#	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed