
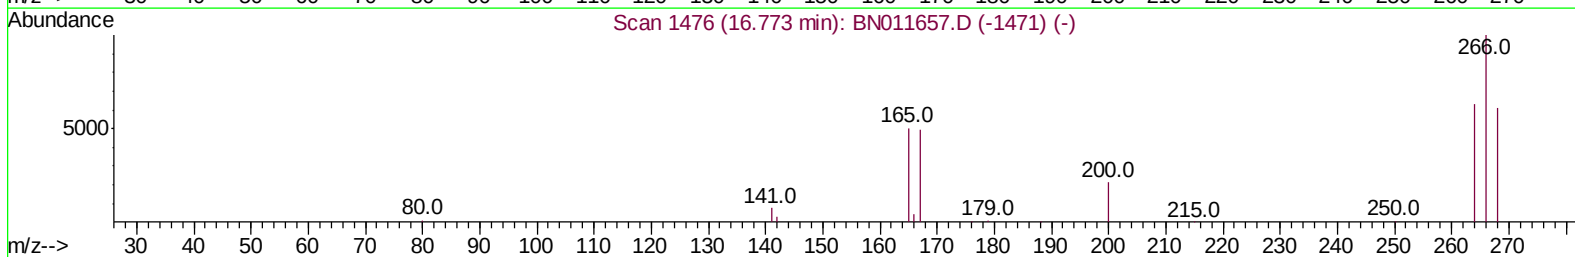
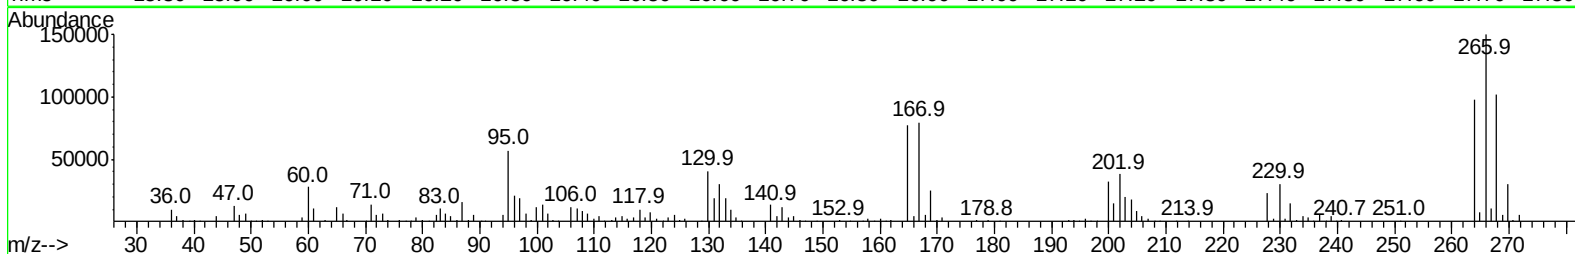


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN090920\
Data File : BN011776.D
Acq On : 10 Sep 2020 00:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 01:22:54 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN082720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 09 10:54:46 2020
Response via : Initial Calibration

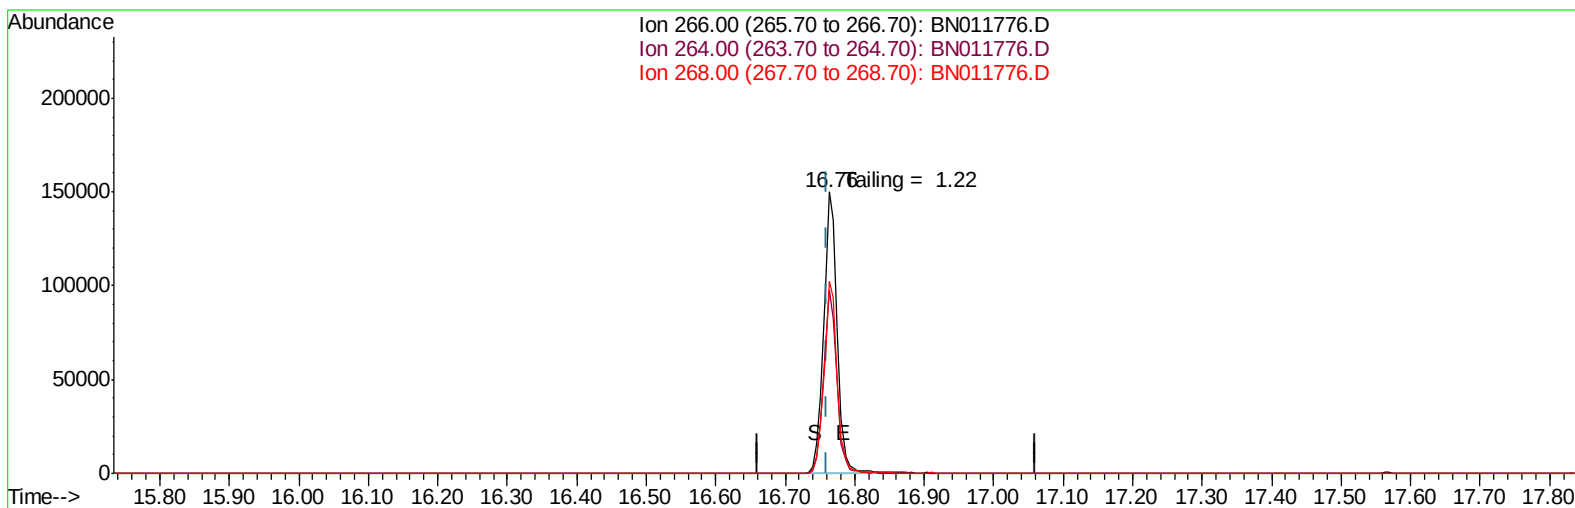

TIC: BN011776.D

(24) Pentachlorophenol

16.763min (+0.002) 5967.22ng

response 198889

Ion	Exp%	Act%
266.00	100	100
264.00	61.90	64.83
268.00	66.20	66.79
0.00	0.00	0.00