


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090920\
 Data File : BN011761.D
 Acq On : 09 Sep 2020 09:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 09 10:54:46 2020

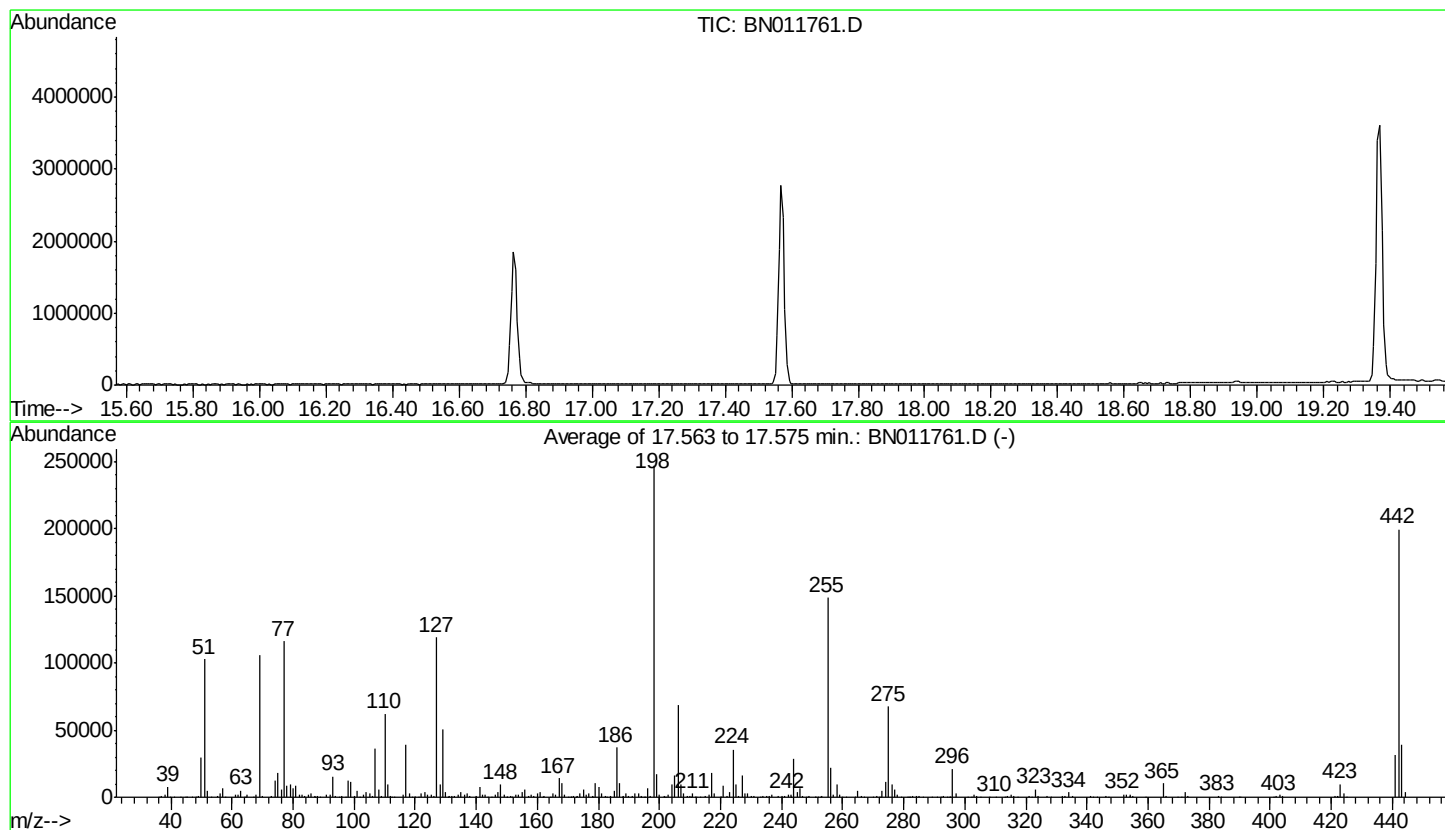

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.6	102605	PASS
68	69	0.00	2	1.5	1634	PASS
69	198	0.00	100	43.0	106112	PASS
70	69	0.00	2	0.5	545	PASS
127	198	10	80	48.1	118824	PASS
197	198	0.00	2	0.4	1015	PASS
198	198	100	100	100.0	246869	PASS
199	198	5	9	6.8	16737	PASS
275	198	10	60	27.3	67493	PASS
365	198	1	100	4.1	10166	PASS
441	198	0.01	100	12.9	31925	PASS
442	198	50	100	80.7	199330	PASS
443	442	15	24	19.4	38765	PASS