


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN090920\
 Data File : BN011776.D
 Acq On : 10 Sep 2020 00:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 09 10:54:46 2020

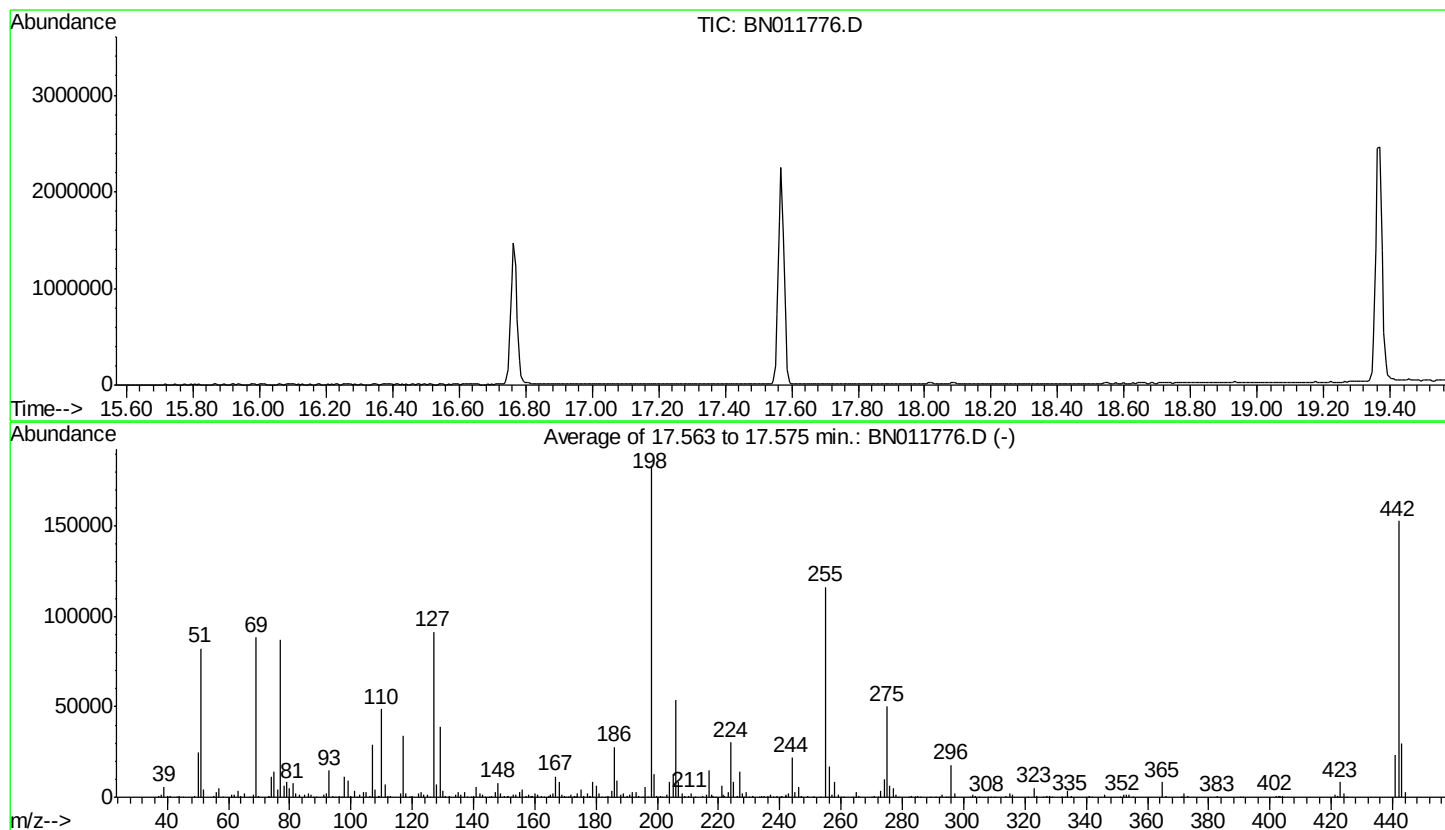

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.8	82224	PASS
68	69	0.00	2	1.5	1363	PASS
69	198	0.00	100	48.2	88442	PASS
70	69	0.00	2	0.6	573	PASS
127	198	10	80	49.9	91485	PASS
197	198	0.00	2	0.2	337	PASS
198	198	100	100	100.0	183424	PASS
199	198	5	9	6.9	12603	PASS
275	198	10	60	27.4	50216	PASS
365	198	1	100	4.6	8414	PASS
441	198	0.01	100	12.6	23133	PASS
442	198	50	100	83.4	152890	PASS
443	442	15	24	19.2	29413	PASS