

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090924\
 Data File : BN033818.D
 Acq On : 09 Sep 2024 14:49
 Operator : MA/JU
 Sample : P3886-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MW-06-6.5-090624

Quant Time: Sep 10 03:16:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN090424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 04 18:36:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.509	152	4033	0.400	ng	0.00
7) Naphthalene-d8	10.271	136	10158	0.400	ng	# 0.00
13) Acenaphthene-d10	14.146	164	4614	0.400	ng	-0.01
19) Phenanthrene-d10	16.892	188	9323	0.400	ng	#-0.01
29) Chrysene-d12	21.112	240	7273	0.400	ng	0.00
35) Perylene-d12	23.265	264	7730	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.154	112	1481	0.120	ng	0.00
5) Phenol-d6	6.700	99	1008	0.069	ng	0.00
8) Nitrobenzene-d5	8.649	82	2872	0.332	ng	0.00
11) 2-Methylnaphthalene-d10	11.865	152	4653	0.324	ng	0.00
14) 2,4,6-Tribromophenol	15.651	330	755	0.324	ng	0.00
15) 2-Fluorobiphenyl	12.767	172	6688	0.348	ng	0.00
27) Fluoranthene-d10	18.938	212	9569	0.416	ng	0.00
31) Terphenyl-d14	19.555	244	6857	0.442	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.168	88	981	0.214	ng	# 1
3) n-Nitrosodimethylamine	3.392	42	1585	0.294	ng	# 1
18) Fluorene	15.215	166	374	0.022	ng	# 26
34) Bis(2-ethylhexyl)phtha...	21.059	149	2134	0.151	ng	# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090924\
Data File : BN033818.D
Acq On : 09 Sep 2024 14:49
Operator : MA/JU
Sample : P3886-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MW-06-6.5-090624


Quant Time: Sep 10 03:16:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 18:36:01 2024
Response via : Initial Calibration

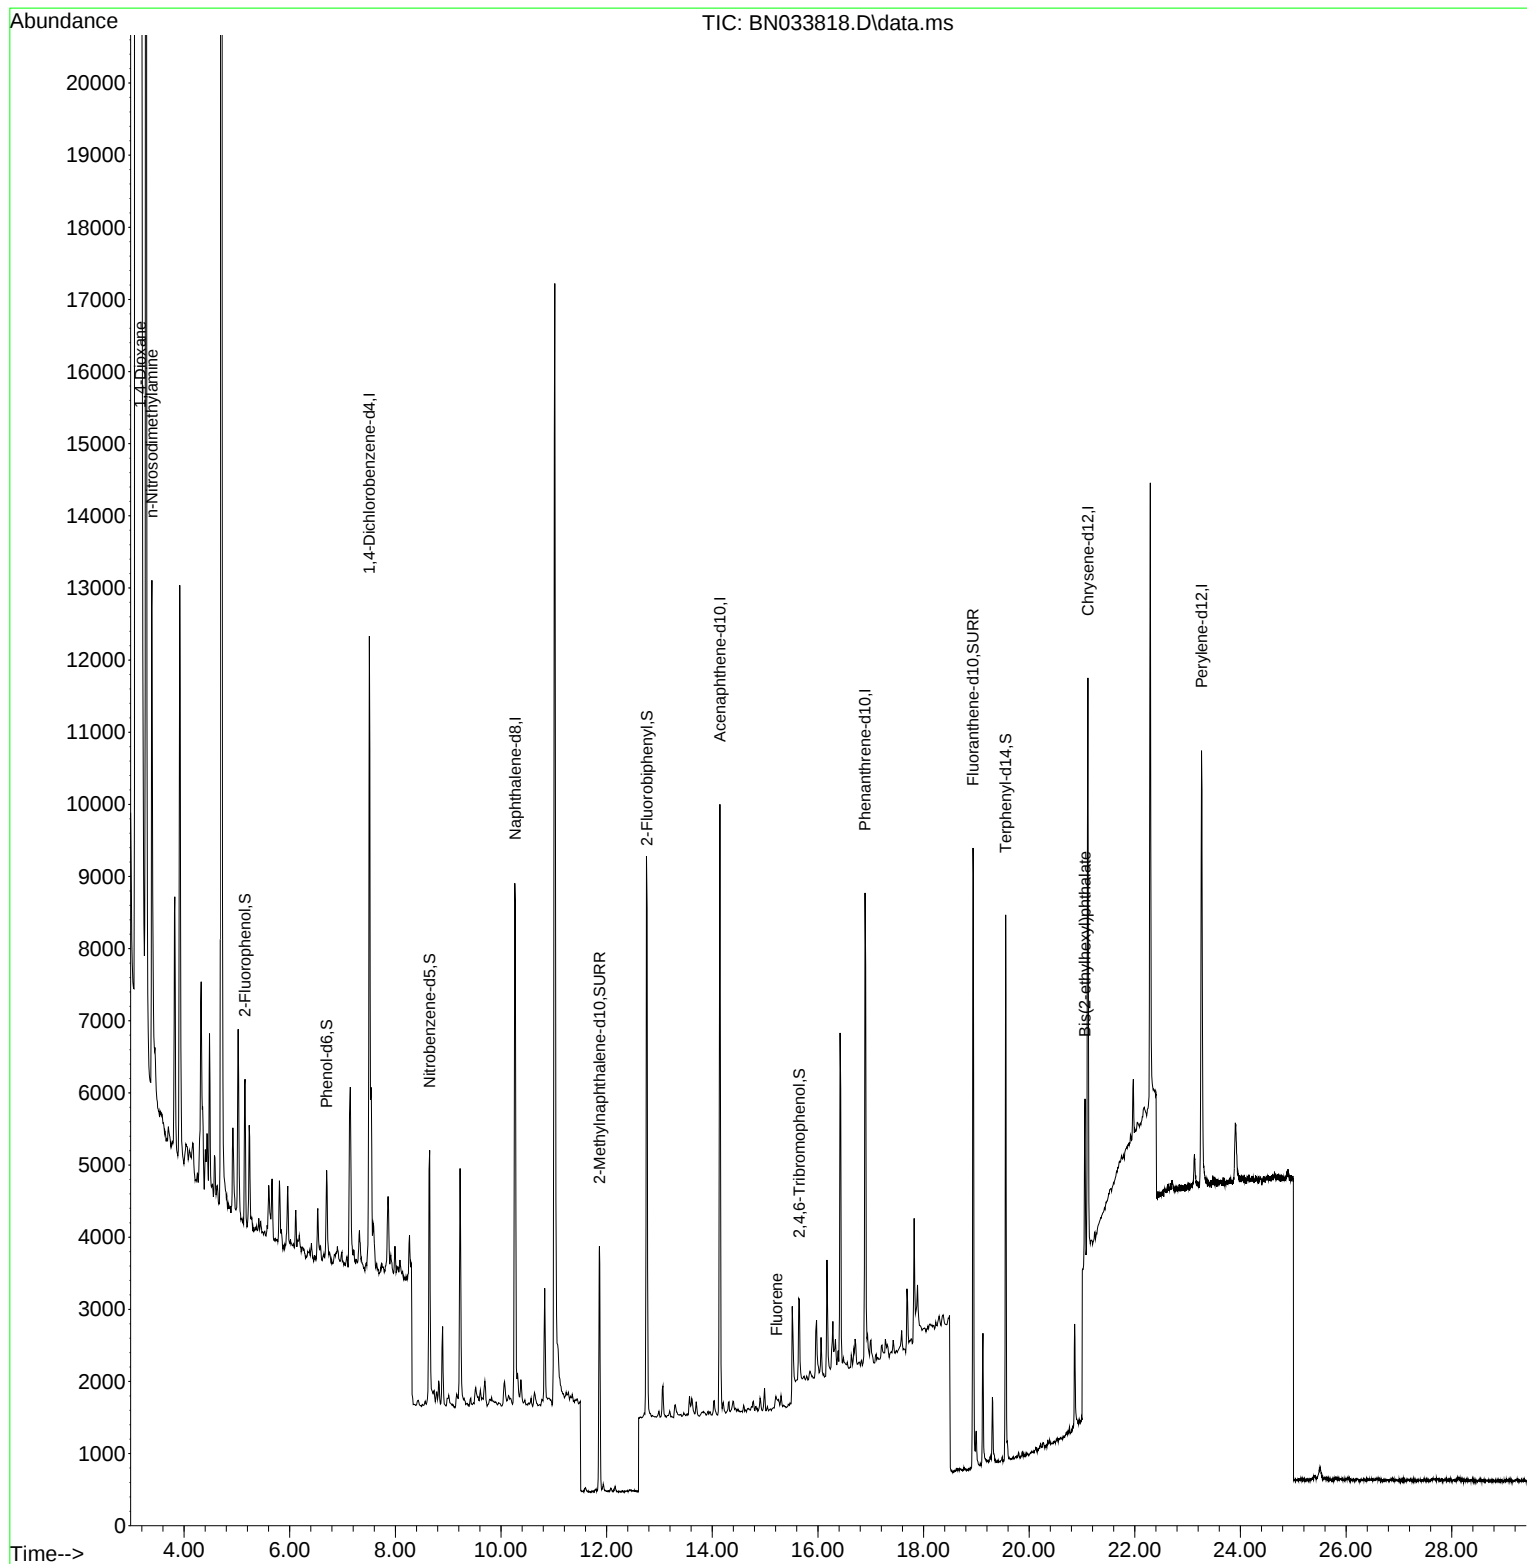

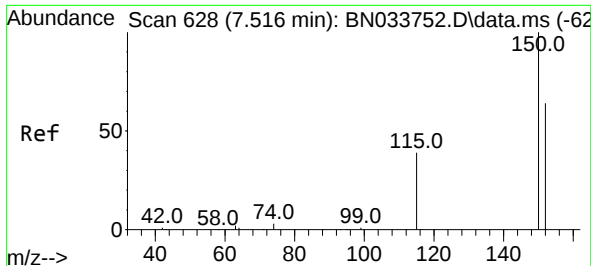




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.509 min Scan# 61
 Delta R.T. -0.007 min
 Lab File: BN033818.D
 Acq: 09 Sep 2024 14:49

Instrument :
 BNA_N
 ClientSampleId :
 MW-06-6.5-090624

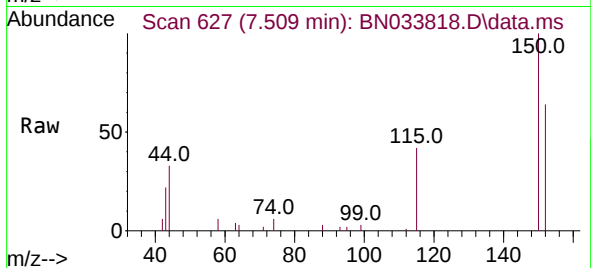

Tgt Ion:152 Resp: 4033




Ion	Ratio	Lower	Upper
152	100		
150	155.5	123.3	184.9
115	64.9	51.0	76.4

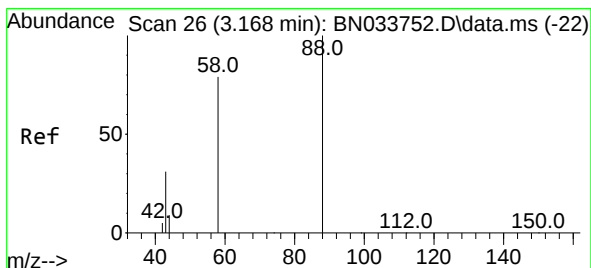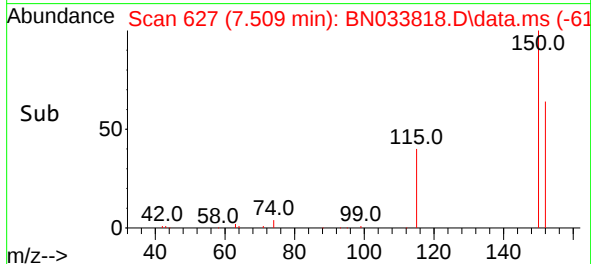


#2
 1,4-Dioxane
 Concen: 0.214 ng
 RT: 3.168 min Scan# 26
 Delta R.T. 0.000 min
 Lab File: BN033818.D
 Acq: 09 Sep 2024 14:49

Tgt Ion: 88 Resp: 981

Ion	Ratio	Lower	Upper
88	100		
43	956.7	29.0	43.4#
58	76.2	64.1	96.1


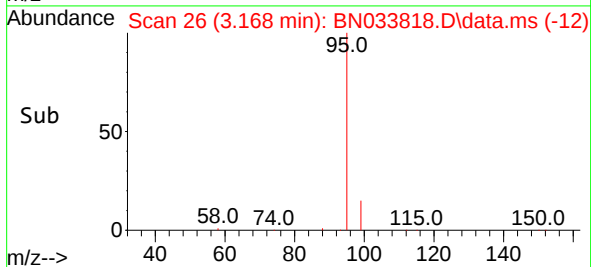

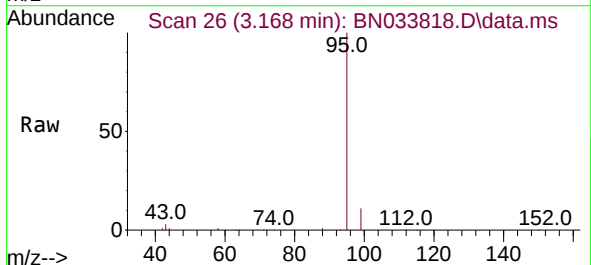


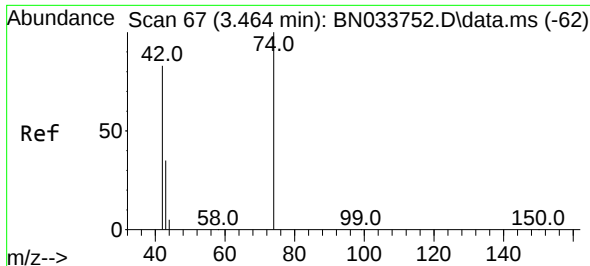

#3
n-Nitrosodimethylamine
Concen: 0.294 ng
RT: 3.392 min Scan# 51
Delta R.T. -0.072 min
Lab File: BN033818.D
Acq: 09 Sep 2024 14:49




Instrument :
BNA_N
ClientSampleId :
MW-06-6.5-090624


Tgt Ion: 42 Resp: 1585
Ion Ratio Lower Upper
42 100
74 2.6 93.5 140.3#
44 125.7 7.4 11.0#

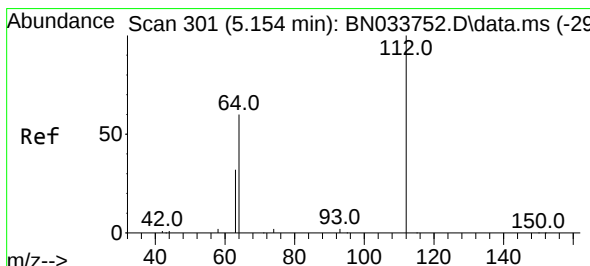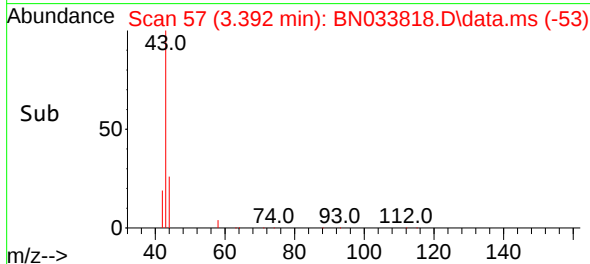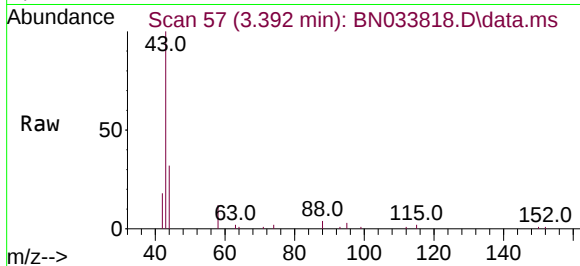

#4
2-Fluorophenol
Concen: 0.120 ng
RT: 5.154 min Scan# 301
Delta R.T. -0.000 min
Lab File: BN033818.D
Acq: 09 Sep 2024 14:49

Tgt Ion: 112 Resp: 1481
Ion Ratio Lower Upper
112 100
64 59.6 47.6 71.4
63 33.2 25.9 38.9


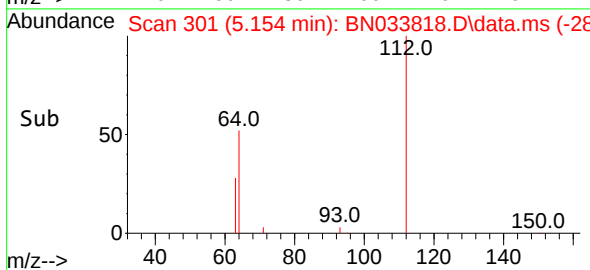

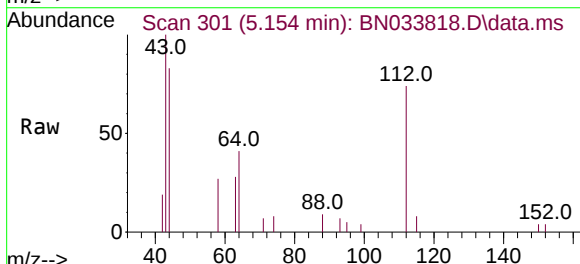


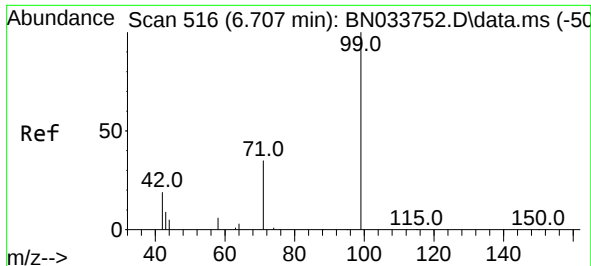

#5
Phenol-d6
Concen: 0.069 ng
RT: 6.700 min Scan# 516
Delta R.T. -0.007 min
Lab File: BN033818.D
Acq: 09 Sep 2024 14:49




Instrument :
BNA_N
ClientSampleId :
MW-06-6.5-090624


Tgt Ion: 99 Resp: 1008
Ion Ratio Lower Upper
99 100
42 33.2 18.0 27.0#
71 44.1 28.7 43.1#

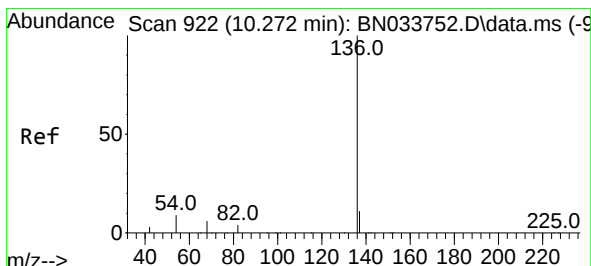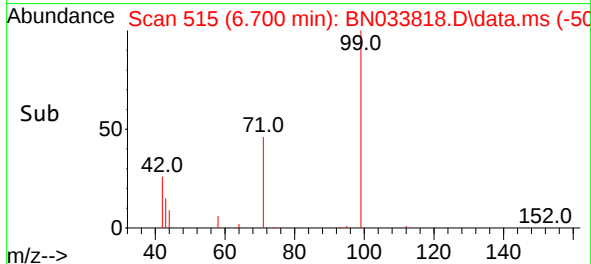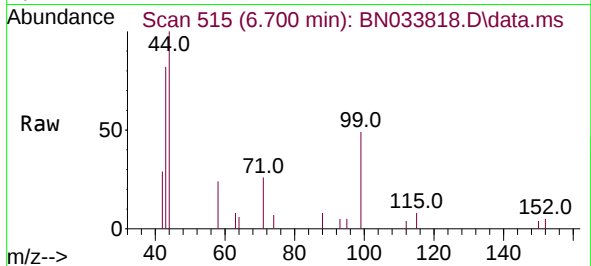

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.271 min Scan# 922
Delta R.T. -0.000 min
Lab File: BN033818.D
Acq: 09 Sep 2024 14:49

Tgt Ion: 136 Resp: 10158
Ion Ratio Lower Upper
136 100
137 11.4 9.0 13.4
54 7.1 8.1 12.1#
68 4.7 5.8 8.8#


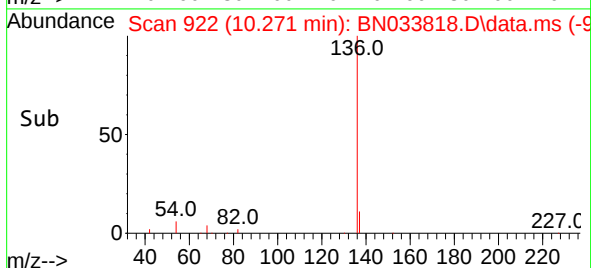
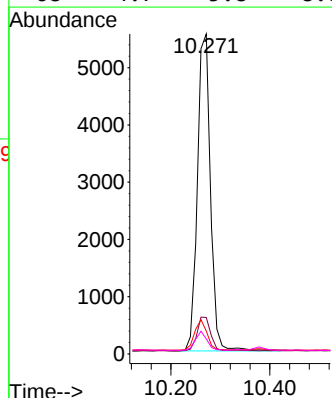
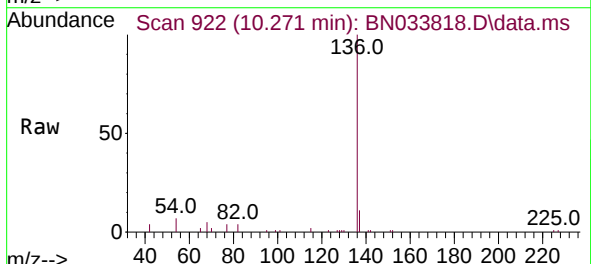


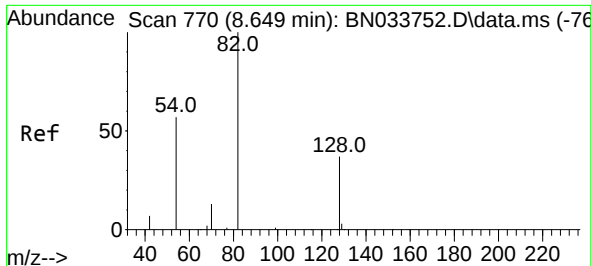

#8
Nitrobenzene-d5
Concen: 0.332 ng
RT: 8.649 min Scan# 770
Delta R.T. -0.000 min
Lab File: BN033818.D
Acq: 09 Sep 2024 14:49




Instrument :
BNA_N
ClientSampleId :
MW-06-6.5-090624


Tgt Ion: 82 Resp: 2872
Ion Ratio Lower Upper
82 100
128 46.8 31.3 46.9
54 55.9 46.9 70.3

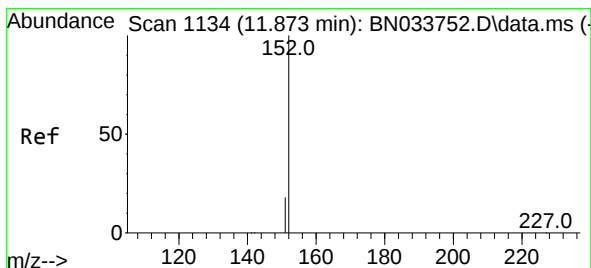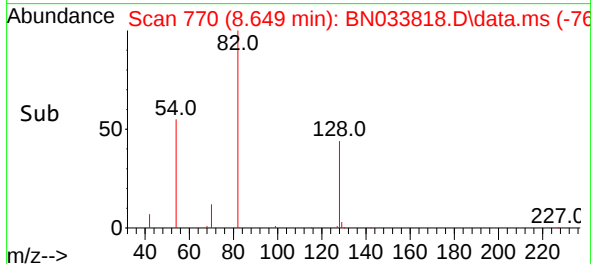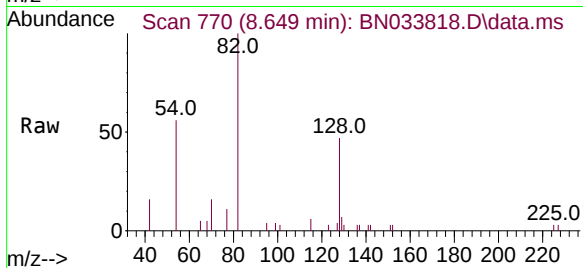

#11
2-Methylnaphthalene-d10
Concen: 0.324 ng
RT: 11.865 min Scan# 1132
Delta R.T. -0.008 min
Lab File: BN033818.D
Acq: 09 Sep 2024 14:49

Tgt Ion: 152 Resp: 4653
Ion Ratio Lower Upper
152 100
151 21.2 16.7 25.1


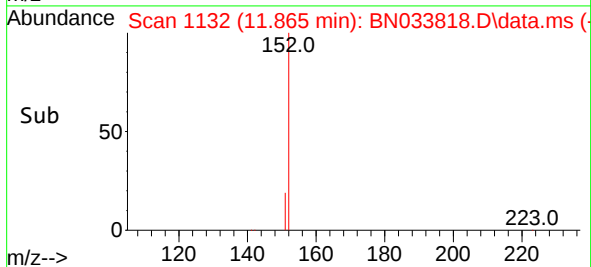

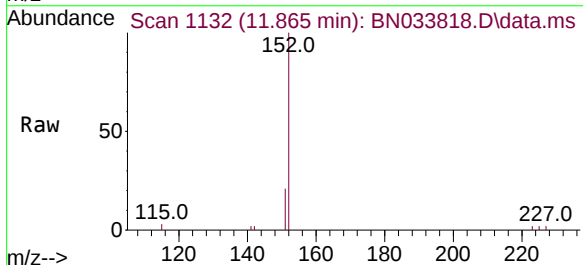


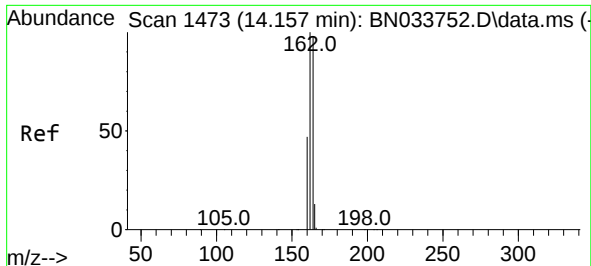

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.146 min Scan# 1472
Delta R.T. -0.011 min
Lab File: BN033818.D
Acq: 09 Sep 2024 14:49




Instrument :
BNA_N
ClientSampleId :
MW-06-6.5-090624


Tgt Ion:164 Resp: 4614
Ion Ratio Lower Upper
164 100
162 103.9 82.0 123.0
160 50.1 39.1 58.7

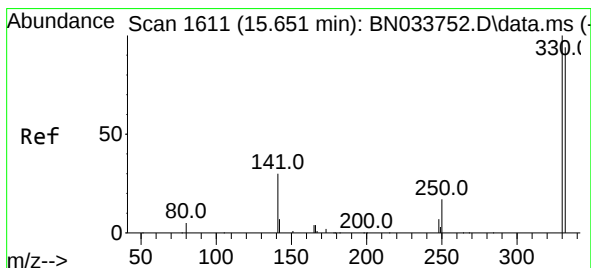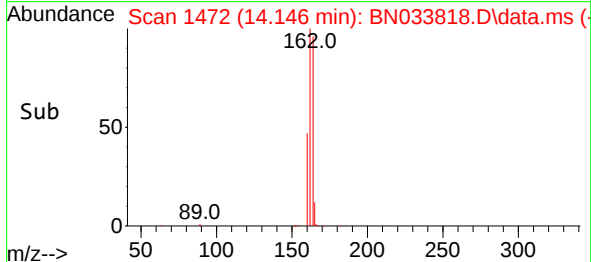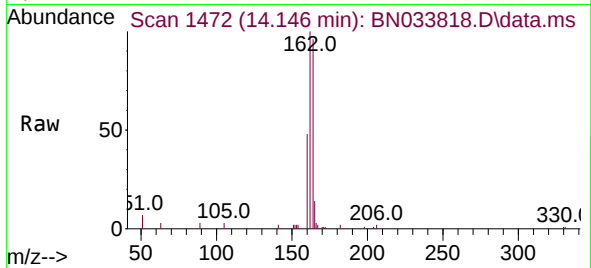

#14
2,4,6-Tribromophenol
Concen: 0.324 ng
RT: 15.651 min Scan# 1611
Delta R.T. -0.000 min
Lab File: BN033818.D
Acq: 09 Sep 2024 14:49

Tgt Ion:330 Resp: 755
Ion Ratio Lower Upper
330 100
332 96.7 74.2 111.4
141 47.7 33.9 50.9


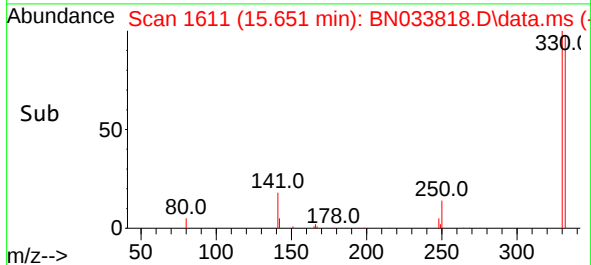

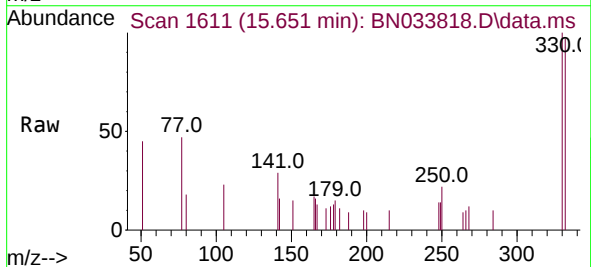


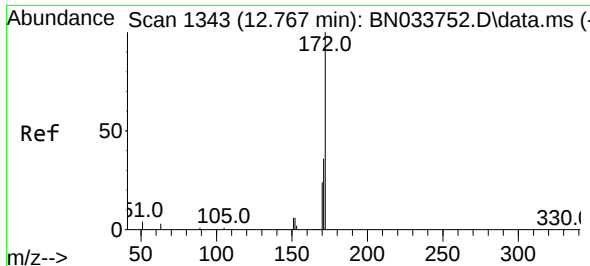

#15
2-Fluorobiphenyl
Concen: 0.348 ng
RT: 12.767 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN033818.D
Acq: 09 Sep 2024 14:49




Instrument :
BNA_N
ClientSampleId :
MW-06-6.5-090624


Tgt Ion:	172	Resp:	6688
Ion	Ratio	Lower	Upper
172	100		
171	34.2	28.8	43.2
170	22.7	19.7	29.5

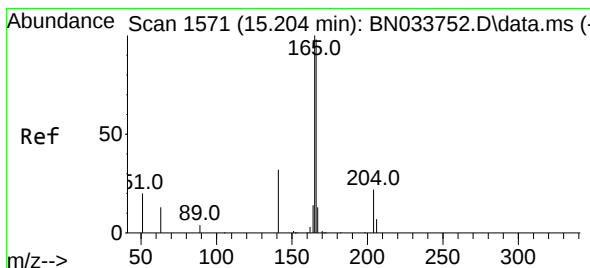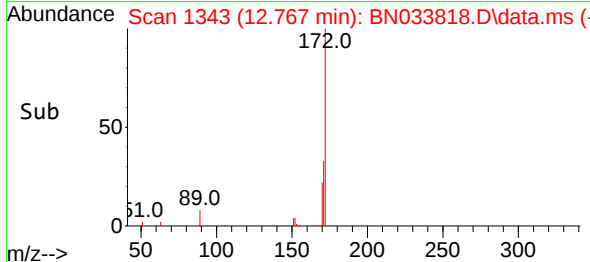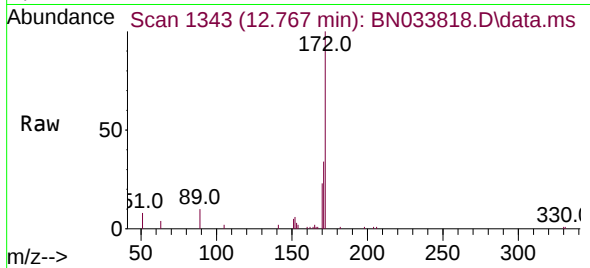

#18
Fluorene
Concen: 0.022 ng
RT: 15.215 min Scan# 1572
Delta R.T. 0.010 min
Lab File: BN033818.D
Acq: 09 Sep 2024 14:49

Tgt Ion:	166	Resp:	374
Ion	Ratio	Lower	Upper
166	100		
165	19.3	78.8	118.2#
167	0.0	10.6	16.0#


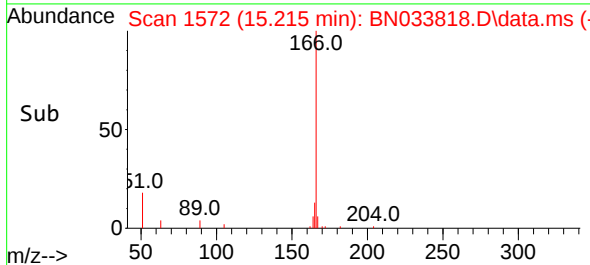

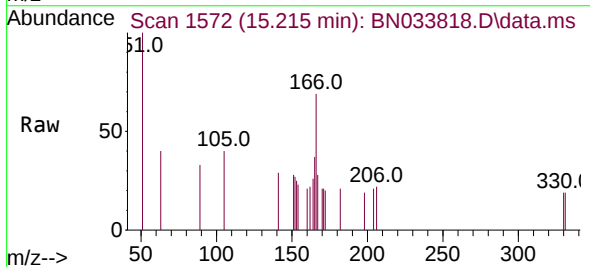


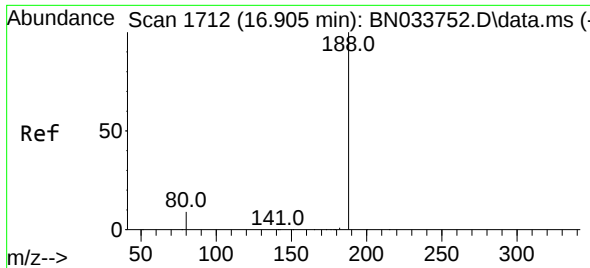

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.892 min Scan# 1711
Delta R.T. -0.013 min
Lab File: BN033818.D
Acq: 09 Sep 2024 14:49




Instrument :
BNA_N
ClientSampleId :
MW-06-6.5-090624


Tgt Ion:188 Resp: 9323
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 14.7 7.9 11.9#

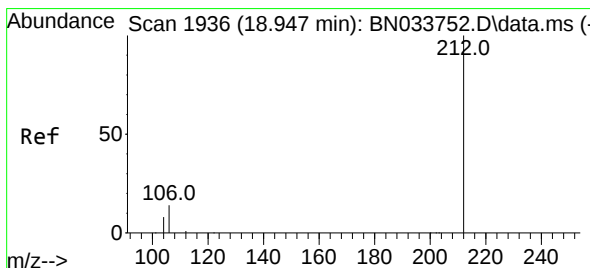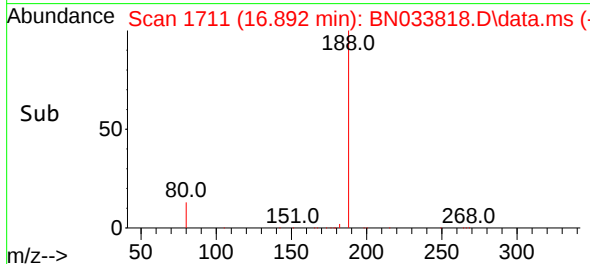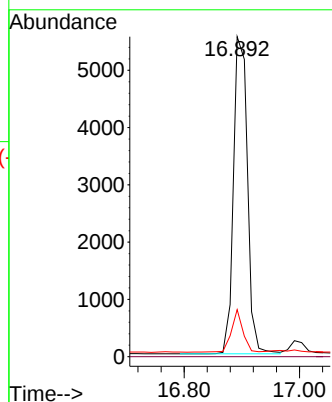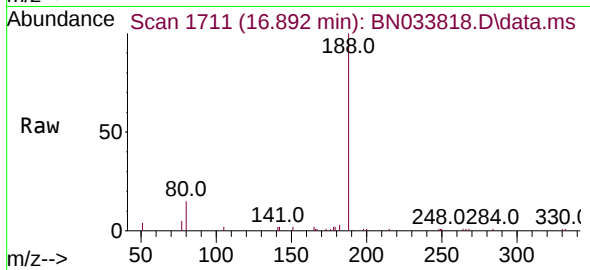

#27
Fluoranthene-d10
Concen: 0.416 ng
RT: 18.938 min Scan# 1934
Delta R.T. -0.009 min
Lab File: BN033818.D
Acq: 09 Sep 2024 14:49

Tgt Ion:212 Resp: 9569
Ion Ratio Lower Upper
212 100
106 13.5 11.5 17.3
104 7.7 6.6 9.8


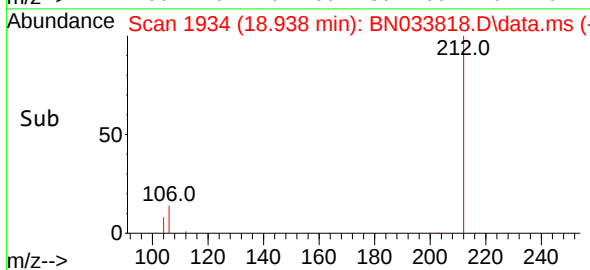
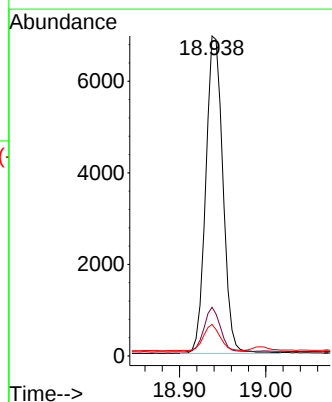
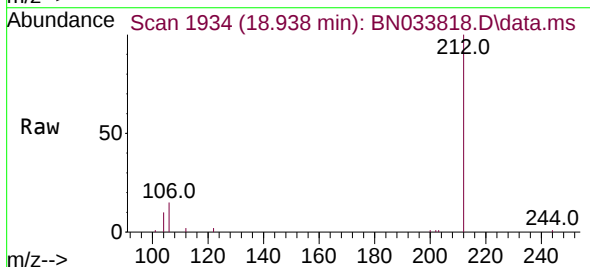


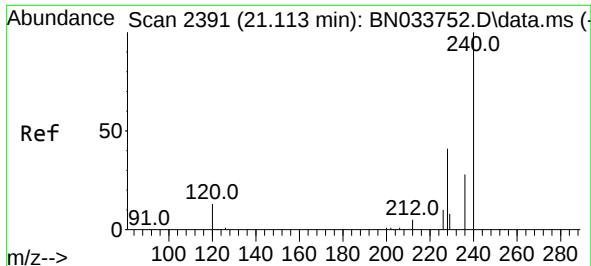

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.112 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN033818.D
Acq: 09 Sep 2024 14:49




Instrument :
BNA_N
ClientSampleId :
MW-06-6.5-090624


Tgt Ion:240 Resp: 7273
Ion Ratio Lower Upper
240 100
120 14.0 13.7 20.5
236 28.9 23.4 35.2

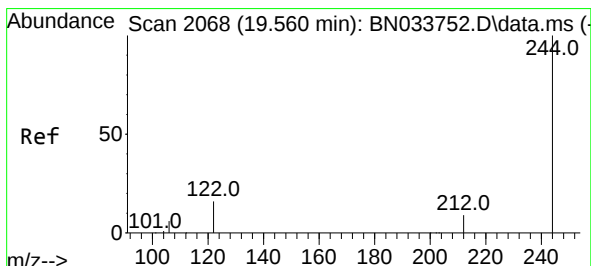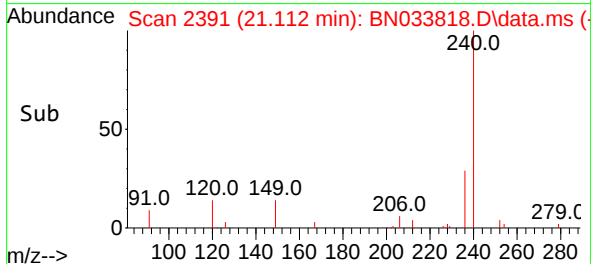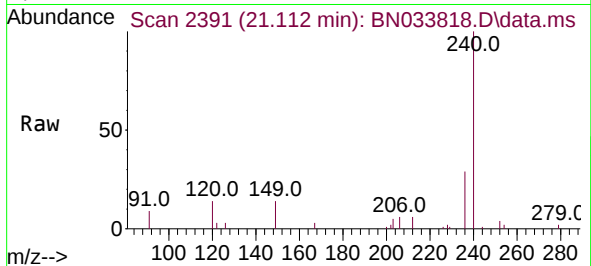

#31
Terphenyl-d14
Concen: 0.442 ng
RT: 19.555 min Scan# 2067
Delta R.T. -0.005 min
Lab File: BN033818.D
Acq: 09 Sep 2024 14:49

Tgt Ion:244 Resp: 6857
Ion Ratio Lower Upper
244 100
212 10.5 7.9 11.9
122 16.8 13.2 19.8


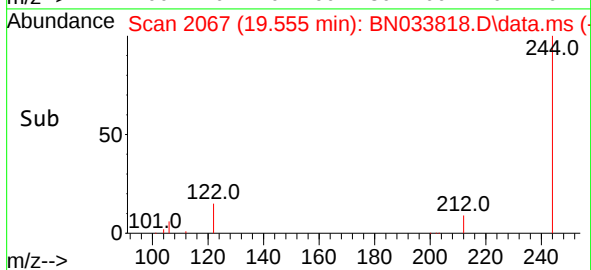

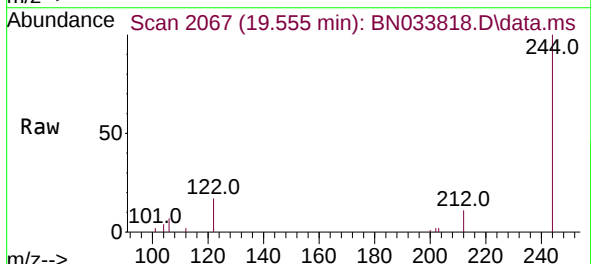


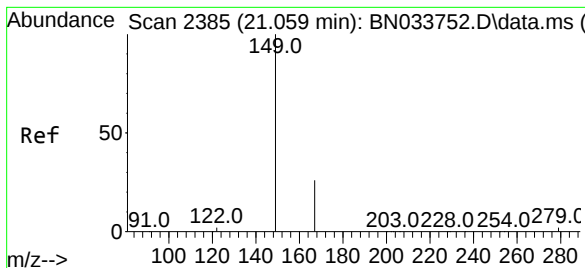

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.151 ng
 RT: 21.059 min Scan# 2134
 Delta R.T. -0.000 min
 Lab File: BN033818.D
 Acq: 09 Sep 2024 14:49

Instrument :
 BNA_N
 ClientSampleId :
 MW-06-6.5-090624

Tgt Ion:149 Resp: 2134
 Ion Ratio Lower Upper
 149 100
 167 25.0 21.0 31.4
 279 3.8 2.4 3.6#

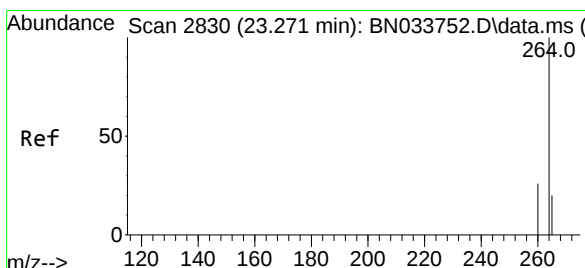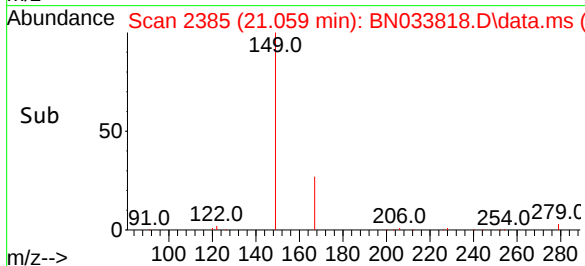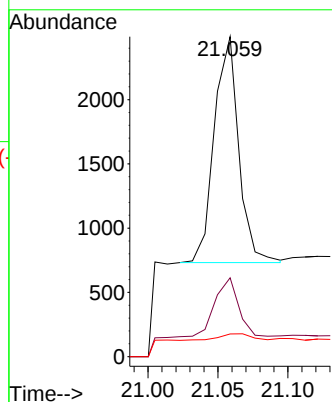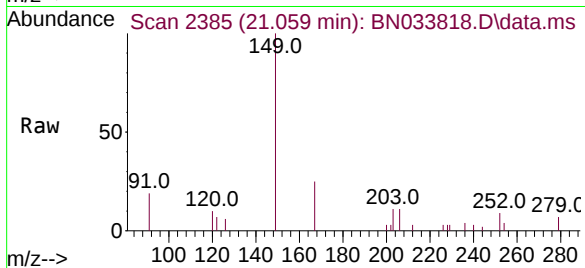

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.265 min Scan# 2828
 Delta R.T. -0.006 min
 Lab File: BN033818.D
 Acq: 09 Sep 2024 14:49

Tgt Ion:264 Resp: 7730
 Ion Ratio Lower Upper
 264 100
 260 26.2 21.1 31.7
 265 92.4 72.0 108.0

