
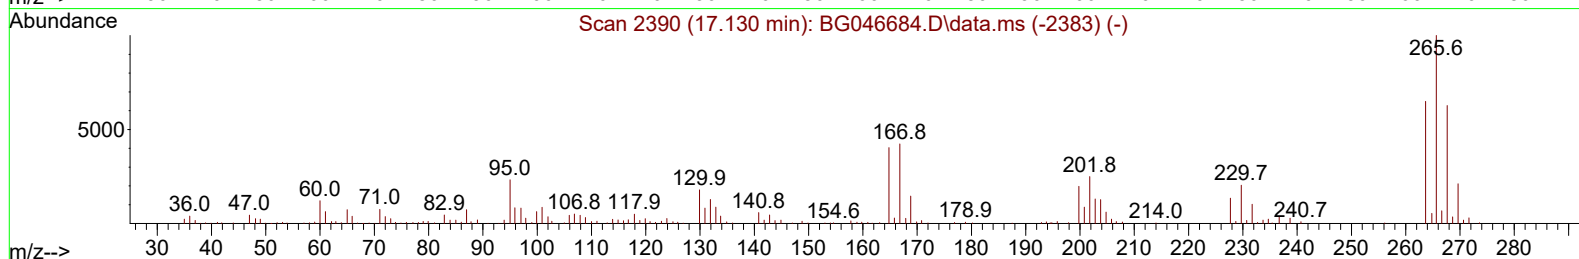
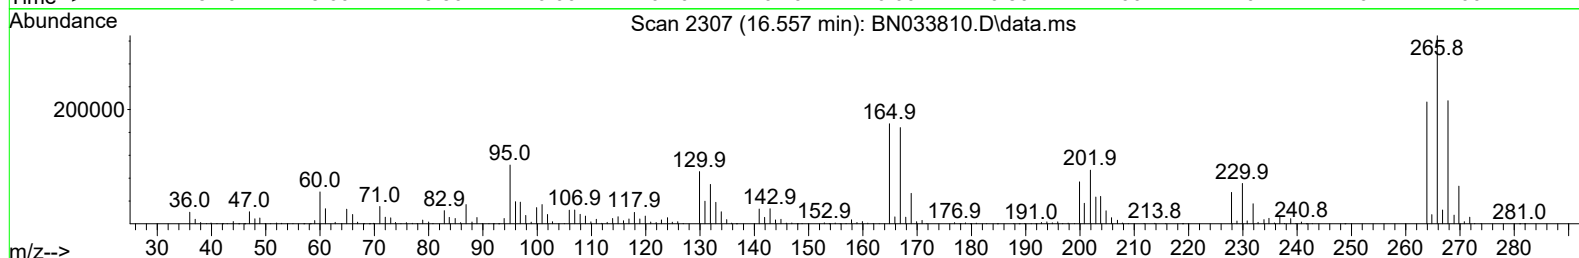


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090924\
Data File : BN033810.D
Acq On : 09 Sep 2024 09:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 09 11:55:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 07 02:00:52 2024
Response via : Initial Calibration

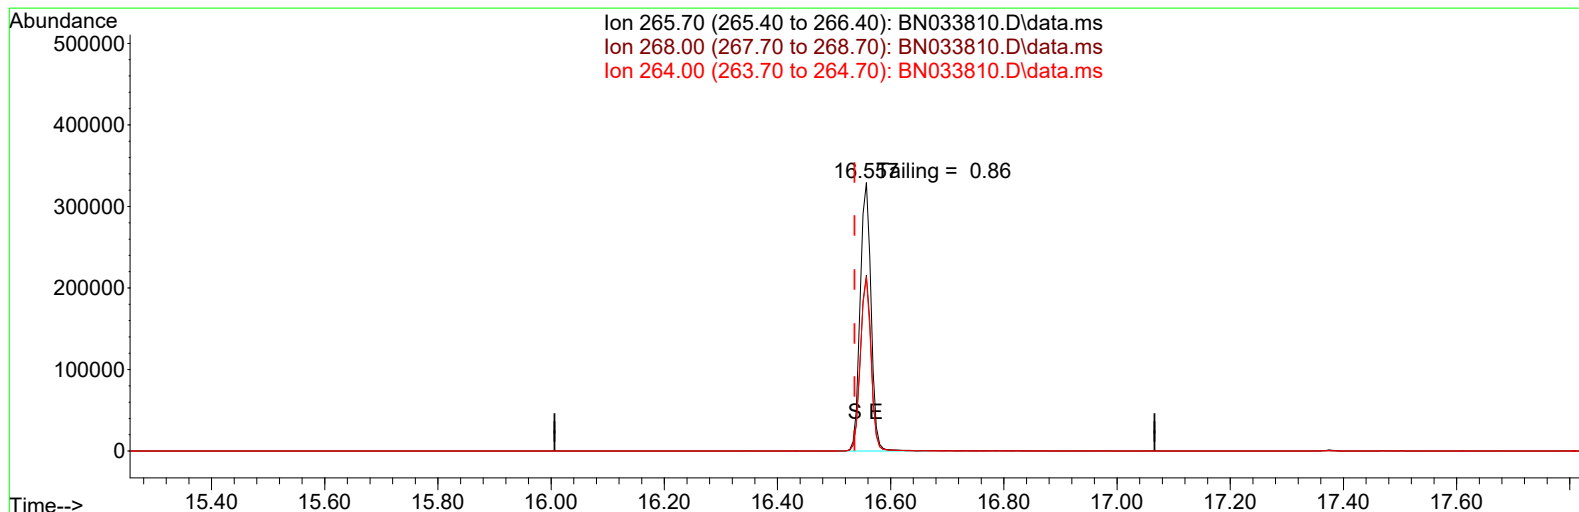

TIC: BN033810.D\data.ms

(70) Pentachlorophenol (C)




16.557min (+ 0.021) 19790.47 ng

response 438442

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.49
264.00	61.60	64.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090924\
Data File : BN033810.D
Acq On : 09 Sep 2024 09:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 09 11:55:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 07 02:00:52 2024
Response via : Initial Calibration

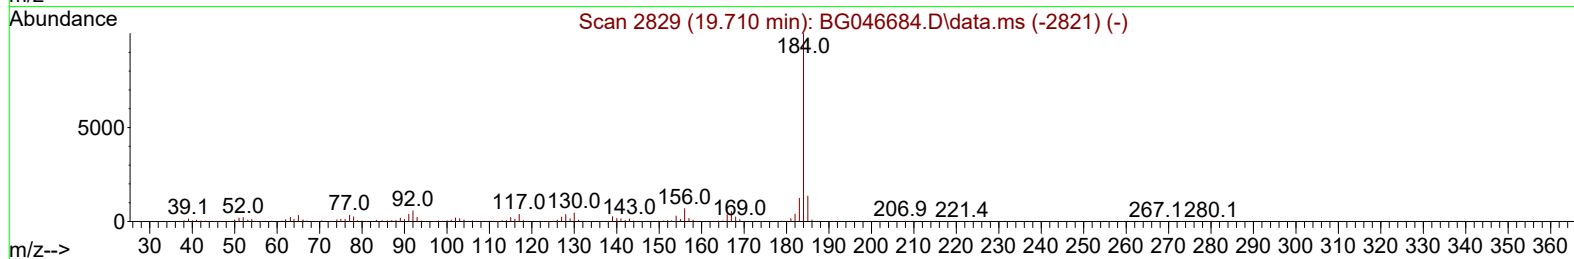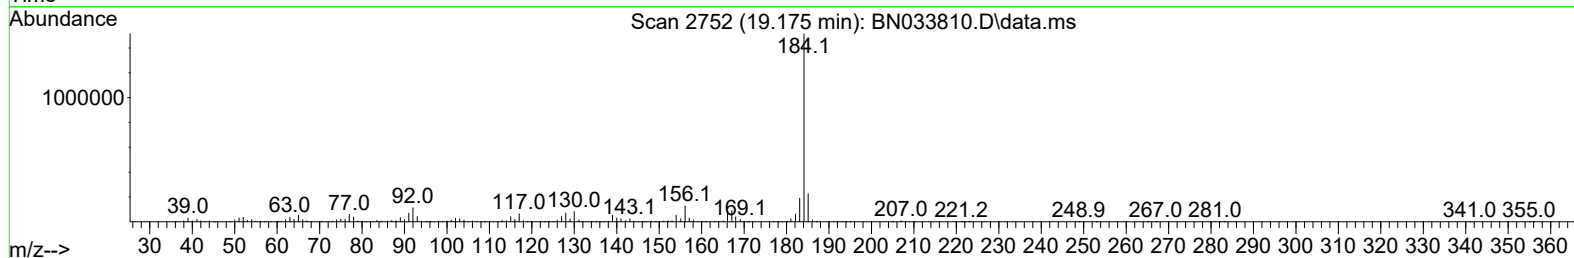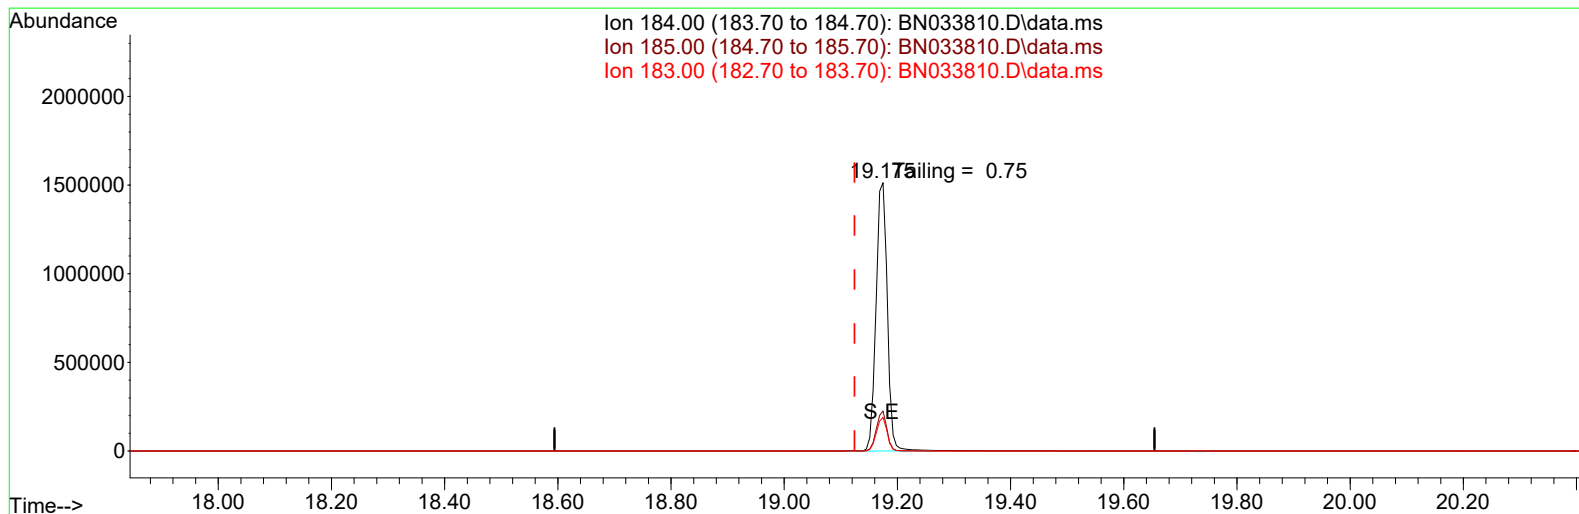

TIC: BN033810.D\data.ms

(77) Benzidine

19.175min (+ 0.050) 0.00 ng

response 2100370

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.95
183.00	13.20	12.52
0.00	0.00	0.00