

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091022\
 Data File : BN021712.D
 Acq On : 10 Sep 2022 23:50
 Operator : CG/JU
 Sample : N4558-09
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BP-VPB-RW5-GW-278-280

Quant Time: Sep 12 01:15:14 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 09 23:19:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.062	152	5893	0.400	ng	0.00
7) Naphthalene-d8	10.887	136	19651	0.400	ng	-0.01
13) Acenaphthene-d10	14.707	164	11557	0.400	ng	-0.01
19) Phenanthrene-d10	17.459	188	23200	0.400	ng	-0.01
29) Chrysene-d12	21.646	240	14118	0.400	ng	# 0.00
35) Perylene-d12	24.159	264	10951	0.400	ng	#-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.592	112	2111	0.183	ng	0.00
5) Phenol-d6	7.217	99	1721	0.117	ng	0.00
8) Nitrobenzene-d5	9.232	82	4402	0.332	ng	0.00
11) 2-Methylnaphthalene-d10	12.474	152	14665	0.331	ng	0.00
14) 2,4,6-Tribromophenol	16.208	330	1540	0.406	ng	0.00
15) 2-Fluorobiphenyl	13.339	172	16654	0.330	ng	0.00
27) Fluoranthene-d10	19.489	212	21844	0.366	ng	0.00
31) Terphenyl-d14	20.079	244	15446	0.487	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.403	88	8686	1.178	ng	# 91
12) 2-Methylnaphthalene	12.180	142	11	0.128	ng	# 1
24) Pentachlorophenol	17.121	266	18	0.206	ng	# 59
34) Bis(2-ethylhexyl)phtha...	21.539	149	2978	0.150	ng	# 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091022\
Data File : BN021712.D
Acq On : 10 Sep 2022 23:50
Operator : CG/JU
Sample : N4558-09
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BP-VPB-RW5-GW-278-280

Quant Time: Sep 12 01:15:14 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 09 23:19:14 2022
Response via : Initial Calibration



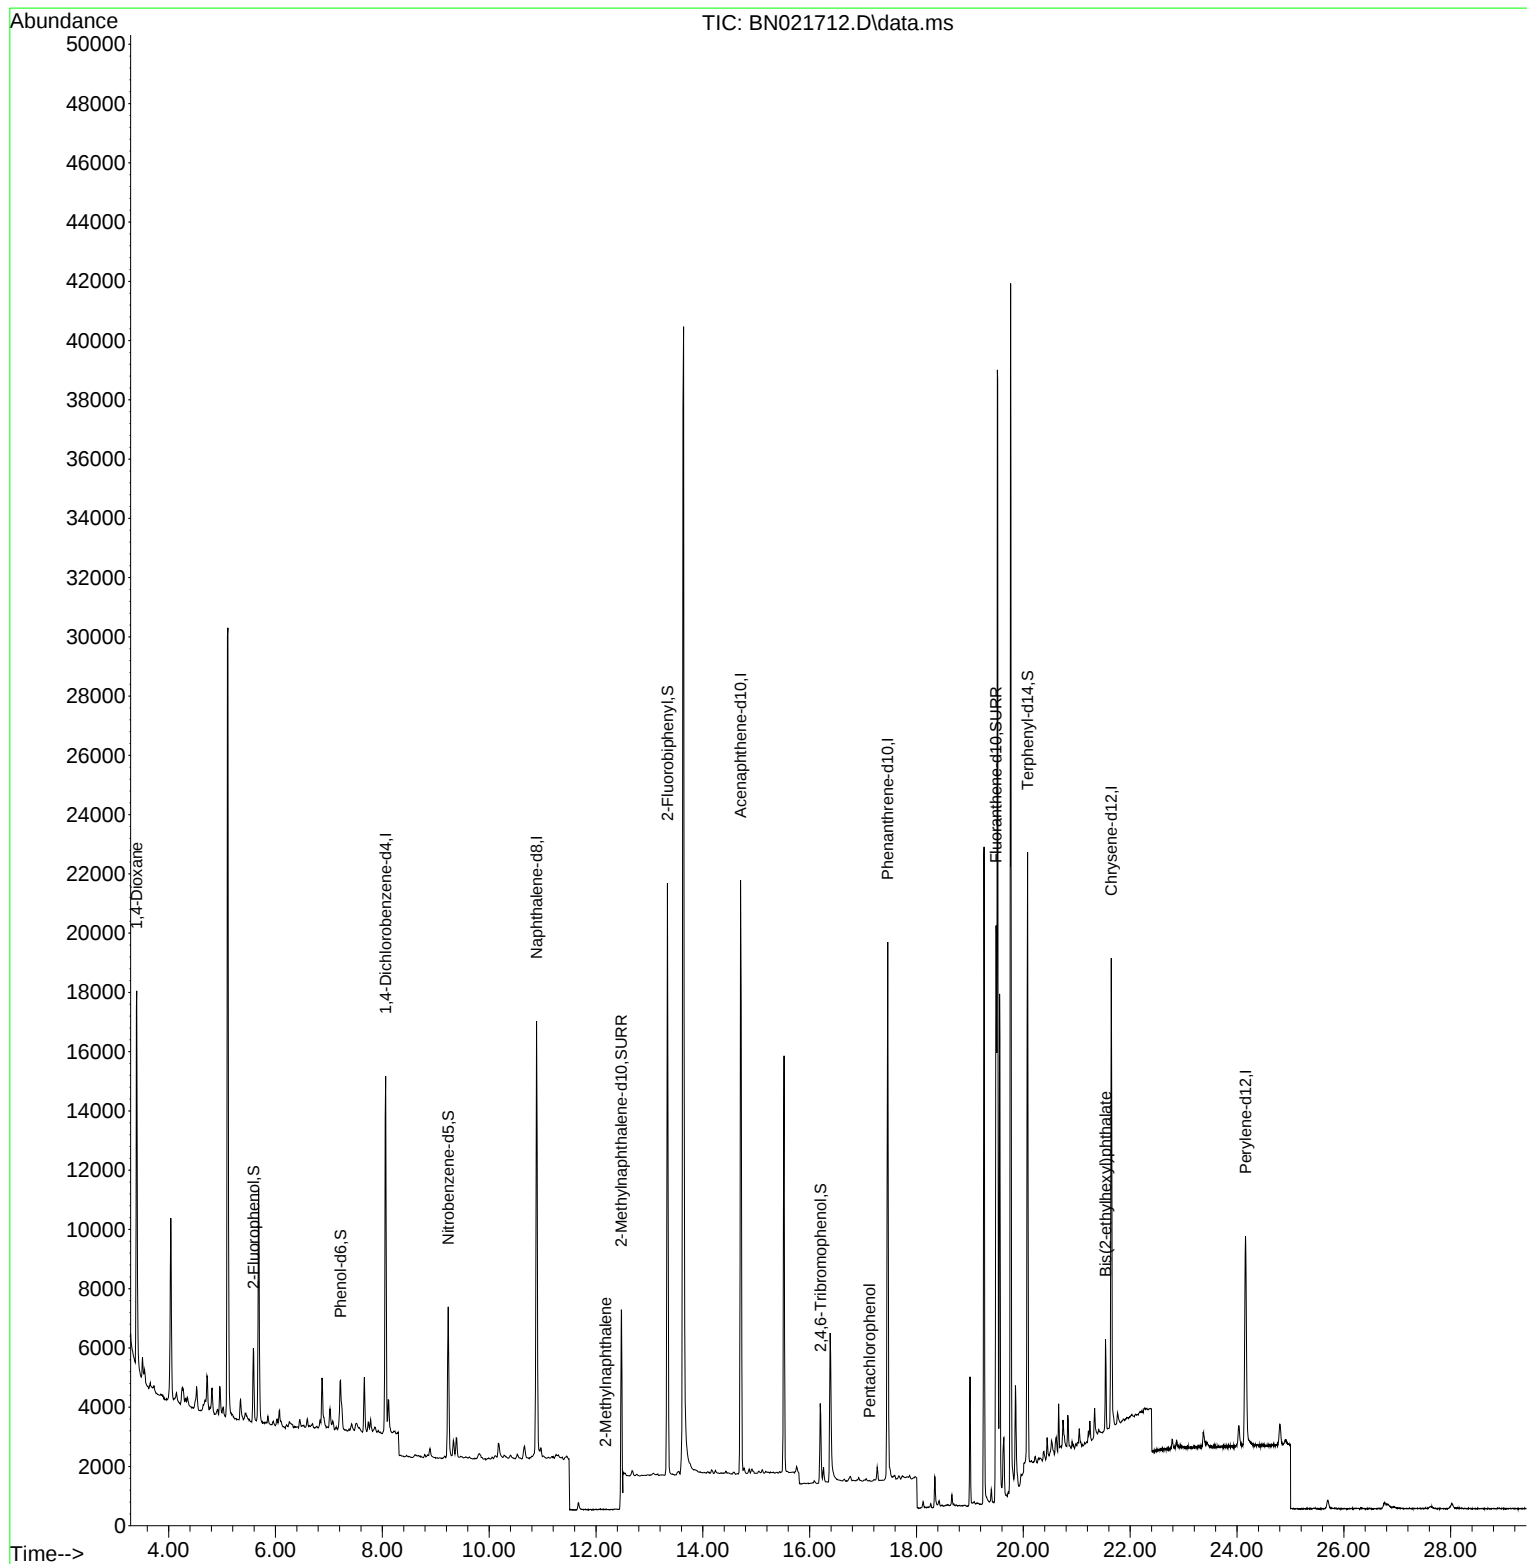




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 8.062 min Scan# 6
 Delta R.T. -0.000 min
 Lab File: BN021712.D
 Acq: 10 Sep 2022 23:50




Instrument :
 BNA_N
 ClientSampleId :
 BP-VPB-RW5-GW-278-280

Tgt Ion:152 Resp: 5893
 Ion Ratio Lower Upper
 152 100
 150 153.5 121.4 182.0
 115 61.3 48.6 72.8

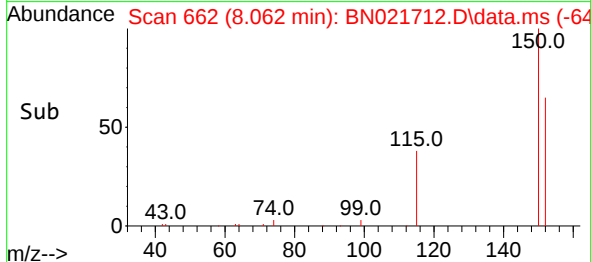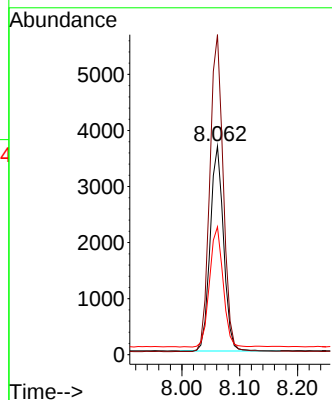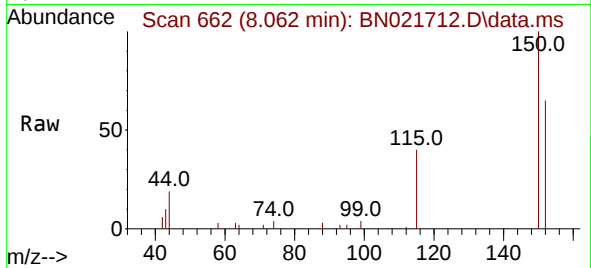

#2
 1,4-Dioxane
 Concen: 1.178 ng
 RT: 3.403 min Scan# 17
 Delta R.T. -0.000 min
 Lab File: BN021712.D
 Acq: 10 Sep 2022 23:50

Tgt Ion: 88 Resp: 8686
 Ion Ratio Lower Upper
 88 100
 43 30.7 35.8 53.8#
 58 70.9 57.1 85.7

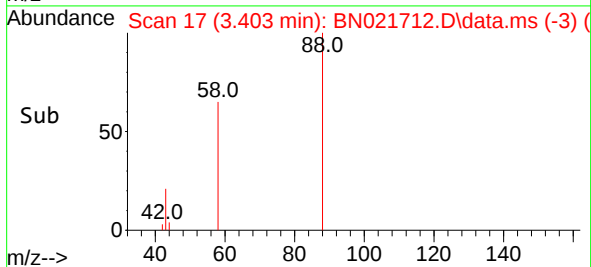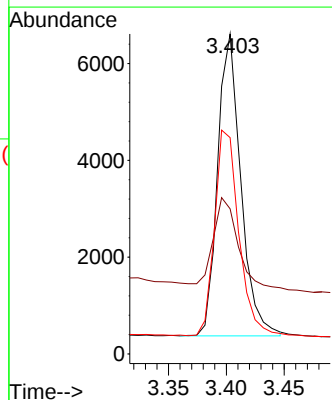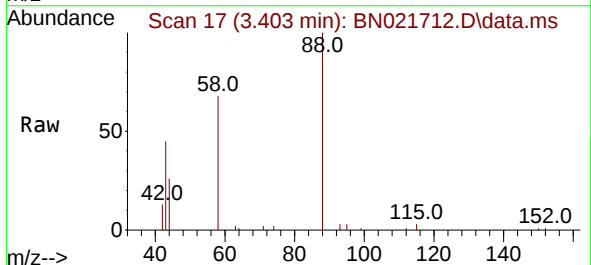



#4

2-Fluorophenol

Concen: 0.183 ng

RT: 5.592 min Scan# 31

Delta R.T. -0.000 min

Lab File: BN021712.D

Acq: 10 Sep 2022 23:50

Instrument :

BNA_N

ClientSampleId :

BP-VPB-RW5-GW-278-280





Tgt Ion:112 Resp: 2111

Ion Ratio Lower Upper

112 100

64 57.3 43.5 65.3

63 29.7 22.6 34.0

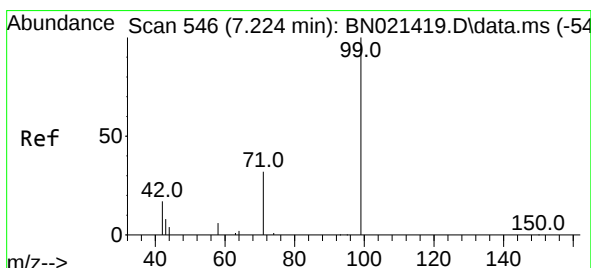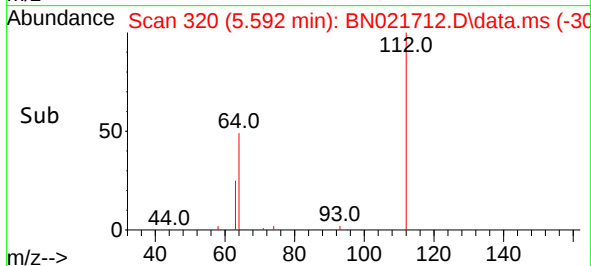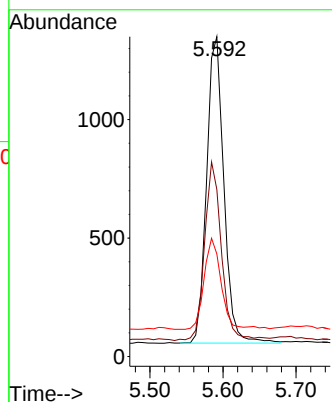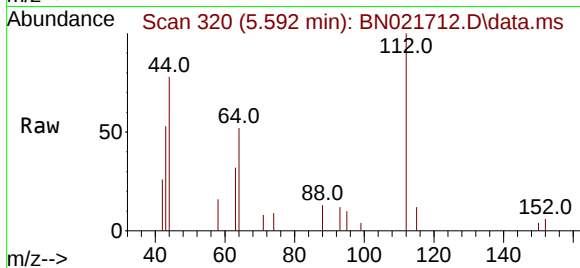

#5

Phenol-d6

Concen: 0.117 ng

RT: 7.217 min Scan# 545

Delta R.T. -0.000 min

Lab File: BN021712.D

Acq: 10 Sep 2022 23:50




Tgt Ion: 99 Resp: 1721

Ion Ratio Lower Upper

99 100

42 22.0 15.5 23.3

71 36.3 24.2 36.2#

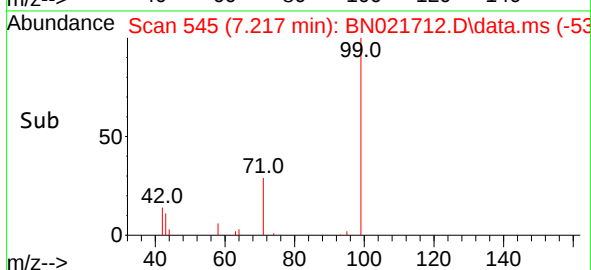
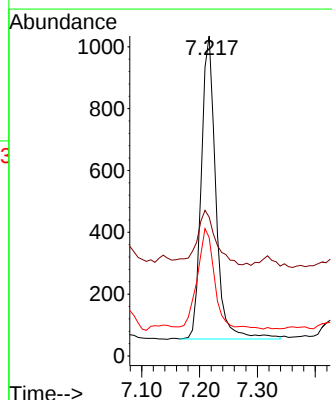
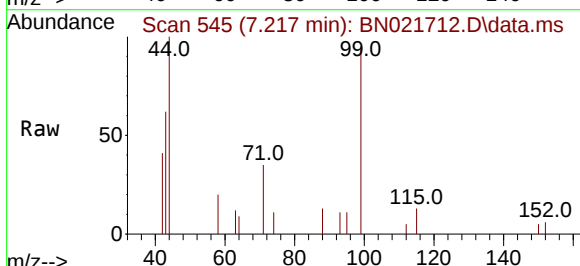




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.887 min Scan# 91
Delta R.T. -0.011 min
Lab File: BN021712.D
Acq: 10 Sep 2022 23:50




Instrument :
BNA_N
ClientSampleId :
BP-VPB-RW5-GW-278-280

Tgt Ion:	136	Resp:	19651
Ion Ratio	Lower	Upper	
136	100		
137	11.4	9.3	13.9
54	8.6	6.9	10.3
68	7.4	6.1	9.1

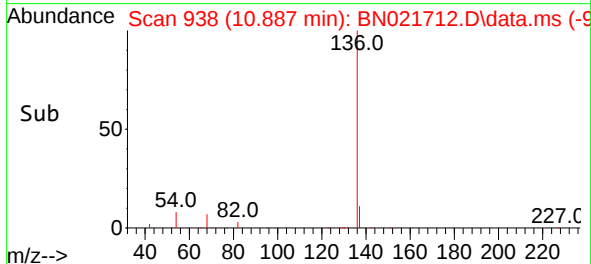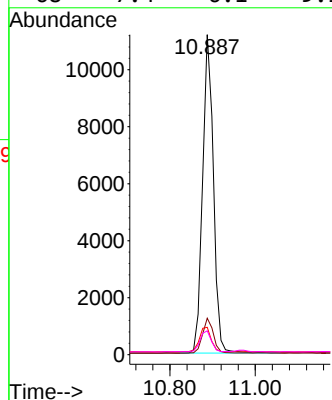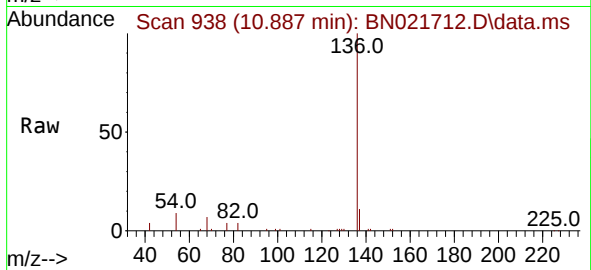

#8
Nitrobenzene-d5
Concen: 0.332 ng
RT: 9.232 min Scan# 783
Delta R.T. -0.000 min
Lab File: BN021712.D
Acq: 10 Sep 2022 23:50

Tgt Ion:	82	Resp:	4402
Ion Ratio	Lower	Upper	
82	100		
128	41.6	30.9	46.3
54	47.8	42.7	64.1

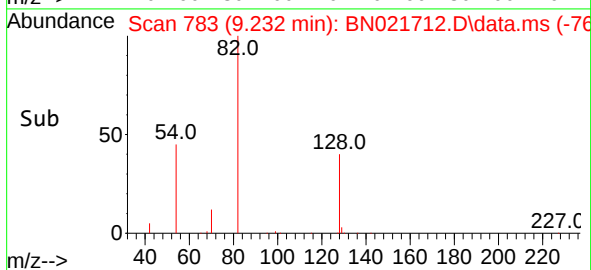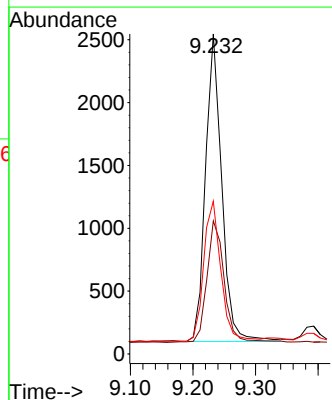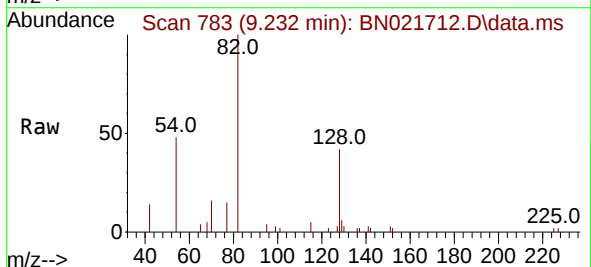



#11

2-Methylnaphthalene-d10

Concen: 0.331 ng

RT: 12.474 min Scan# 1174

Delta R.T. -0.004 min

Lab File: BN021712.D

Acq: 10 Sep 2022 23:50

Instrument :

BNA_N

ClientSampleId :





BP-VPB-RW5-GW-278-280

Tgt Ion:152 Resp: 14665

Ion Ratio Lower Upper

152 100

151 21.4 14.5 21.7

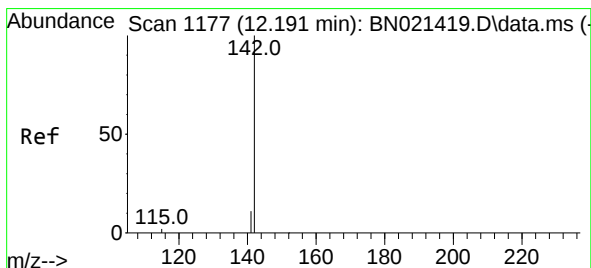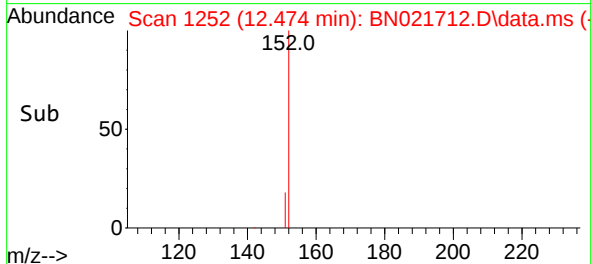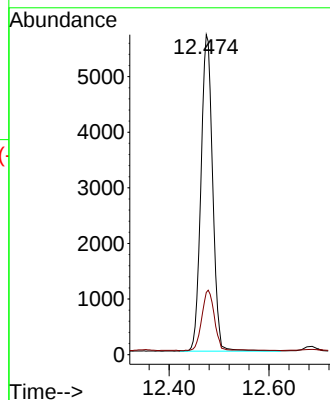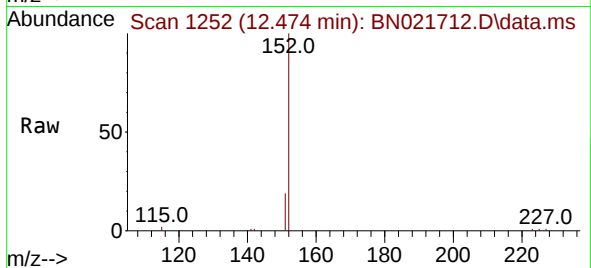

#12

2-Methylnaphthalene

Concen: 0.128 ng

RT: 12.180 min Scan# 1174

Delta R.T. -0.000 min

Lab File: BN021712.D

Acq: 10 Sep 2022 23:50




Tgt Ion:142 Resp: 11

Ion Ratio Lower Upper

142 100

141 105.9 12.2 18.2#

115 185.3 7.9 11.9#

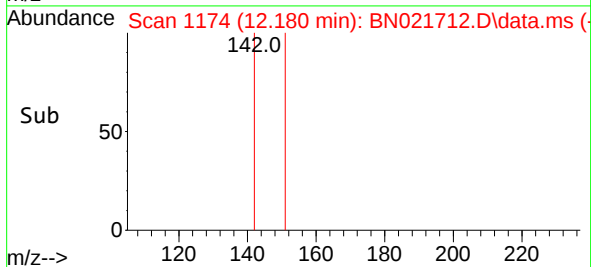
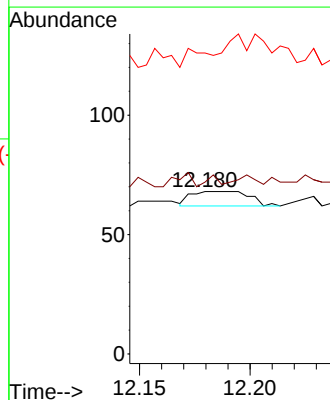
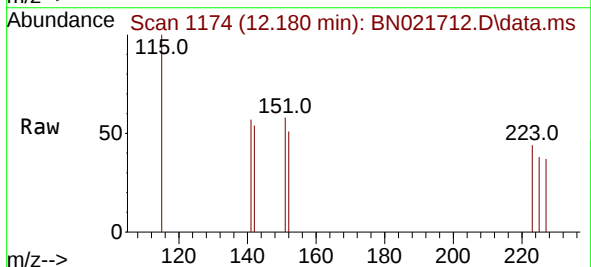




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.707 min Scan# 14
Delta R.T. -0.011 min
Lab File: BN021712.D
Acq: 10 Sep 2022 23:50




Instrument :
BNA_N
ClientSampleId :
BP-VPB-RW5-GW-278-280

Tgt Ion:164 Resp: 11557
Ion Ratio Lower Upper
164 100
162 104.3 82.2 123.4
160 51.0 39.5 59.3

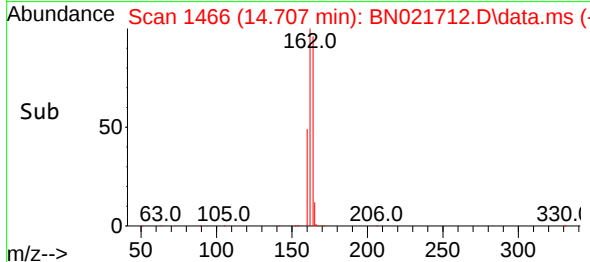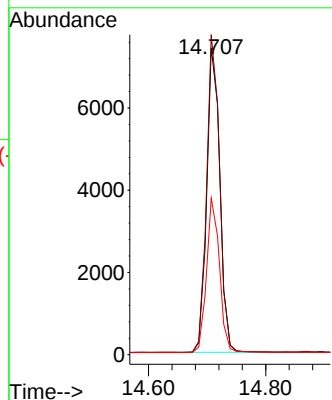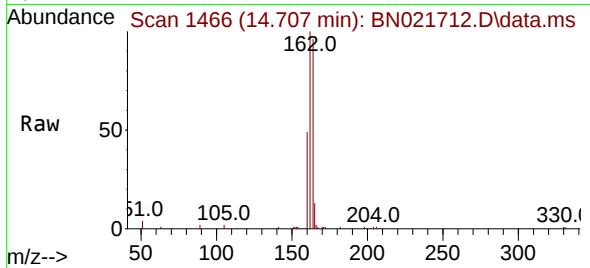

#14
2,4,6-Tribromophenol
Concen: 0.406 ng
RT: 16.208 min Scan# 1608
Delta R.T. -0.000 min
Lab File: BN021712.D
Acq: 10 Sep 2022 23:50

Tgt Ion:330 Resp: 1540
Ion Ratio Lower Upper
330 100
332 97.7 79.3 118.9
141 43.6 37.1 55.7

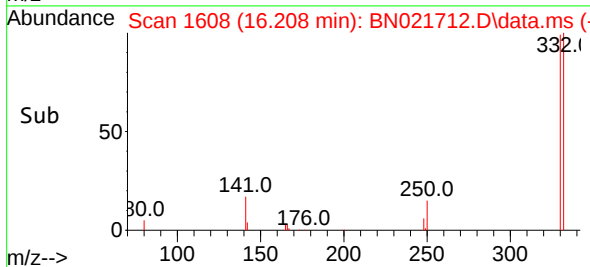
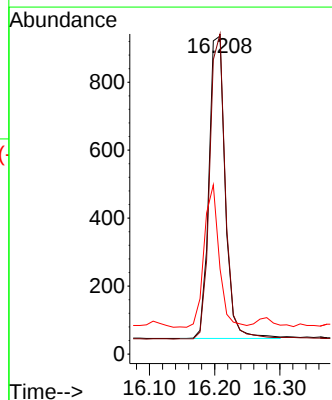
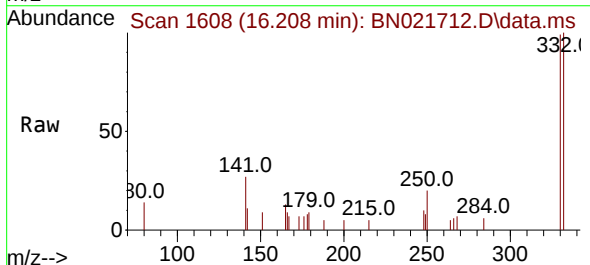




#15
2-Fluorobiphenyl
Concen: 0.330 ng
RT: 13.339 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN021712.D
Acq: 10 Sep 2022 23:50




Instrument :
BNA_N
ClientSampleId :
BP-VPB-RW5-GW-278-280


Tgt Ion:172 Resp: 16654
Ion Ratio Lower Upper
172 100
171 34.4 27.8 41.6
170 23.4 18.6 28.0

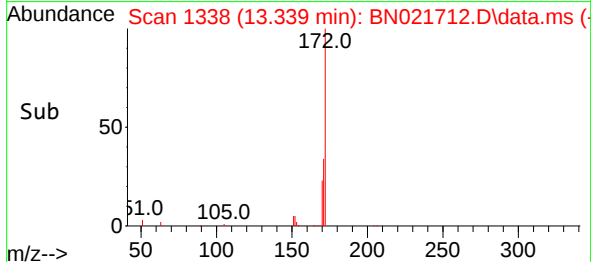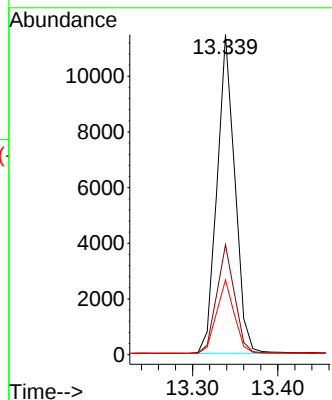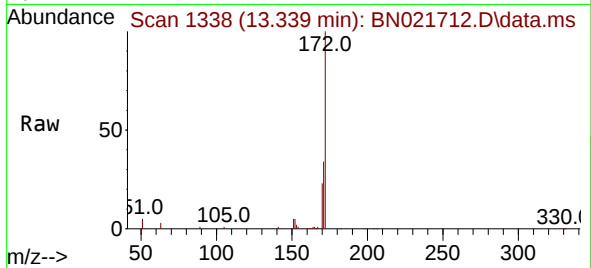

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.459 min Scan# 1730
Delta R.T. -0.010 min
Lab File: BN021712.D
Acq: 10 Sep 2022 23:50

Tgt Ion:188 Resp: 23200
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 12.5 9.5 14.3

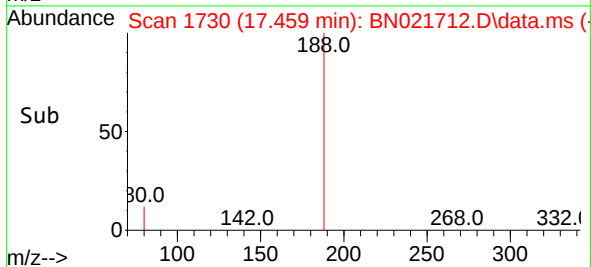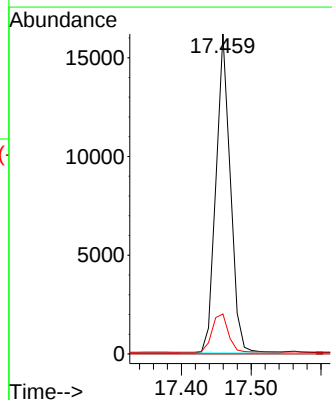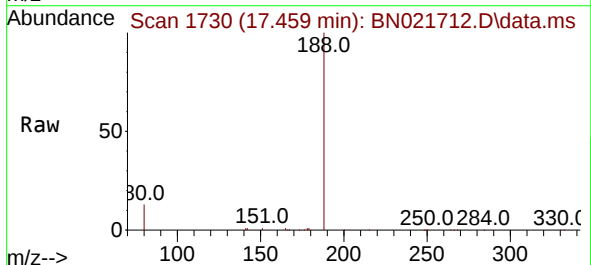

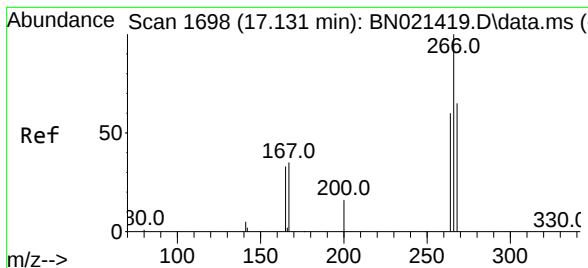

#24

Pentachlorophenol

Concen: 0.206 ng

RT: 17.121 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN021712.D

Acq: 10 Sep 2022 23:50





Instrument :

BNA_N

ClientSampleId :

BP-VPB-RW5-GW-278-280

Tgt Ion:266	Resp:	18
Ion Ratio	Lower	Upper
266	100	
264	88.9	49.0 73.6#
268	27.8	50.9 76.3#

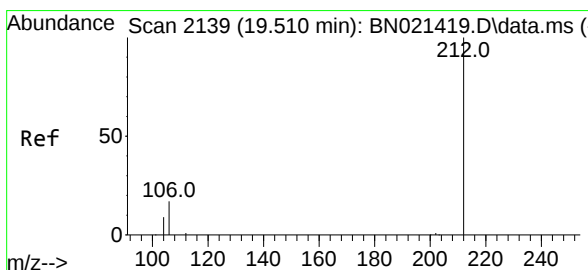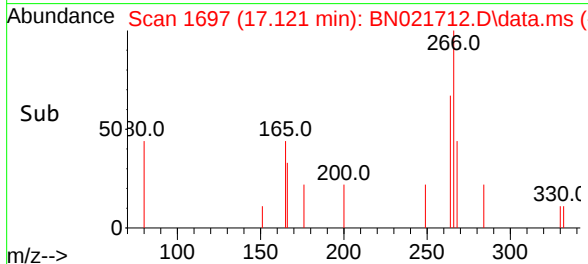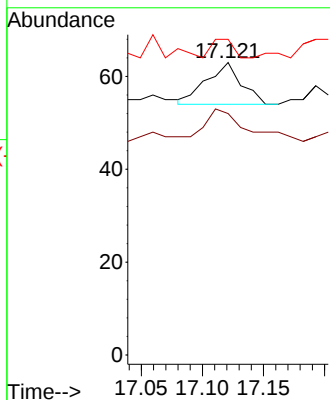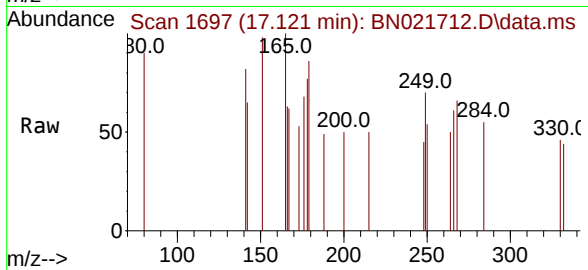

#27

Fluoranthene-d10

Concen: 0.366 ng




RT: 19.489 min Scan# 2134


Delta R.T. -0.008 min

Lab File: BN021712.D

Acq: 10 Sep 2022 23:50

Tgt Ion:212	Resp:	21844
Ion Ratio	Lower	Upper
212	100	
106	18.2	14.2 21.2
104	9.9	7.8 11.6

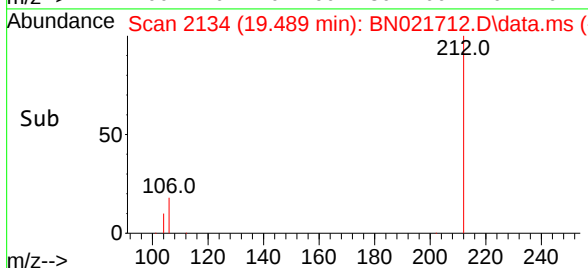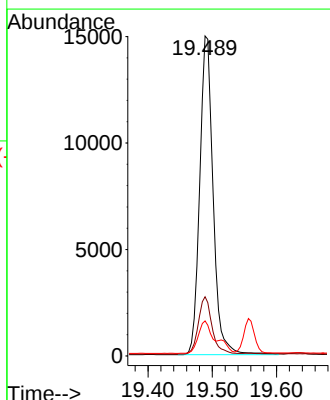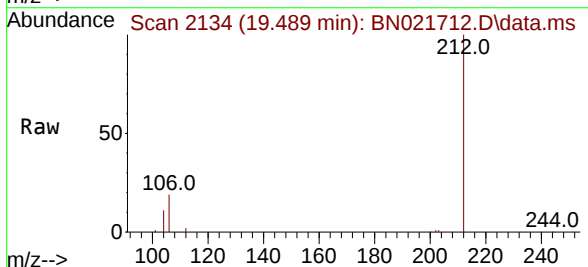

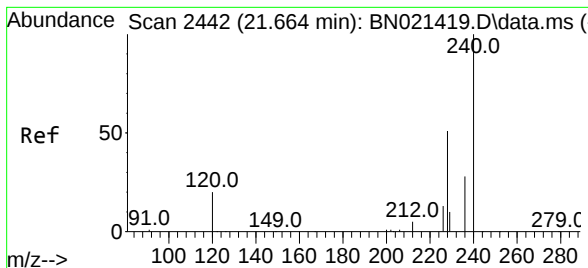

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.646 min Scan# 2440

Delta R.T. -0.009 min

Lab File: BN021712.D

Acq: 10 Sep 2022 23:50

Instrument :

BNA_N

ClientSampleId :

BP-VPB-RW5-GW-278-280





Tgt Ion:240 Resp: 14118

Ion Ratio Lower Upper

240 100

120 18.3 10.2 15.4#

236 28.4 22.1 33.1

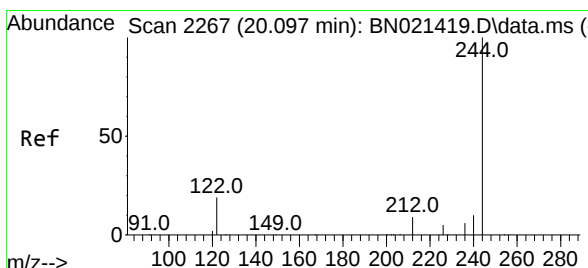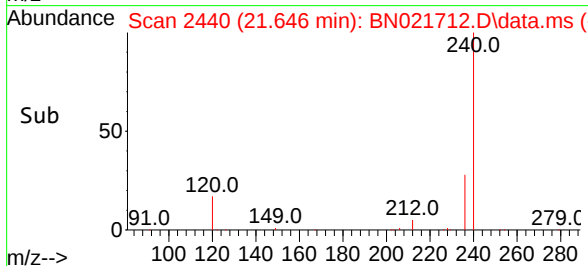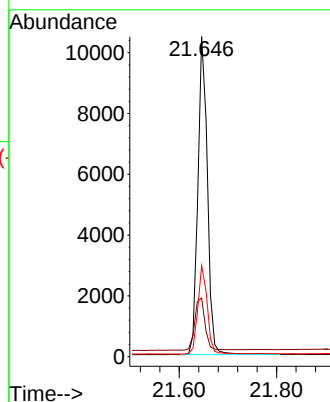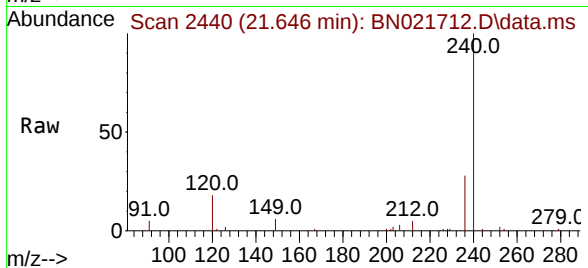

#31

Terphenyl-d14

Concen: 0.487 ng

RT: 20.079 min Scan# 2265

Delta R.T. -0.009 min

Lab File: BN021712.D

Acq: 10 Sep 2022 23:50




Tgt Ion:244 Resp: 15446


Ion Ratio Lower Upper

244 100

212 12.8 6.5 9.7#

122 15.8 9.1 13.7#


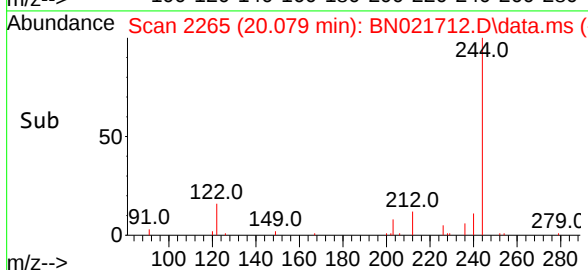
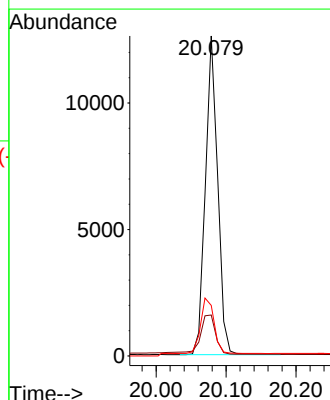
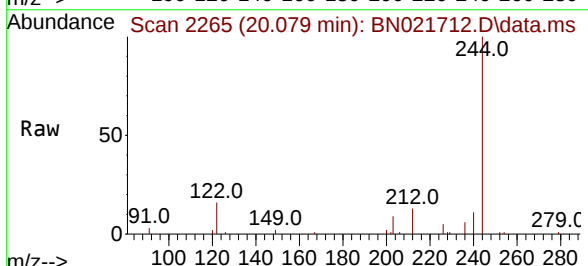


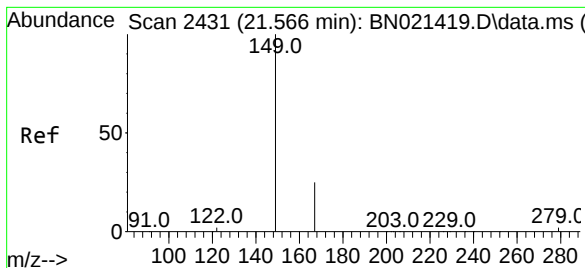

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.150 ng
 RT: 21.539 min Scan# 2428
 Delta R.T. -0.009 min
 Lab File: BN021712.D
 Acq: 10 Sep 2022 23:50

Instrument :
 BNA_N
 ClientSampleId :
 BP-VPB-RW5-GW-278-280

Tgt Ion:149 Resp: 2978
 Ion Ratio Lower Upper
 149 100
 167 25.7 21.4 32.0
 279 3.7 2.2 3.2#

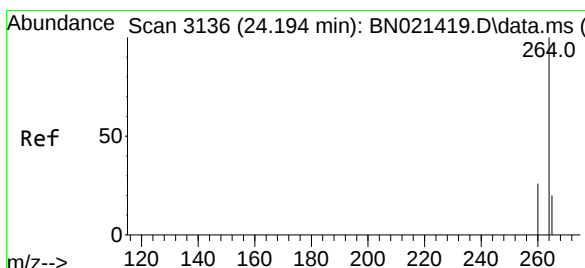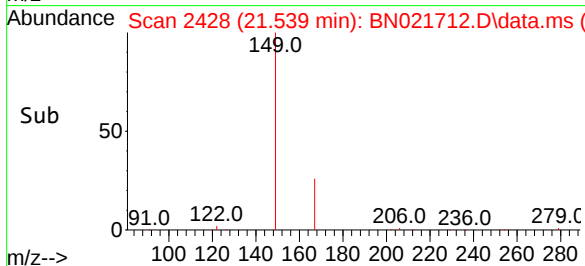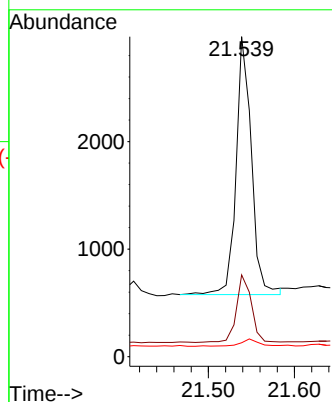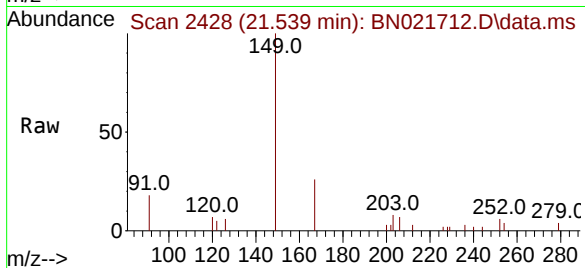

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.159 min Scan# 3124
 Delta R.T. -0.015 min
 Lab File: BN021712.D
 Acq: 10 Sep 2022 23:50

Tgt Ion:264 Resp: 10951
 Ion Ratio Lower Upper
 264 100
 260 25.7 21.0 31.6
 265 48.3 32.2 48.2#

