
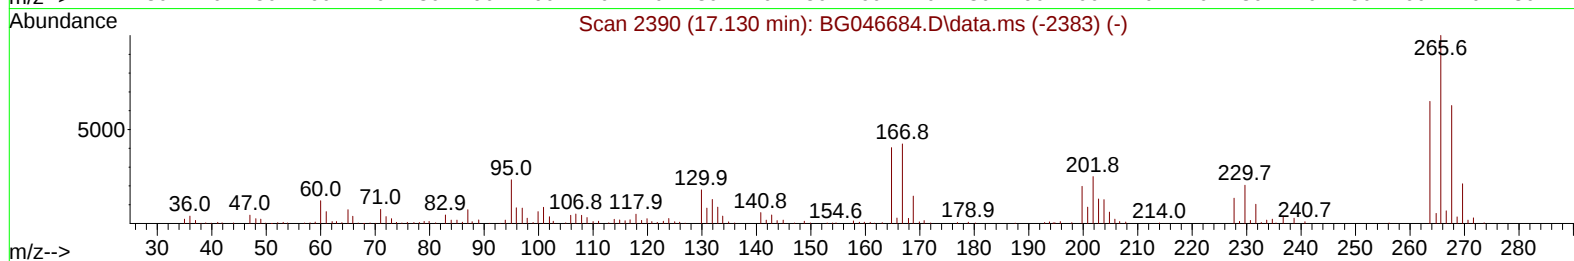
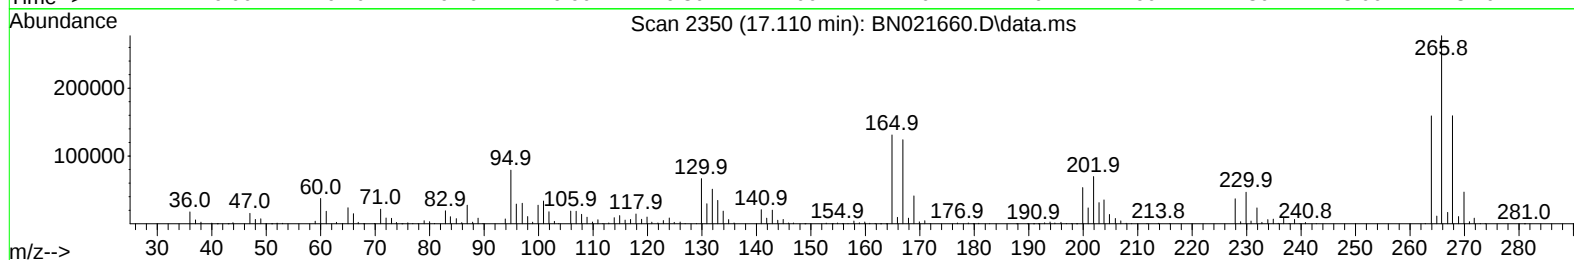


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091022\
Data File : BN021660.D
Acq On : 09 Sep 2022 14:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 05:04:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 10 05:03:56 2022
Response via : Initial Calibration

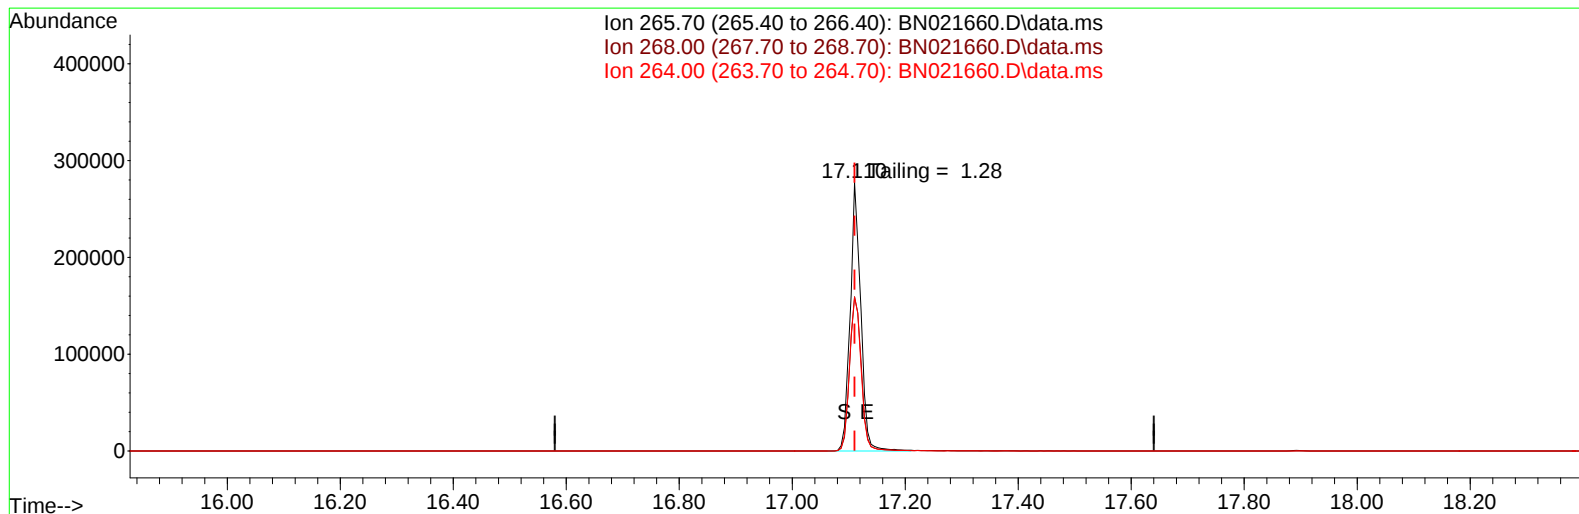

TIC: BN021660.D\data.ms

(70) Pentachlorophenol (C)




17.110min (0.000) 22230.16 ng

response 364789

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.48
264.00	61.60	57.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091022\
Data File : BN021660.D
Acq On : 09 Sep 2022 14:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 05:04:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 10 05:03:56 2022
Response via : Initial Calibration

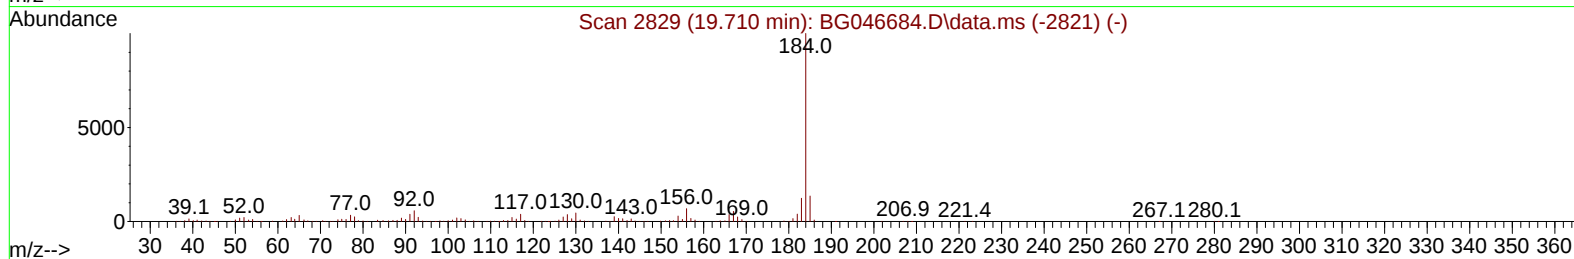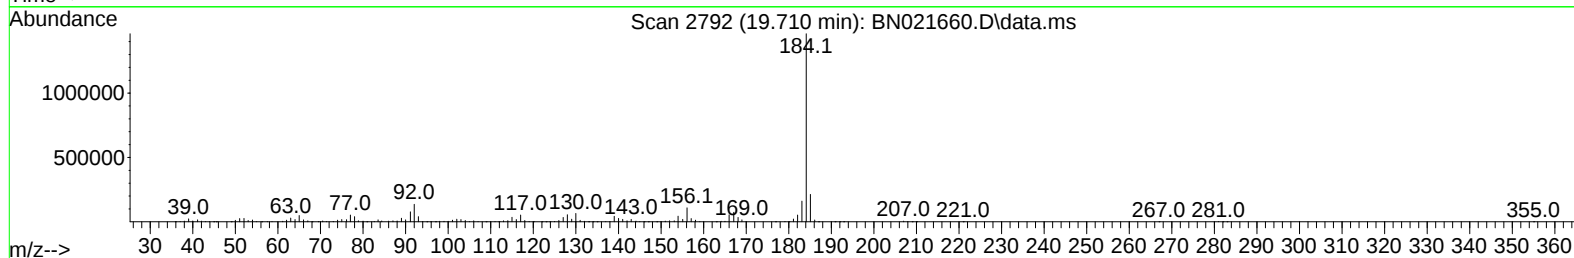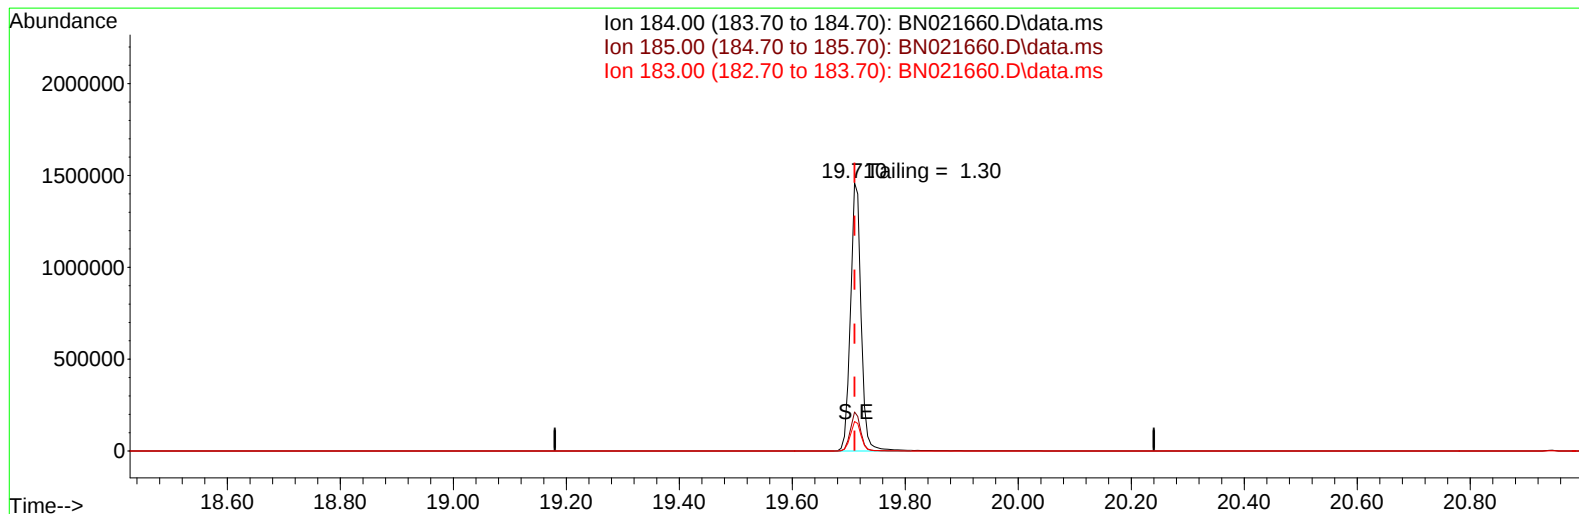

TIC: BN021660.D\data.ms

(77) Benzidine**19.710min (0.000) 1016832.70 ng****response 1911999**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.58
183.00	13.20	10.99
0.00	0.00	0.00