
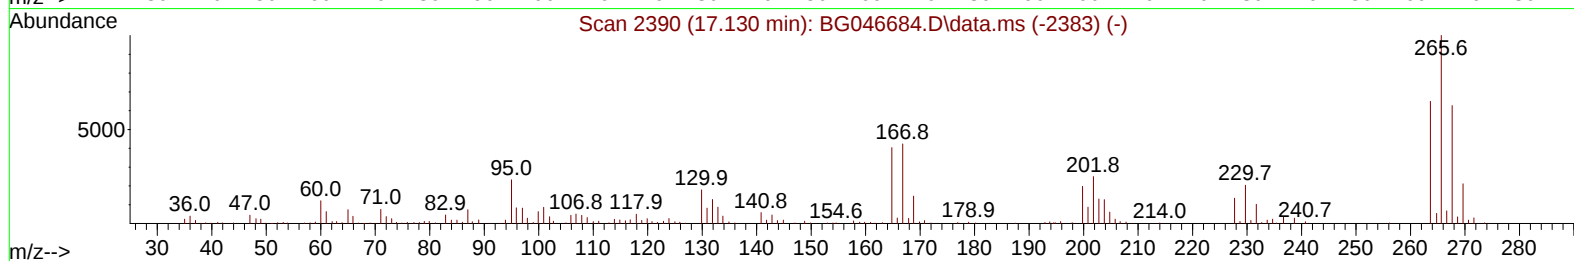
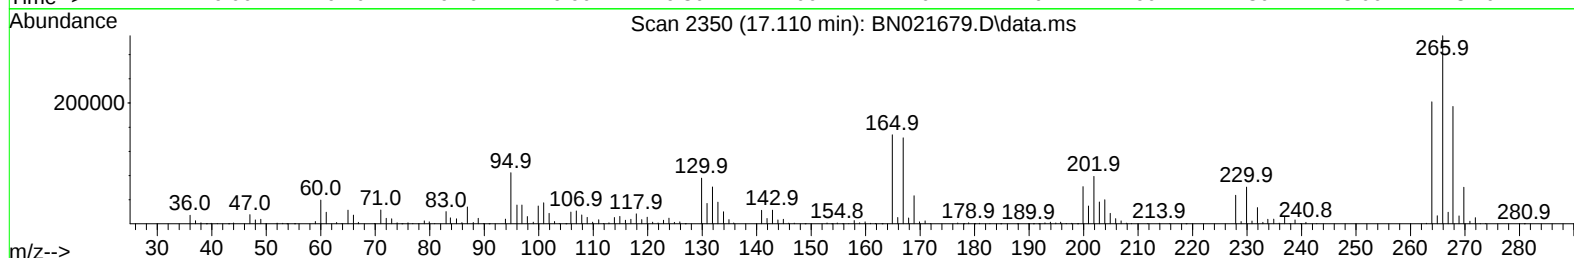


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091022\
Data File : BN021679.D
Acq On : 10 Sep 2022 03:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 05:05:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 10 05:03:56 2022
Response via : Initial Calibration

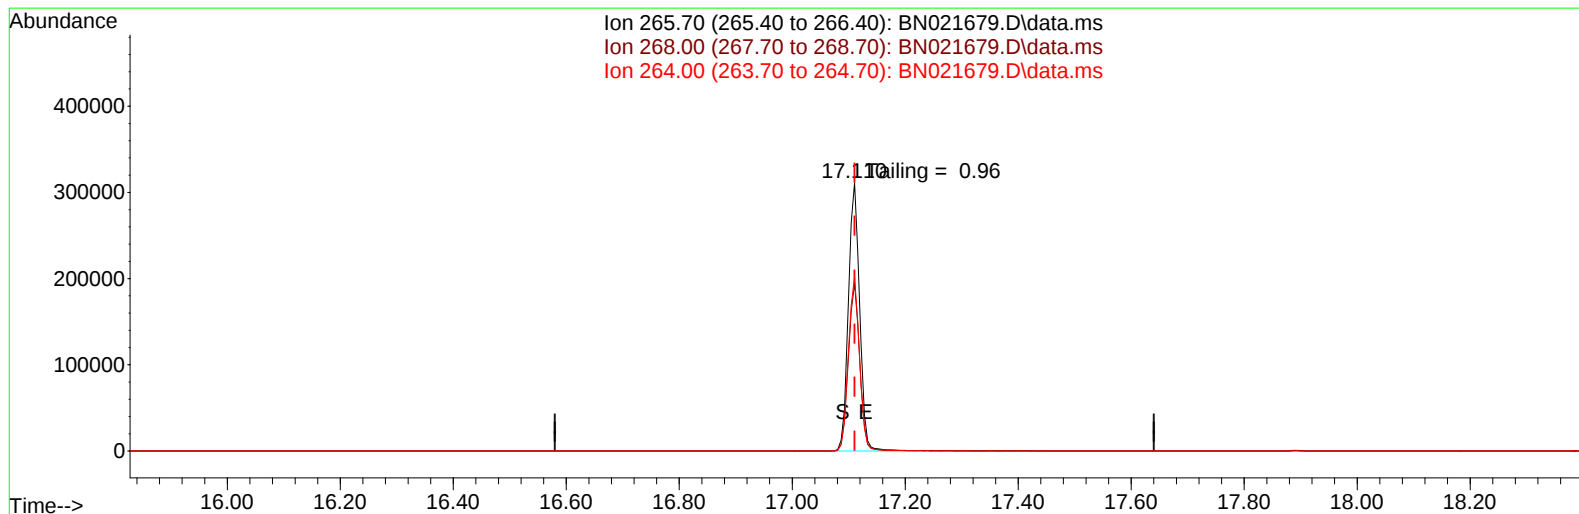

TIC: BN021679.D\data.ms

(70) Pentachlorophenol (C)




17.110min (+ 0.000) 24135.18 ng

response 431090

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.43
264.00	61.60	64.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091022\
Data File : BN021679.D
Acq On : 10 Sep 2022 03:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 05:05:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 10 05:03:56 2022
Response via : Initial Calibration

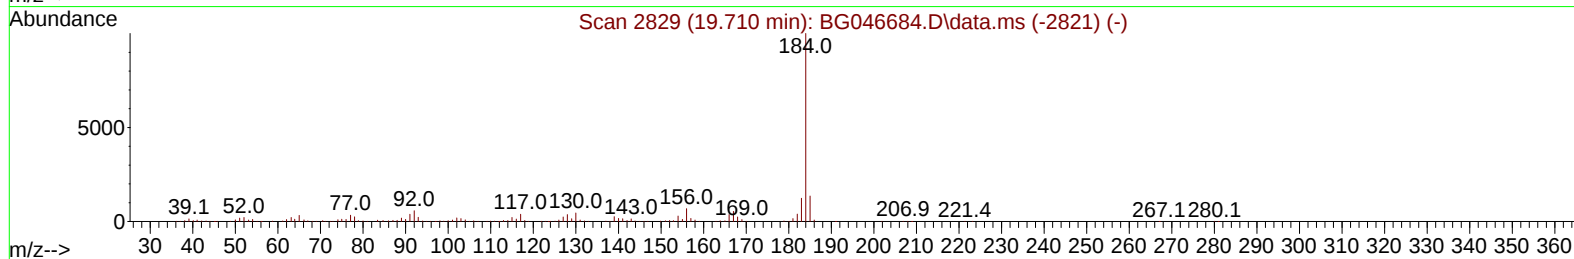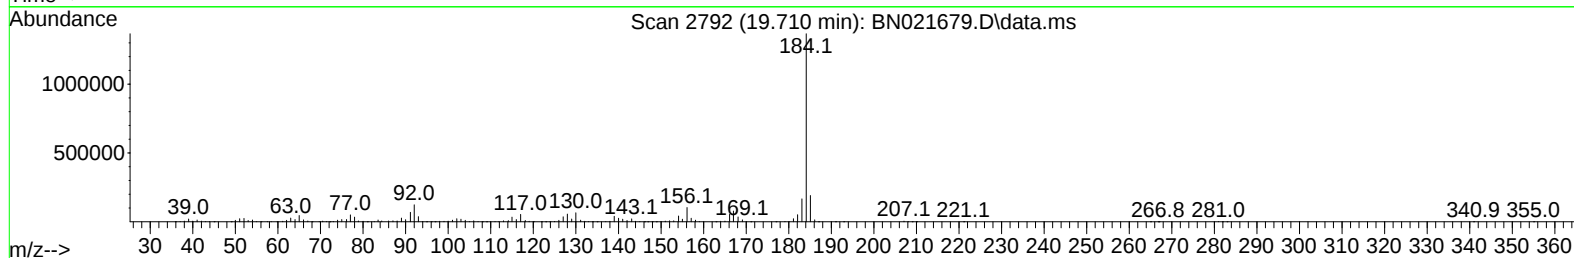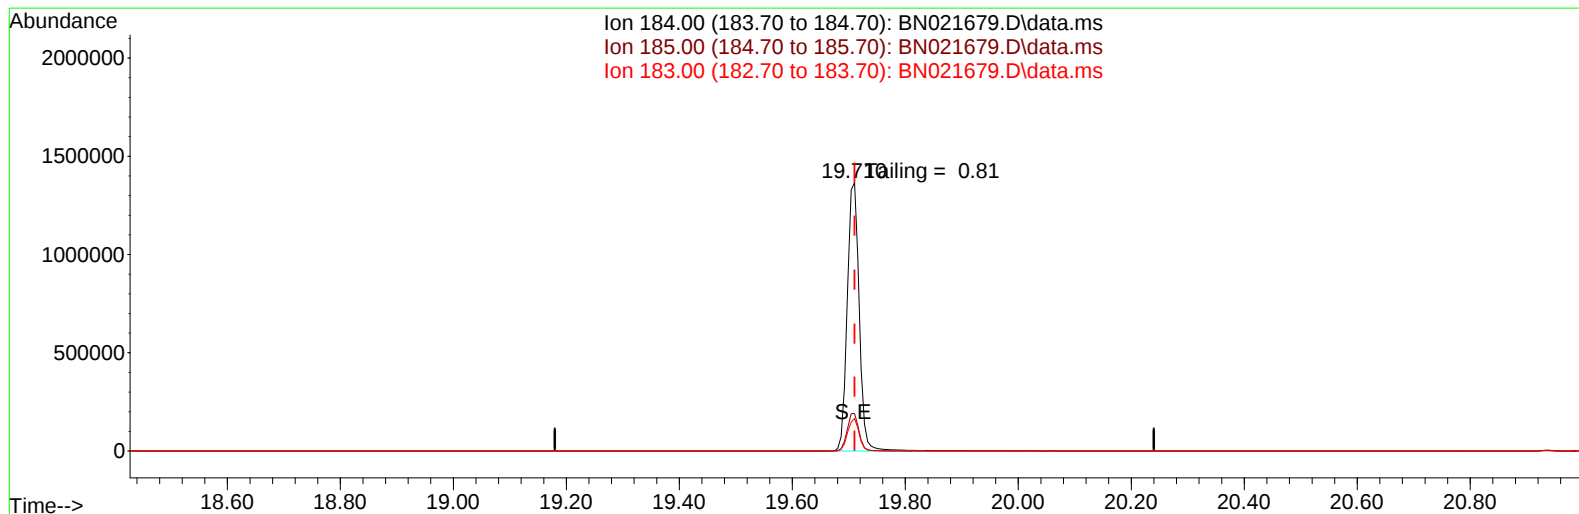

TIC: BN021679.D\data.ms

(77) Benzidine**19.710min (+ 0.000) 1228464.27 ng****response 2006997**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.98
183.00	13.20	12.16
0.00	0.00	0.00