
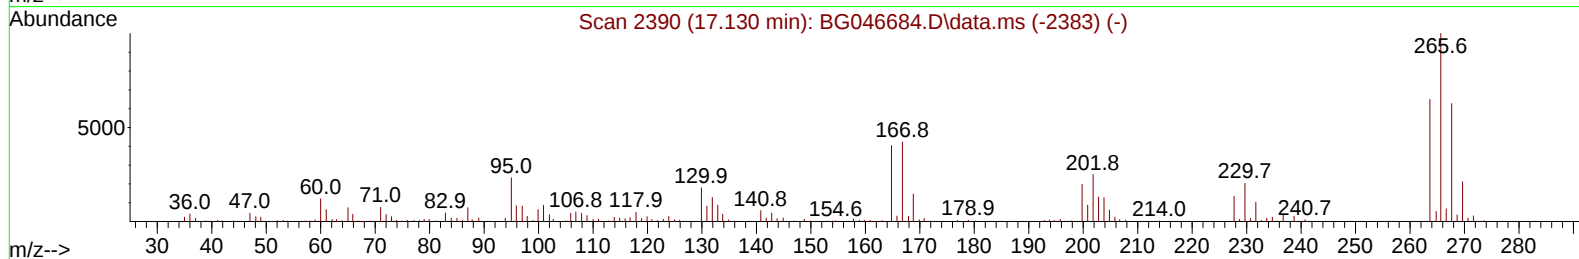
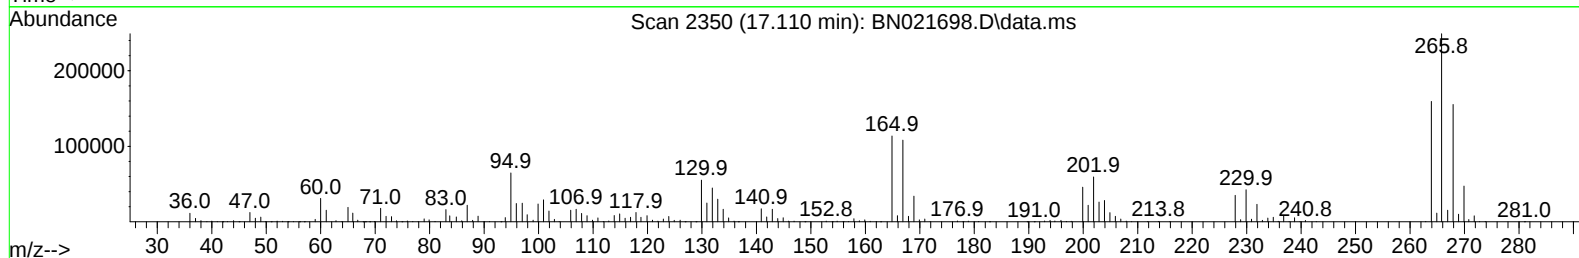


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091022\
 Data File : BN021698.D
 Acq On : 10 Sep 2022 14:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: Sep 12 02:31:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 12 02:31:07 2022
 Response via : Initial Calibration

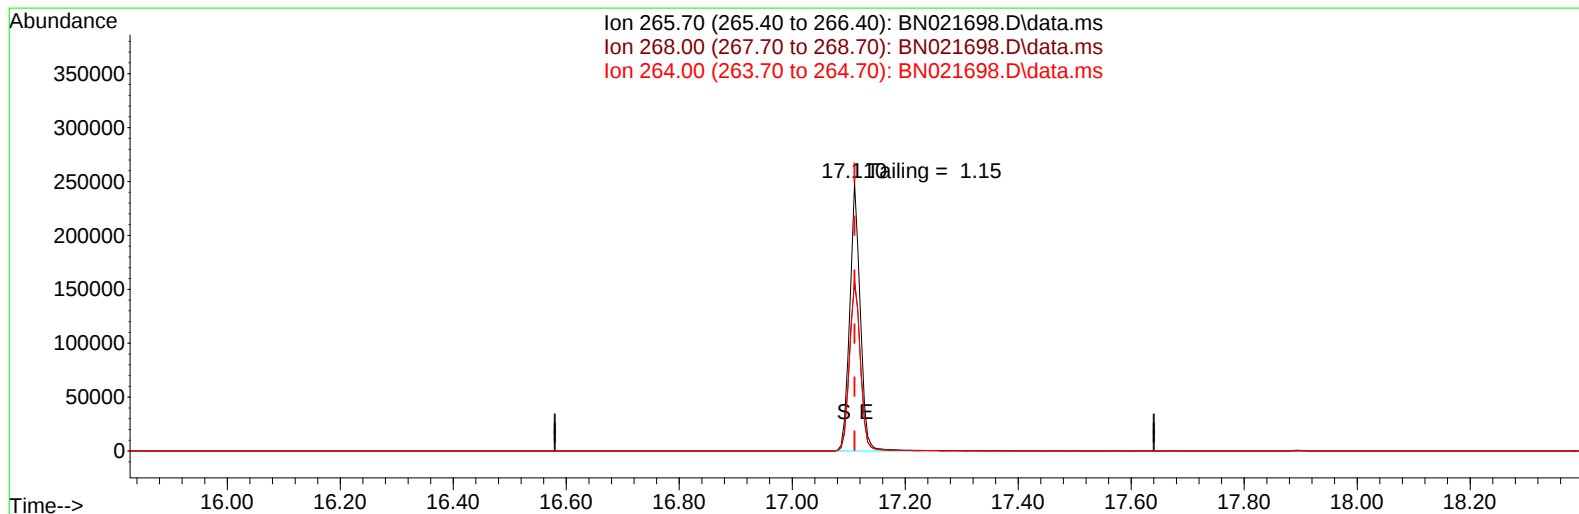

TIC: BN021698.D\data.ms

(70) Pentachlorophenol (C)




17.110min (0.000) 20049.45 ng

response 324756

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.44
264.00	61.60	64.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091022\
Data File : BN021698.D
Acq On : 10 Sep 2022 14:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 37 Sample Multiplier: 1

Quant Time: Sep 12 02:31:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 12 02:31:07 2022
Response via : Initial Calibration

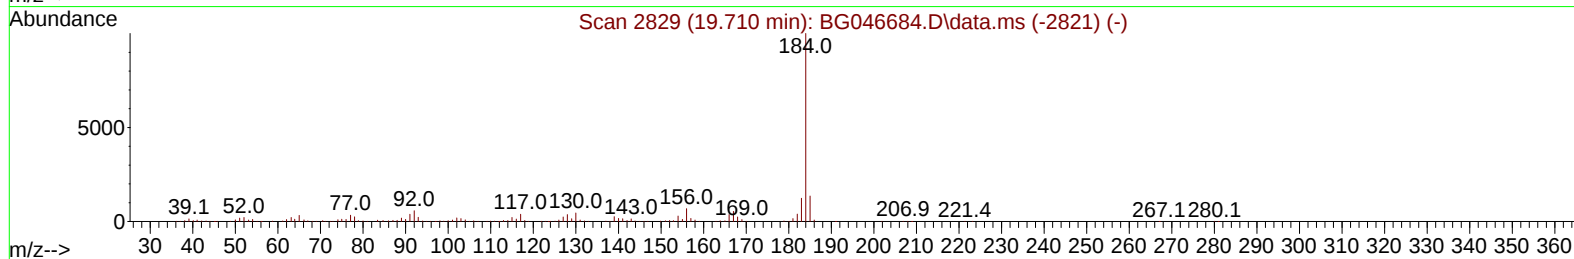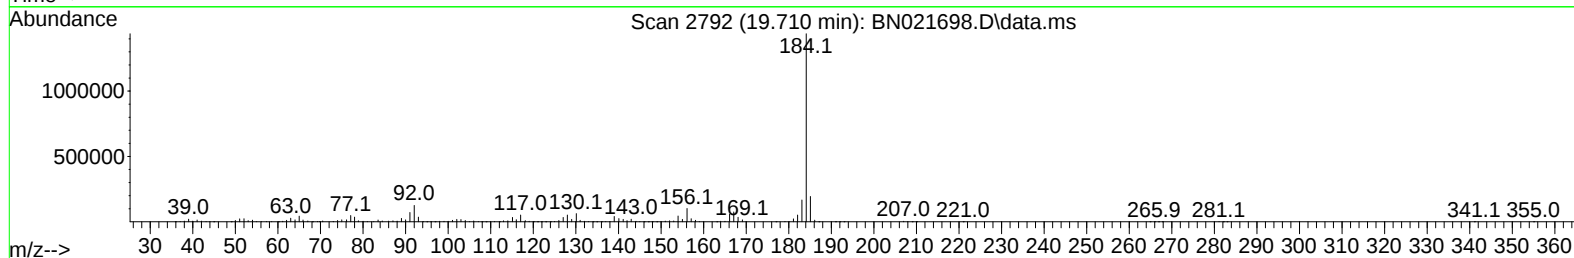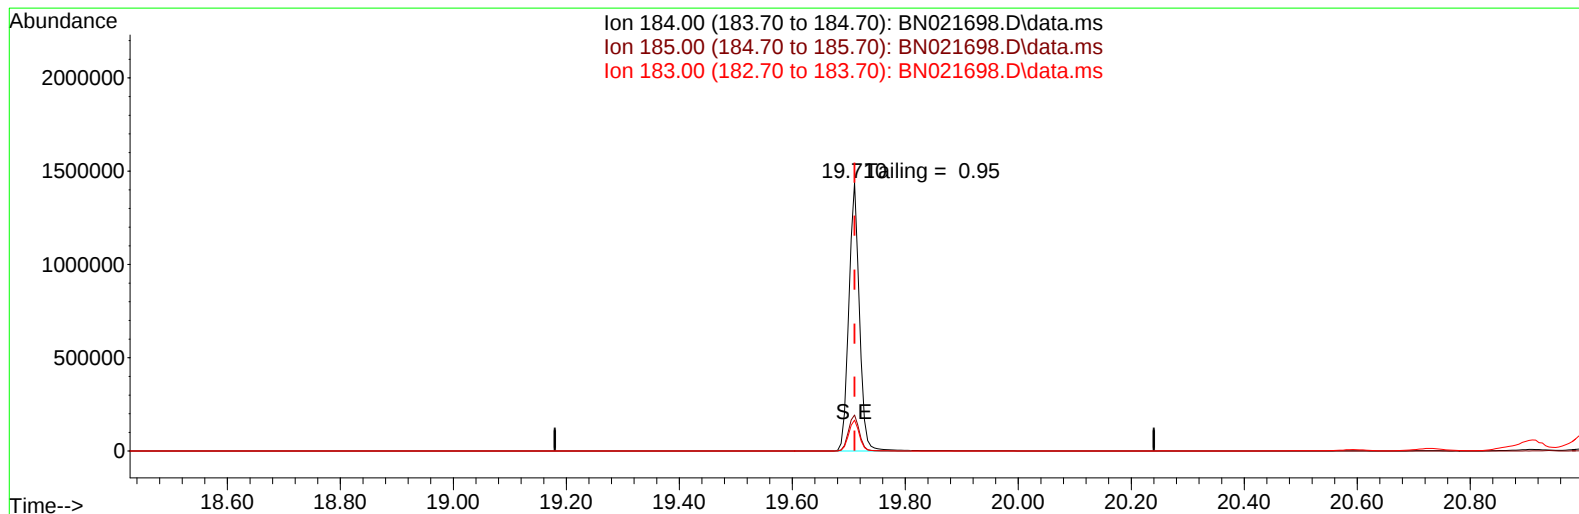

TIC: BN021698.D\data.ms

(77) Benzidine**19.710min (0.000) 1090023.93 ng****response 1881622**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.43
183.00	13.20	11.55
0.00	0.00	0.00