

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091022\
 Data File : BN021687.D
 Acq On : 10 Sep 2022 07:54
 Operator : CG/JU
 Sample : N4492-16
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EB02-090122

Quant Time: Sep 12 01:06:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 09 23:19:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.062	152	5081	0.400	ng	0.00
7) Naphthalene-d8	10.888	136	16956	0.400	ng	-0.01
13) Acenaphthene-d10	14.707	164	9746	0.400	ng	-0.01
19) Phenanthrene-d10	17.459	188	20388	0.400	ng	-0.01
29) Chrysene-d12	21.655	240	14502	0.400	ng	0.00
35) Perylene-d12	24.165	264	10522	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.592	112	2112	0.212	ng	0.00
5) Phenol-d6	7.217	99	1686	0.133	ng	0.00
8) Nitrobenzene-d5	9.233	82	4224	0.369	ng	0.00
11) 2-Methylnaphthalene-d10	12.475	152	13800	0.361	ng	0.00
14) 2,4,6-Tribromophenol	16.208	330	1395	0.436	ng	0.00
15) 2-Fluorobiphenyl	13.339	172	12920	0.303	ng	0.00
27) Fluoranthene-d10	19.493	212	22512	0.429	ng	0.00
31) Terphenyl-d14	20.079	244	15151	0.465	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.403	88	617	0.097	ng	# 49
34) Bis(2-ethylhexyl)phtha...	21.548	149	3785	0.186	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091022\
Data File : BN021687.D
Acq On : 10 Sep 2022 07:54
Operator : CG/JU
Sample : N4492-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EB02-090122


Quant Time: Sep 12 01:06:28 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 09 23:19:14 2022
Response via : Initial Calibration

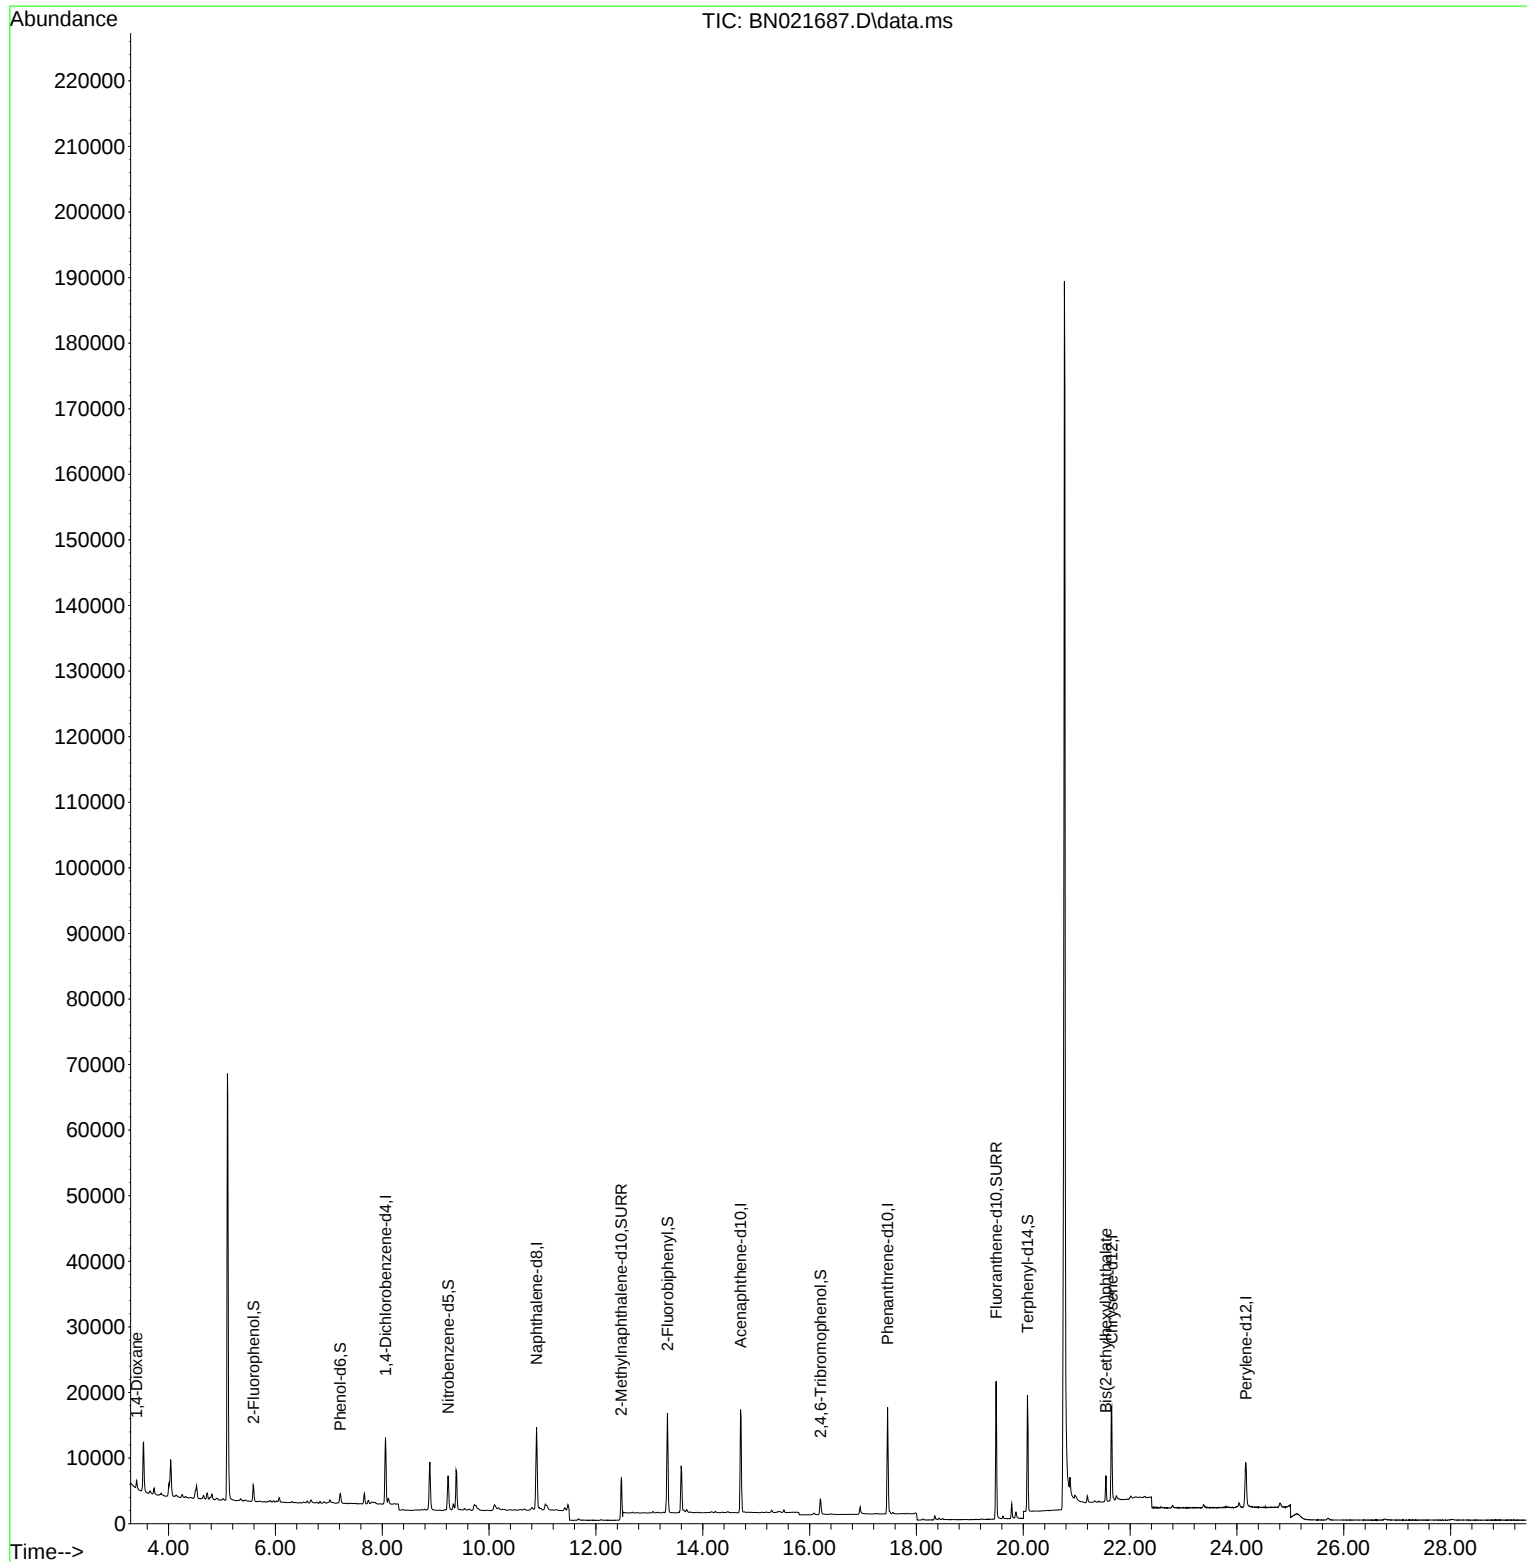






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 8.062 min Scan# 60
 Delta R.T. -0.000 min
 Lab File: BN021687.D
 Acq: 10 Sep 2022 07:54


Instrument :
 BNA_N
 ClientSampleId :
 EB02-090122

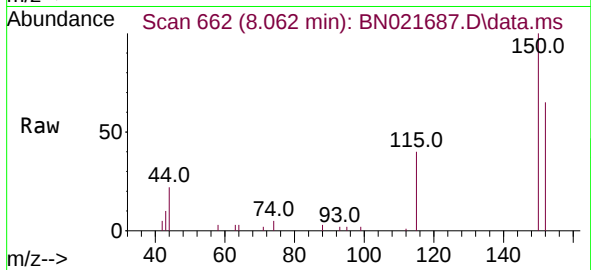



Tgt Ion:152 Resp: 5081
 Ion Ratio Lower Upper
 152 100
 150 153.5 121.4 182.0
 115 60.9 48.6 72.8

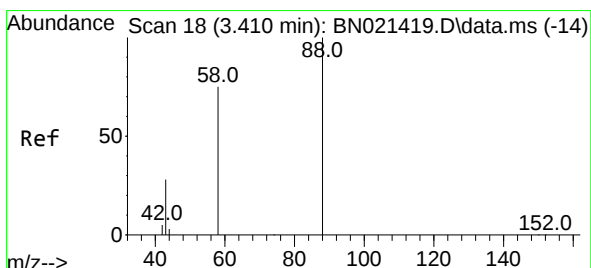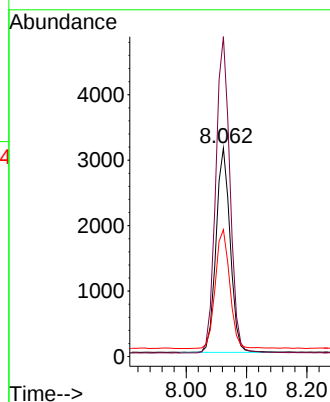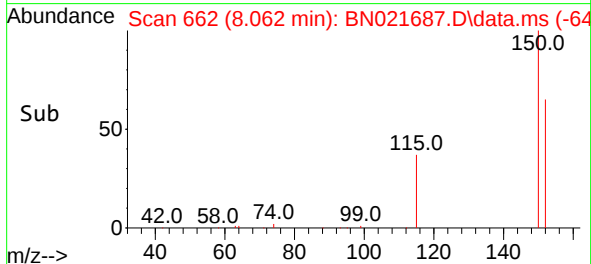

#2
 1,4-Dioxane
 Concen: 0.097 ng
 RT: 3.403 min Scan# 17
 Delta R.T. 0.000 min
 Lab File: BN021687.D
 Acq: 10 Sep 2022 07:54

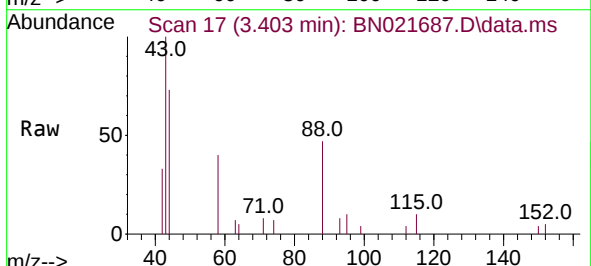

Tgt Ion: 88 Resp: 617
 Ion Ratio Lower Upper
 88 100
 43 116.4 35.8 53.8#
 58 83.6 57.1 85.7



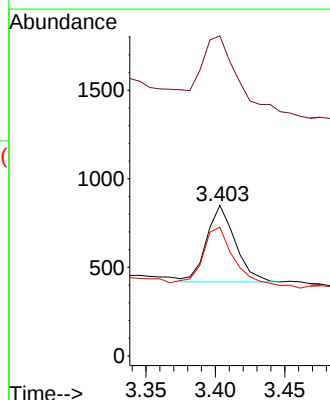
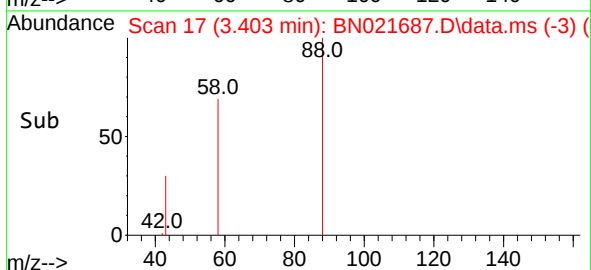




#4
2-Fluorophenol
Concen: 0.212 ng
RT: 5.592 min Scan# 31
Delta R.T. 0.000 min
Lab File: BN021687.D
Acq: 10 Sep 2022 07:54




Instrument :
BNA_N
ClientSampleId :
EB02-090122


Tgt Ion: 112 Resp: 2112
Ion Ratio Lower Upper
112 100
64 55.4 43.5 65.3
63 28.2 22.6 34.0

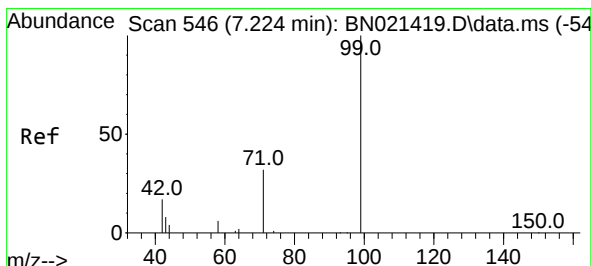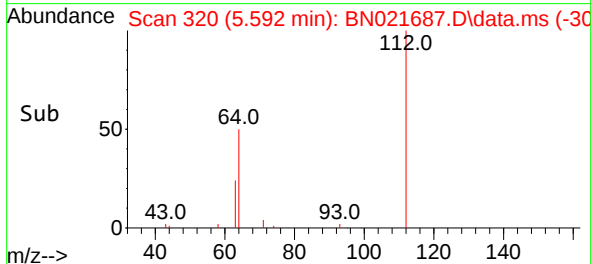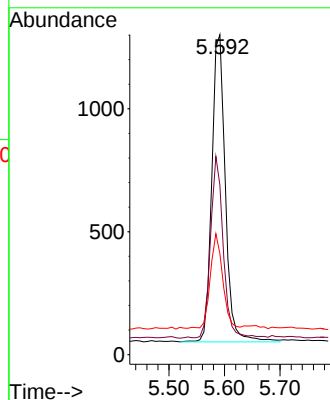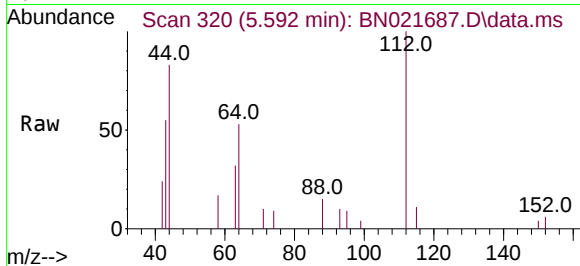

#5
Phenol-d6
Concen: 0.133 ng
RT: 7.217 min Scan# 545
Delta R.T. 0.000 min
Lab File: BN021687.D
Acq: 10 Sep 2022 07:54

Tgt Ion: 99 Resp: 1686
Ion Ratio Lower Upper
99 100
42 17.9 15.5 23.3
71 35.8 24.2 36.2


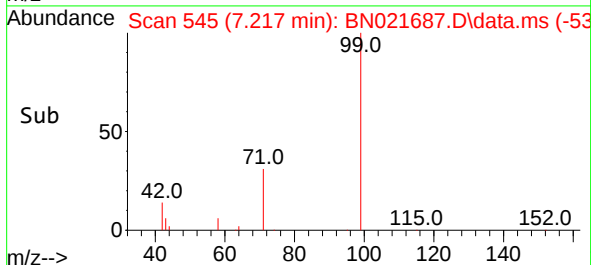
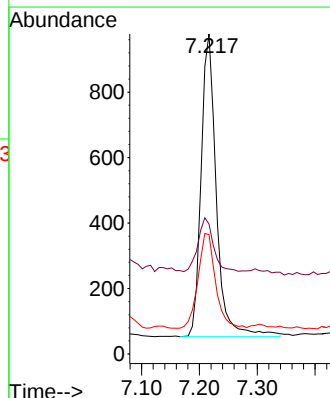
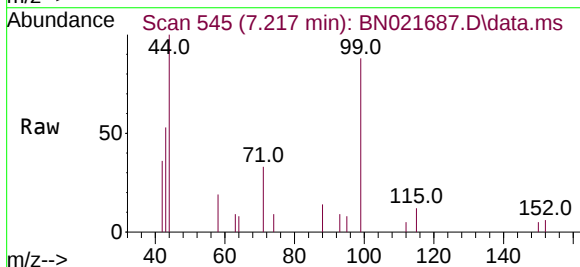


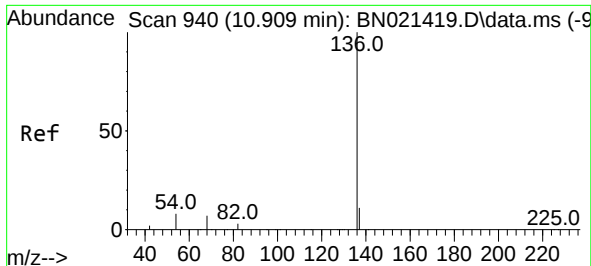

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.888 min Scan# 91
Delta R.T. -0.011 min
Lab File: BN021687.D
Acq: 10 Sep 2022 07:54




Instrument :
BNA_N
ClientSampleId :
EB02-090122

Tgt Ion:	136	Resp:	16956
Ion Ratio	Lower	Upper	
136	100		
137	11.5	9.3	13.9
54	8.8	6.9	10.3
68	7.5	6.1	9.1

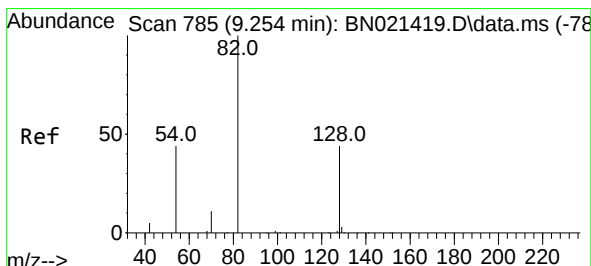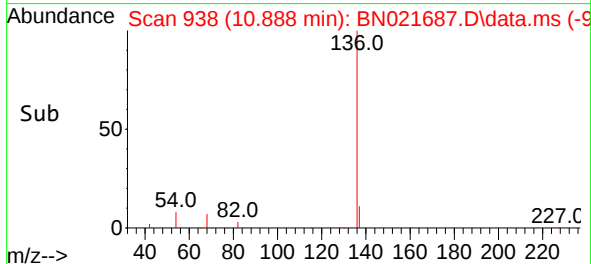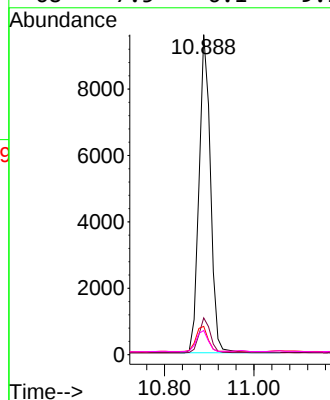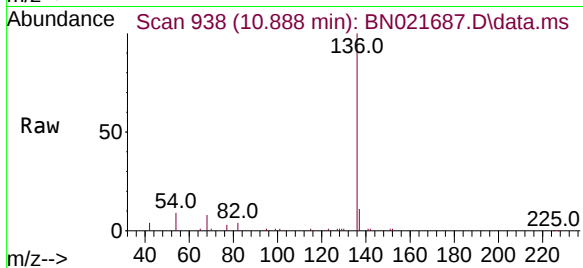

#8
Nitrobenzene-d5
Concen: 0.369 ng
RT: 9.233 min Scan# 783
Delta R.T. 0.000 min
Lab File: BN021687.D
Acq: 10 Sep 2022 07:54

Tgt Ion:	82	Resp:	4224
Ion Ratio	Lower	Upper	
82	100		
128	41.7	30.9	46.3
54	53.0	42.7	64.1


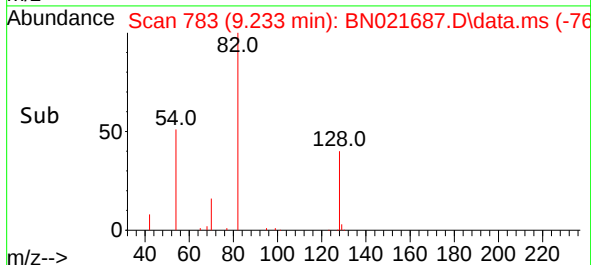
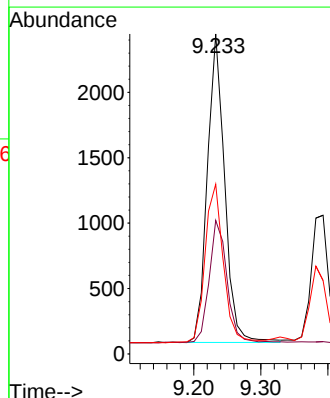
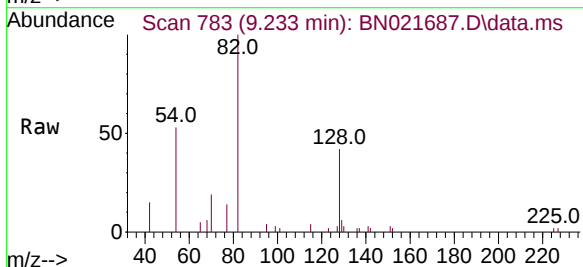




#11
2-Methylnaphthalene-d10
Concen: 0.361 ng
RT: 12.475 min Scan# 11
Delta R.T. -0.004 min
Lab File: BN021687.D
Acq: 10 Sep 2022 07:54




Instrument :
BNA_N
ClientSampleId :
EB02-090122


Tgt Ion:152 Resp: 13800
Ion Ratio Lower Upper
152 100
151 18.6 14.5 21.7

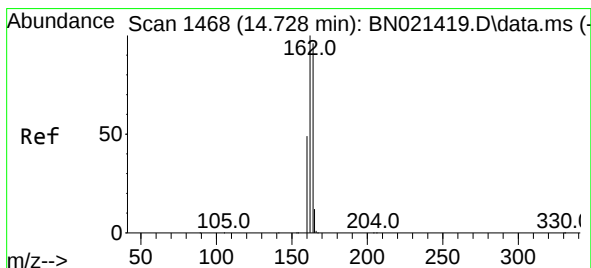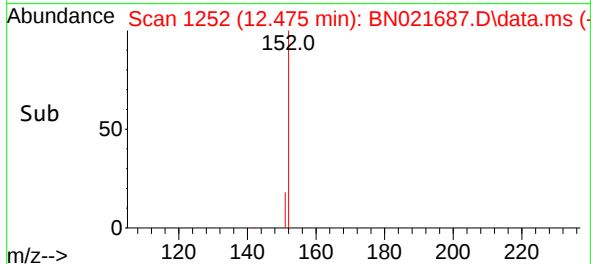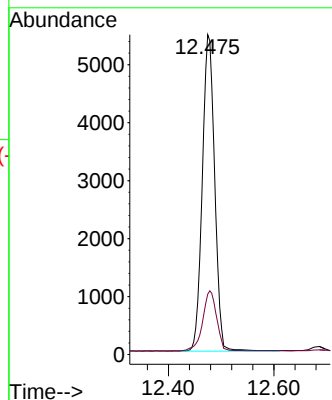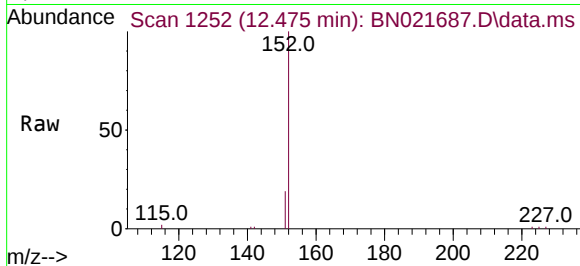

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.707 min Scan# 1466
Delta R.T. -0.011 min
Lab File: BN021687.D
Acq: 10 Sep 2022 07:54

Tgt Ion:164 Resp: 9746
Ion Ratio Lower Upper
164 100
162 105.6 82.2 123.4
160 51.5 39.5 59.3


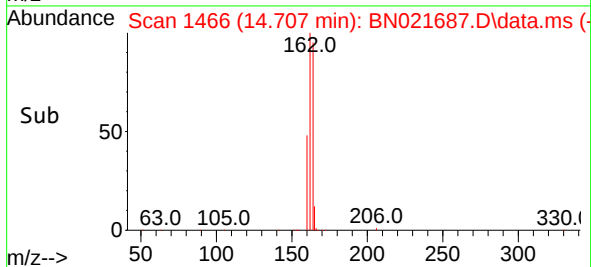
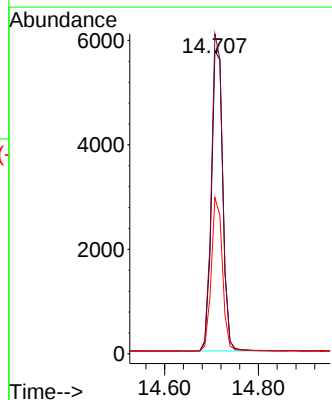
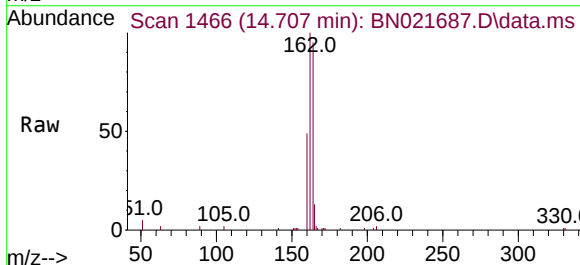


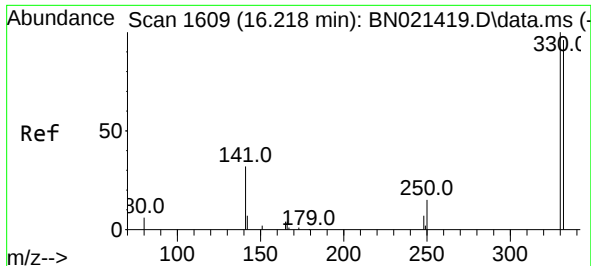

#14
2,4,6-Tribromophenol
Concen: 0.436 ng
RT: 16.208 min Scan# 1608
Delta R.T. 0.000 min
Lab File: BN021687.D
Acq: 10 Sep 2022 07:54




Instrument :
BNA_N
ClientSampleId :
EB02-090122


Tgt Ion:330 Resp: 1395
Ion Ratio Lower Upper
330 100
332 96.6 79.3 118.9
141 46.5 37.1 55.7

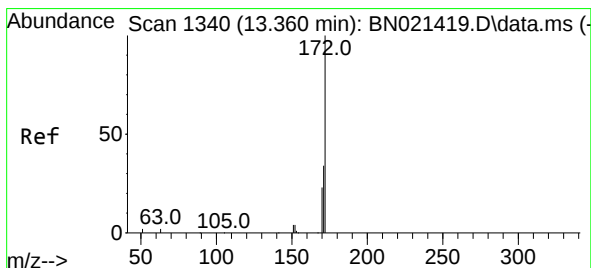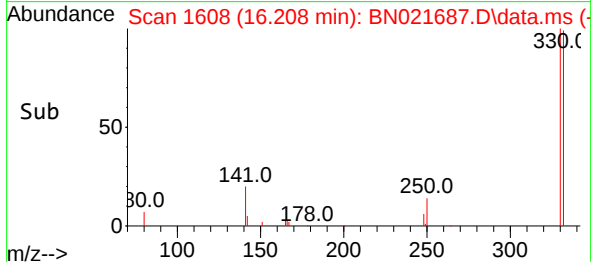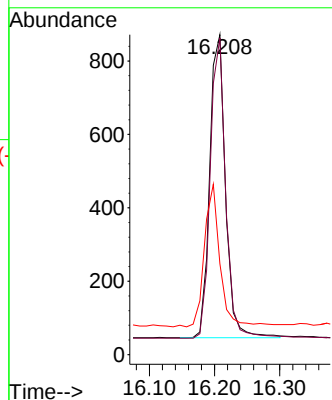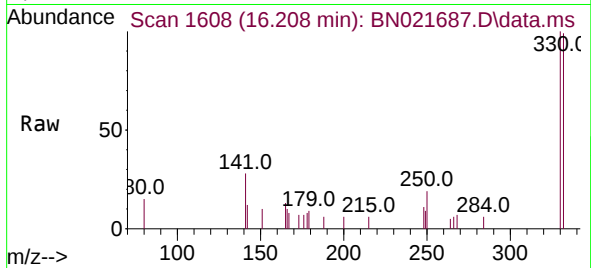

#15
2-Fluorobiphenyl
Concen: 0.303 ng
RT: 13.339 min Scan# 1338
Delta R.T. 0.000 min
Lab File: BN021687.D
Acq: 10 Sep 2022 07:54

Tgt Ion:172 Resp: 12920
Ion Ratio Lower Upper
172 100
171 34.8 27.8 41.6
170 23.9 18.6 28.0


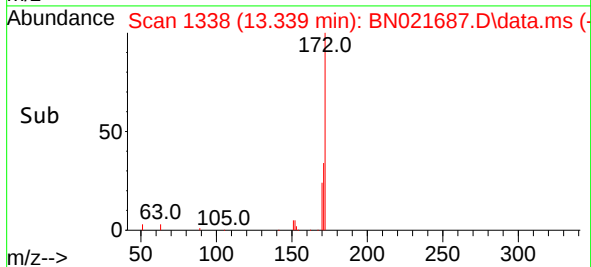
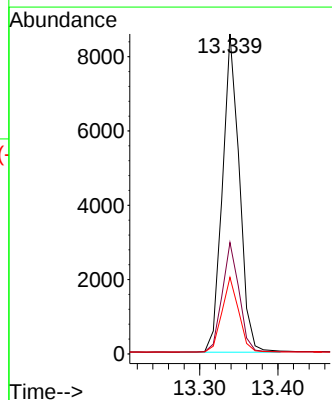
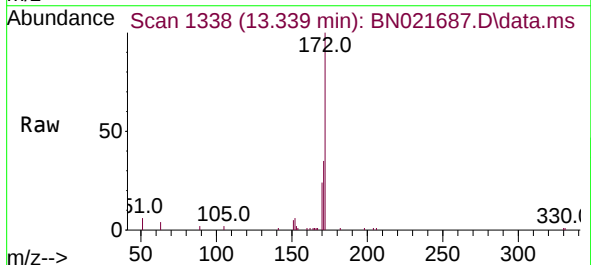


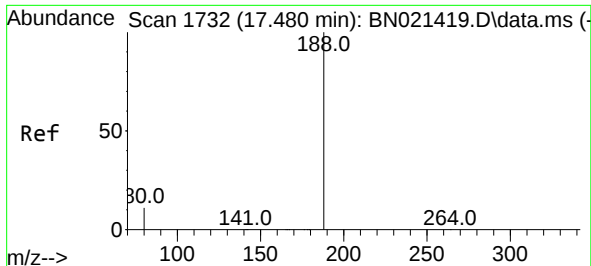

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.459 min Scan# 1730
Delta R.T. -0.010 min
Lab File: BN021687.D
Acq: 10 Sep 2022 07:54




Instrument :
BNA_N
ClientSampleId :
EB02-090122


Tgt Ion:188 Resp: 20388
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 13.1 9.5 14.3

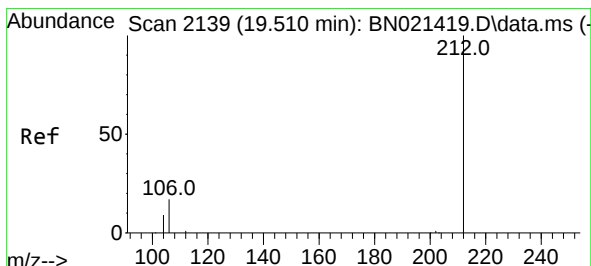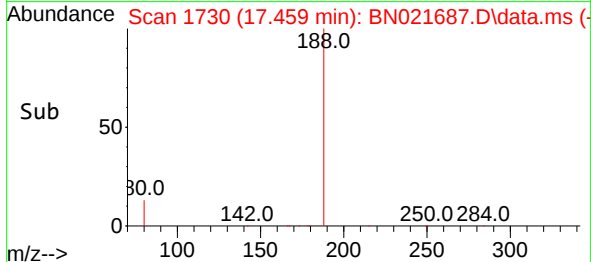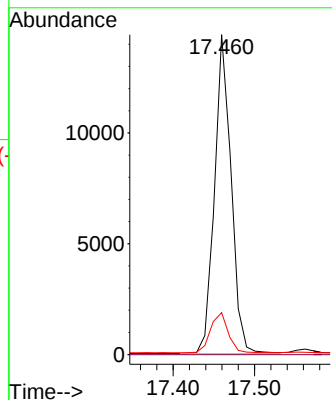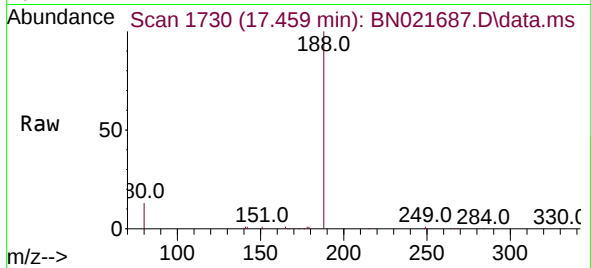

#27
Fluoranthene-d10
Concen: 0.429 ng
RT: 19.493 min Scan# 2135
Delta R.T. -0.004 min
Lab File: BN021687.D
Acq: 10 Sep 2022 07:54

Tgt Ion:212 Resp: 22512
Ion Ratio Lower Upper
212 100
106 17.9 14.2 21.2
104 10.1 7.8 11.6

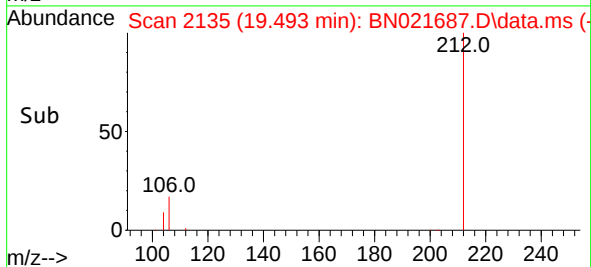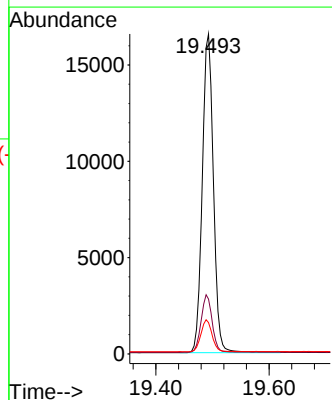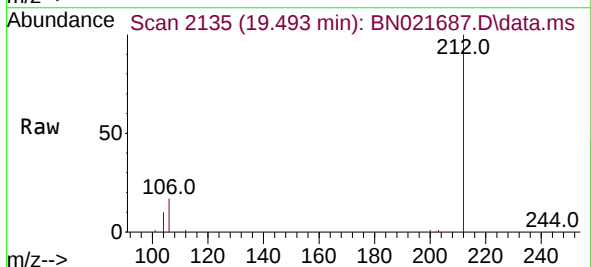

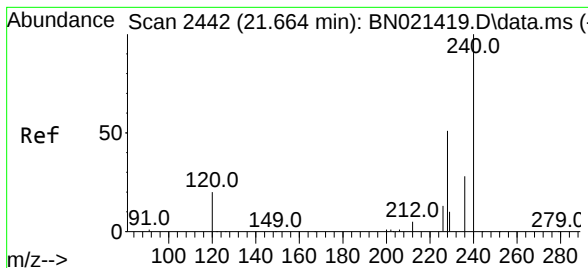

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.655 min Scan# 2441

Delta R.T. 0.000 min

Lab File: BN021687.D

Acq: 10 Sep 2022 07:54

Instrument :

BNA_N

ClientSampleId :

EB02-090122





Tgt Ion:240 Resp: 14502

Ion Ratio Lower Upper

240 100

120 12.9 10.2 15.4

236 27.6 22.1 33.1

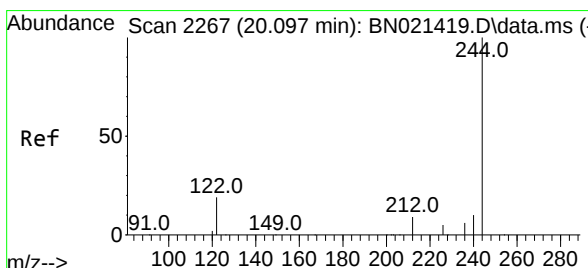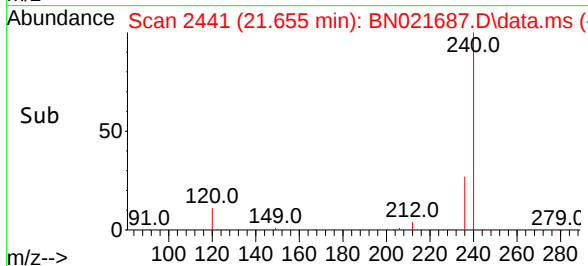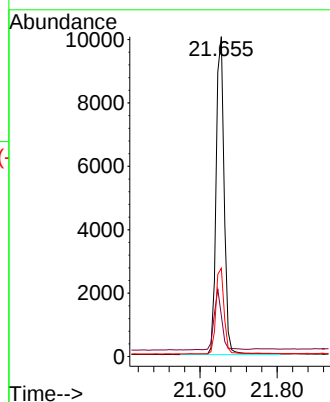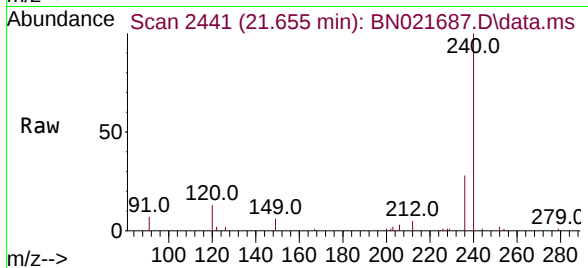

#31

Terphenyl-d14

Concen: 0.465 ng

RT: 20.079 min Scan# 2265

Delta R.T. -0.009 min

Lab File: BN021687.D

Acq: 10 Sep 2022 07:54




Tgt Ion:244 Resp: 15151


Ion Ratio Lower Upper

244 100

212 9.8 6.5 9.7#

122 19.2 9.1 13.7#


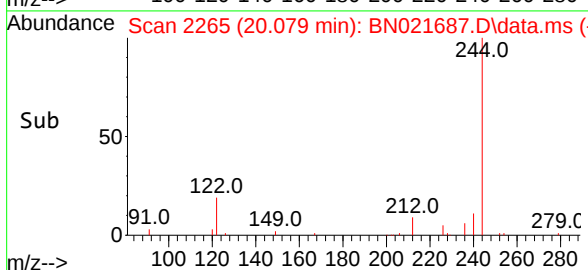
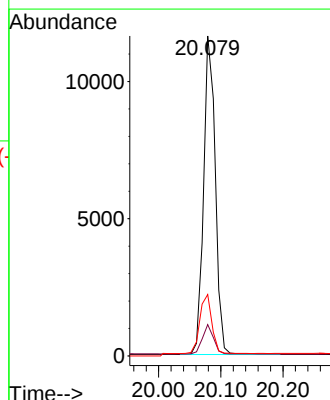
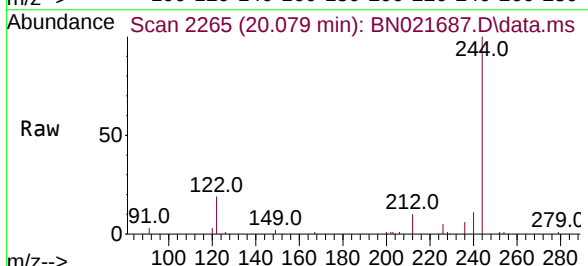


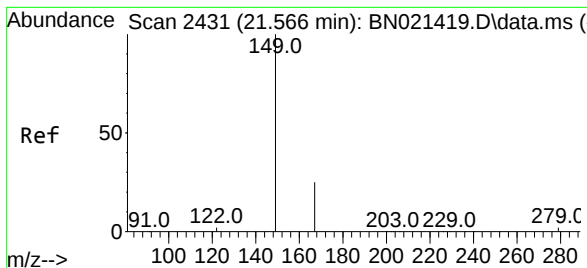

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.186 ng
 RT: 21.548 min Scan# 2431
 Delta R.T. 0.000 min
 Lab File: BN021687.D
 Acq: 10 Sep 2022 07:54

Instrument :
 BNA_N
 ClientSampleId :
 EB02-090122

Tgt Ion:149 Resp: 3785
 Ion Ratio Lower Upper
 149 100
 167 25.0 21.4 32.0
 279 3.1 2.2 3.2

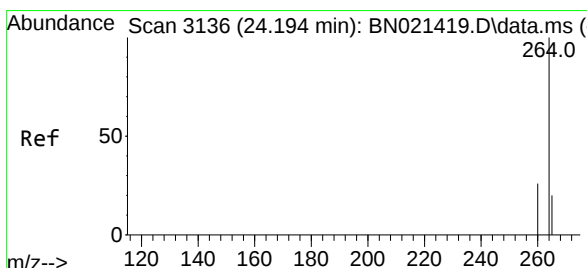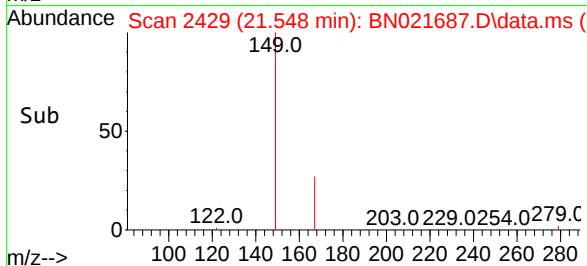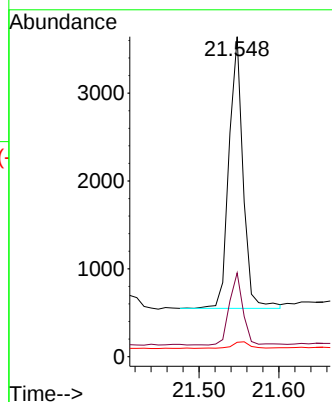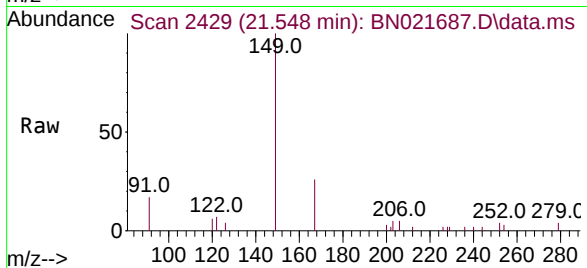

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.165 min Scan# 3126
 Delta R.T. -0.009 min
 Lab File: BN021687.D
 Acq: 10 Sep 2022 07:54

Tgt Ion:264 Resp: 10522
 Ion Ratio Lower Upper
 264 100
 260 26.9 21.0 31.6
 265 47.9 32.2 48.2

