


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091022\
 Data File : BN021660.D
 Acq On : 09 Sep 2022 14:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 13 02:32:27 2022

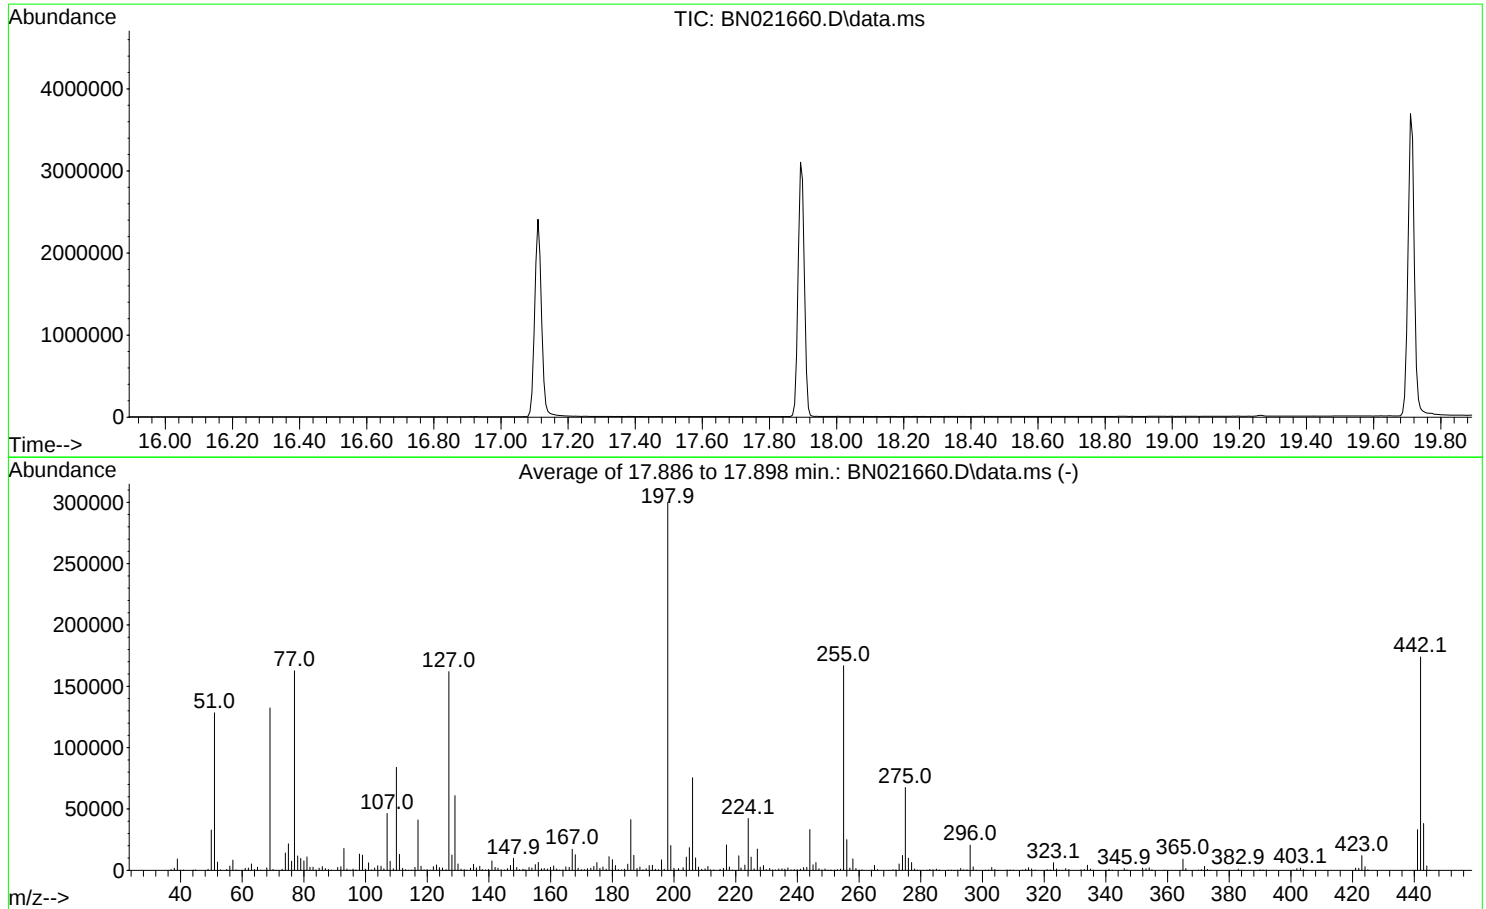




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.8	128403	PASS
68	69	0.00	2	1.5	2035	PASS
69	198	0.00	100	44.1	132384	PASS
70	69	0.00	2	0.5	722	PASS
127	198	10	80	54.0	161941	PASS
197	198	0.00	2	0.3	896	PASS
198	198	100	100	100.0	299904	PASS
199	198	5	9	6.7	20205	PASS
275	198	10	60	22.5	67472	PASS
365	198	1	100	3.0	9029	PASS
441	198	0.01	100	11.0	33035	PASS
442	442	50	100	100.0	173923	PASS
443	442	15	24	22.0	38224	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091022\
 Data File : BN021660.D
 Acq On : 09 Sep 2022 14:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 10 05:04:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 10 05:03:56 2022
 Response via : Initial Calibration

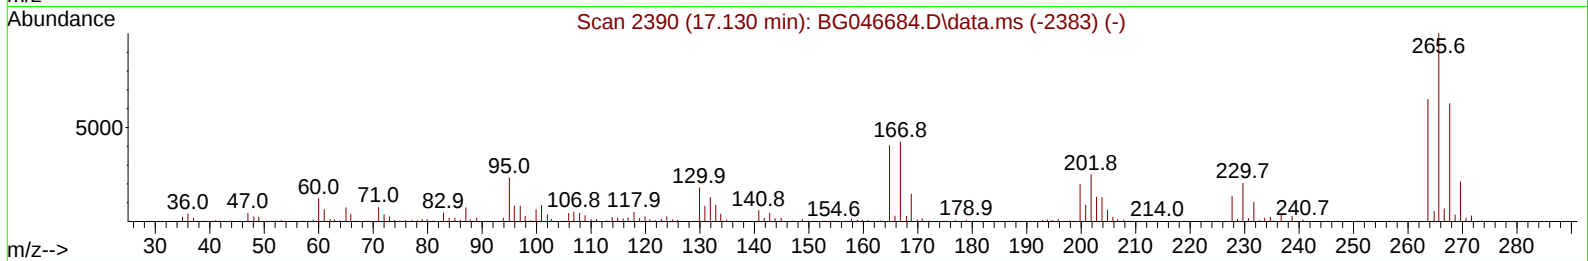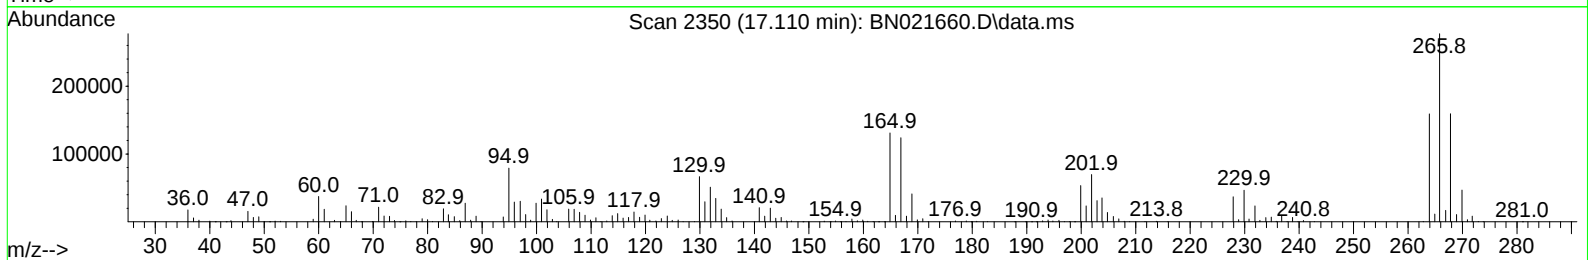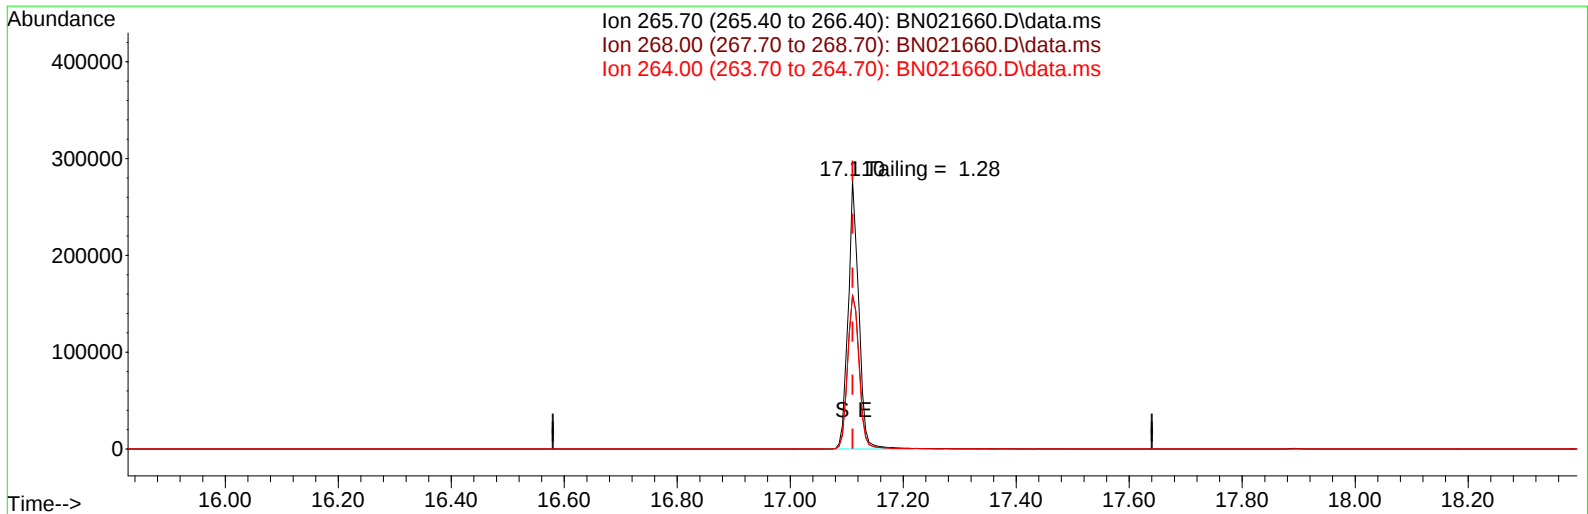

TIC: BN021660.D\data.ms

(70) Pentachlorophenol (C)

17.110min (0.000) 22230.16 ng




response 364789

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.48
264.00	61.60	57.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091022\
Data File : BN021660.D
Acq On : 09 Sep 2022 14:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 10 05:04:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 10 05:03:56 2022
Response via : Initial Calibration

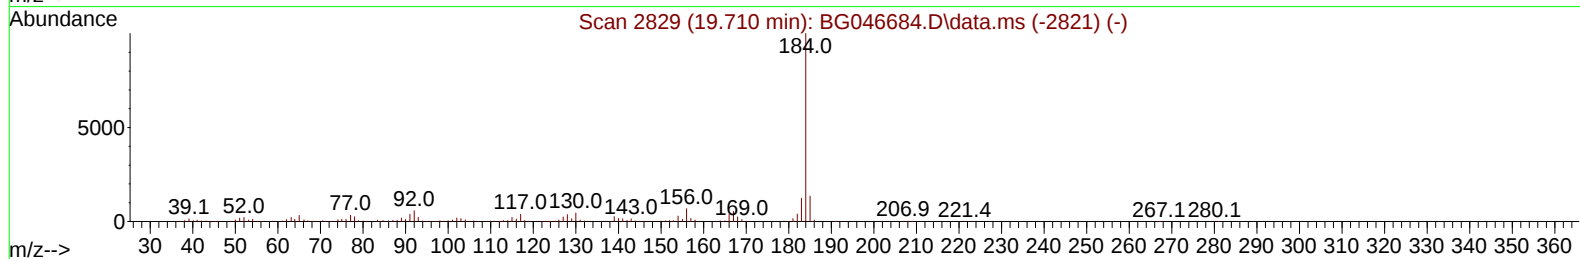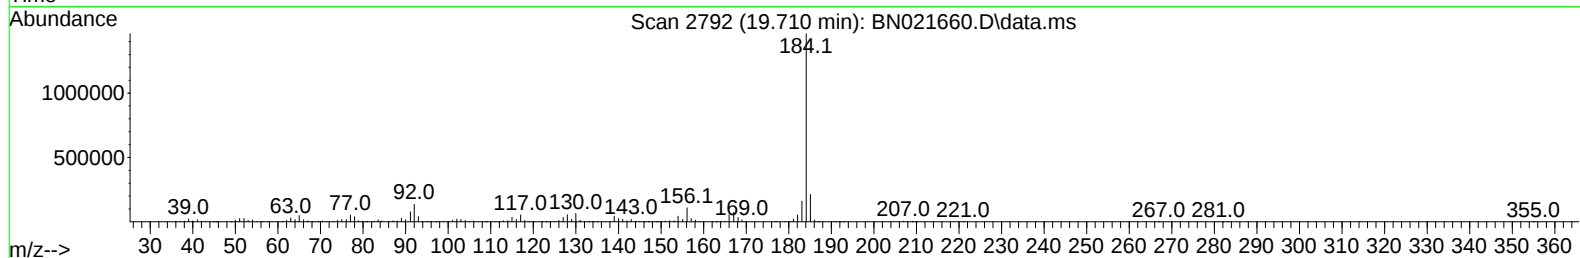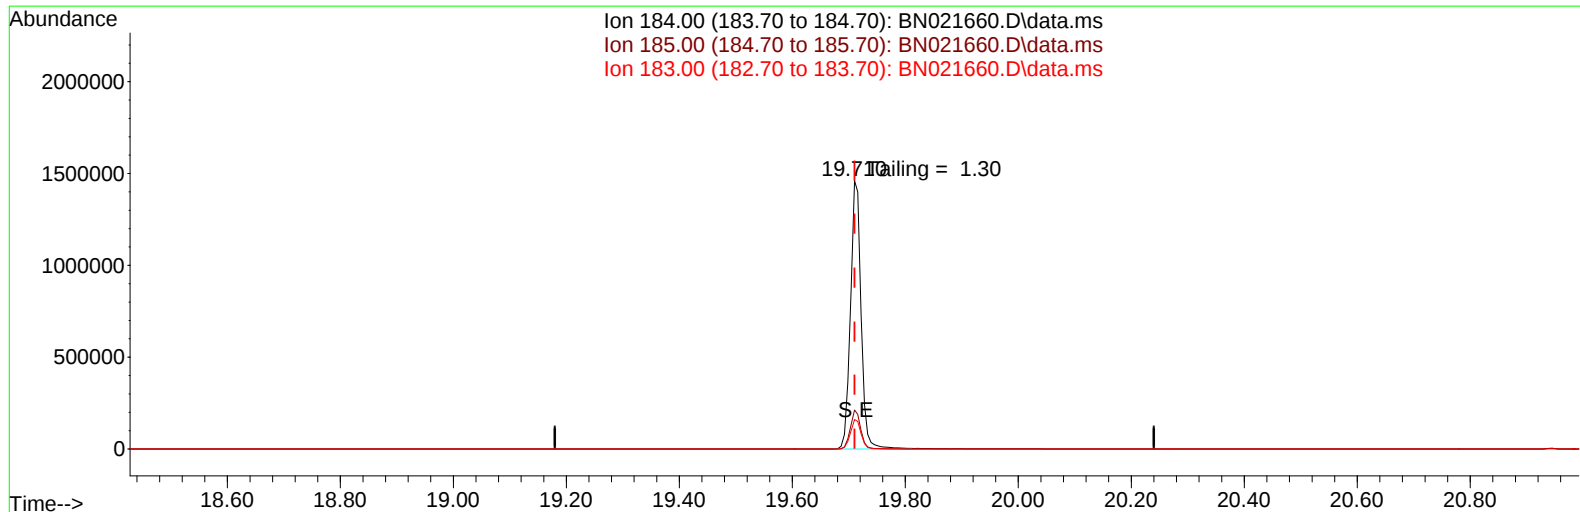

TIC: BN021660.D\data.ms

(77) Benzidine

19.710min (0.000) 1016832.70 ng

response 1911999

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.58
183.00	13.20	10.99
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/10/2022	BNA_N	<u>BN021660.D</u>
Compound Name	Response	Retention Time
DDT	1004498	20.945
DDD	14592	20.504
DDE	1461	19.992
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16053	1020551	1.57

Instrument :
BNA_N
ClientSampleId :
DFTPP