
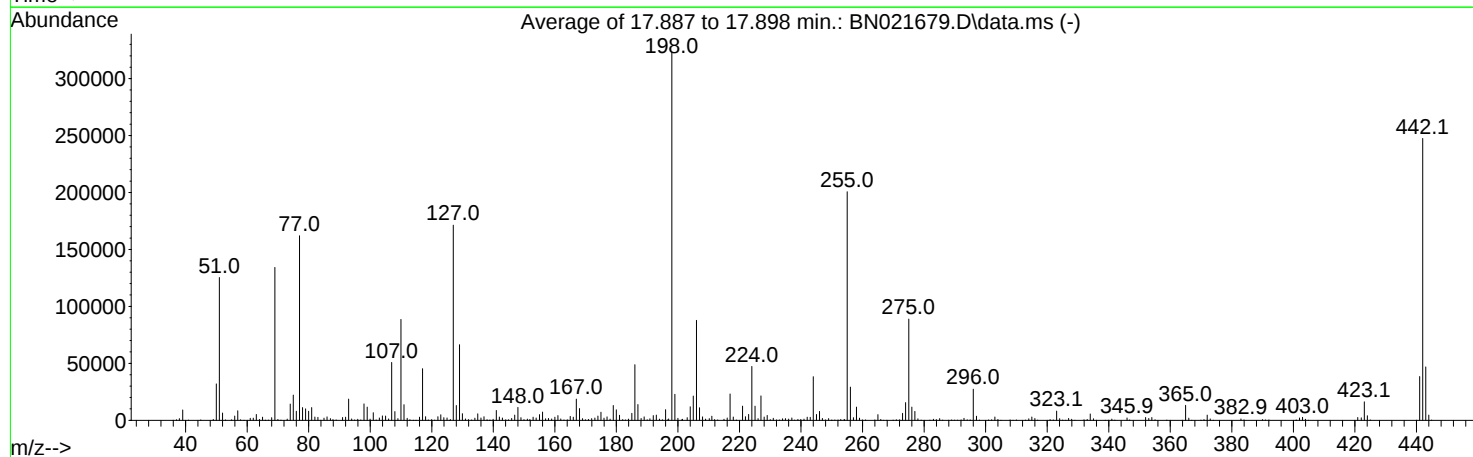


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091022\
 Data File : BN021679.D
 Acq On : 10 Sep 2022 03:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 13 02:32:27 2022

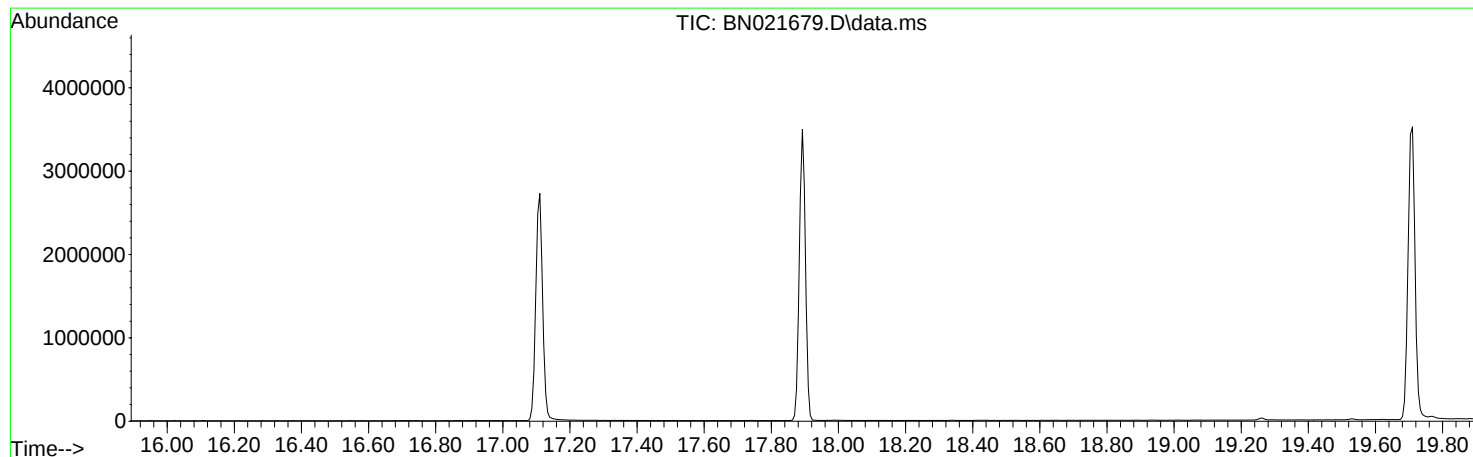




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	125451	PASS
68	69	0.00	2	1.7	2322	PASS
69	198	0.00	100	41.5	134165	PASS
70	69	0.00	2	0.6	757	PASS
127	198	10	80	53.0	171307	PASS
197	198	0.00	2	0.4	1138	PASS
198	198	100	100	100.0	322965	PASS
199	198	5	9	7.1	22843	PASS
275	198	10	60	27.5	88915	PASS
365	198	1	100	4.1	13183	PASS
441	198	0.01	100	11.9	38429	PASS
442	442	50	100	100.0	247488	PASS
443	442	15	24	18.9	46816	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091022\
 Data File : BN021679.D
 Acq On : 10 Sep 2022 03:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 10 05:05:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 10 05:03:56 2022
 Response via : Initial Calibration

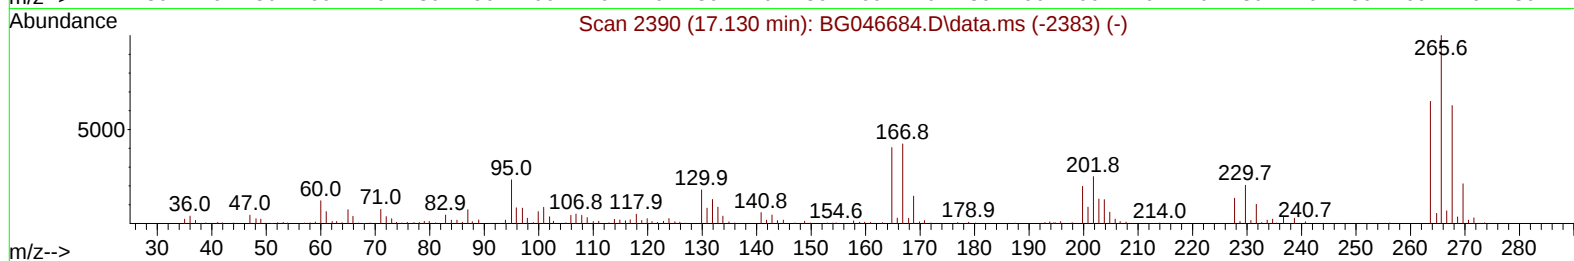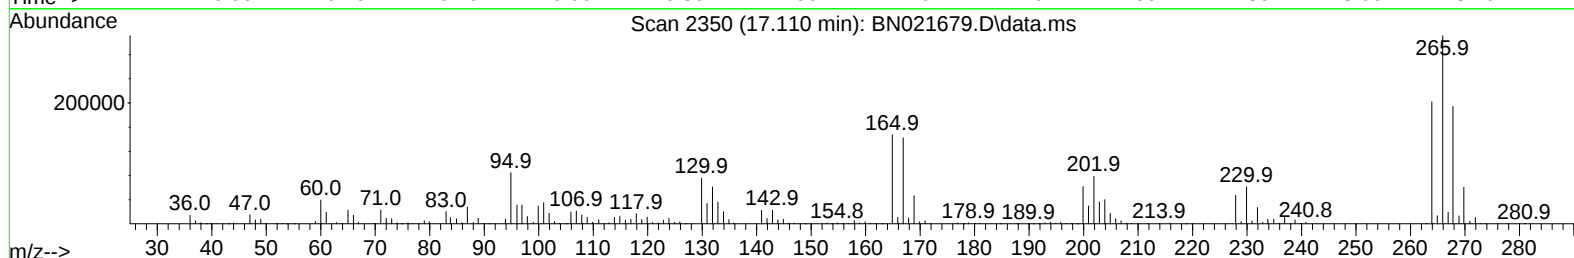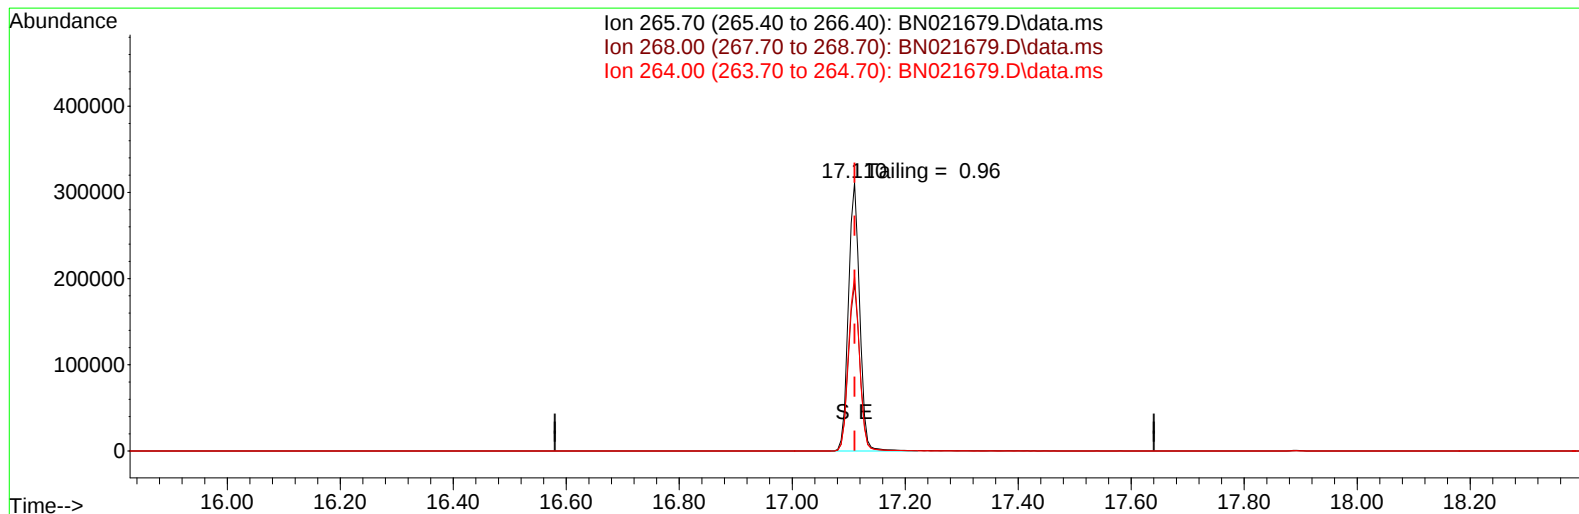

TIC: BN021679.D\data.ms

(70) Pentachlorophenol (C)

17.110min (+ 0.000) 24135.18 ng




response 431090

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.43
264.00	61.60	64.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091022\
Data File : BN021679.D
Acq On : 10 Sep 2022 03:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 10 05:05:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 10 05:03:56 2022
Response via : Initial Calibration

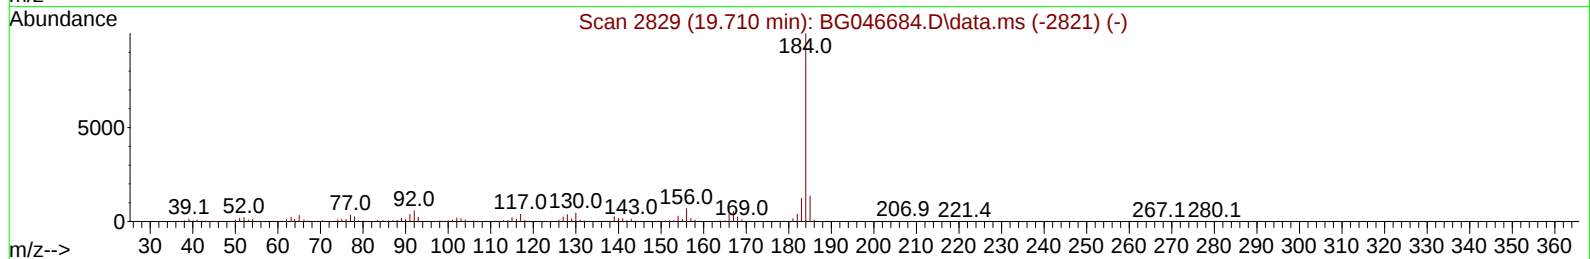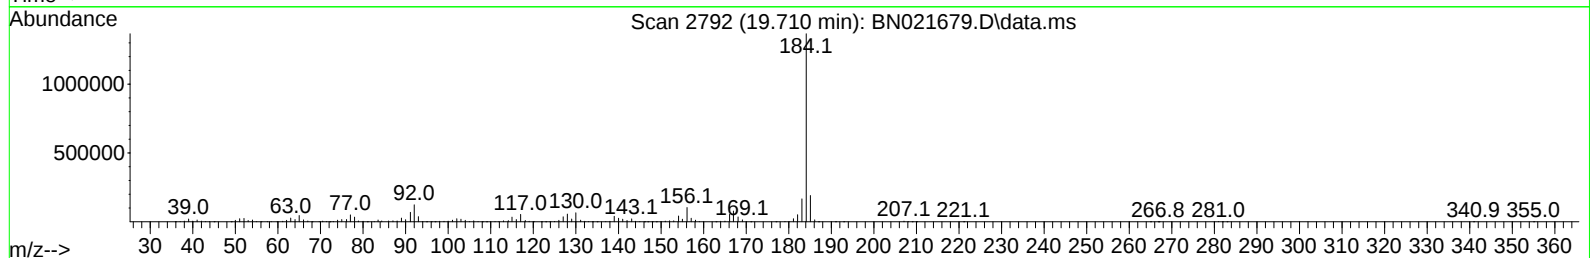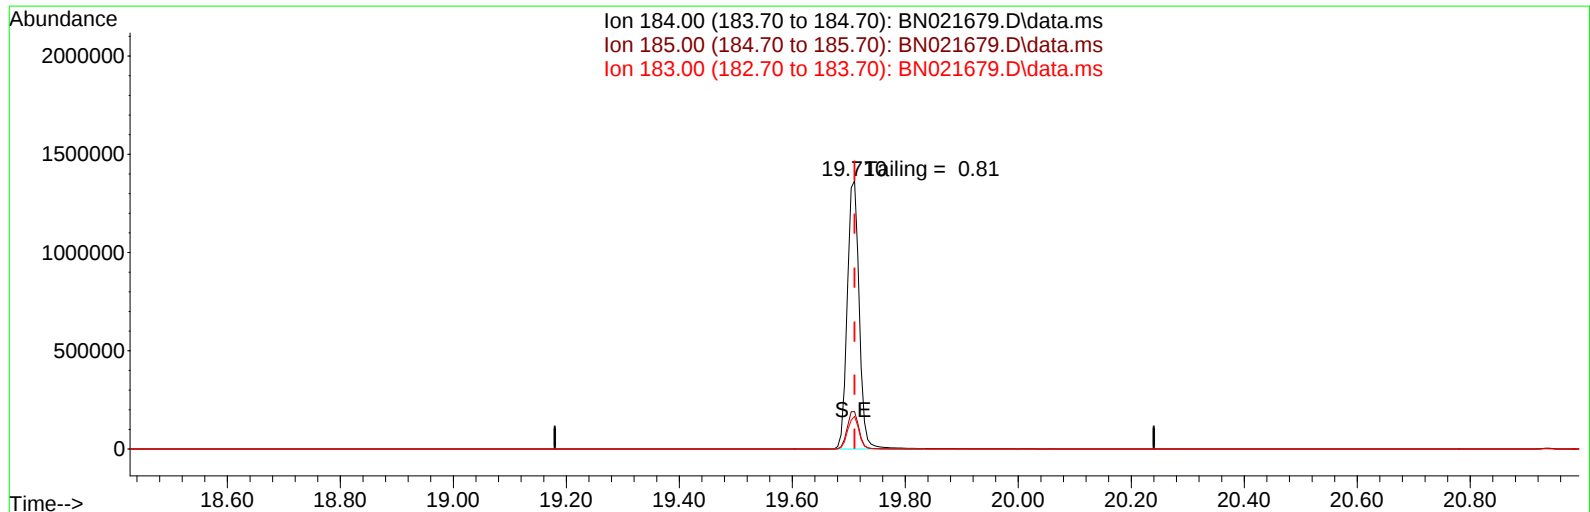

TIC: BN021679.D\data.ms

(77) Benzidine

19.710min (+ 0.000) 1228464.27 ng

response 2006997

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.98
183.00	13.20	12.16
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/10/2022	BNA_N	<u>BN021679.D</u>
Compound Name	Response	Retention Time
DDT	1046202	20.939
DDD	79716	20.498
DDE	2153	19.986
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
81869	1128071	7.26

Instrument :
BNA_N
ClientSampleId :
DFTPP