
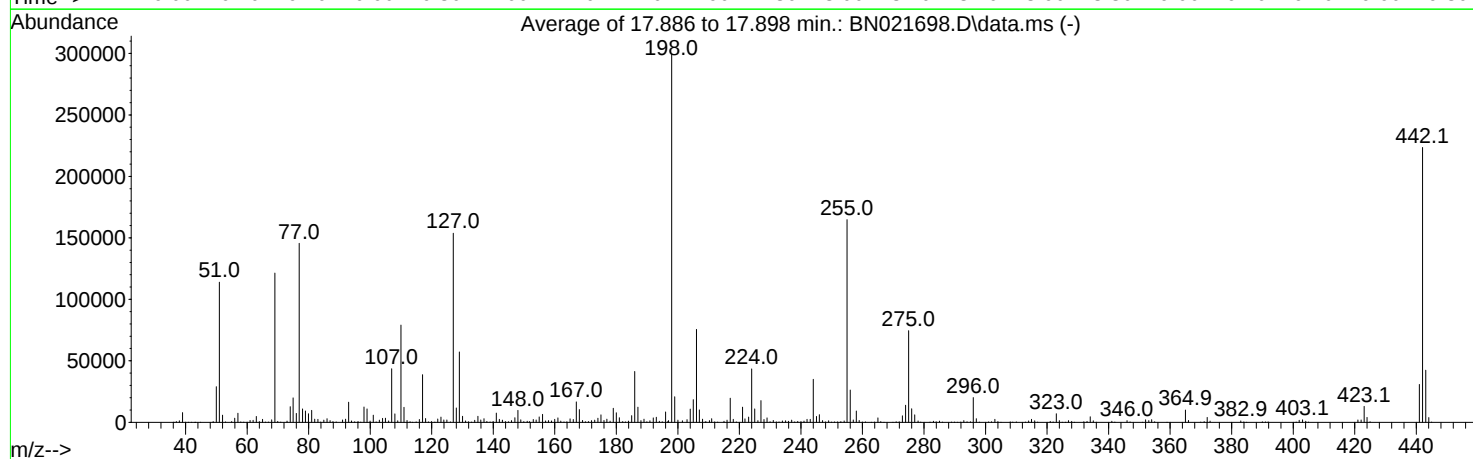


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091022\
 Data File : BN021698.D
 Acq On : 10 Sep 2022 14:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 13 02:32:27 2022

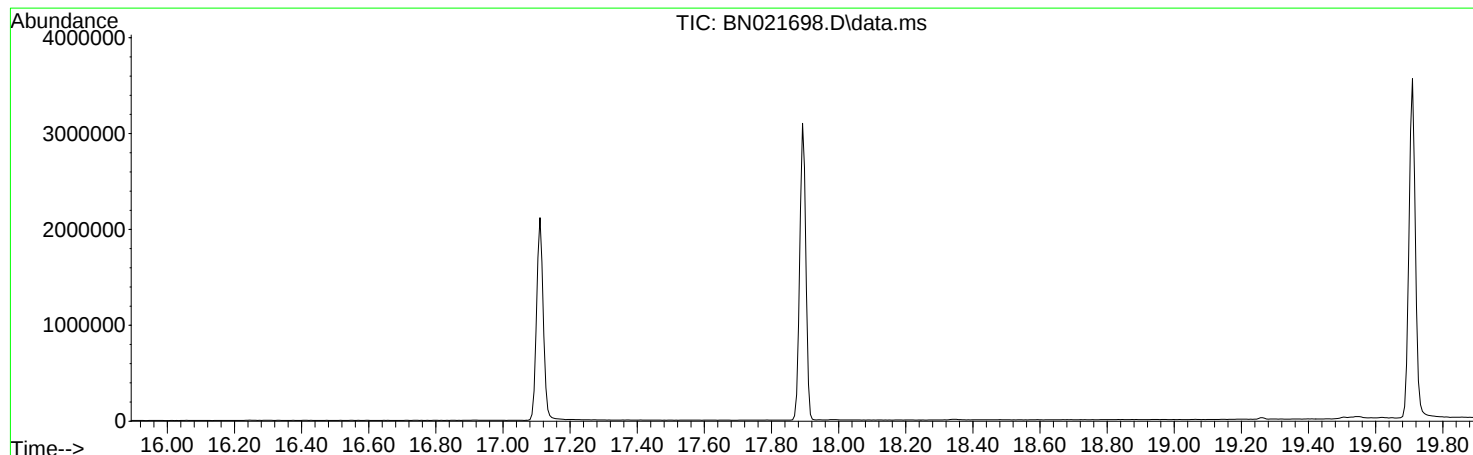




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	113992	PASS
68	69	0.00	2	1.7	2013	PASS
69	198	0.00	100	40.6	121333	PASS
70	69	0.00	2	0.6	736	PASS
127	198	10	80	51.4	153728	PASS
197	198	0.00	2	0.5	1378	PASS
198	198	100	100	100.0	299200	PASS
199	198	5	9	6.9	20717	PASS
275	198	10	60	24.9	74507	PASS
365	198	1	100	3.3	9998	PASS
441	198	0.01	100	10.3	30837	PASS
442	442	50	100	100.0	223531	PASS
443	442	15	24	19.0	42363	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091022\
Data File : BN021698.D
Acq On : 10 Sep 2022 14:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 12 02:31:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 12 02:31:07 2022
Response via : Initial Calibration

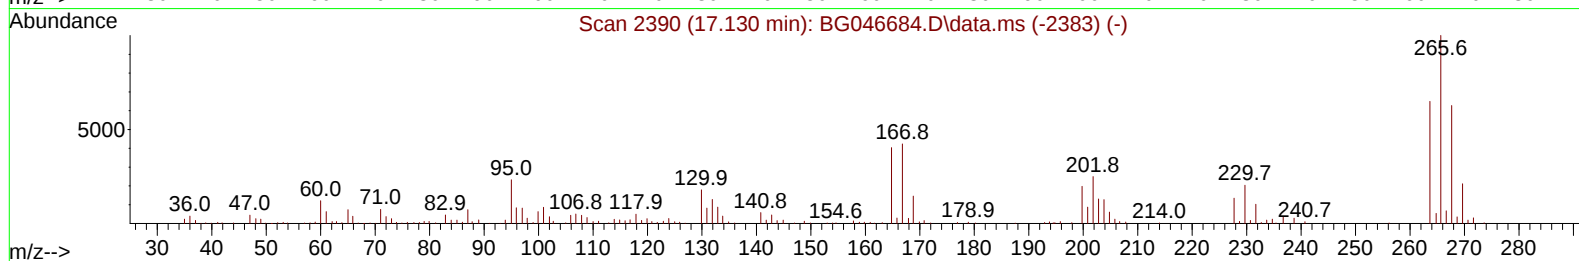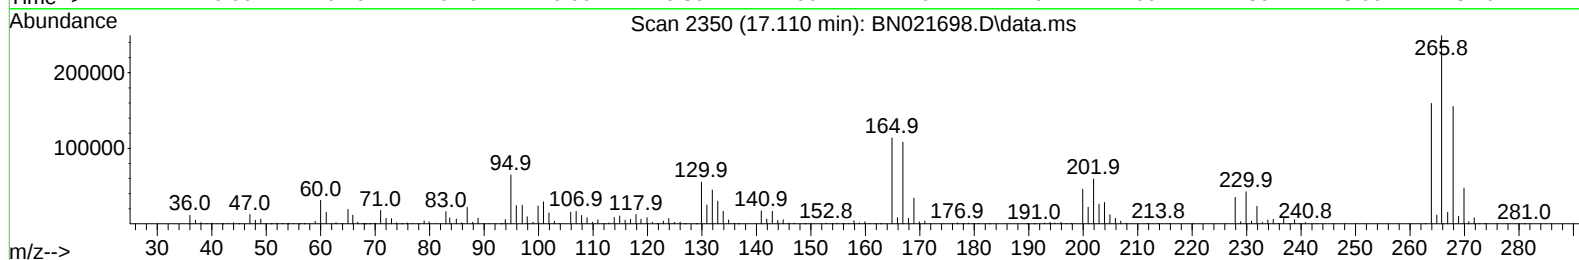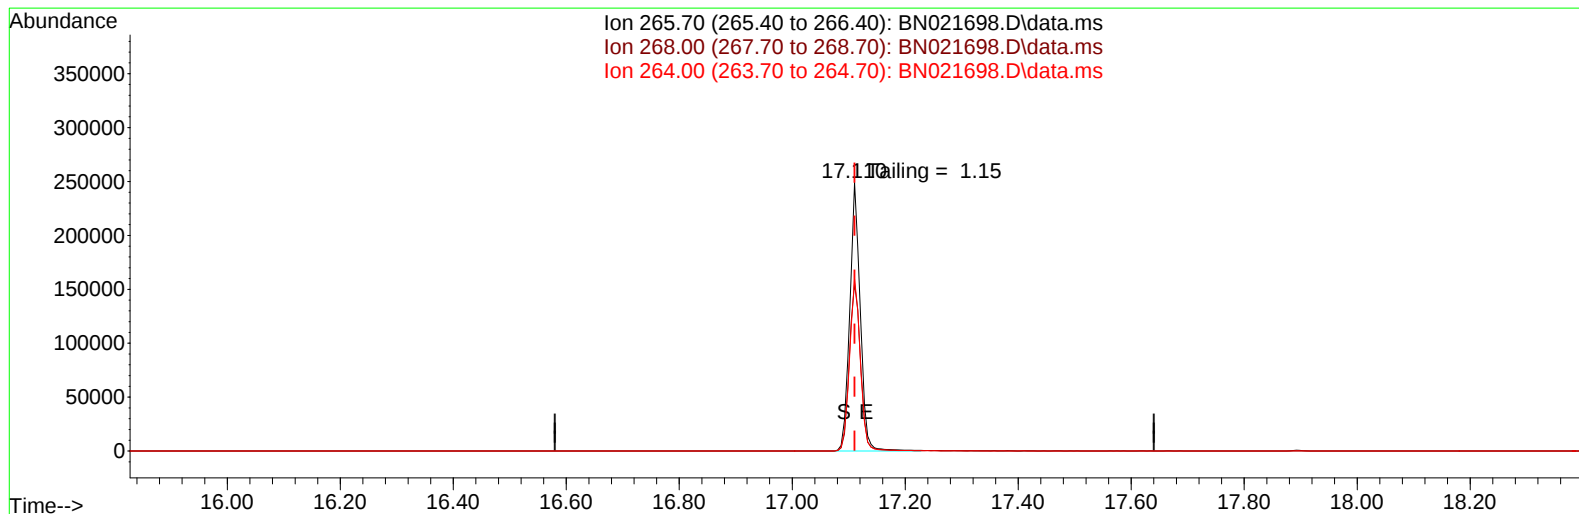

TIC: BN021698.D\data.ms

(70) Pentachlorophenol (C)

17.110min (0.000) 20049.45 ng




response 324756

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.44
264.00	61.60	64.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091022\
Data File : BN021698.D
Acq On : 10 Sep 2022 14:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 12 02:31:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 12 02:31:07 2022
Response via : Initial Calibration

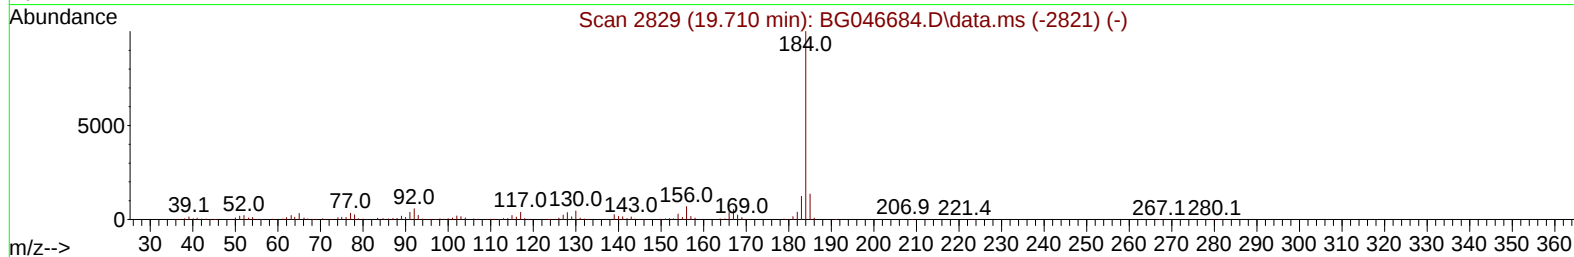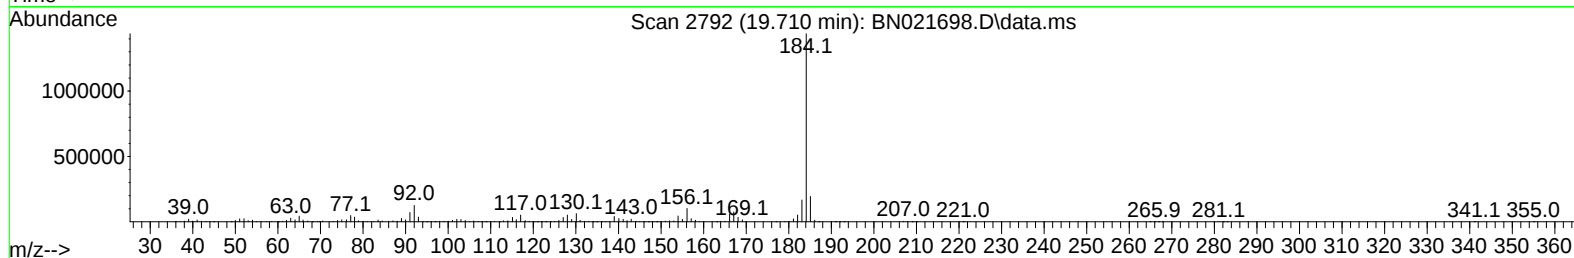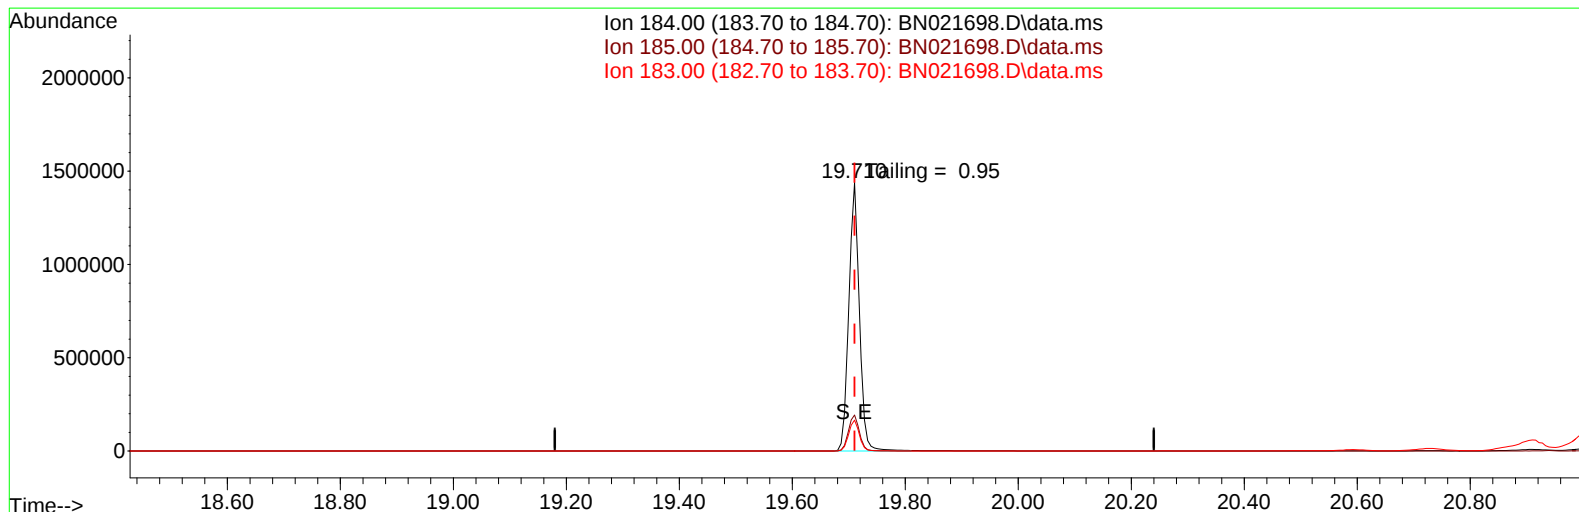

TIC: BN021698.D\data.ms

(77) Benzidine

19.710min (0.000) 1090023.93 ng

response 1881622

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.43
183.00	13.20	11.55
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/10/2022	BNA_N	<u>BN021698.D</u>
Compound Name	Response	Retention Time
DDT	839538	20.939
DDD	103964	20.498
DDE	1134	19.986
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
105098	944636	11.13

Instrument :
BNA_N
ClientSampleId :
DFTPP