
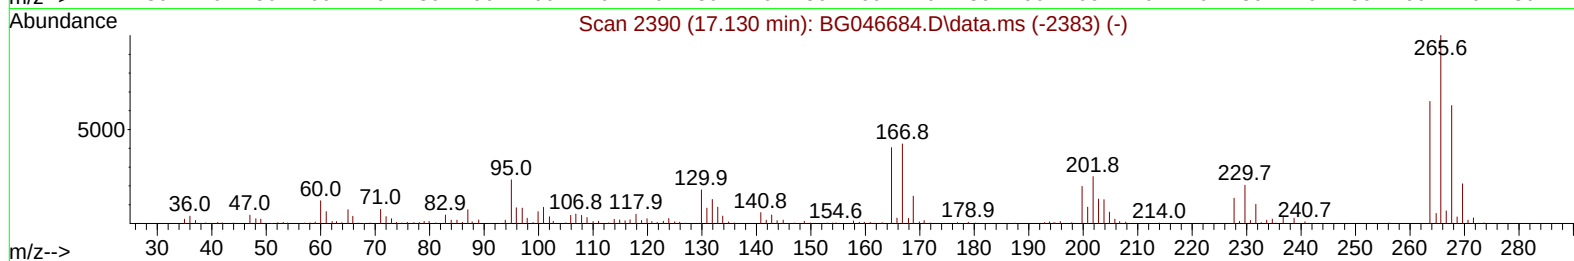
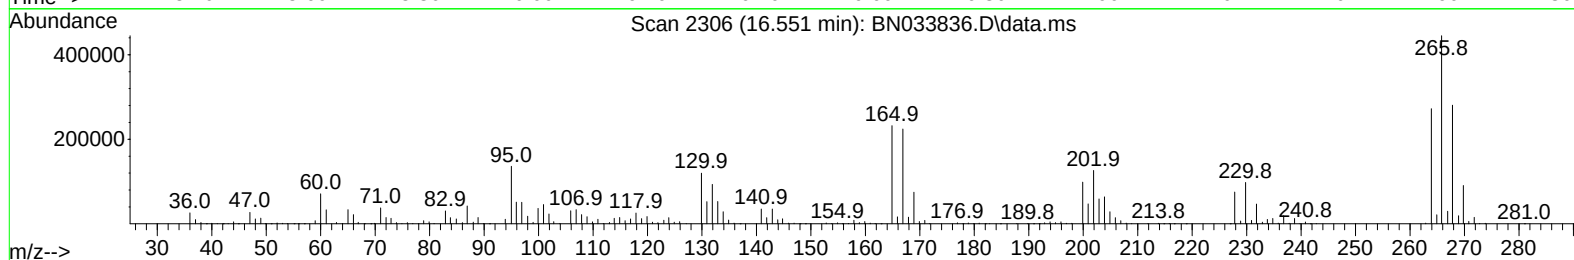


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN091024\  
Data File : BN033836.D  
Acq On : 10 Sep 2024 10:37  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 13:55:21 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Sep 10 04:22:28 2024  
Response via : Initial Calibration

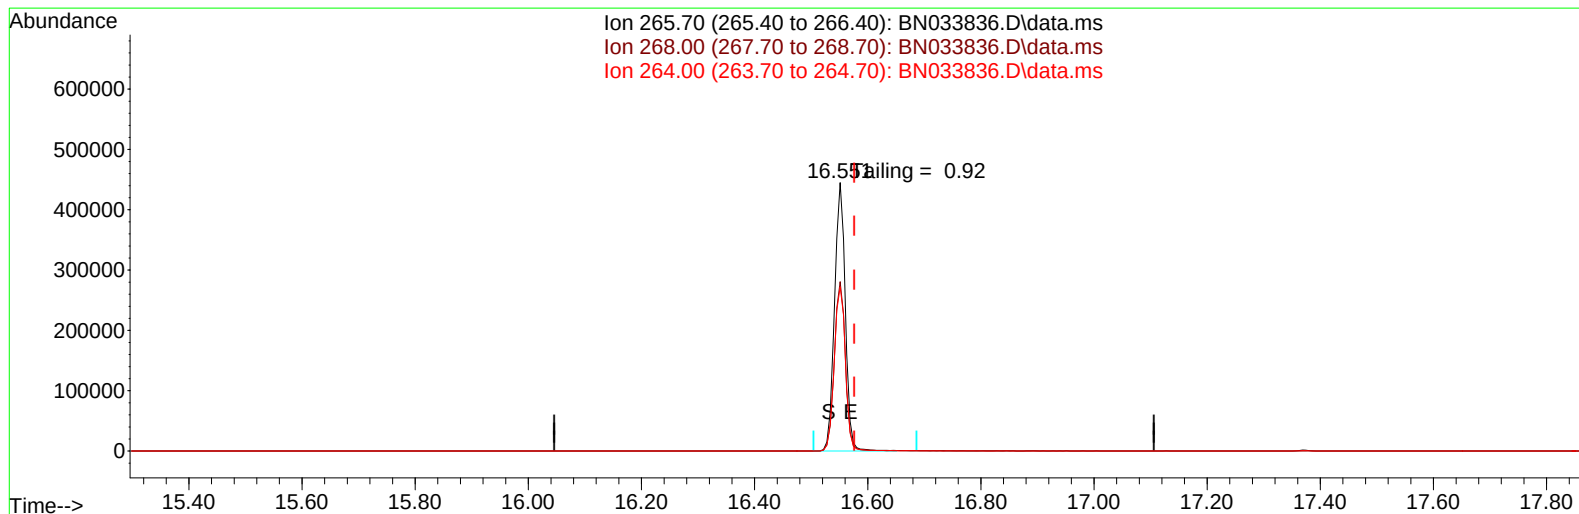

TIC: BN033836.D\data.ms




**(70) Pentachlorophenol (C)**

16.551min (-0.025) 22069.97 ng

response 591823

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 63.08  |
| 264.00 | 61.60  | 61.17  |
| 0.00   | 0.00   | 0.00   |

Quant Time: Sep 10 13:58:28 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Sep 10 04:22:28 2024  
Response via : Initial Calibration

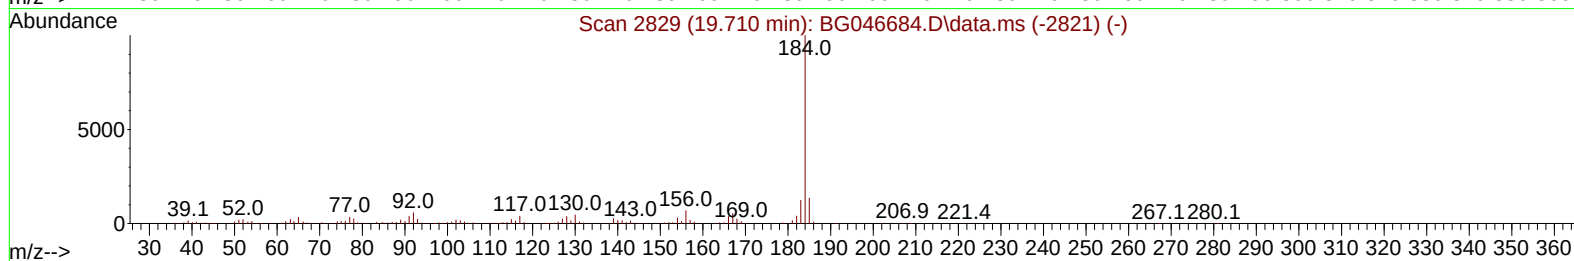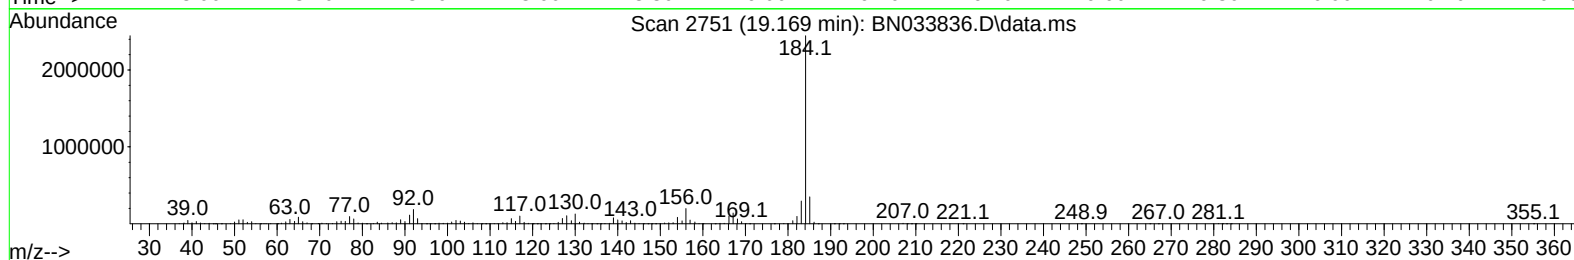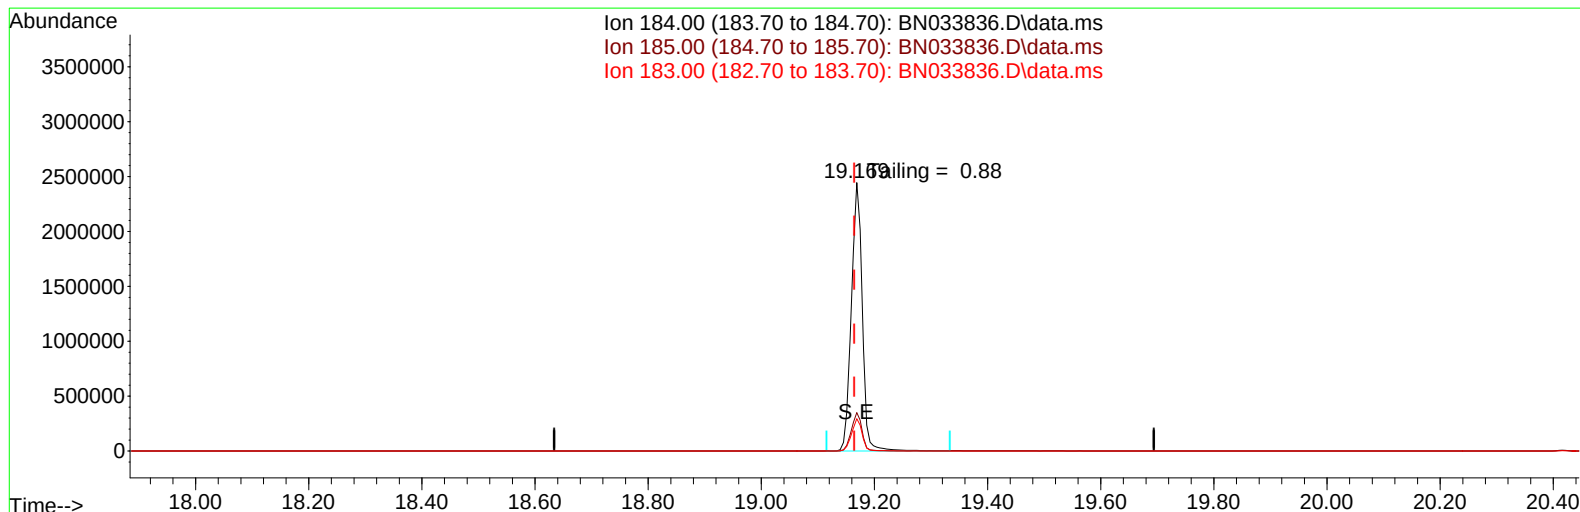

TIC: BN033836.D\data.ms

(77) Benzidine

**19.169min (+ 0.005) 0.00 ng**

response 3272624

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.34  |
| 183.00 | 13.20  | 12.08  |
| 0.00   | 0.00   | 0.00   |