


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091024\
Data File : BN033836.D
Acq On : 10 Sep 2024 10:37
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN090424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 04 18:36:01 2024

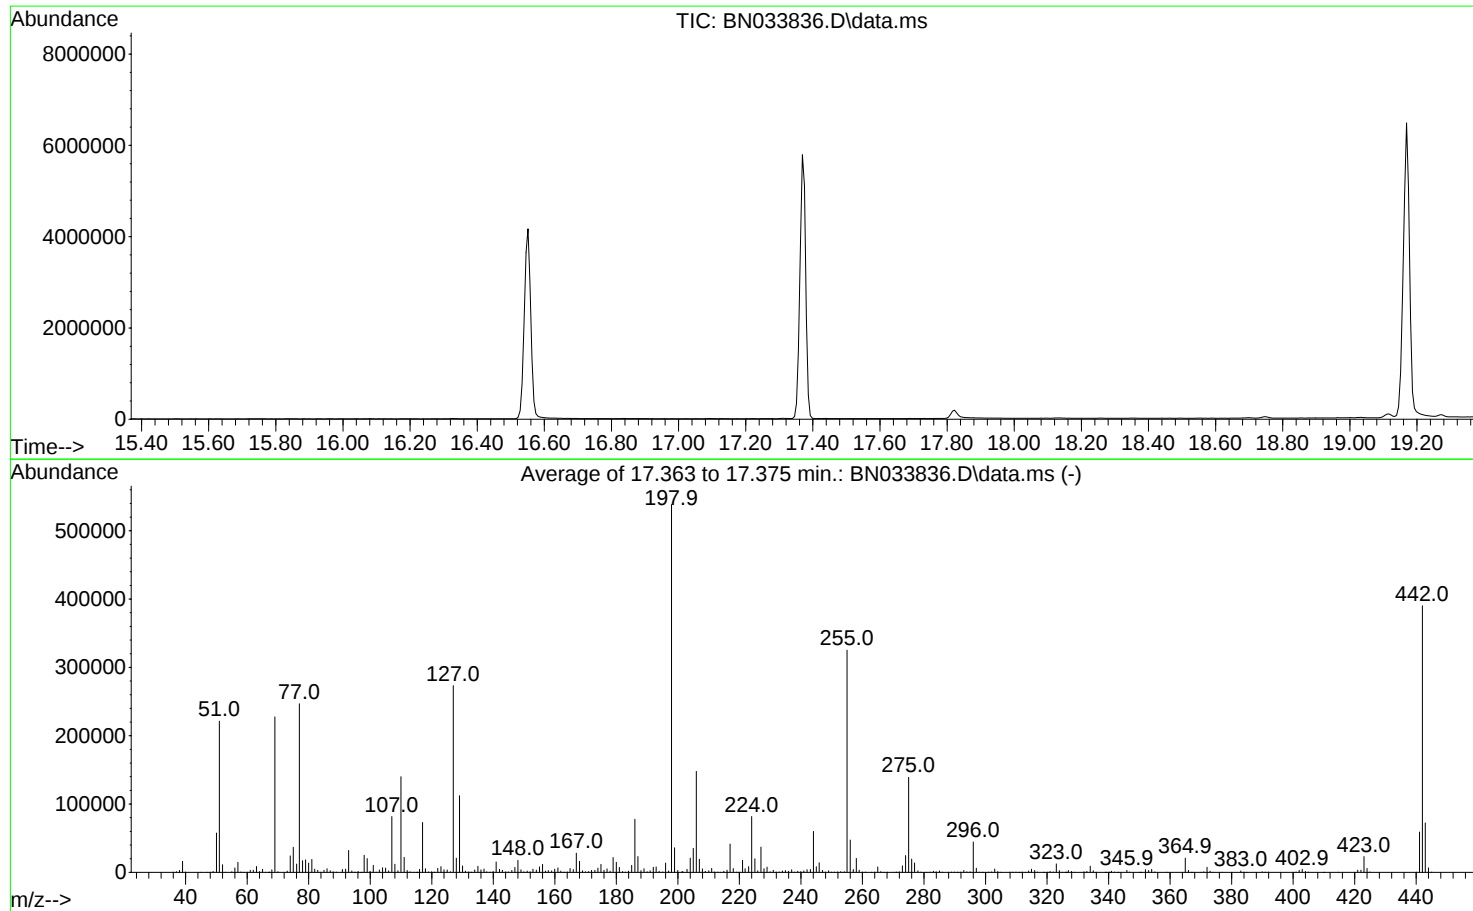

AutoFind: Scans 2444, 2445, 2446; Background Corrected with Scan 2437

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	221365	PASS
68	69	0.00	2	1.6	3705	PASS
69	198	0.00	100	42.3	227597	PASS
70	69	0.00	2	0.5	1040	PASS
127	198	10	80	50.7	273195	PASS
197	198	0.00	2	0.4	2201	PASS
198	198	100	100	100.0	538411	PASS
199	198	5	9	6.7	36131	PASS
275	198	10	60	25.8	139125	PASS
365	198	1	100	3.9	20890	PASS
441	198	0.01	100	11.0	59021	PASS
442	442	50	100	100.0	390080	PASS
443	442	15	24	18.6	72501	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/10/2024	BNA_N	<u>BN033836.D</u>
Compound Name	Response	Retention Time
DDT	1781963	20.416
DDD	37253	19.969
DDE	1595	19.463
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
38848	1820811	2.13

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091024\
Data File : BN033836.D
Acq On : 10 Sep 2024 10:37
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 10 13:55:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 04:22:28 2024
Response via : Initial Calibration

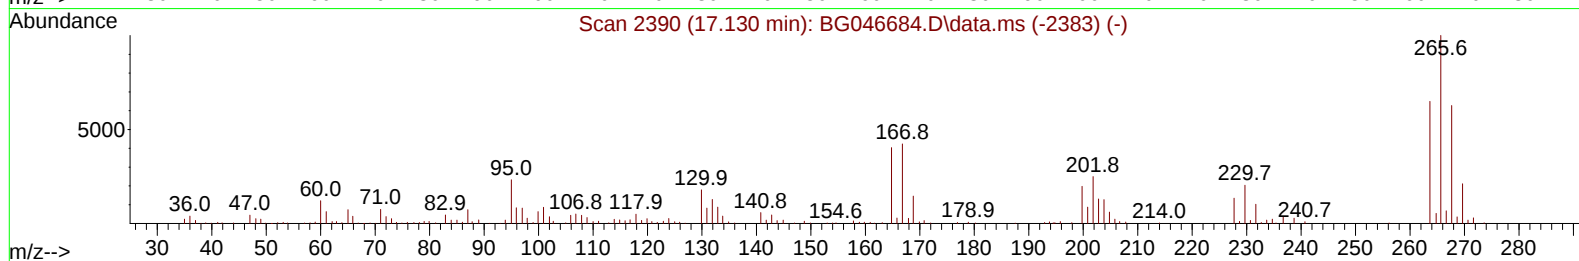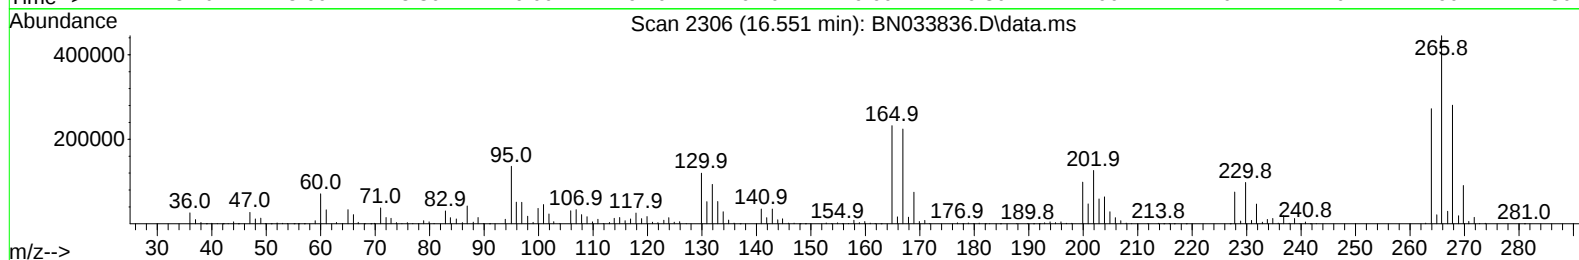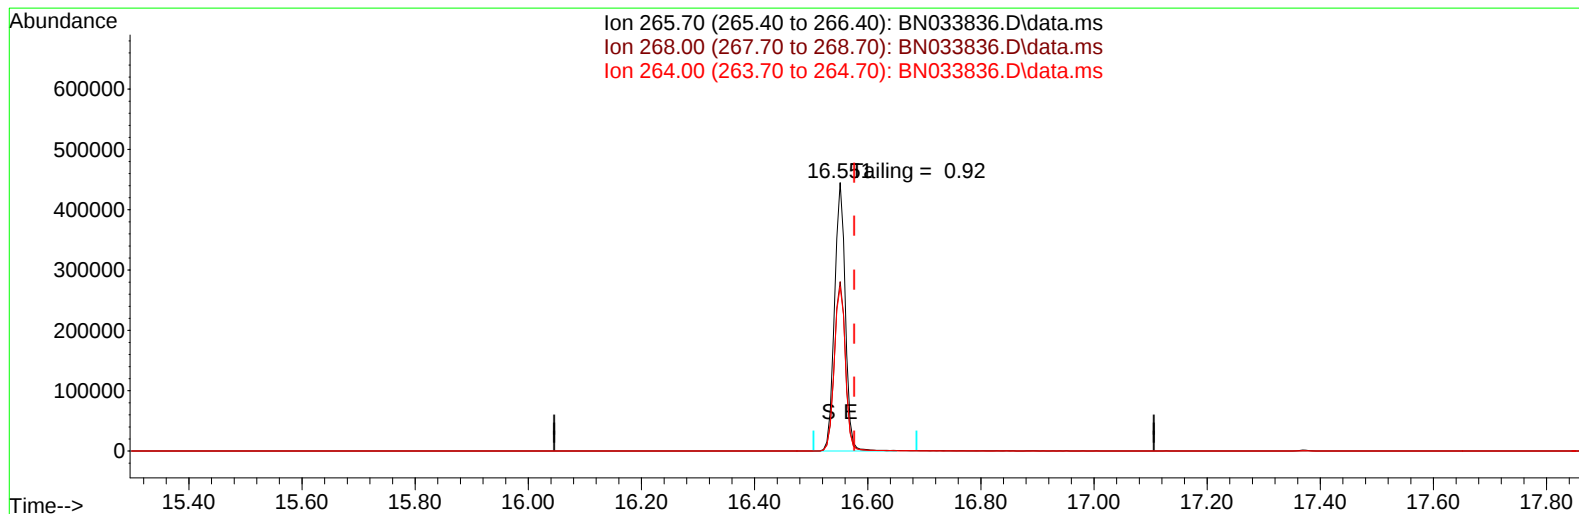

TIC: BN033836.D\data.ms

(70) Pentachlorophenol (C)

16.551min (-0.025) 22069.97 ng




response 591823

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.08
264.00	61.60	61.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091024\
Data File : BN033836.D
Acq On : 10 Sep 2024 10:37
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 10 13:58:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 04:22:28 2024
Response via : Initial Calibration

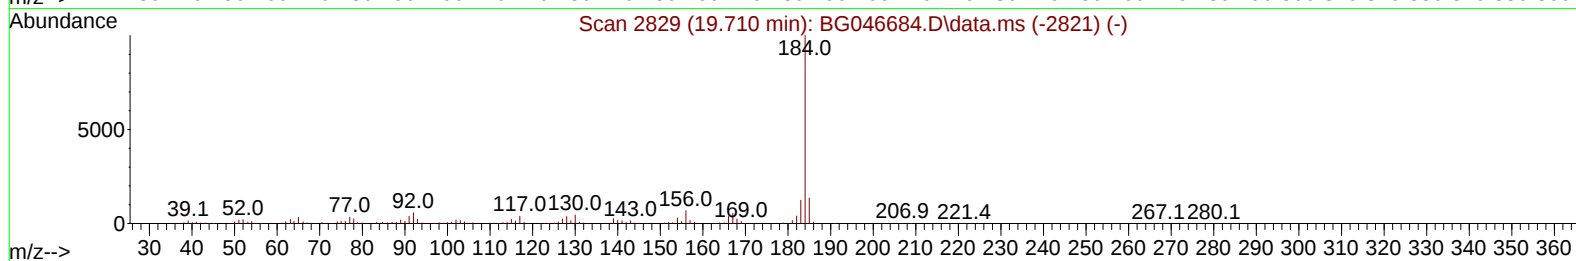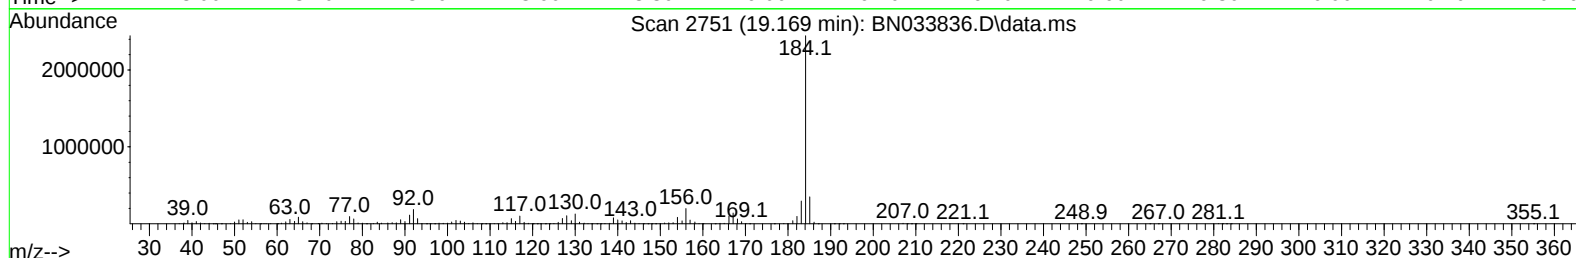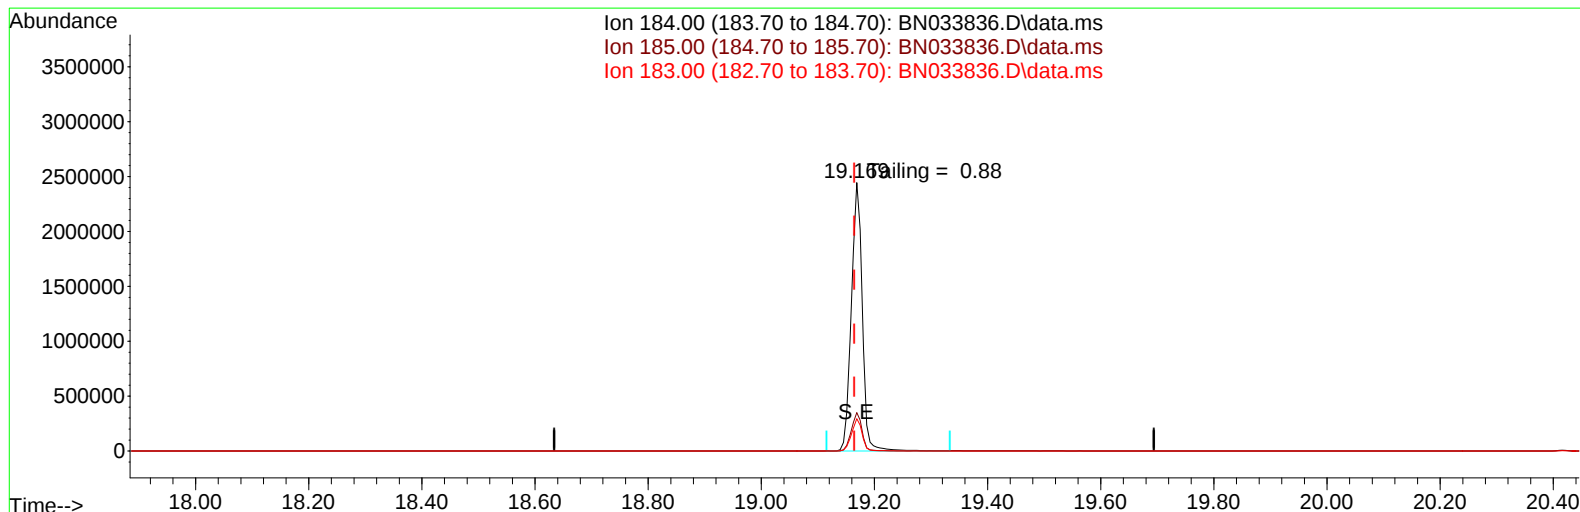

TIC: BN033836.D\data.ms

(77) Benzidine

19.169min (+ 0.005) 0.00 ng

response 3272624

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.34
183.00	13.20	12.08
0.00	0.00	0.00