


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091025\
Data File : BN037676.D
Acq On : 10 Sep 2025 09:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN090925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 10 02:02:04 2025

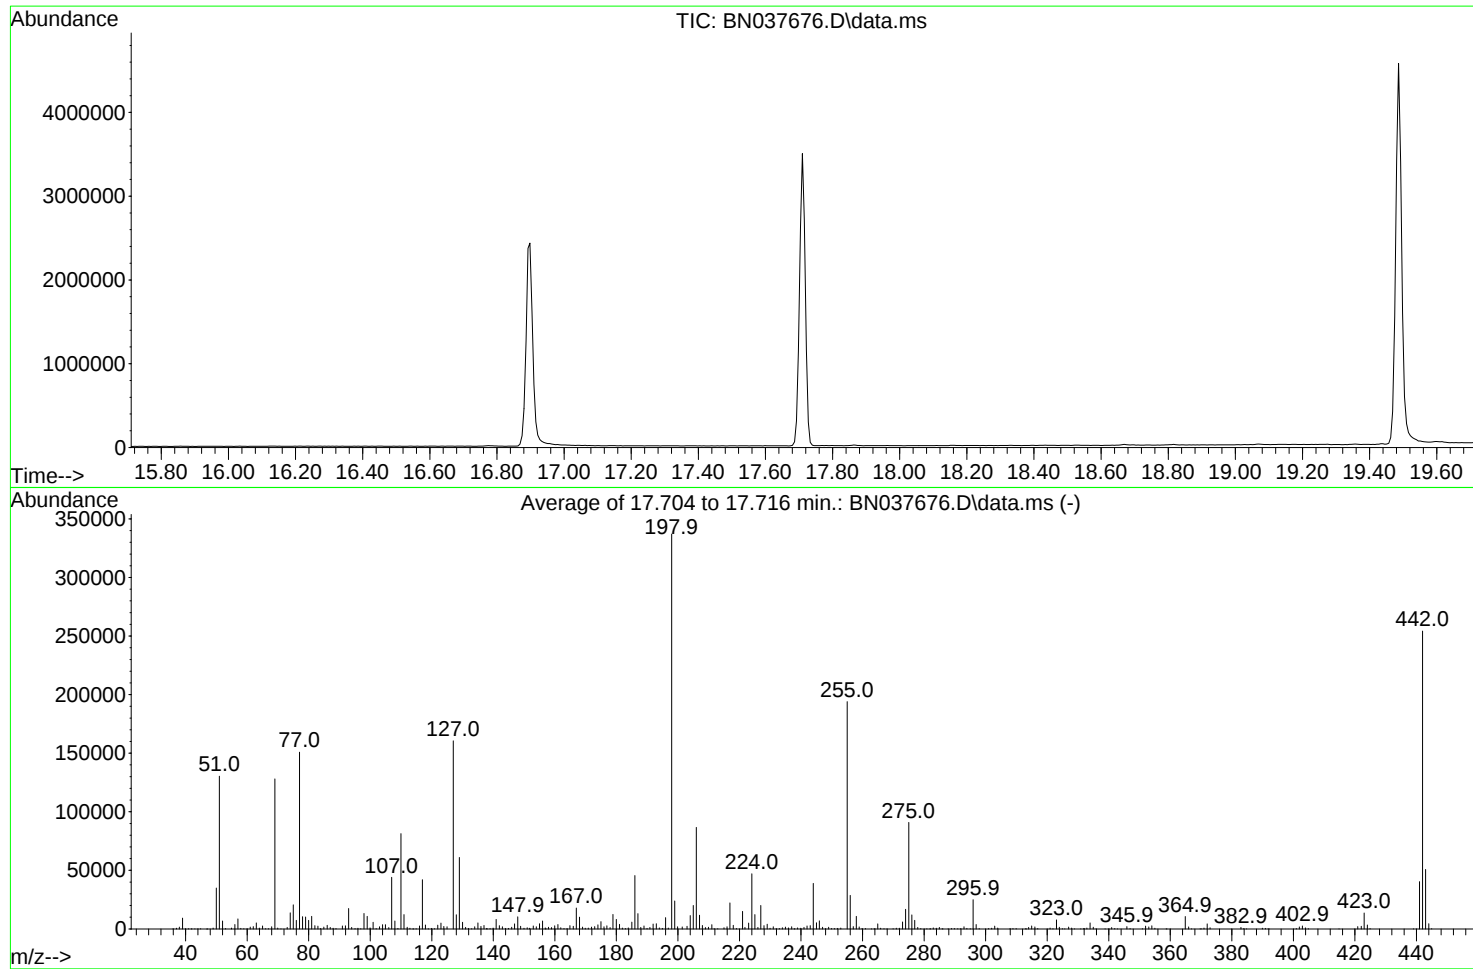

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.4	1798	PASS
69	69	100	100	100.0	128077	PASS
70	69	0.00	2	0.6	752	PASS
197	198	0.00	2	0.2	753	PASS
198	198	100	100	100.0	337024	PASS
199	198	5	9	7.1	23811	PASS
365	198	1	100	3.1	10612	PASS
441	443	0.01	150	79.7	40411	PASS
442	442	100	100	100.0	254187	PASS
443	442	15	24	20.0	50720	PASS