

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN091118\
 Data File : BN002634.D
 Acq On : 11 Sep 2018 18:34
 Operator : JU/SJ
 Sample : J4837-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C08J6

Manual Integrations
 APPROVED

Sohil
 9/12/2018 4:54:56 PM

Quant Time: Sep 12 08:10:27 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 12 07:54:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	151006	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	685278	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.29	164	426347	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.05	188	995534	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	1091512	20.00	ng/ul	0.00
85) Perylene-d12	23.46	264	1087513	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.23	96	11931	3.73	ng/uL	0.00
5) Phenol-d5	6.85	99	89824	6.49	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	276698	31.82	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	283102	26.84	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	177480	16.03	ng/ul	0.00
19) Nitrobenzene-d5	8.81	128	180295	33.05	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	210164	36.64	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	331742	31.47	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	0.00
43) Dimethylphthalate-d6	13.71	166	1326533	37.53	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	1522390	35.11	ng/ul	0.00
51) 4-Nitrophenol-d4	14.53	143	39055m	5.85	ng/ul	0.01
57) Fluorene-d10	15.29	176	1131424	36.92	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	214906	33.91	ng/ul	0.00
70) Anthracene-d10	17.15	188	1825844	38.39	ng/ul	0.00
78) Pyrene-d10	19.45	212	2058761	39.42	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.33	264	2225597	39.14	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.76	163	35172	1.015	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN091118\
Data File : BN002634.D
Acq On : 11 Sep 2018 18:34
Operator : JU/SJ
Sample : J4837-13
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C08J6

Quant Time: Sep 12 08:10:27 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 12 07:54:03 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
9/12/2018 4:54:56 PM

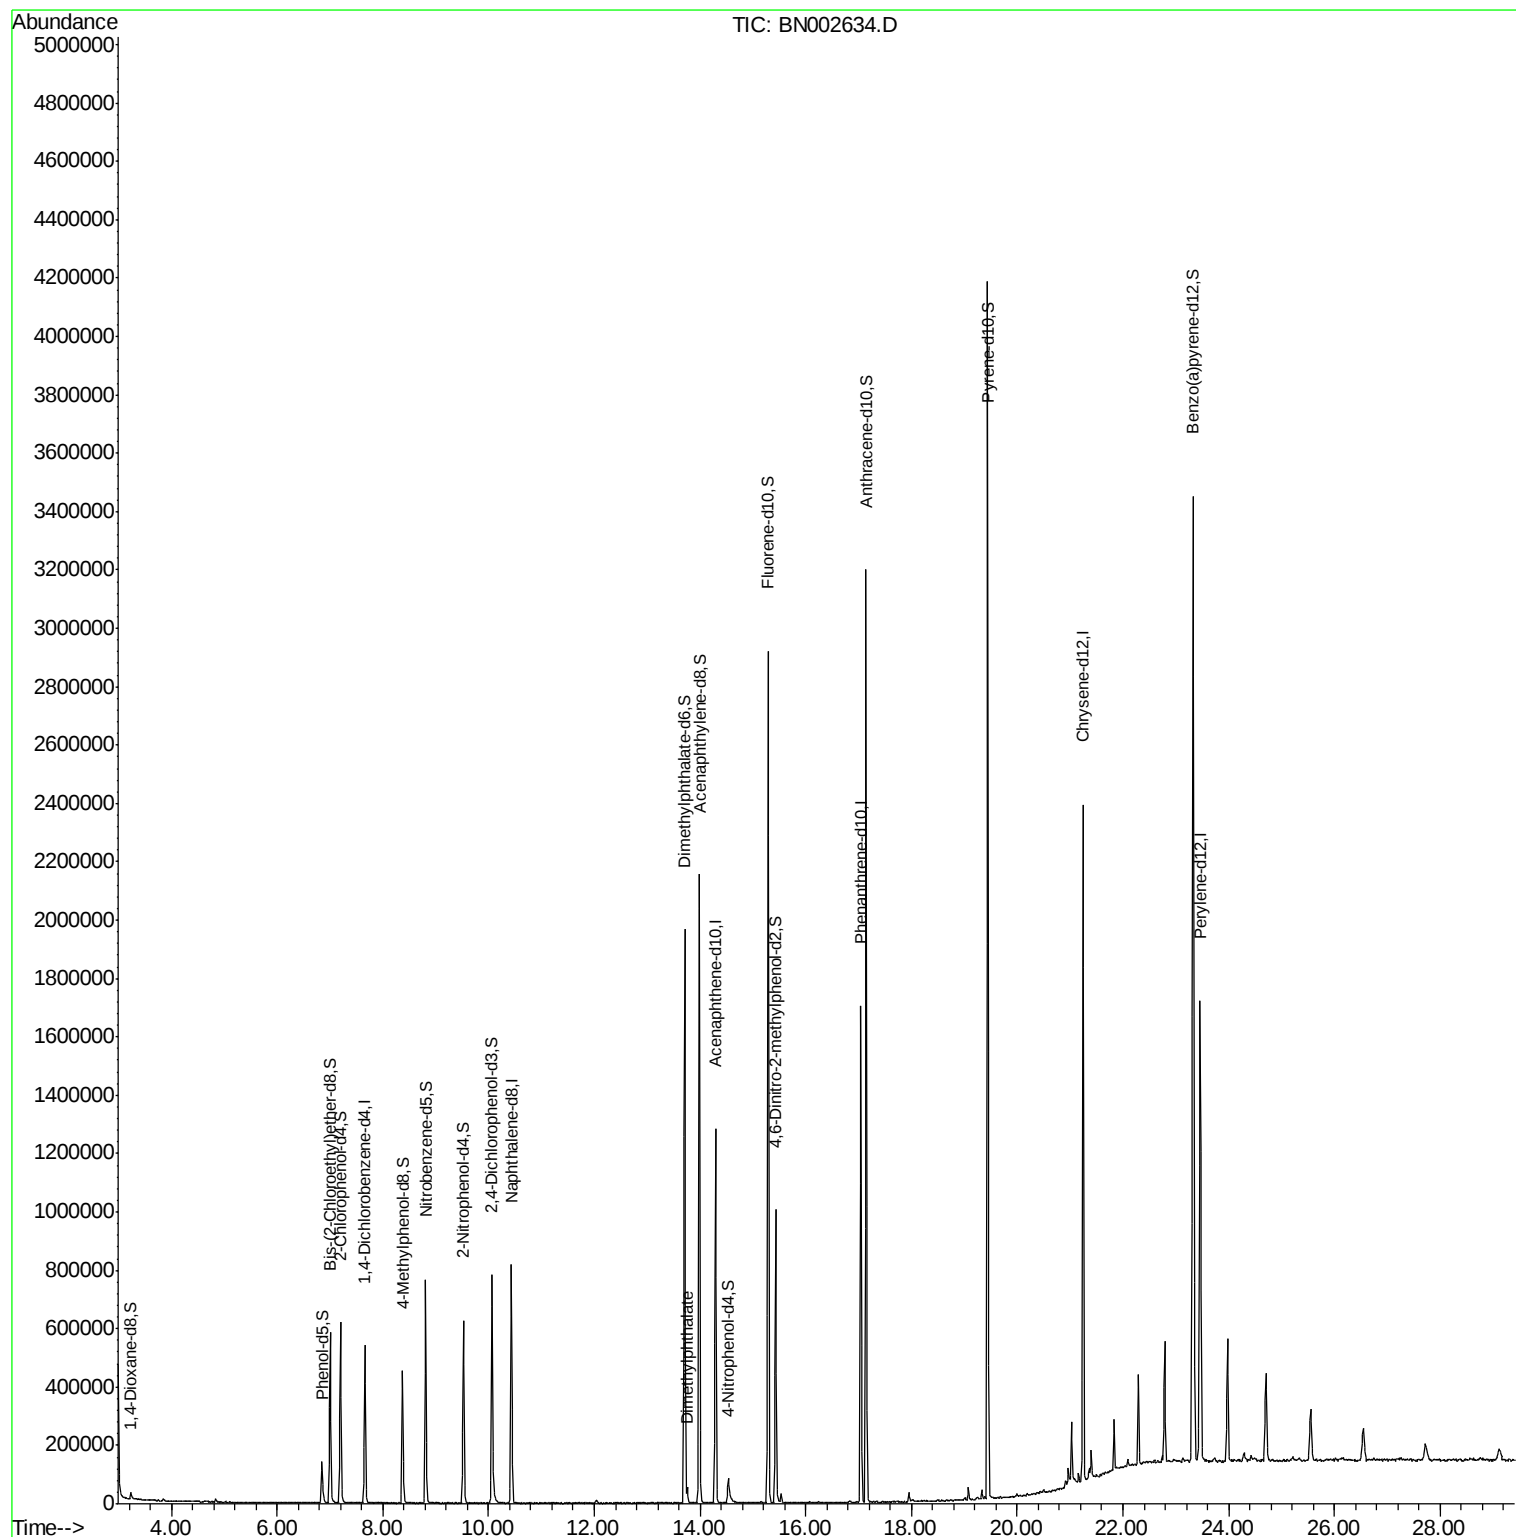

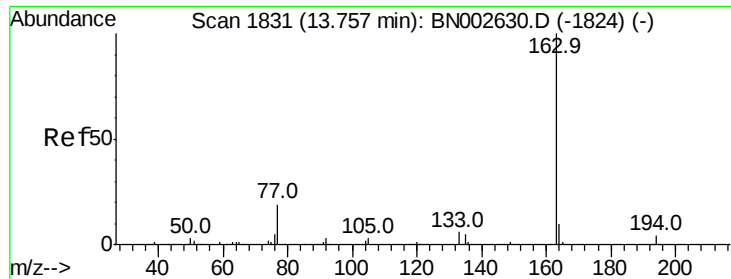


#44
 Dimethylphthalate
 Concen: 1.015 ng/ul
 RT: 13.76 min Scan# 1831
 Delta R.T. -0.00 min
 Lab File: BN002634.D
 Acq: 11 Sep 2018 18:34

Instrument :
 BNA_N
 ClientSampleId :
 C08J6

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.7	3.2	4.8
164	10.1	7.8	11.8

Manual Integrations
 APPROVED

Sohil
 9/12/2018 4:54:56 PM

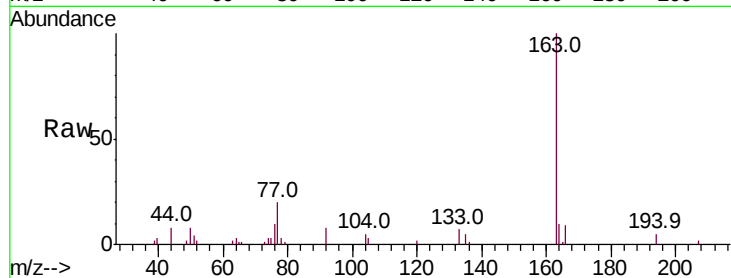

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

