

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN091118\
 Data File : BN002641.D
 Acq On : 11 Sep 2018 22:40
 Operator : JU/SJ
 Sample : J4837-16
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C08S0

Manual Integrations
 APPROVED

Sohil
 9/12/2018 4:55:07 PM

Quant Time: Sep 12 08:33:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 12 07:54:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	158198	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	724757	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.29	164	451123	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.05	188	1051771	20.00	ng/ul	0.00
77) Chrysene-d12	21.24	240	1095029	20.00	ng/ul	0.00
85) Perylene-d12	23.46	264	1004770	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	16837	5.02	ng/uL	0.00
5) Phenol-d5	6.85	99	74592	5.14	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	235002	25.79	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	242375	21.94	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	146494	12.63	ng/ul	0.00
19) Nitrobenzene-d5	8.81	128	156242	27.08	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	182270	30.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	285091	25.57	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
43) Dimethylphthalate-d6	13.71	166	1114522	29.80	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	1201749	26.20	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	29632m	4.19	ng/ul	0.02
57) Fluorene-d10	15.29	176	962632	29.69	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	173936	25.97	ng/ul	0.00
70) Anthracene-d10	17.14	188	1521017	30.27	ng/ul	0.00
78) Pyrene-d10	19.45	212	1715889	32.75	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.32	264	1646837	31.34	ng/ul	0.00

Target Compounds					Ovalue	
44) Dimethylphthalate	13.76	163	283897	7.740	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN091118\
Data File : BN002641.D
Acq On : 11 Sep 2018 22:40
Operator : JU/SJ
Sample : J4837-16
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C08S0

Quant Time: Sep 12 08:33:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 12 07:54:03 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
9/12/2018 4:55:07 PM

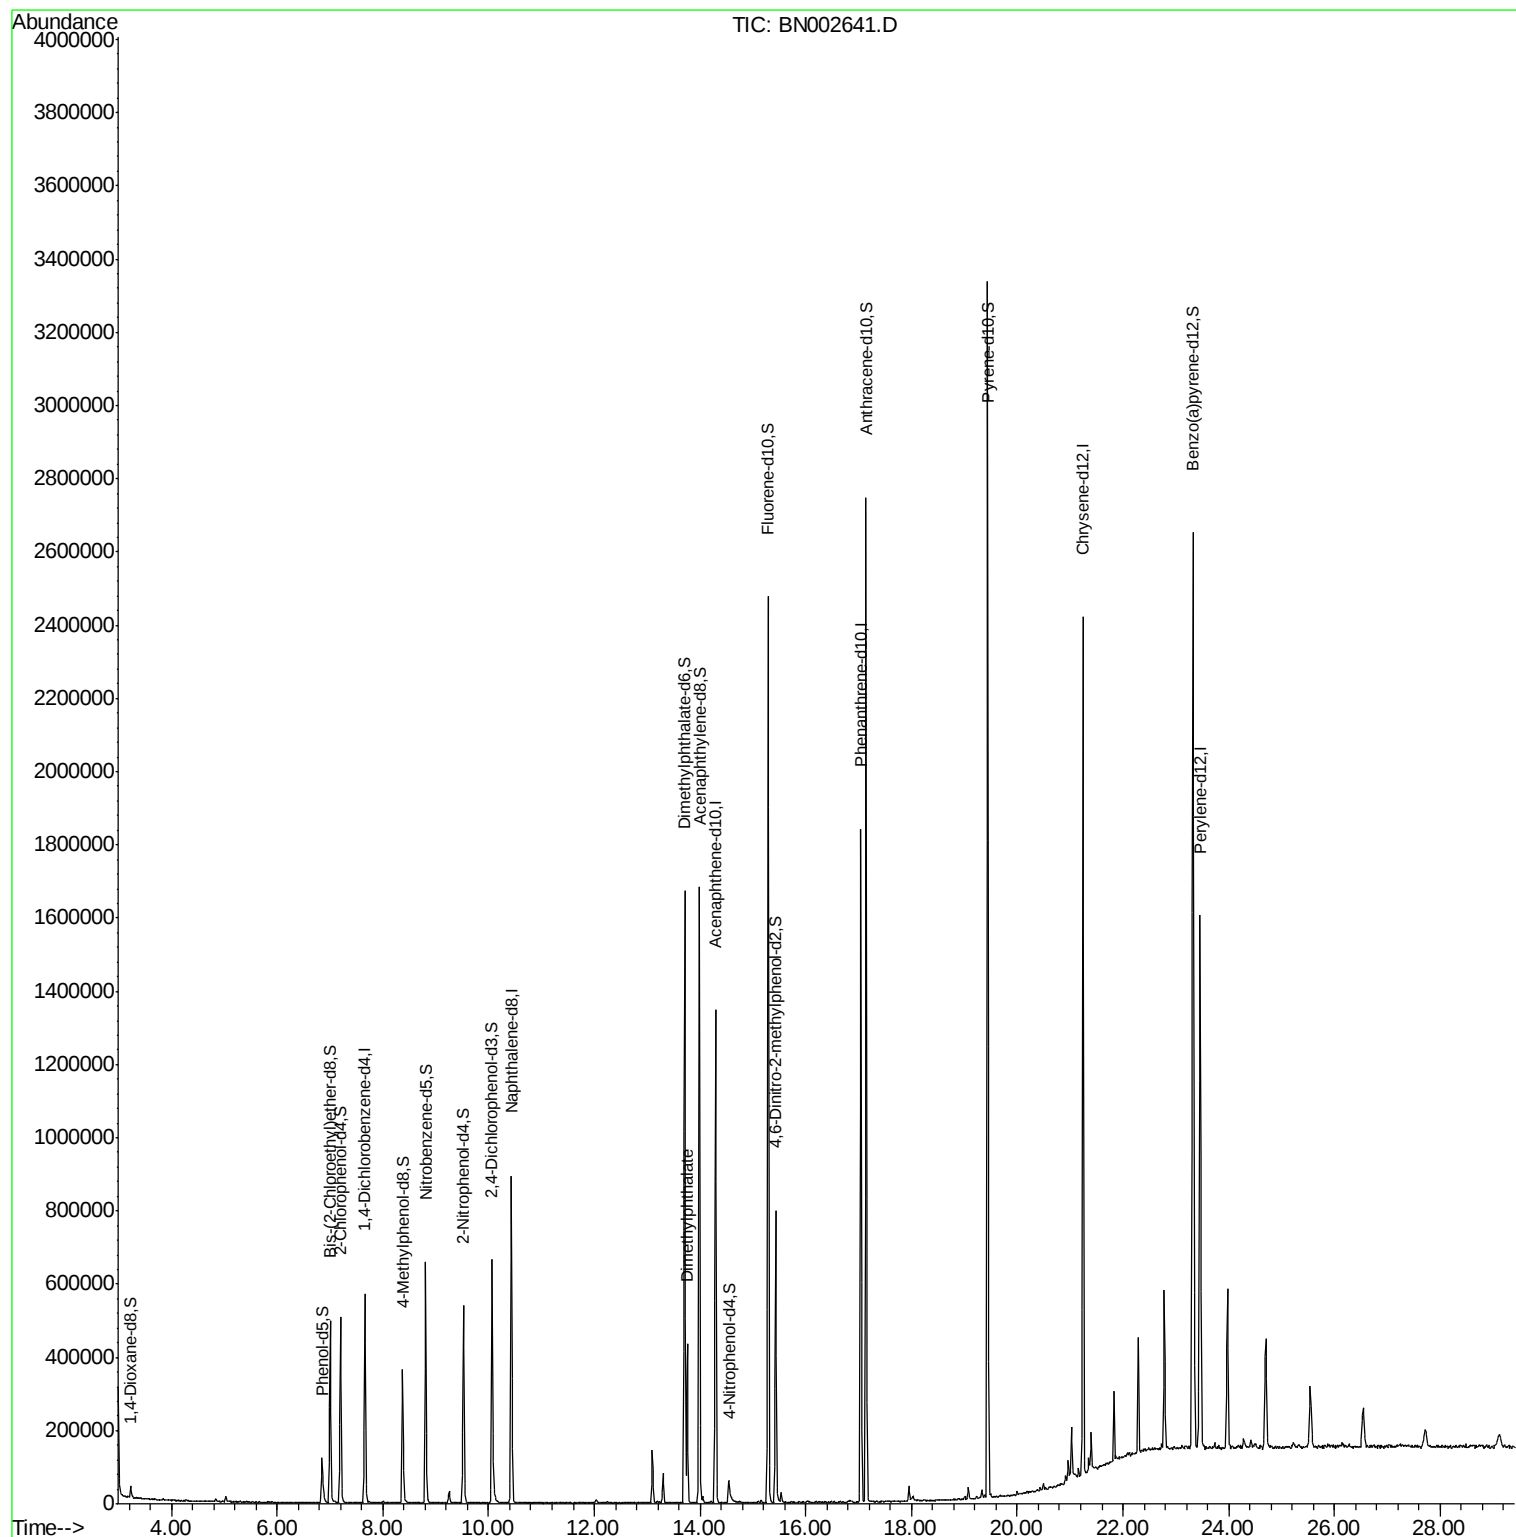

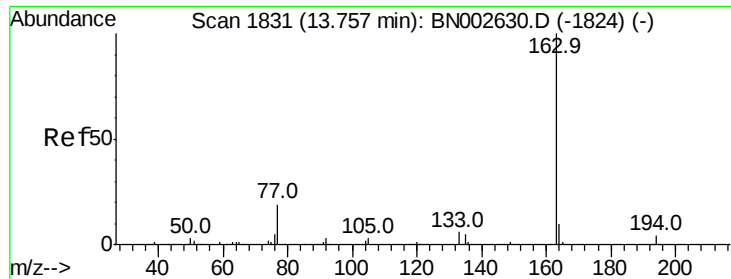

#44
 Dimethylphthalate
 Concen: 7.740 ng/ul
 RT: 13.76 min Scan# 1831
 Delta R.T. -0.00 min
 Lab File: BN002641.D
 Acq: 11 Sep 2018 22:40

Instrument :
 BNA_N
 ClientSampleId :
 C08S0

Tot Ion:	163	Resp:	283897
Ion Ratio	Lower	Upper	
163	100		
194	3.9	3.2	4.8
164	9.0	7.8	11.8

Manual Integrations
 APPROVED

Sohil
 9/12/2018 4:55:07 PM

