

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091124\
 Data File : BN033850.D
 Acq On : 10 Sep 2024 20:39
 Operator : JU/RC
 Sample : SSTD16085
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD160222

Quant Time: Sep 11 01:36:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 11 01:28:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.499	152	205438	20.000	ng/u1	0.00
20) Naphthalene-d8	10.263	136	915976	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.145	164	615445	20.000	ng/u1	0.00
64) Phenanthrene-d10	16.904	188	1277823	20.000	ng/u1	0.00
79) Chrysene-d12	21.145	240	1235380	20.000	ng/u1	0.02
88) Perylene-d12	23.927	264	1534346	20.000	ng/u1	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.111	96	319239	63.398	ng/uL	0.00
4) Pyridine-d5	3.499	84	2387781	156.274	ng/u1	0.00
7) Phenol-d5	6.710	99	2978351	158.061	ng/u1	0.02
9) Bis-(2-Chloroethyl)eth...	6.863	67	1744931	144.420	ng/u1	0.01
11) 2-Chlorophenol-d4	7.052	132	2424415	170.672	ng/u1	0.01
15) 4-Methylphenol-d8	8.234	113	2458638	157.791	ng/u1	0.02
21) Nitrobenzene-d5	8.657	128	1226767	175.972	ng/u1	0.02
24) 2-Nitrophenol-d4	9.369	143	1369243	223.057	ng/u1	0.02
28) 2,4-Dichlorophenol-d3	9.904	165	2365913	173.122	ng/u1	0.02
31) 4-Chloroaniline-d4	10.416	131	3322239	145.817	ng/u1	0.02
46) Dimethylphthalate-d6	13.581	166	6841652	146.074	ng/u1	0.02
49) Acenaphthylene-d8	13.840	160	7830257	149.320	ng/u1	0.01
54) 4-Nitrophenol-d4	14.404	143	1497963	165.513	ng/u1	0.04
60) Fluorene-d10	15.157	176	5766675	143.559	ng/u1	0.01
65) 4,6-Dinitro-2-methylph...	15.298	200	1403546	233.216	ng/u1	0.03
73) Anthracene-d10	17.010	188	9037571	149.174	ng/u1	0.02
81) Pyrene-d10	19.310	212	10288064	150.811	ng/u1	0.01
92) Benzo(a)pyrene-d12	23.757	264	12583487	157.729	ng/u1	0.04
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.146	88	336620	63.711	ng/uL	95
5) Pyridine	3.517	79	2420098	154.070	ng/u1	94
6) Benzaldehyde	6.658	77	1067919	109.071	ng/u1	97
8) Phenol	6.740	94	3075575	155.327	ng/u1	99
10) Bis(2-Chloroethyl)ether	6.958	93	2281856	144.724	ng/u1	98
12) 2-Chlorophenol	7.081	128	2440398	164.674	ng/u1	99
13) 2-Methylphenol	7.957	108	2295012	153.206	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.028	45	3218434	125.745	ng/u1	97
16) Acetophenone	8.334	105	3683470	145.564	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.352	70	1845102	142.686	ng/u1	96
18) 4-Methylphenol	8.310	108	2536634	151.277	ng/u1	98
19) Hexachloroethane	8.563	117	1004894	162.273	ng/u1	94
22) Nitrobenzene	8.699	77	2875395	164.033	ng/u1	98
23) Isophorone	9.246	82	5368528	150.920	ng/u1	98
25) 2-Nitrophenol	9.399	139	1438319	200.783	ng/u1	97
26) 2,4-Dimethylphenol	9.475	107	2706234	159.600	ng/u1	97
27) Bis(2-Chloroethoxy)met...	9.710	93	3155549	143.240	ng/u1	97
29) 2,4-Dichlorophenol	9.934	162	2345964	165.976	ng/u1	98
30) Naphthalene	10.316	128	7539469	147.628	ng/u1	99
32) 4-Chloroaniline	10.446	127	3262858	146.435	ng/u1	99
33) Hexachlorobutadiene	10.604	225	1466901	166.032	ng/u1	97
34) Caprolactam	11.287	113	465399	82.448	ng/u1	96
35) 4-Chloro-3-methylphenol	11.598	107	2680575	164.857	ng/u1	96
36) 2-Methylnaphthalene	11.940	142	5239062	145.757	ng/u1	98


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091124\
 Data File : BN033850.D
 Acq On : 10 Sep 2024 20:39
 Operator : JU/RC
 Sample : SSTD16085
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD160222

Quant Time: Sep 11 01:36:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 11 01:28:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.163	142	5283528	145.434	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.322	216	2754828	156.333	ng/ul	98
40) Hexachlorocyclopentadiene	12.298	237	1652102	169.188	ng/ul	98
41) 2,4,6-Trichlorophenol	12.569	196	1950318	180.382	ng/ul	98
42) 2,4,5-Trichlorophenol	12.645	196	2126926	174.677	ng/ul	99
43) 1,1'-Biphenyl	12.981	154	6758623	145.608	ng/ul	100
44) 2-Chloronaphthalene	13.016	162	5422455	150.697	ng/ul	97
45) 2-Nitroaniline	13.240	65	1915374	185.275	ng/ul	96
47) Dimethylphthalate	13.634	163	6897131	146.693	ng/ul	99
48) 2,6-Dinitrotoluene	13.751	165	1558383	182.371	ng/ul	97
50) Acenaphthylene	13.875	152	8401812	146.716	ng/ul	99
51) 3-Nitroaniline	14.081	138	1518364	156.914	ng/ul	99
52) Acenaphthene	14.222	153	5945620	146.932	ng/ul	98
53) 2,4-Dinitrophenol	14.287	184	1099422	260.452	ng/ul	87
55) 4-Nitrophenol	14.422	109	1210323	170.756	ng/ul	95
56) Dibenzofuran	14.557	168	7975560	141.163	ng/ul	98
57) 2,4-Dinitrotoluene	14.545	165	2284928	177.927	ng/ul	91
58) 2,3,4,6-Tetrachlorophenol	14.792	232	1770203	178.894	ng/ul	99
59) Diethylphthalate	15.016	149	7304415	148.914	ng/ul	98
61) Fluorene	15.216	166	6297515	135.430	ng/ul	95
62) 4-Chlorophenyl-phenyle...	15.210	204	3037764	136.155	ng/ul	99
63) 4-Nitroaniline	15.269	138	1368217	137.378	ng/ul	98
66) 4,6-Dinitro-2-methylph...	15.316	198	1501375	220.745	ng/ul#	98
67) N-Nitrosodiphenylamine	15.434	169	5705399	148.473	ng/ul	99
68) 4-Bromophenyl-phenylether	16.104	248	2108276	161.643	ng/ul	93
69) Hexachlorobenzene	16.216	284	2430404	162.753	ng/ul	96
70) Atrazine	16.410	200	1973506	138.038	ng/ul	99
71) Pentachlorophenol	16.563	266	1716372	182.704	ng/ul	97
72) Phenanthrene	16.951	178	10360527	145.002	ng/ul	98
74) Anthracene	17.045	178	10399164	142.862	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	12.934	216	2821510	163.775	ng/ul	98
76) Pentachlorobenzene	14.475	250	2889106	162.951	ng/ul	98
77) Carbazole	17.316	167	9784361	145.798	ng/ul	98
78) Di-n-butylphthalate	17.898	149	11863116	141.540	ng/ul	97
80) Fluoranthene	18.975	202	11747587	147.277	ng/ul	100
82) Pyrene	19.345	202	12295223	142.219	ng/ul	100
83) Butylbenzylphthalate	20.269	149	5926809	171.089	ng/ul	98
84) 3,3'-Dichlorobenzidine	21.063	252	3977158	141.220	ng/ul	99
85) Benzo(a)anthracene	21.127	228	13132307	147.728	ng/ul	95
86) Bis(2-ethylhexyl)phtha...	21.080	149	8264084	147.042	ng/ul#	96
87) Chrysene	21.192	228	12088555	144.594	ng/ul	96
89) Di-n-octyl phthalate	22.145	149	14852552	150.296	ng/ul	100
90) Benzo(b)fluoranthene	23.074	252	14365195	150.597	ng/ul	99
91) Benzo(k)fluoranthene	23.139	252	14132986	149.240	ng/ul	98
93) Benzo(a)pyrene	23.833	252	13843715	153.143	ng/ul	94
94) Indeno(1,2,3-cd)pyrene	27.068	276	17698718	157.762	ng/ul	97
95) Dibenzo(a,h)anthracene	27.151	278	14605330	158.975	ng/ul	98
96) Benzo(g,h,i)perylene	28.074	276	13649557	158.322	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2

1,4-Dioxane

Concen: 63.711 ng/uL

RT: 3.146 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39

Instrument :

BNA_N

ClientSampleId :

SSTD160222





Tgt Ion: 88 Resp: 336620

Ion Ratio Lower Upper

88 100

43 29.6 24.7 37.1

58 75.5 64.6 96.8

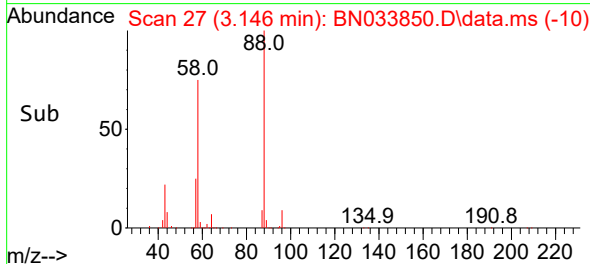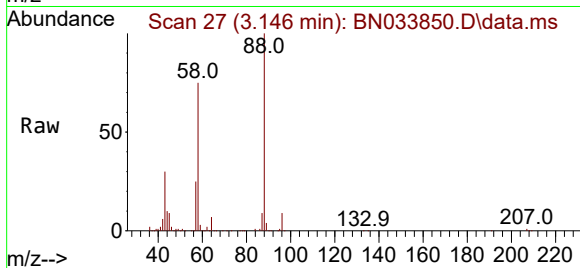

#5

Pyridine

Concen: 154.070 ng/uL

RT: 3.517 min Scan# 90

Delta R.T. -0.006 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39




Tgt Ion: 79 Resp: 2420098


Ion Ratio Lower Upper

79 100

52 88.2 65.2 97.8

51 38.1 29.7 44.5


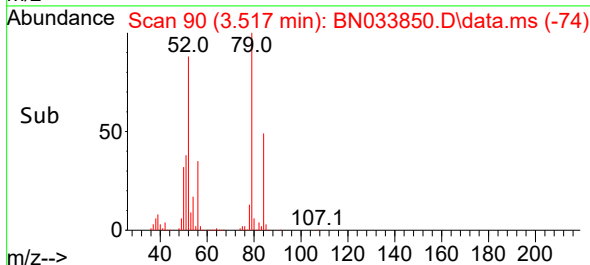

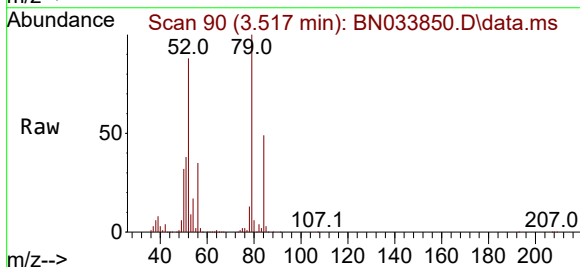




#6
Benzaldehyde
Concen: 109.071 ng/ul
RT: 6.658 min Scan# 61
Delta R.T. 0.000 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39




Instrument :
BNA_N
ClientSampleId :
SSTD160222


Tgt Ion: 77 Resp: 1067919
Ion Ratio Lower Upper
77 100
105 94.6 76.4 114.6
106 91.7 69.8 104.6



#8
Phenol
Concen: 155.327 ng/ul
RT: 6.740 min Scan# 638
Delta R.T. 0.024 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39

Tgt Ion: 94 Resp: 3075575
Ion Ratio Lower Upper
94 100
65 29.7 24.3 36.5
66 39.4 31.8 47.6









#10
Bis(2-Chloroethyl)ether
Concen: 144.724 ng/ul
RT: 6.958 min Scan# 61
Delta R.T. 0.018 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39




Instrument :
BNA_N
ClientSampleId :
SSTD160222


Tgt Ion: 93 Resp: 2281856
Ion Ratio Lower Upper
93 100
63 76.5 63.6 95.4
95 32.1 25.7 38.5

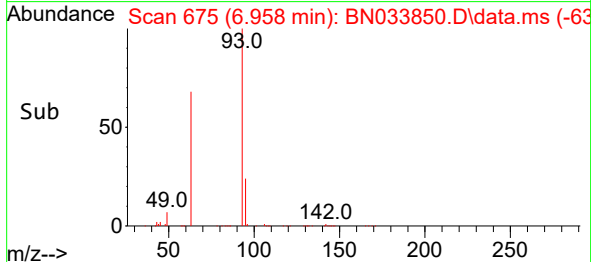

#12
2-Chlorophenol
Concen: 164.674 ng/ul
RT: 7.081 min Scan# 696
Delta R.T. 0.012 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39

Tgt Ion:128 Resp: 2440398
Ion Ratio Lower Upper
128 100
64 48.5 39.1 58.7
130 32.7 25.8 38.6

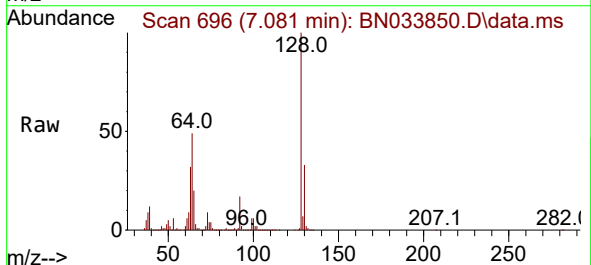



#13

2-Methylphenol

Concen: 153.206 ng/ul

RT: 7.957 min Scan# 84

Delta R.T. 0.012 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39

Instrument :

BNA_N

ClientSampleId :





SSTD160222

Tgt Ion:108 Resp: 2295012

Ion Ratio Lower Upper

108 100

107 90.5 71.9 107.9

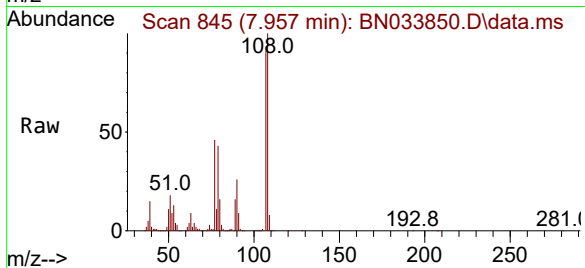

#14

2,2'-oxybis(1-Chloropropane)

Concen: 125.745 ng/ul

RT: 8.028 min Scan# 857

Delta R.T. 0.006 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39




Tgt Ion: 45 Resp: 3218434


Ion Ratio Lower Upper

45 100

77 15.0 11.0 16.6

79 10.8 7.8 11.8


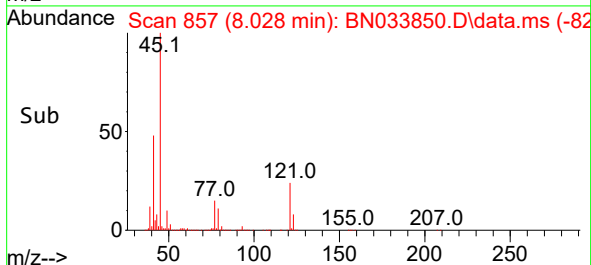
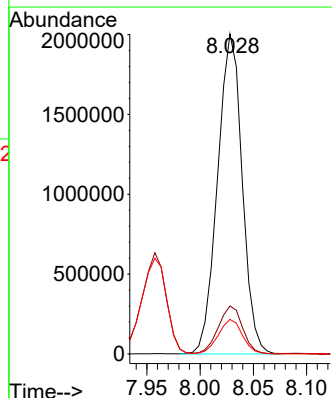
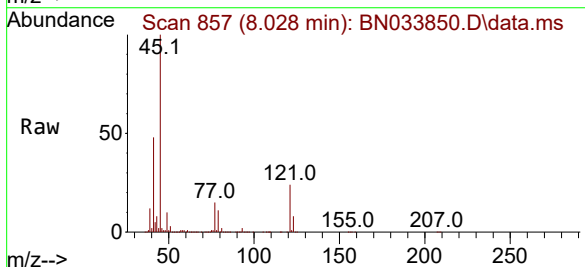




#16
Acetophenone
Concen: 145.564 ng/ul
RT: 8.334 min Scan# 906
Delta R.T. 0.018 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39




Instrument :
BNA_N
ClientSampleId :
SSTD160222


Tgt Ion:105 Resp: 3683470
Ion Ratio Lower Upper
105 100
77 76.8 61.1 91.7
51 26.9 22.6 33.8

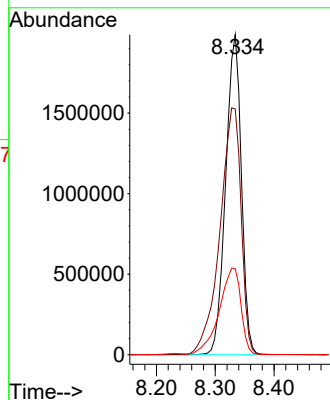

#17
N-Nitroso-di-n-propylamine
Concen: 142.686 ng/ul
RT: 8.352 min Scan# 912
Delta R.T. 0.047 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39

Tgt Ion: 70 Resp: 1845102
Ion Ratio Lower Upper
70 100
42 56.6 47.9 71.9
101 10.2 7.5 11.3
130 21.8 16.2 24.2

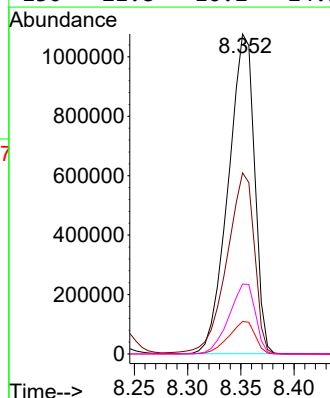



#18

4-Methylphenol

Concen: 151.277 ng/ul

RT: 8.310 min Scan# 905

Delta R.T. 0.035 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39

Instrument :

BNA_N

ClientSampleId :





SSTD160222

Tgt Ion:108 Resp: 2536634

Ion Ratio Lower Upper

108 100

107 109.2 89.4 134.2



#19

Hexachloroethane

Concen: 162.273 ng/ul

RT: 8.563 min Scan# 948

Delta R.T. 0.006 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39




Tgt Ion:117 Resp: 1004894


Ion Ratio Lower Upper

117 100

201 95.9 73.9 110.9

199 62.1 44.0 66.0









#22
Nitrobenzene
Concen: 164.033 ng/ul
RT: 8.699 min Scan# 91
Delta R.T. 0.018 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39




Instrument :
BNA_N
ClientSampleId :
SSTD160222


Tgt Ion: 77 Resp: 2875395
Ion Ratio Lower Upper
77 100
123 44.8 34.5 51.7
65 13.7 11.0 16.6

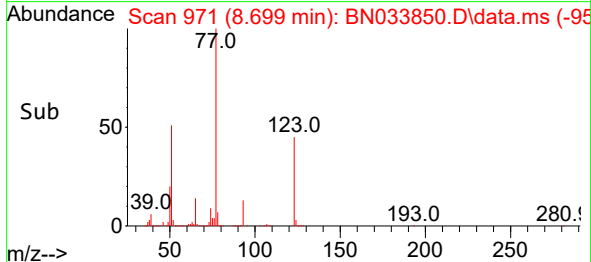

#23
Isophorone
Concen: 150.920 ng/ul
RT: 9.246 min Scan# 1064
Delta R.T. 0.035 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39

Tgt Ion: 82 Resp: 5368528
Ion Ratio Lower Upper
82 100
95 7.5 6.1 9.1
138 18.2 13.4 20.0

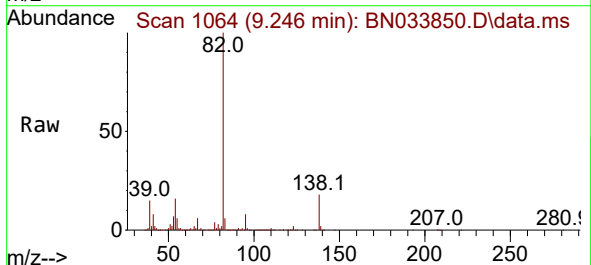



#25

2-Nitrophenol

Concen: 200.783 ng/ul

RT: 9.399 min Scan# 1103

Delta R.T. 0.012 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39

Instrument :

BNA_N

ClientSampleId :

SSTD160222





Tgt Ion:139 Resp: 1438319

Ion Ratio Lower Upper

139 100

65 55.6 42.0 63.0

109 33.3 26.5 39.7

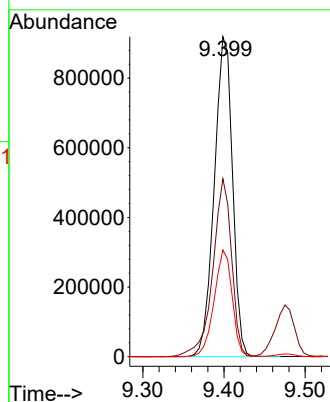

#26

2,4-Dimethylphenol

Concen: 159.600 ng/ul

RT: 9.475 min Scan# 1103

Delta R.T. 0.018 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39




Tgt Ion:107 Resp: 2706234


Ion Ratio Lower Upper

107 100

121 48.5 38.4 57.6

122 81.7 62.9 94.3

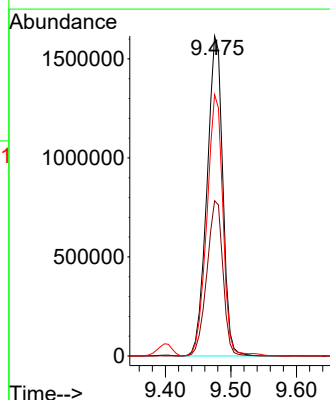



#27

Bis(2-Chloroethoxy)methane

Concen: 143.240 ng/ul

RT: 9.710 min Scan# 1143

Delta R.T. 0.018 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39

Instrument :

BNA_N

ClientSampleId :

SSTD160222





Tgt Ion: 93 Resp: 3155549

Ion Ratio Lower Upper

93 100

95 32.7 24.9 37.3

123 11.6 8.8 13.2

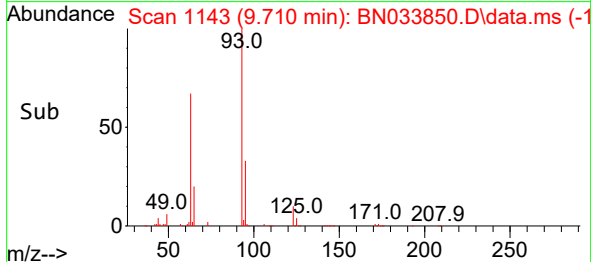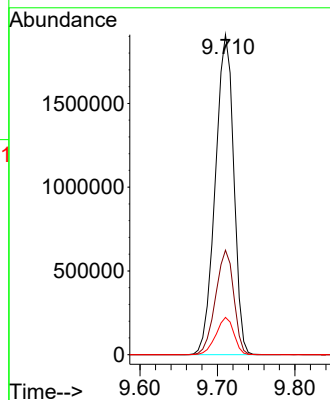

#29

2,4-Dichlorophenol

Concen: 165.976 ng/ul

RT: 9.934 min Scan# 1181

Delta R.T. 0.018 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39




Tgt Ion:162 Resp: 2345964


Ion Ratio Lower Upper

162 100

164 64.0 53.0 79.6

98 37.8 30.6 46.0

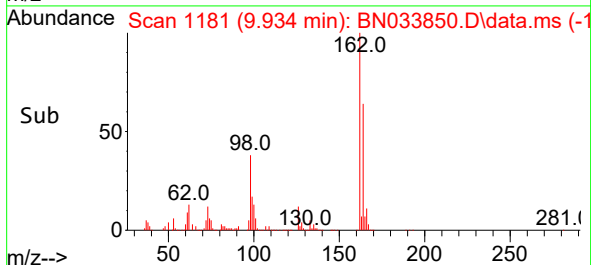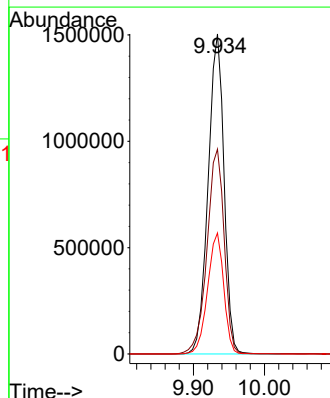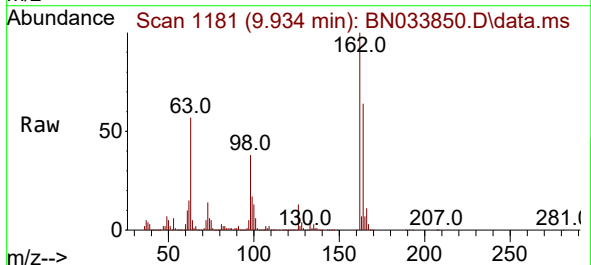



#30

Naphthalene

Concen: 147.628 ng/ul

RT: 10.316 min Scan# 1245

Delta R.T. 0.006 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39

Instrument :

BNA_N

ClientSampleId :

SSTD160222





Tgt Ion:128 Resp: 7539469

Ion Ratio Lower Upper

128 100

129 11.3 8.7 13.1

127 13.5 10.6 16.0

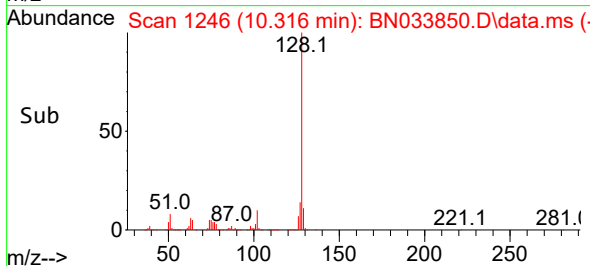

#32

4-Chloroaniline

Concen: 146.435 ng/ul

RT: 10.446 min Scan# 1268

Delta R.T. 0.024 min

Lab File: BN033850.D




Acq: 10 Sep 2024 20:39


Tgt Ion:127 Resp: 3262858

Ion Ratio Lower Upper

127 100

129 32.2 26.2 39.2


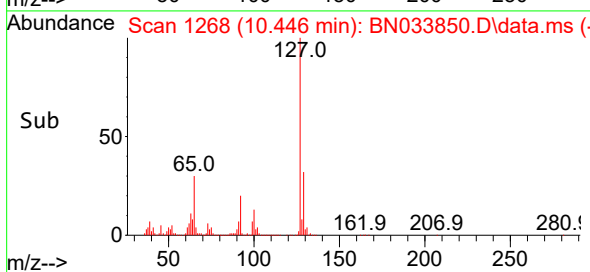

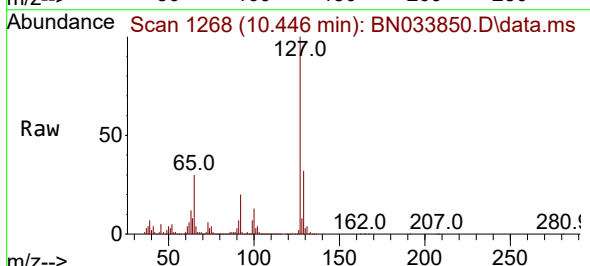




#33
Hexachlorobutadiene
Concen: 166.032 ng/ul
RT: 10.604 min Scan# 1410
Delta R.T. 0.000 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39




Instrument :
BNA_N
ClientSampleId :
SSTD160222


Tgt Ion:225 Resp: 1466901
Ion Ratio Lower Upper
225 100
223 62.9 52.2 78.2
227 65.4 50.1 75.1



#34
Caprolactam
Concen: 82.448 ng/ul
RT: 11.287 min Scan# 1411
Delta R.T. 0.088 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39

Tgt Ion:113 Resp: 465399
Ion Ratio Lower Upper
113 100
55 163.1 137.0 205.6
56 123.4 99.7 149.5









#35
4-Chloro-3-methylphenol
Concen: 164.857 ng/ul
RT: 11.598 min Scan# 1464
Delta R.T. 0.035 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39




Instrument :
BNA_N
ClientSampleId :
SSTD160222


Tgt Ion:107 Resp: 2680575
Ion Ratio Lower Upper
107 100
144 25.8 19.1 28.7
142 80.6 61.4 92.0

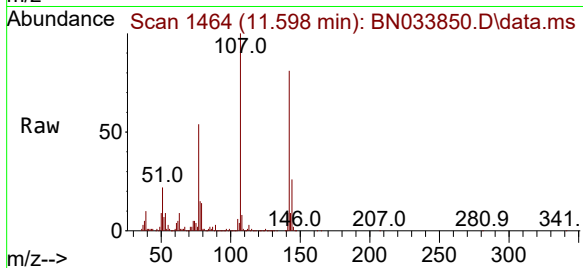

#36
2-Methylnaphthalene
Concen: 145.757 ng/ul
RT: 11.940 min Scan# 1522
Delta R.T. 0.012 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39

Tgt Ion:142 Resp: 5239062
Ion Ratio Lower Upper
142 100
141 88.7 72.2 108.2




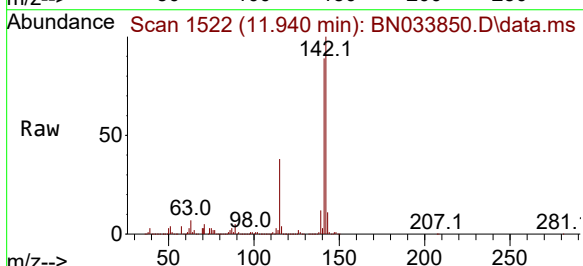




#37
1-Methylnaphthalene
Concen: 145.434 ng/ul
RT: 12.163 min Scan# 1560
Delta R.T. 0.006 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39




Instrument :
BNA_N
ClientSampleId :
SSTD160222


Tgt Ion:142 Resp: 5283528
Ion Ratio Lower Upper
142 100
141 91.7 72.5 108.7
116 4.1 3.2 4.8



#39
1,2,4,5-Tetrachlorobenzene
Concen: 156.333 ng/ul
RT: 12.322 min Scan# 1587
Delta R.T. 0.012 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39

Tgt Ion:216 Resp: 2754828
Ion Ratio Lower Upper
216 100
214 80.6 63.0 94.6
179 22.0 18.2 27.2
108 17.2 15.0 22.4









#40
Hexachlorocyclopentadiene
Concen: 169.188 ng/ul
RT: 12.298 min Scan# 1582
Delta R.T. 0.006 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39




Instrument :
BNA_N
ClientSampleId :
SSTD160222


Tgt Ion:237 Resp: 1652102
Ion Ratio Lower Upper
237 100
235 64.9 50.7 76.1
272 12.9 10.1 15.1

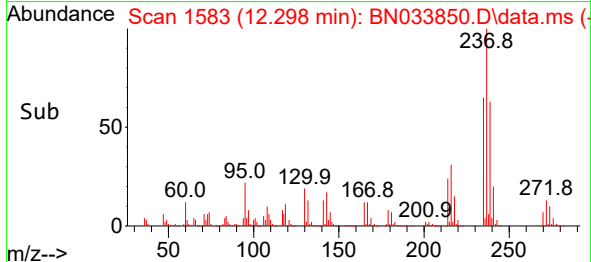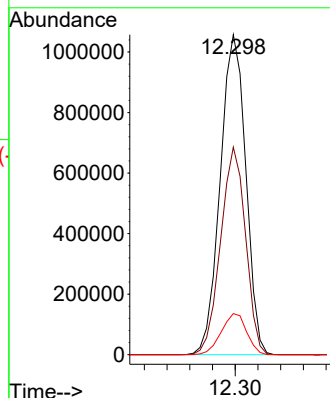

#41
2,4,6-Trichlorophenol
Concen: 180.382 ng/ul
RT: 12.569 min Scan# 1629
Delta R.T. 0.012 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39

Tgt Ion:196 Resp: 1950318
Ion Ratio Lower Upper
196 100
198 95.5 75.0 112.4
200 29.6 24.7 37.1

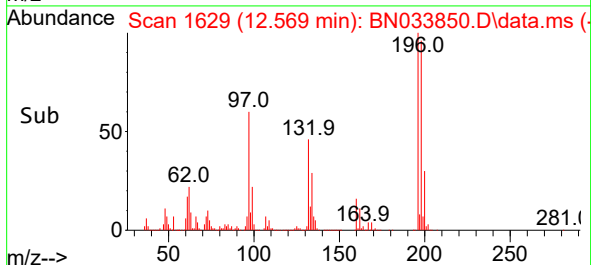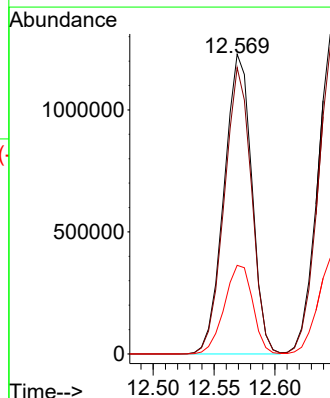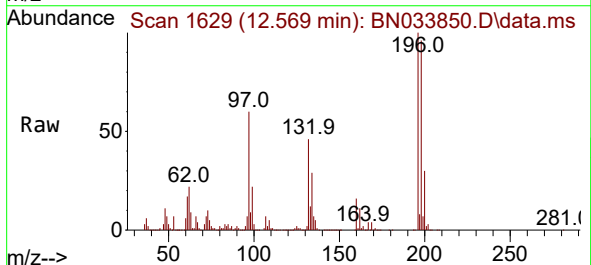



#42

2,4,5-Trichlorophenol

Concen: 174.677 ng/ul

RT: 12.645 min Scan# 1

Delta R.T. 0.018 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39

Instrument :

BNA_N

ClientSampleId :

SSTD160222





Tgt Ion:196 Resp: 2126926

Ion Ratio Lower Upper

196 100

198 95.9 77.1 115.7

200 30.0 25.2 37.8



#43

1,1'-Biphenyl

Concen: 145.608 ng/ul

RT: 12.981 min Scan# 1699

Delta R.T. 0.012 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39




Tgt Ion:154 Resp: 6758623


Ion Ratio Lower Upper

154 100

153 41.4 33.3 49.9

76 12.6 10.2 15.4





#44

2-Chloronaphthalene

Concen: 150.697 ng/ul

RT: 13.016 min Scan# 1705

Delta R.T. 0.012 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39

Instrument :

BNA_N

ClientSampleId :

SSTD160222





Tgt Ion:162 Resp: 5422455

Ion Ratio Lower Upper

162 100

164 33.1 25.1 37.7

127 42.4 32.6 48.8

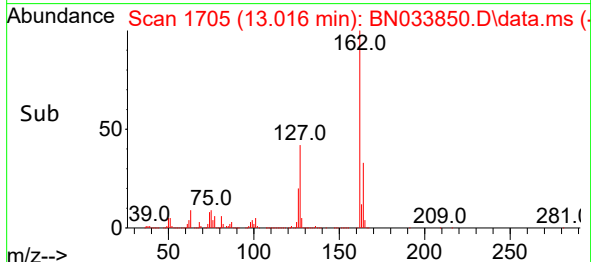

#45

2-Nitroaniline

Concen: 185.275 ng/ul

RT: 13.240 min Scan# 1743

Delta R.T. 0.024 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39




Tgt Ion: 65 Resp: 1915374


Ion Ratio Lower Upper

65 100

92 67.9 53.2 79.8

138 106.2 80.9 121.3


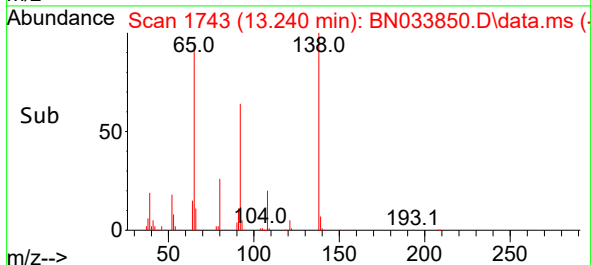




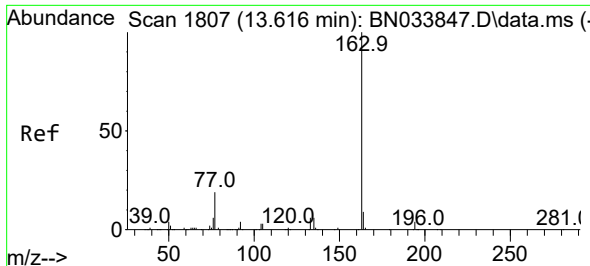

#47
Dimethylphthalate
Concen: 146.693 ng/ul
RT: 13.634 min Scan# 1810
Delta R.T. 0.018 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39




Instrument :
BNA_N
ClientSampleId :
SSTD160222


Tgt Ion:163 Resp: 6897131
Ion Ratio Lower Upper
163 100
194 4.1 3.0 4.6
164 10.1 7.7 11.5

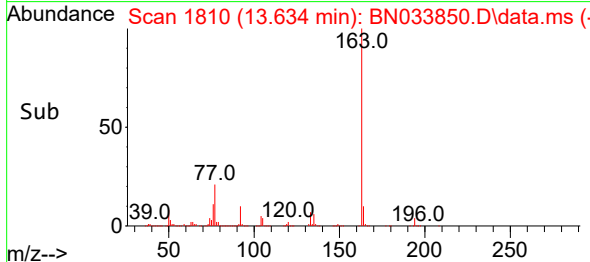

#48
2,6-Dinitrotoluene
Concen: 182.371 ng/ul
RT: 13.751 min Scan# 1830
Delta R.T. 0.024 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39

Tgt Ion:165 Resp: 1558383
Ion Ratio Lower Upper
165 100
89 59.0 48.6 72.8
121 21.3 19.0 28.6


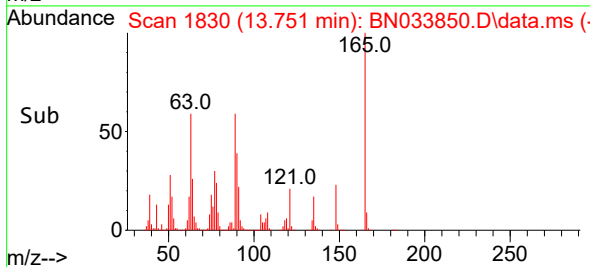

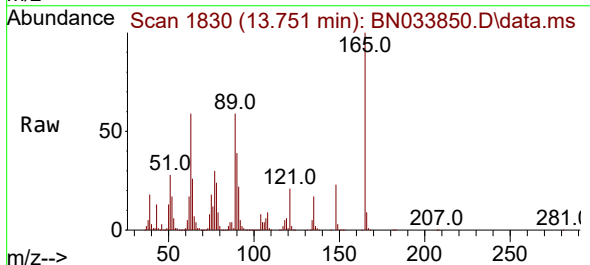




#50
Acenaphthylene
Concen: 146.716 ng/ul
RT: 13.875 min Scan# 1851
Delta R.T. 0.018 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39




Instrument :
BNA_N
ClientSampleId :
SSTD160222


Tgt Ion:152 Resp: 8401812
Ion Ratio Lower Upper
152 100
151 20.9 16.2 24.4
153 13.4 10.6 16.0

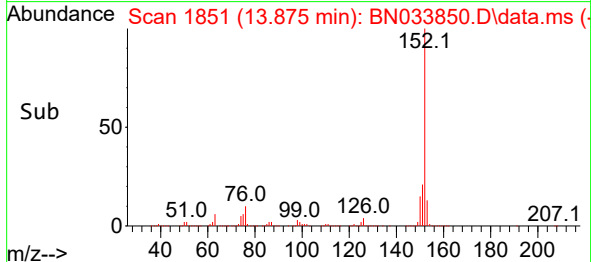

#51
3-Nitroaniline
Concen: 156.914 ng/ul
RT: 14.081 min Scan# 1886
Delta R.T. 0.029 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39

Tgt Ion:138 Resp: 1518364
Ion Ratio Lower Upper
138 100
108 10.9 9.0 13.4
92 119.8 94.6 141.8

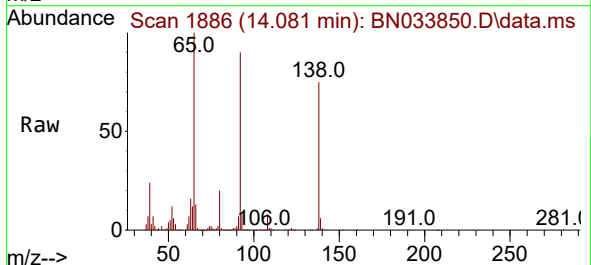

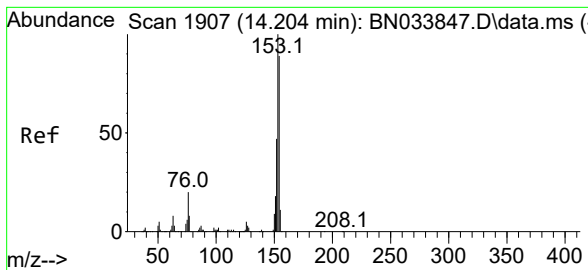

#52

Acenaphthene

Concen: 146.932 ng/ul

RT: 14.222 min Scan# 1910

Delta R.T. 0.018 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39

Instrument :

BNA_N

ClientSampleId :

SSTD160222





Tgt Ion:153 Resp: 5945620

Ion Ratio Lower Upper

153 100

152 46.4 37.8 56.8

154 86.8 71.2 106.8

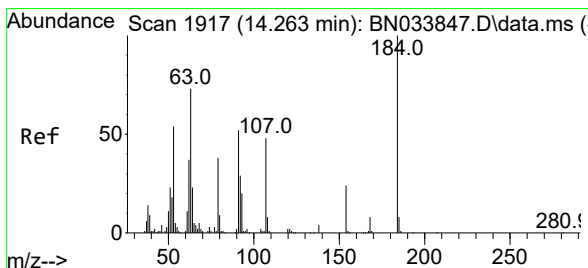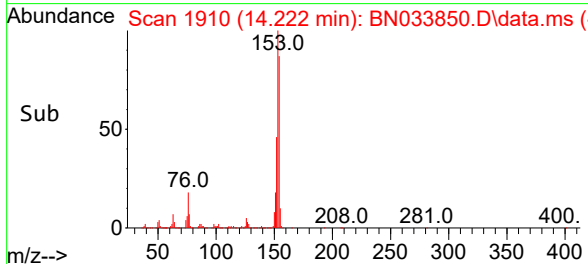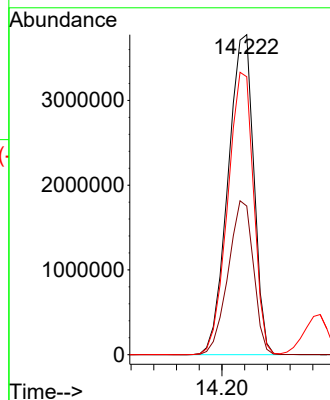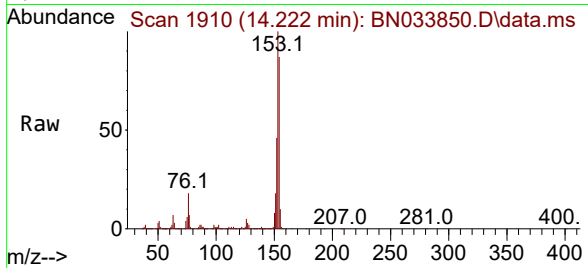

#53

2,4-Dinitrophenol

Concen: 260.452 ng/ul

RT: 14.287 min Scan# 1921

Delta R.T. 0.024 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39




Tgt Ion:184 Resp: 1099422


Ion Ratio Lower Upper

184 100

63 64.6 61.1 91.7

154 62.6 58.5 87.7


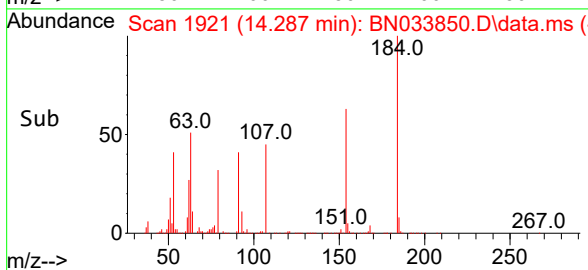
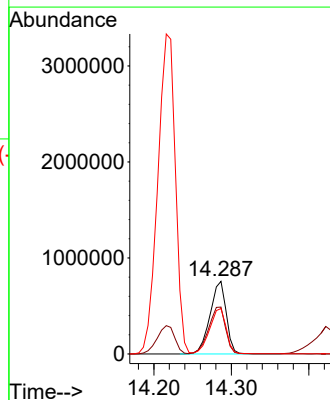
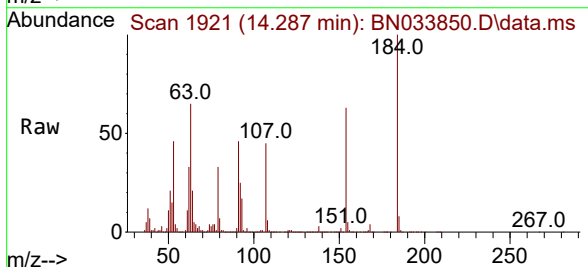




#55
4-Nitrophenol
Concen: 170.756 ng/ul
RT: 14.422 min Scan# 1944
Delta R.T. 0.041 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39




Instrument :
BNA_N
ClientSampleId :
SSTD160222


Tgt Ion:109 Resp: 1210323
Ion Ratio Lower Upper
109 100
139 126.7 102.8 154.2
65 131.5 97.7 146.5



#56
Dibenzofuran
Concen: 141.163 ng/ul
RT: 14.557 min Scan# 1967
Delta R.T. 0.012 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39

Tgt Ion:168 Resp: 7975560
Ion Ratio Lower Upper
168 100
139 40.7 31.7 47.5







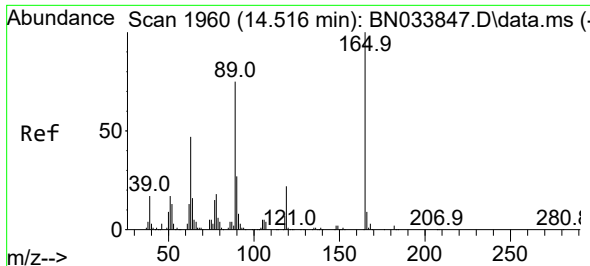

#57
2,4-Dinitrotoluene
Concen: 177.927 ng/ul
RT: 14.545 min Scan# 1965
Delta R.T. 0.029 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39




Instrument :
BNA_N
ClientSampleId :
SSTD160222


Tgt Ion:165 Resp: 2284928
Ion Ratio Lower Upper
165 100
63 53.8 37.8 56.8
182 3.0 2.3 3.5

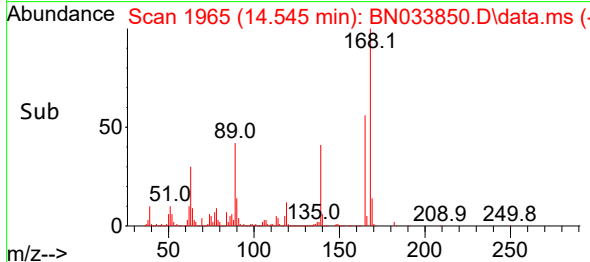

#58
2,3,4,6-Tetrachlorophenol
Concen: 178.894 ng/ul
RT: 14.792 min Scan# 2007
Delta R.T. 0.018 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39

Tgt Ion:232 Resp: 1770203
Ion Ratio Lower Upper
232 100
131 50.9 41.0 61.6
130 2.7 2.2 3.2
166 34.5 27.1 40.7

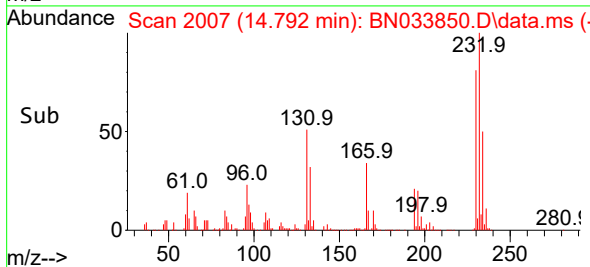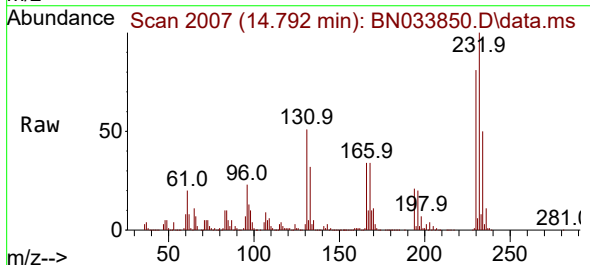



#59

Diethylphthalate

Concen: 148.914 ng/ul

RT: 15.016 min Scan# 2045

Delta R.T. 0.024 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39

Instrument :

BNA_N

ClientSampleId :

SSTD160222





Tgt Ion:149 Resp: 7304415

Ion Ratio Lower Upper

149 100

177 22.0 16.9 25.3

150 13.0 9.9 14.9



#61

Fluorene

Concen: 135.430 ng/ul

RT: 15.216 min Scan# 2079

Delta R.T. 0.018 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39




Tgt Ion:166 Resp: 6297515


Ion Ratio Lower Upper

166 100

165 96.2 81.9 122.9

167 13.5 10.9 16.3







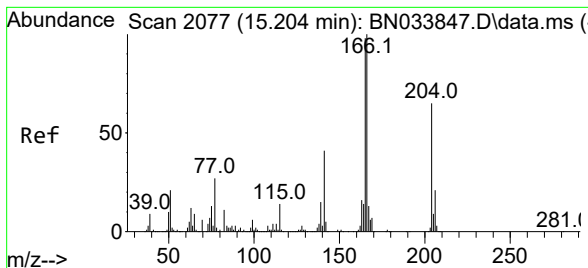

#62
4-Chlorophenyl-phenylether
Concen: 136.155 ng/ul
RT: 15.210 min Scan# 2077
Delta R.T. 0.006 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39




Instrument :
BNA_N
ClientSampleId :
SSTD160222


Tgt Ion:204 Resp: 3037764
Ion Ratio Lower Upper
204 100
206 32.6 26.2 39.4
141 64.3 50.4 75.6

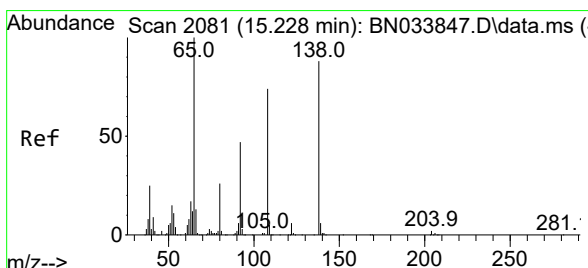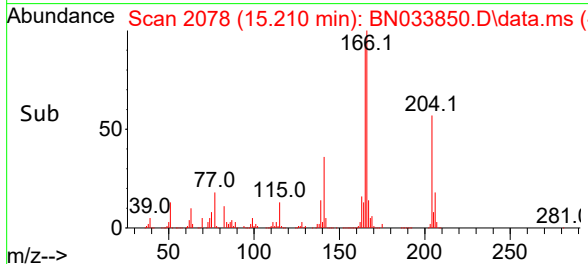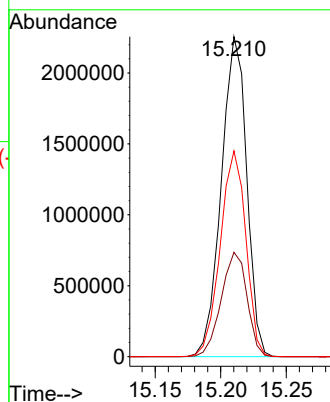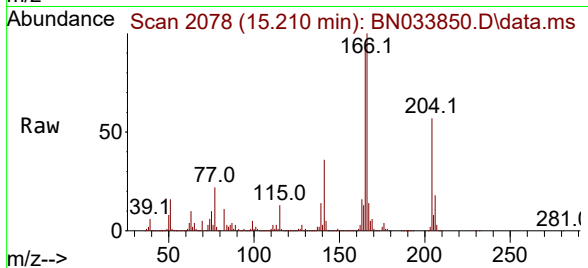

#63
4-Nitroaniline
Concen: 137.378 ng/ul
RT: 15.269 min Scan# 2088
Delta R.T. 0.041 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39

Tgt Ion:138 Resp: 1368217
Ion Ratio Lower Upper
138 100
92 51.3 43.0 64.4
108 82.4 67.0 100.4


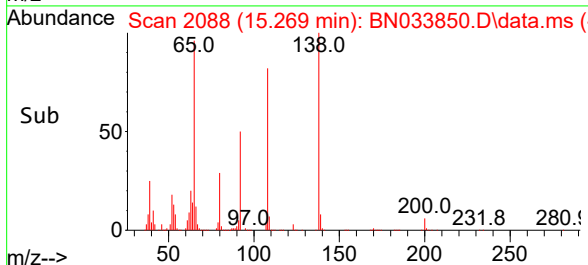
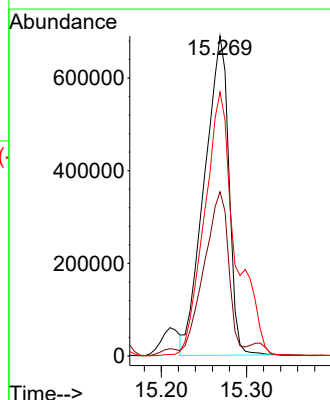
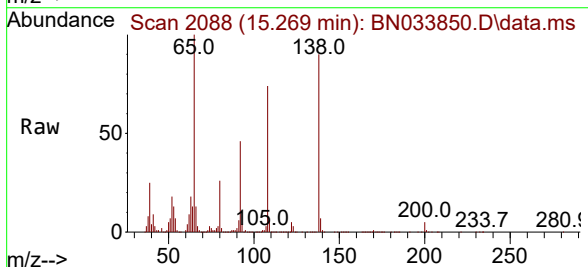


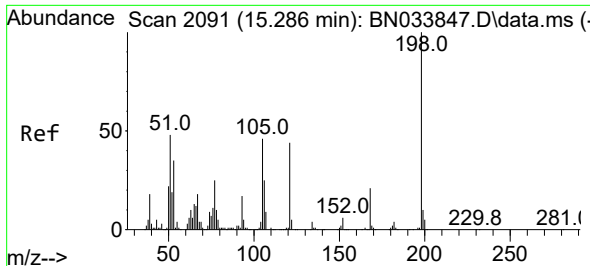

#66
 4,6-Dinitro-2-methylphenol
 Concen: 220.745 ng/ul
 RT: 15.316 min Scan# 2096
 Delta R.T. 0.029 min
 Lab File: BN033850.D
 Acq: 10 Sep 2024 20:39




Instrument :
 BNA_N
 ClientSampleId :
 SSTD160222


Tgt Ion:198 Resp: 1501375
 Ion Ratio Lower Upper
 198 100
 182 3.1 3.2 4.8#
 77 25.5 21.1 31.7

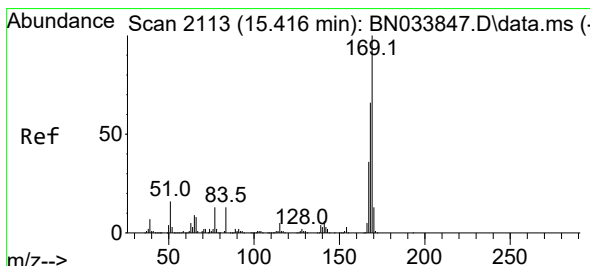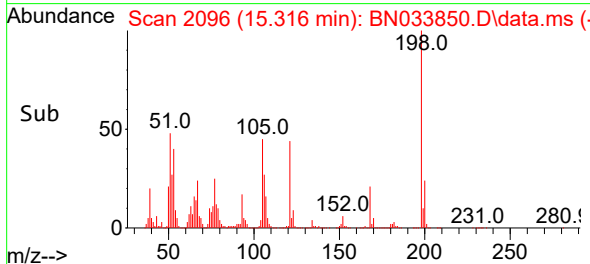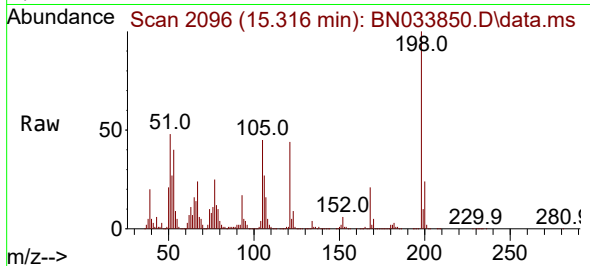

#67
 N-Nitrosodiphenylamine
 Concen: 148.473 ng/ul
 RT: 15.434 min Scan# 2116
 Delta R.T. 0.018 min
 Lab File: BN033850.D
 Acq: 10 Sep 2024 20:39

Tgt Ion:169 Resp: 5705399
 Ion Ratio Lower Upper
 169 100
 168 66.2 52.8 79.2
 167 37.1 28.6 43.0


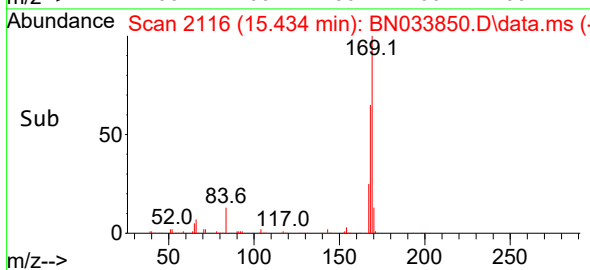

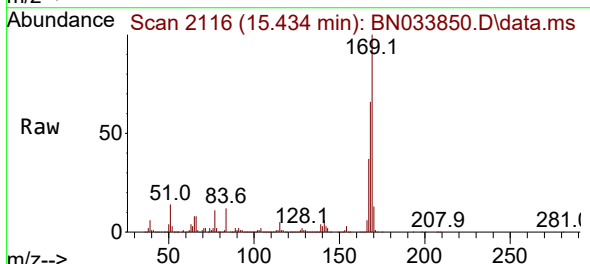




#68
4-Bromophenyl-phenylether
Concen: 161.643 ng/ul
RT: 16.104 min Scan# 21
Delta R.T. 0.006 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39




Instrument :
BNA_N
ClientSampleId :
SSTD160222


Tgt Ion:248 Resp: 2108276
Ion Ratio Lower Upper
248 100
250 92.8 79.8 119.6
141 76.7 67.0 100.4

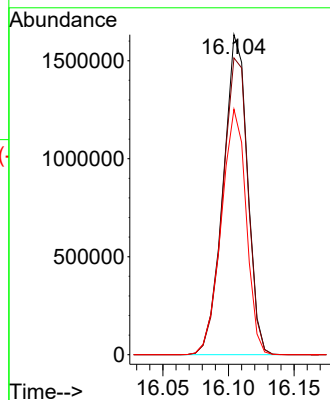

#69
Hexachlorobenzene
Concen: 162.753 ng/ul
RT: 16.216 min Scan# 2249
Delta R.T. 0.012 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39

Tgt Ion:284 Resp: 2430404
Ion Ratio Lower Upper
284 100
142 34.8 31.3 46.9
249 31.2 25.1 37.7

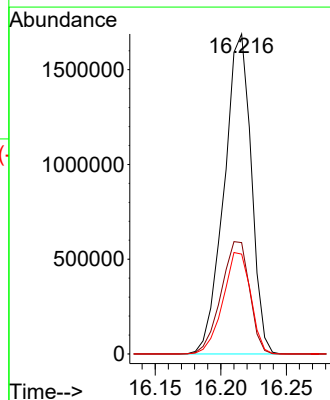

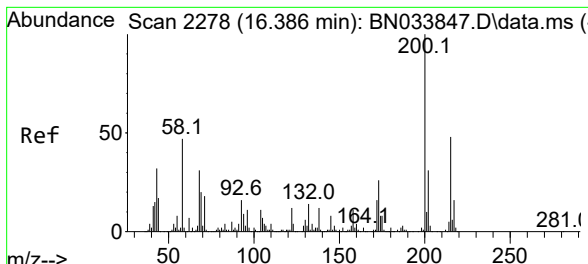

#70

Atrazine

Concen: 138.038 ng/ul

RT: 16.410 min Scan# 21

Delta R.T. 0.024 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39

Instrument :

BNA_N

ClientSampleId :

SSTD160222





Tgt Ion:200 Resp: 1973506

Ion Ratio Lower Upper

200 100

173 26.4 21.3 31.9

215 48.5 38.2 57.4

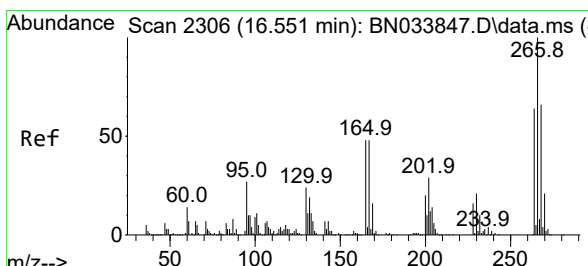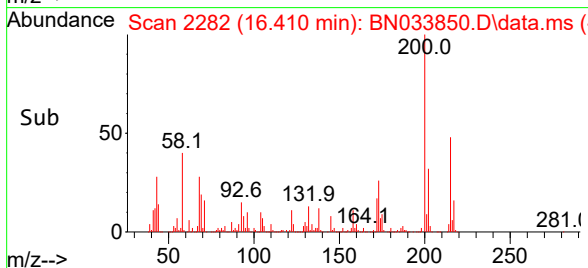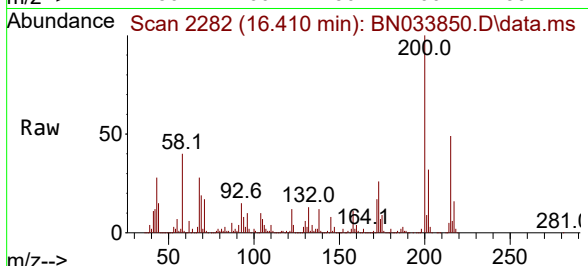

#71

Pentachlorophenol

Concen: 182.704 ng/ul

RT: 16.563 min Scan# 2308

Delta R.T. 0.012 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39




Tgt Ion:266 Resp: 1716372


Ion Ratio Lower Upper

266 100

264 62.0 51.1 76.7

268 68.8 52.8 79.2

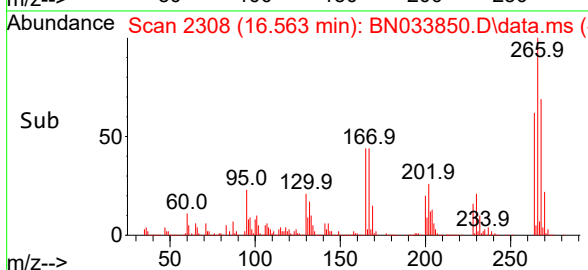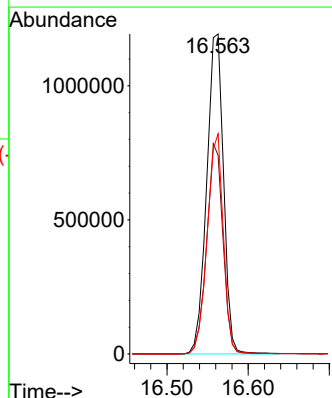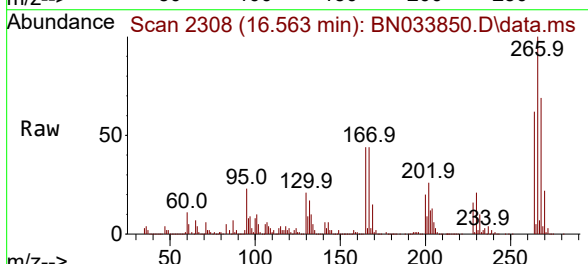

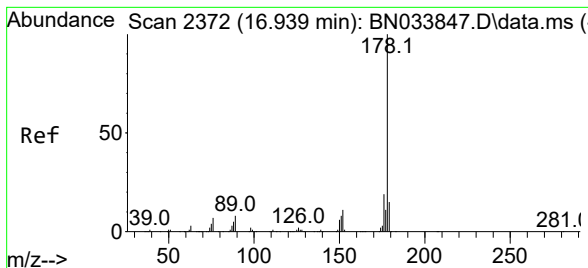

#72

Phenanthrene

Concen: 145.002 ng/u1

RT: 16.951 min Scan# 21

Delta R.T. 0.012 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39

Instrument :

BNA_N

ClientSampleId :

SSTD160222





Tgt Ion:178 Resp:10360527

Ion Ratio Lower Upper

178 100

179 15.7 11.9 17.9

176 19.5 15.2 22.8

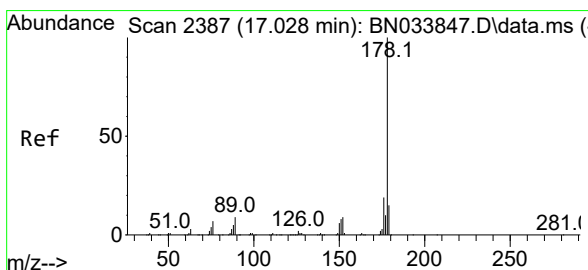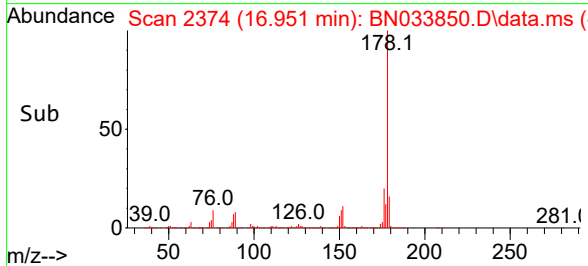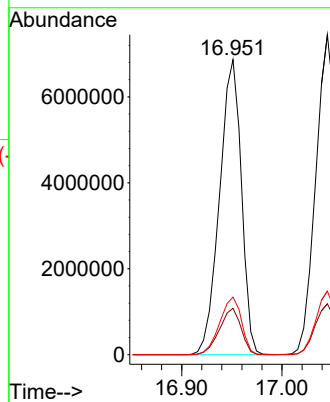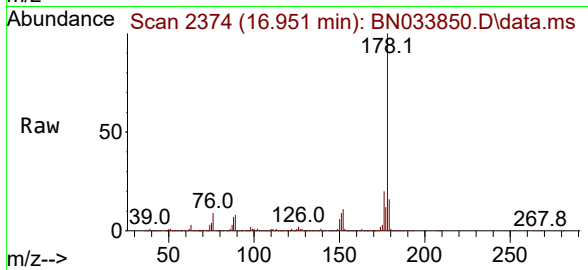

#74

Anthracene

Concen: 142.862 ng/u1

RT: 17.045 min Scan# 2390

Delta R.T. 0.018 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39




Tgt Ion:178 Resp:10399164


Ion Ratio Lower Upper

178 100

179 15.9 12.2 18.2

176 19.9 15.0 22.6


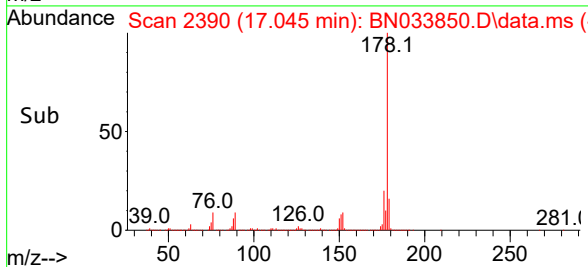
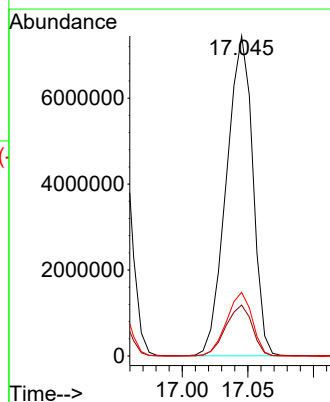
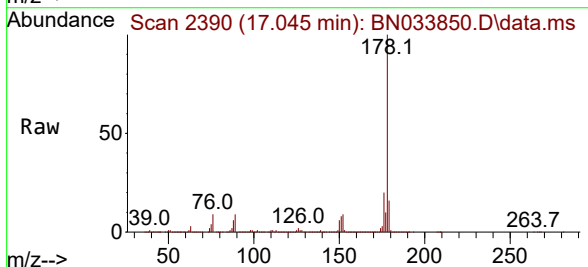


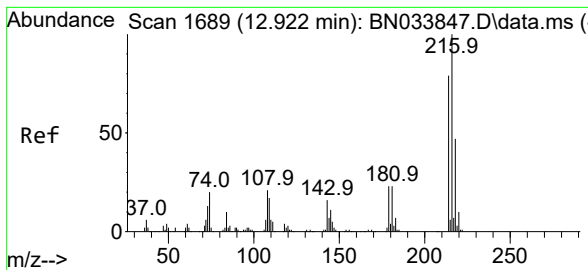

#75
1,2,3,4-Tetrachlorobenzene
Concen: 163.775 ng/uL
RT: 12.934 min Scan# 1691
Delta R.T. 0.012 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39




Instrument :
BNA_N
ClientSampleId :
SSTD160222


Tgt Ion:216 Resp: 2821510
Ion Ratio Lower Upper
216 100
214 78.4 63.6 95.4
218 45.4 37.6 56.4

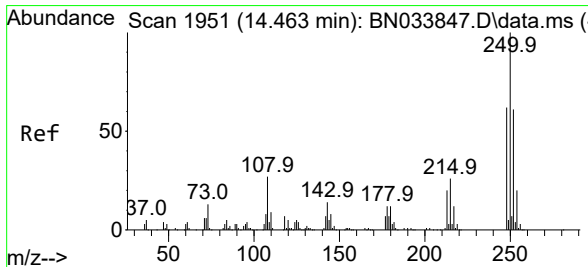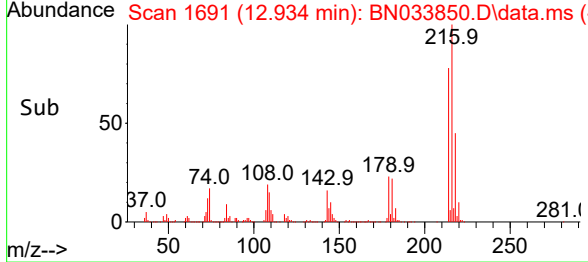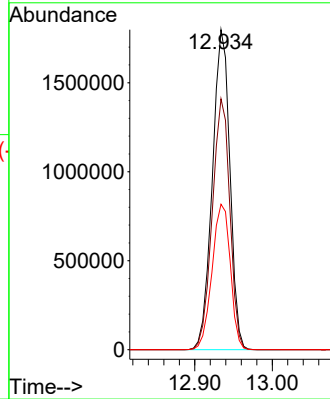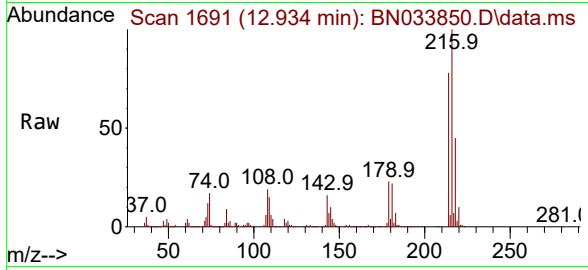

#76
Pentachlorobenzene
Concen: 162.951 ng/uL
RT: 14.475 min Scan# 1953
Delta R.T. 0.012 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39

Tgt Ion:250 Resp: 2889106
Ion Ratio Lower Upper
250 100
248 63.4 49.3 73.9
252 62.2 49.1 73.7

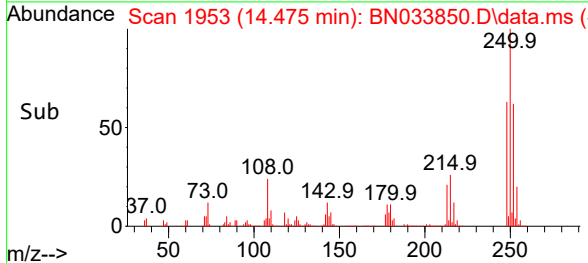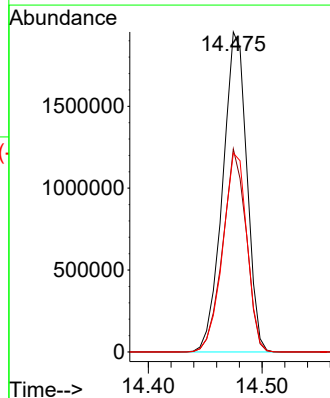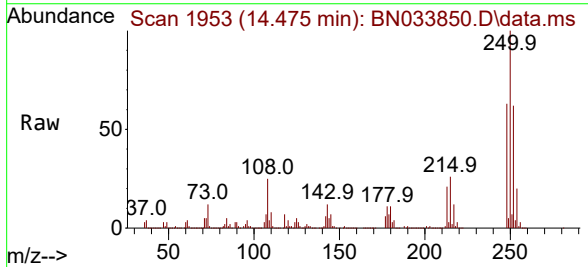




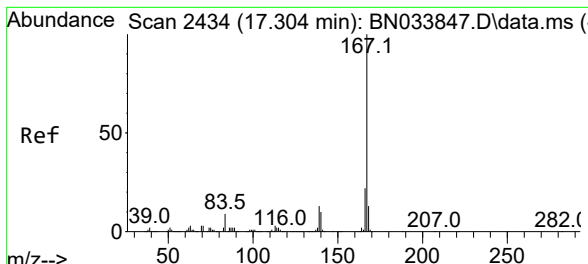


#77
 Carbazole
 Concen: 145.798 ng/ul
 RT: 17.316 min Scan# 2436
 Delta R.T. 0.012 min
 Lab File: BN033850.D
 Acq: 10 Sep 2024 20:39

Instrument :
 BNA_N
 ClientSampleId :
 SSTD160222

Tgt Ion:167 Resp: 9784361




Ion	Ratio	Lower	Upper
167	100		
166	22.3	17.4	26.0
139	14.2	10.5	15.7

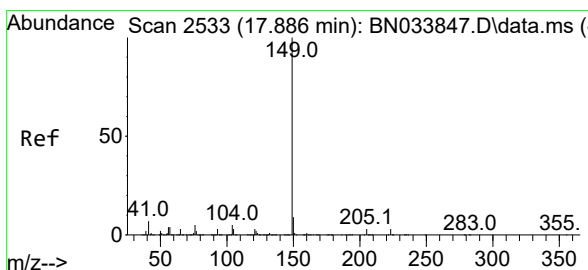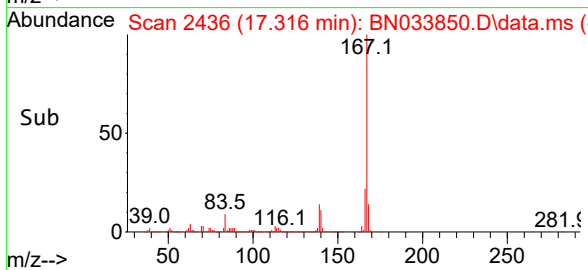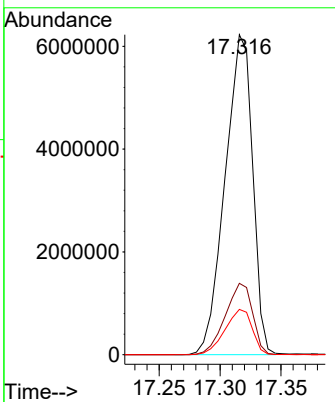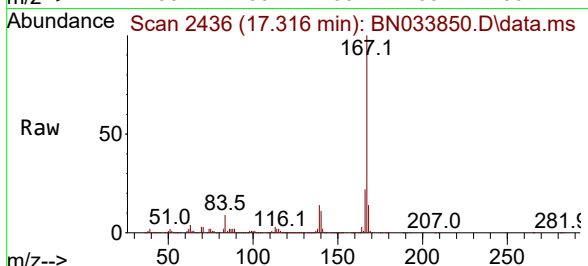


#78
 Di-n-butylphthalate
 Concen: 141.540 ng/ul
 RT: 17.898 min Scan# 2535
 Delta R.T. 0.012 min
 Lab File: BN033850.D
 Acq: 10 Sep 2024 20:39

Tgt Ion:149 Resp:11863116

Ion	Ratio	Lower	Upper
149	100		
150	10.6	7.4	11.2
104	6.1	4.3	6.5


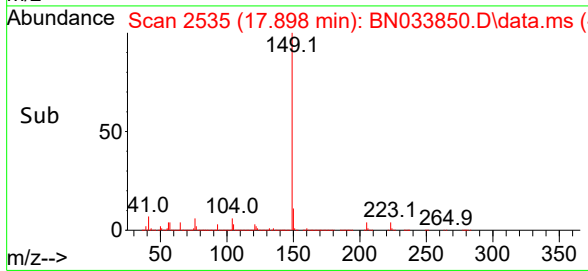
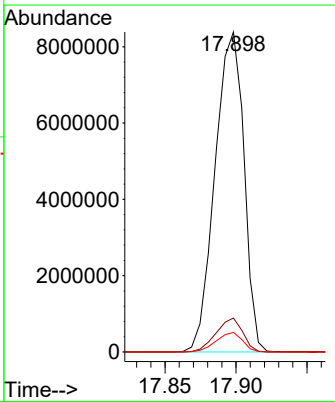
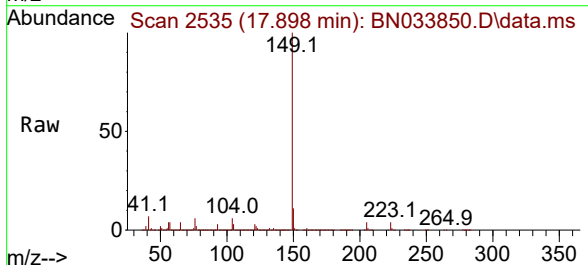




#80
Fluoranthene
Concen: 147.277 ng/ul
RT: 18.975 min Scan# 2716
Delta R.T. 0.012 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39




Instrument :
BNA_N
ClientSampleId :
SSTD160222


Tgt Ion:202 Resp:11747587
Ion Ratio Lower Upper
202 100
101 11.9 9.6 14.4
100 9.4 7.7 11.5



#82
Pyrene
Concen: 142.219 ng/ul
RT: 19.345 min Scan# 2781
Delta R.T. 0.018 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39

Tgt Ion:202 Resp:12295223
Ion Ratio Lower Upper
202 100
101 14.6 11.8 17.8
100 12.4 10.0 15.0





#83

Butylbenzylphthalate

Concen: 171.089 ng/ul

RT: 20.269 min Scan# 2937

Delta R.T. 0.006 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39

Instrument :

BNA_N

ClientSampleId :

SSTD160222





Tgt Ion:149 Resp: 5926809

Ion Ratio Lower Upper

149 100

91 72.2 56.3 84.5

206 21.2 15.9 23.9



#84

3,3'-Dichlorobenzidine

Concen: 141.220 ng/ul

RT: 21.063 min Scan# 3073

Delta R.T. 0.012 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39




Tgt Ion:252 Resp: 3977158


Ion Ratio Lower Upper

252 100

254 64.1 52.0 78.0

126 10.8 9.7 14.5









#85
Benzo(a)anthracene
Concen: 147.728 ng/ul
RT: 21.127 min Scan# 3082
Delta R.T. 0.012 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39




Instrument :
BNA_N
ClientSampleId :
SSTD160222


Tgt Ion:228 Resp:13132307
Ion Ratio Lower Upper
228 100
229 19.0 15.0 22.6
226 29.4 20.2 30.4

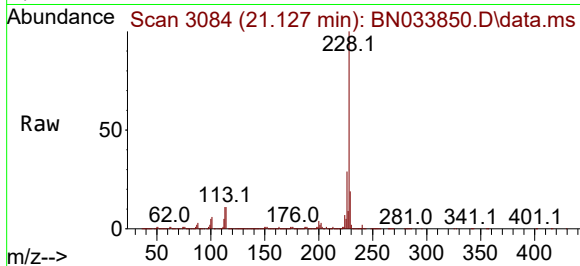

#86
Bis(2-ethylhexyl)phthalate
Concen: 147.042 ng/ul
RT: 21.080 min Scan# 3076
Delta R.T. 0.012 min
Lab File: BN033850.D
Acq: 10 Sep 2024 20:39

Tgt Ion:149 Resp: 8264084
Ion Ratio Lower Upper
149 100
167 27.6 20.6 31.0
279 5.6 3.0 4.6#

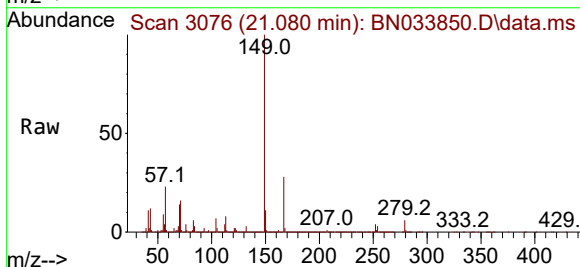



#87

Chrysene

Concen: 144.594 ng/ul

RT: 21.192 min Scan# 3095

Delta R.T. 0.024 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39

Instrument :

BNA_N

ClientSampleId :

SSTD160222





Tgt Ion:228 Resp:12088555

Ion Ratio Lower Upper

228 100

226 31.0 22.5 33.7

229 20.1 15.8 23.6

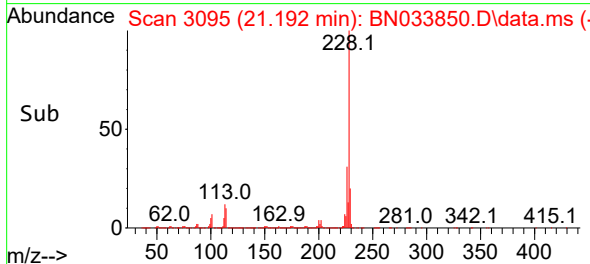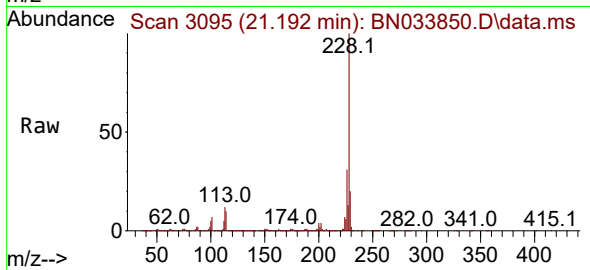

#89

Di-n-octyl phthalate

Concen: 150.296 ng/ul




RT: 22.145 min Scan# 3257


Delta R.T. 0.012 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39

Tgt Ion:149 Resp:14852552

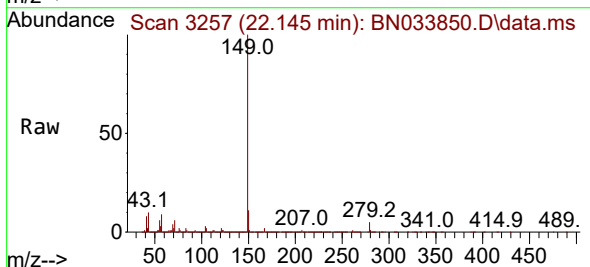



#90

Benzo(b)fluoranthene

Concen: 150.597 ng/ul

RT: 23.074 min Scan# 3409

Delta R.T. 0.035 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39

Instrument :

BNA_N

ClientSampleId :

SSTD160222





Tgt Ion:252 Resp:14365195

Ion Ratio Lower Upper

252 100

253 21.9 17.8 26.6

125 10.9 9.1 13.7

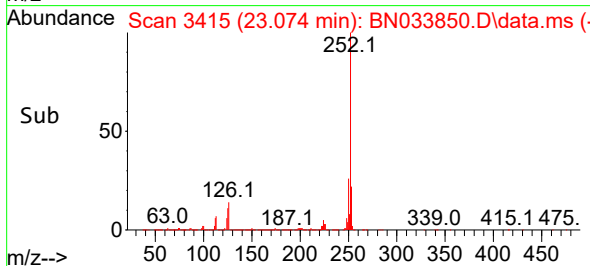

#91

Benzo(k)fluoranthene

Concen: 149.240 ng/ul

RT: 23.139 min Scan# 3426

Delta R.T. 0.041 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39




Tgt Ion:252 Resp:14132986


Ion Ratio Lower Upper

252 100

253 21.2 17.4 26.0

125 9.8 8.8 13.2

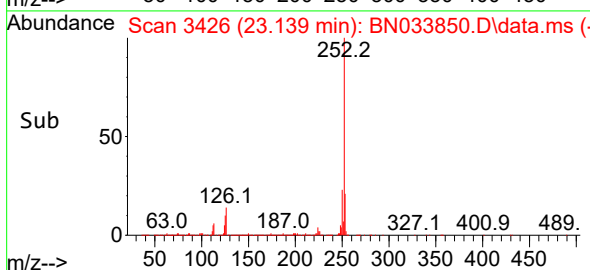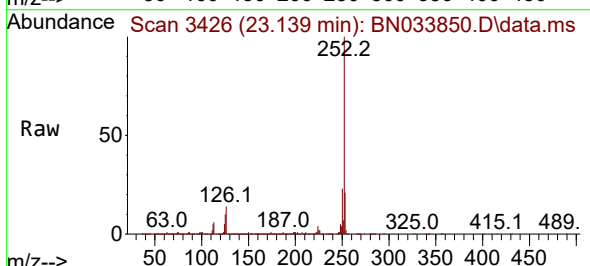



#93

Benzo(a)pyrene

Concen: 153.143 ng/ul

RT: 23.833 min Scan# 3

Delta R.T. 0.047 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39

Instrument :

BNA_N

ClientSampleId :

SSTD160222





Tgt Ion:252 Resp:13843715

Ion Ratio Lower Upper

252 100

253 23.4 15.8 23.8

125 12.1 9.0 13.6

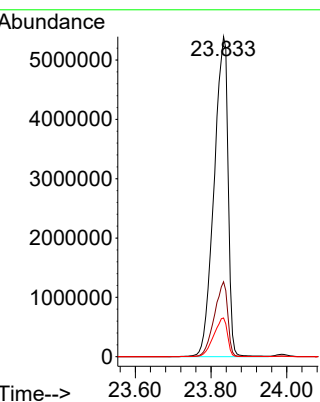

#94

Indeno(1,2,3-cd)pyrene

Concen: 157.762 ng/ul

RT: 27.068 min Scan# 4094

Delta R.T. 0.071 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39




Tgt Ion:276 Resp:17698718


Ion Ratio Lower Upper

276 100

138 21.3 17.7 26.5

277 24.7 18.4 27.6

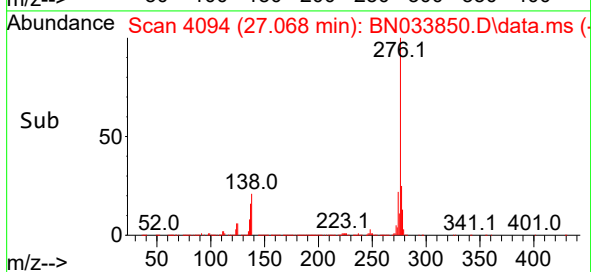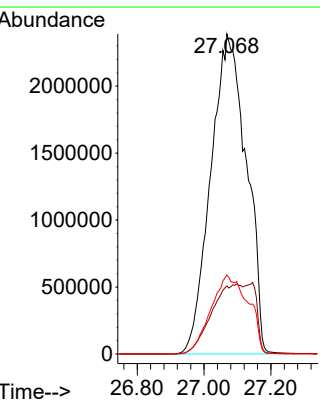



#95

Dibenzo(a,h)anthracene

Concen: 158.975 ng/ul

RT: 27.151 min Scan# 4108

Delta R.T. 0.094 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39

Instrument :

BNA_N

ClientSampleId :

SSTD160222





Tgt Ion:278 Resp:14605330

Ion Ratio Lower Upper

278 100

139 16.2 14.2 21.2

279 23.1 18.1 27.1



#96

Benzo(g,h,i)perylene

Concen: 158.322 ng/ul

RT: 28.074 min Scan# 4265

Delta R.T. 0.118 min

Lab File: BN033850.D

Acq: 10 Sep 2024 20:39

Tgt Ion:276 Resp:13649557

Ion Ratio Lower Upper

276 100

138 21.8 19.0 28.4

277 23.1 18.0 27.0

