




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091124\
Data File : BN033856.D
Acq On : 11 Sep 2024 10:57
Operator : JU/RC
Sample : P3391-01
Misc : SFAM-MDL-Q3-SOIL-01
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-QT3-2024-05

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/12/2024
Supervised By :mohammad ahmed 09/13/2024

Quant Time: Sep 11 11:27:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 11 01:58:59 2024
Response via : Initial Calibration

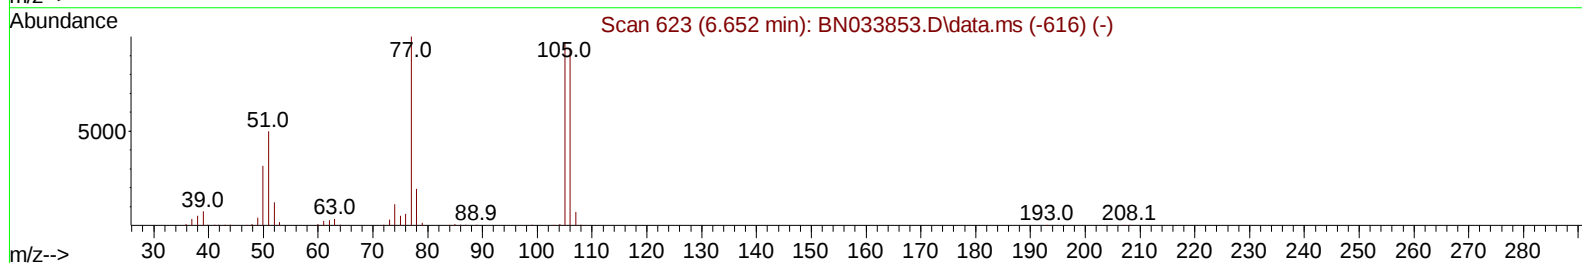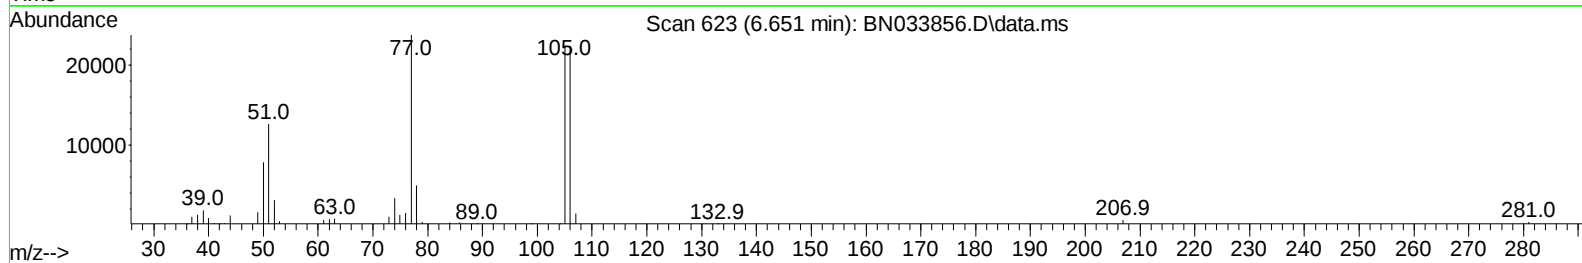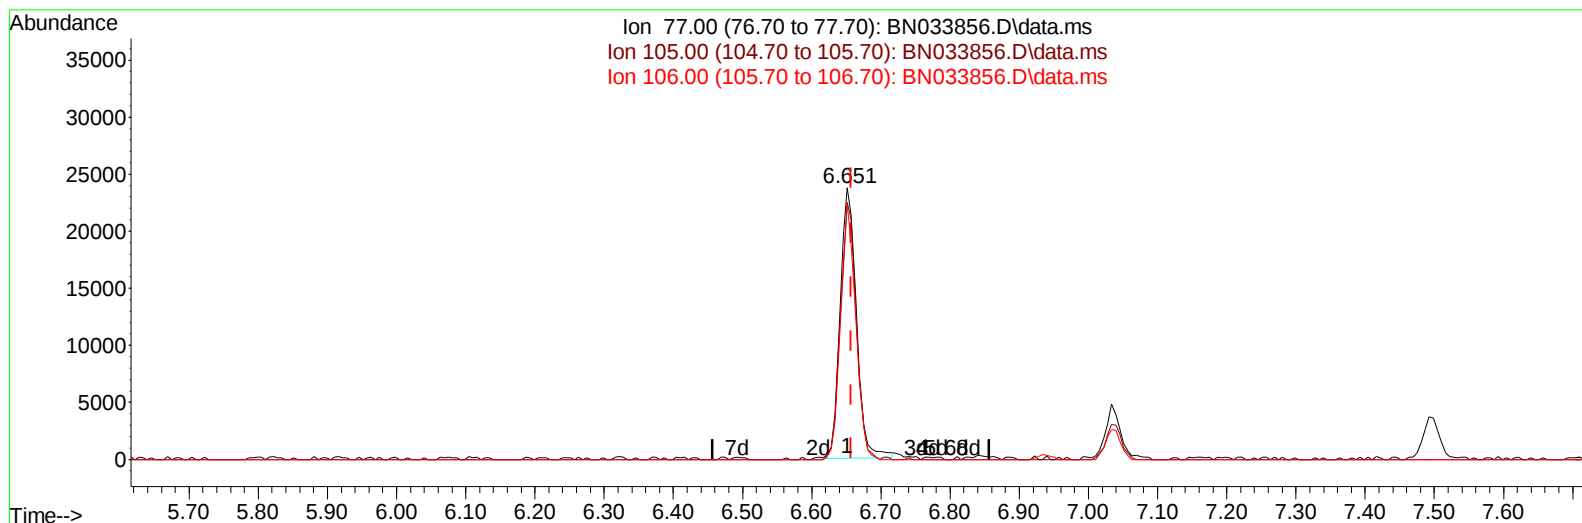

TIC: BN033856.D\data.ms

(6) Benzaldehyde

6.651min (-0.006) 5.49 ng/u1

response 38662

Ion	Exp%	Act%
77.00	100.00	100.00
105.00	95.50	94.72
106.00	87.20	94.18
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091124\
Data File : BN033856.D
Acq On : 11 Sep 2024 10:57
Operator : JU/RC
Sample : P3391-01
Misc : SFAM-MDL-Q3-SOIL-01
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-QT3-2024-05

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/12/2024
Supervised By :mohammad ahmed 09/13/2024

Quant Time: Sep 11 11:27:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 11 01:58:59 2024
Response via : Initial Calibration

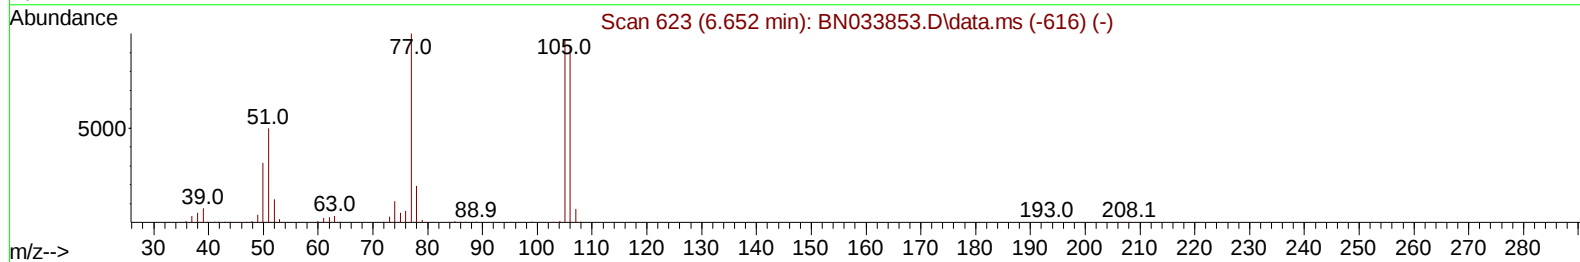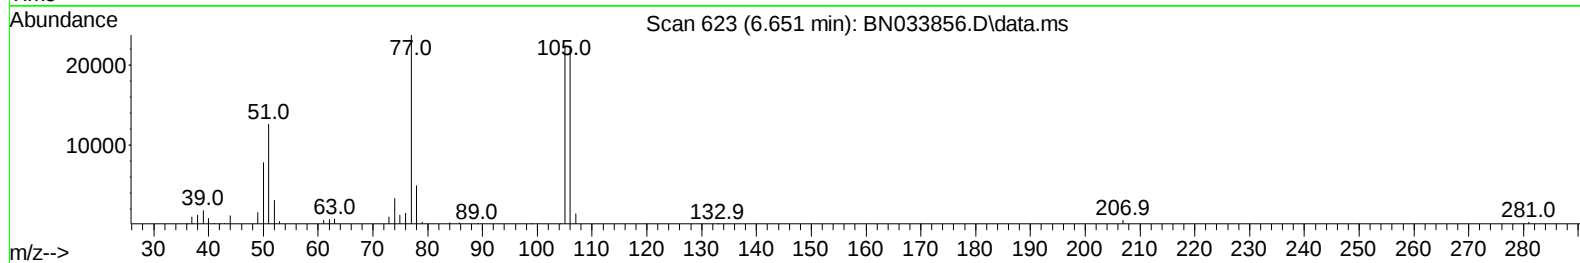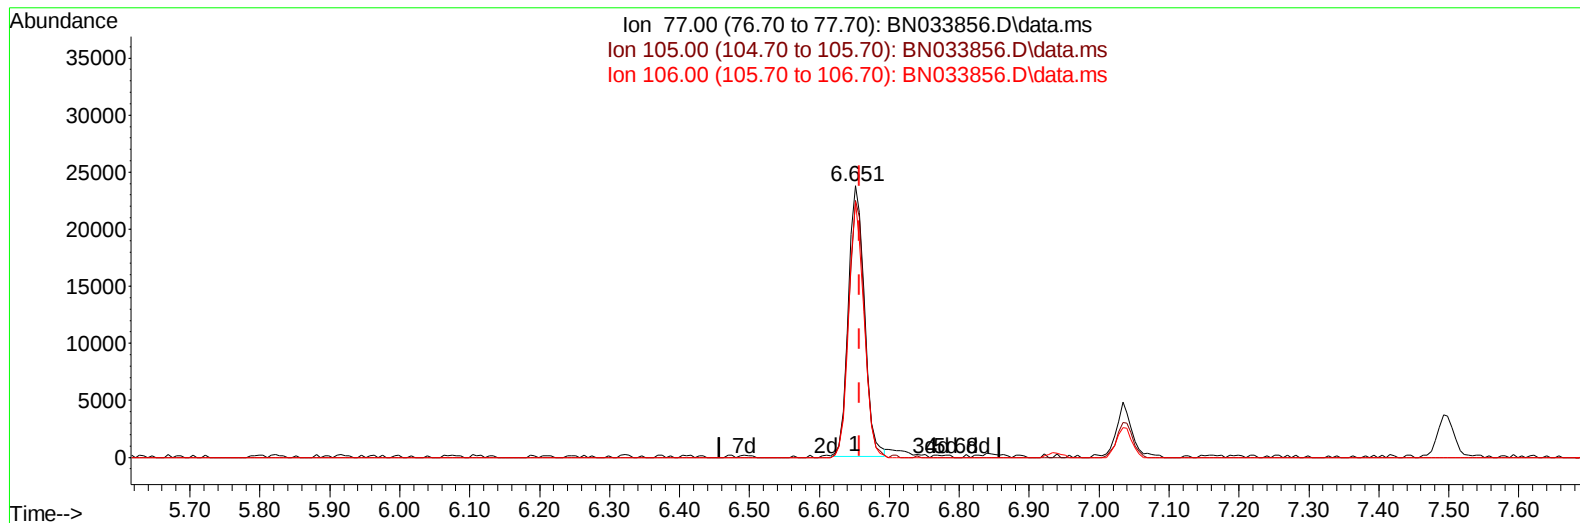

TIC: BN033856.D\data.ms

(6) Benzaldehyde

6.651min (-0.006) 5.41 ng/ul m

response 38114

Ion	Exp%	Act%
77.00	100.00	100.00
105.00	95.50	94.72
106.00	87.20	94.18
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091124\
Data File : BN033856.D
Acq On : 11 Sep 2024 10:57
Operator : JU/RC
Sample : P3391-01
Misc : SFAM-MDL-Q3-SOIL-01
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-QT3-2024-05

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/12/2024
Supervised By :mohammad ahmed 09/13/2024

Quant Time: Sep 11 11:27:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 11 01:58:59 2024
Response via : Initial Calibration

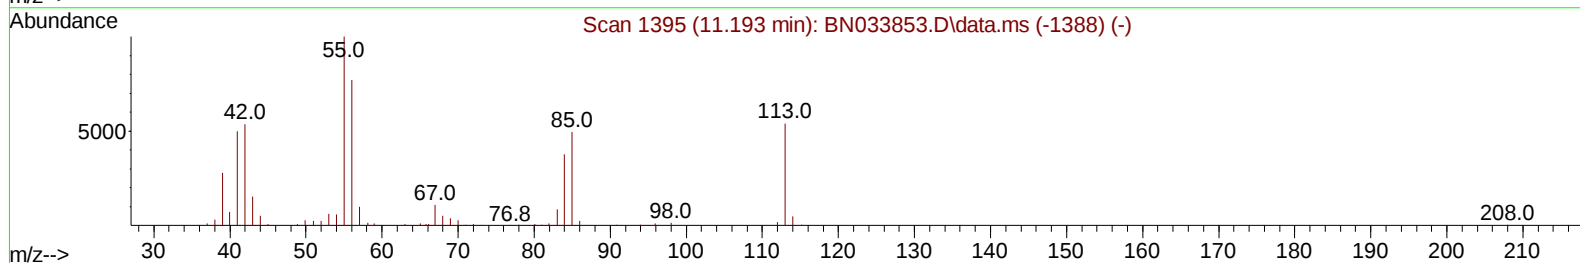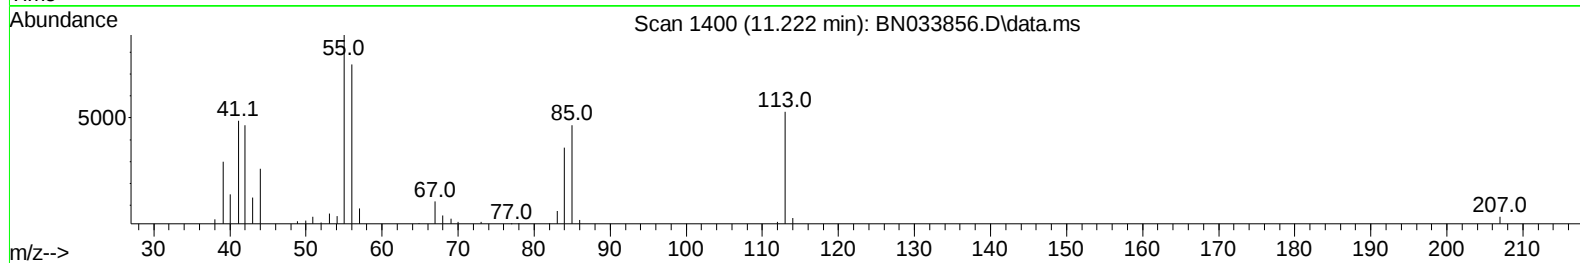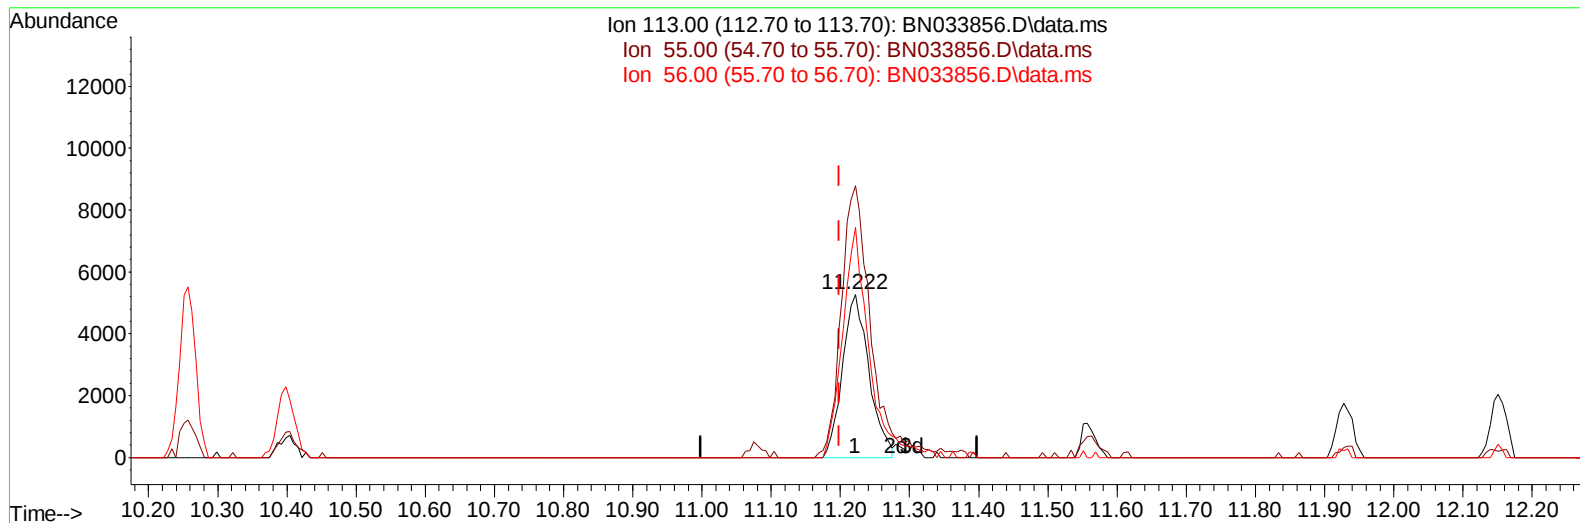

TIC: BN033856.D\data.ms

(34) Caprolactam

11.222min (+ 0.023) 3.35 ng/ul

response 13988

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	171.30	166.31
56.00	124.60	141.02
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091124\
 Data File : BN033856.D
 Acq On : 11 Sep 2024 10:57
 Operator : JU/RC
 Sample : P3391-01
 Misc : SFAM-MDL-Q3-SOIL-01
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-QT3-2024-05

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/12/2024
 Supervised By :mohammad ahmed 09/13/2024

Quant Time: Sep 11 11:27:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 11 01:58:59 2024
 Response via : Initial Calibration

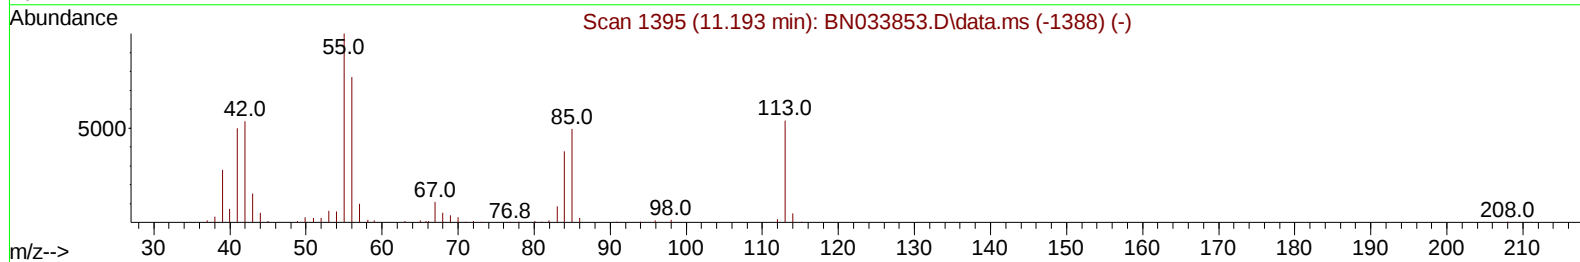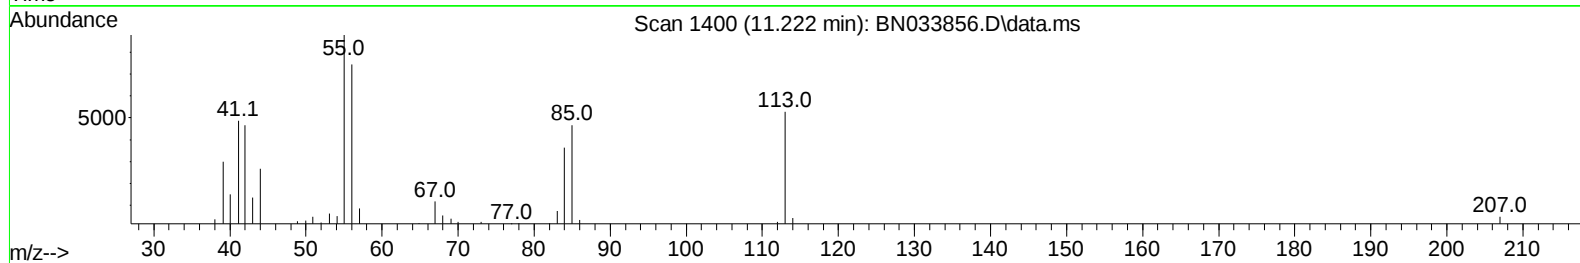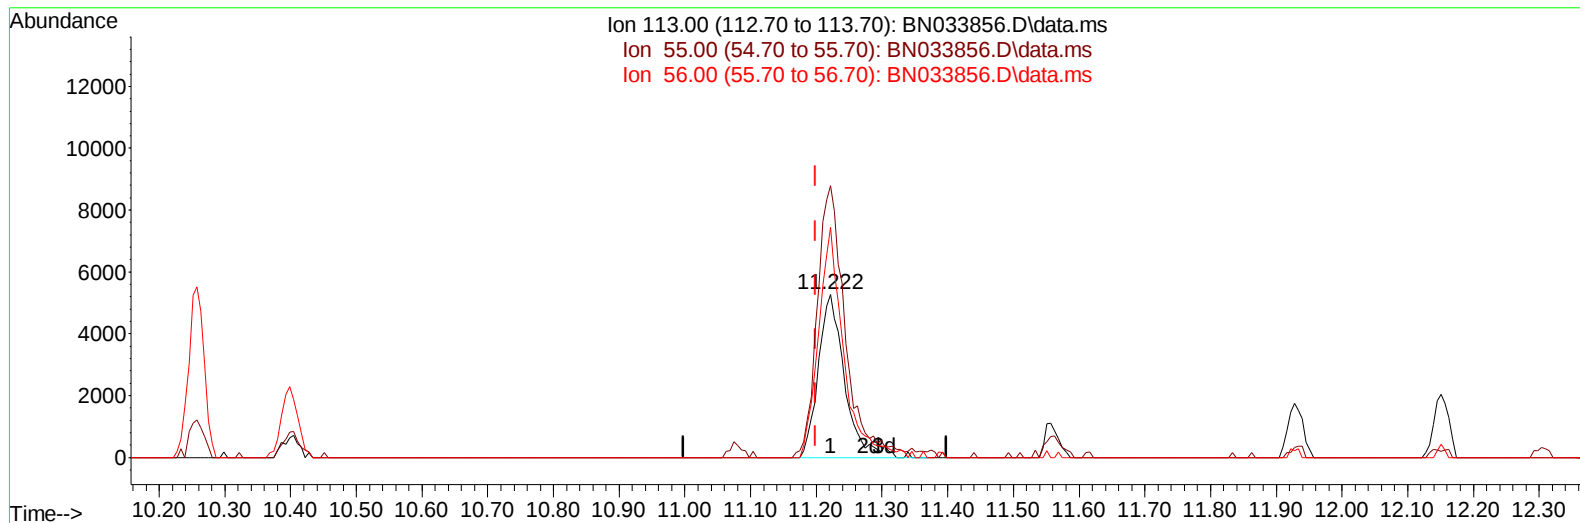

TIC: BN033856.D\data.ms

(34) Caprolactam

11.222min (+ 0.023) 3.53 ng/ul m

response 14739

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	171.30	166.31
56.00	124.60	141.02
0.00	0.00	0.00