

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091124\
 Data File : BN033854.D
 Acq On : 11 Sep 2024 09:28
 Operator : JU/RC
 Sample : PB163198BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK198

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN033854.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	18	22	29	rBV	38595	54528	1.02%	0.114%
2	3.505	84	88	118	rVB	487992	890190	16.60%	1.868%
3	3.811	136	140	146	rVB	10707	16565	0.31%	0.035%
4	4.269	213	218	225	rVB9	5093	13346	0.25%	0.028%
5	6.687	623	629	648	rVB	691172	1091937	20.36%	2.291%
6	6.852	650	657	672	rVB	545258	848016	15.81%	1.779%
7	7.040	682	689	699	rBV	663187	1059713	19.76%	2.224%
8	7.499	760	767	776	rVB	617048	964731	17.99%	2.024%
9	8.204	880	887	899	rBV	862818	1347773	25.13%	2.828%
10	8.640	953	961	972	rBV	688070	1098795	20.49%	2.306%
11	9.351	1074	1082	1090	rBV	555785	874830	16.31%	1.836%
12	9.887	1166	1173	1183	rBV	833207	1337641	24.94%	2.807%
13	10.257	1228	1236	1245	rVB	910768	1463441	27.28%	3.071%
14	10.398	1253	1260	1273	rBV	837948	1366152	25.47%	2.867%
15	11.857	1503	1508	1515	rVB4	12697	20944	0.39%	0.044%
16	13.563	1791	1798	1811	rVB	1681422	2259197	42.12%	4.741%
17	13.828	1836	1843	1854	rBV2	1768630	2519428	46.97%	5.287%
18	14.139	1889	1896	1906	rBV	1481101	2081449	38.81%	4.368%
19	14.357	1926	1933	1944	rBV	920834	1285656	23.97%	2.698%
20	15.139	2059	2066	2075	rBV	2245058	3198182	59.63%	6.711%
21	15.263	2080	2087	2099	rVV	760479	1056162	19.69%	2.216%
22	15.381	2103	2107	2111	rVB4	9925	13079	0.24%	0.027%
23	15.928	2196	2200	2205	rVB5	6560	8678	0.16%	0.018%
24	16.675	2322	2327	2334	rBV5	4286	8066	0.15%	0.017%
25	16.892	2357	2364	2371	rBV	1923119	2576865	48.04%	5.407%
26	16.992	2374	2381	2395	rBV	2629819	3620564	67.50%	7.597%
27	17.586	2477	2482	2484	rBV5	5547	8270	0.15%	0.017%
28	17.822	2518	2522	2527	rBV2	25945	40116	0.75%	0.084%
29	18.857	2694	2698	2705	rBV2	30031	47722	0.89%	0.100%
30	18.927	2706	2710	2716	rVV	30591	43139	0.80%	0.091%
31	19.116	2738	2742	2747	rBV5	16295	22644	0.42%	0.048%
32	19.298	2767	2773	2785	rVB	3254451	4284845	79.89%	8.991%
33	21.127	3078	3084	3092	rBV2	2331736	3116142	58.10%	6.539%
34	23.721	3516	3525	3541	rVB2	2399064	5363621	100.00%	11.255%
35	23.909	3549	3557	3565	rBV	1593101	3652895	68.11%	7.665%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091124\
Data File : BN033854.D
Acq On : 11 Sep 2024 09:28
Operator : JU/RC
Sample : PB163198BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK198

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 47655322

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091124\
Data File : BN033854.D
Acq On : 11 Sep 2024 09:28
Operator : JU/RC
Sample : PB163198BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK198

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

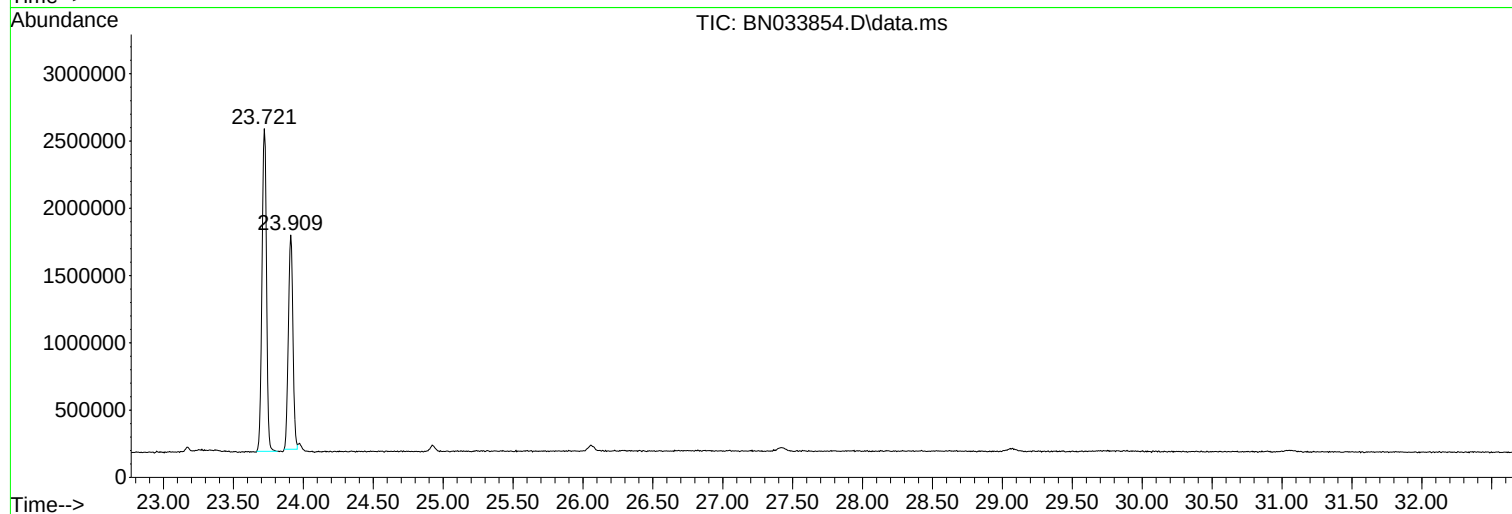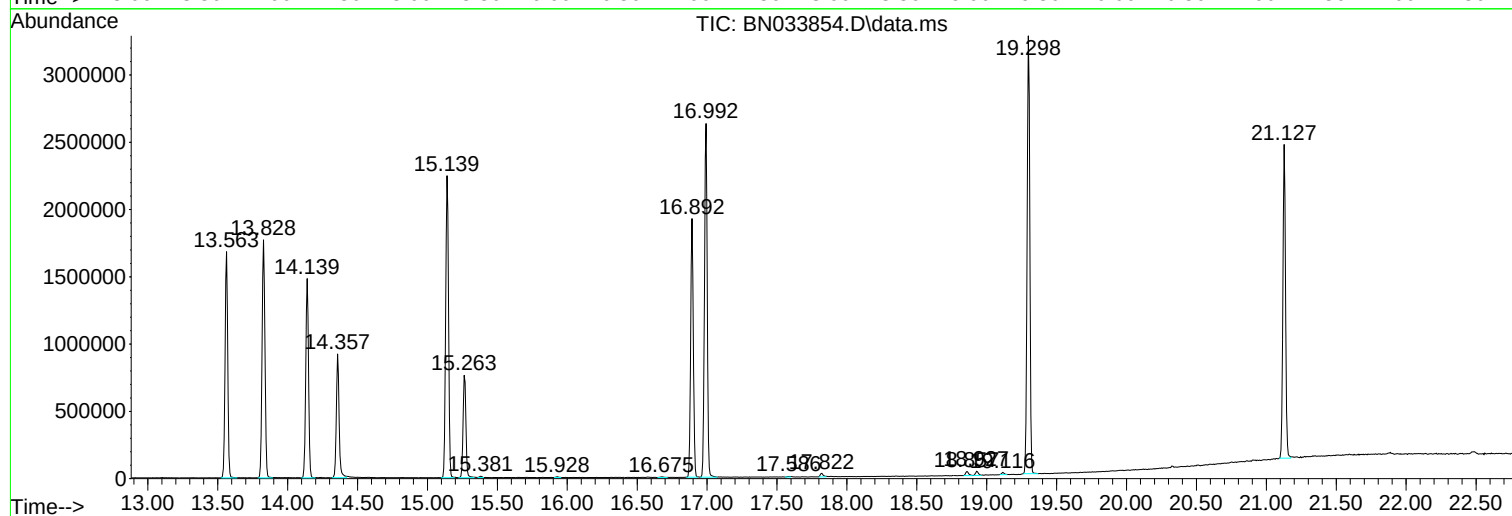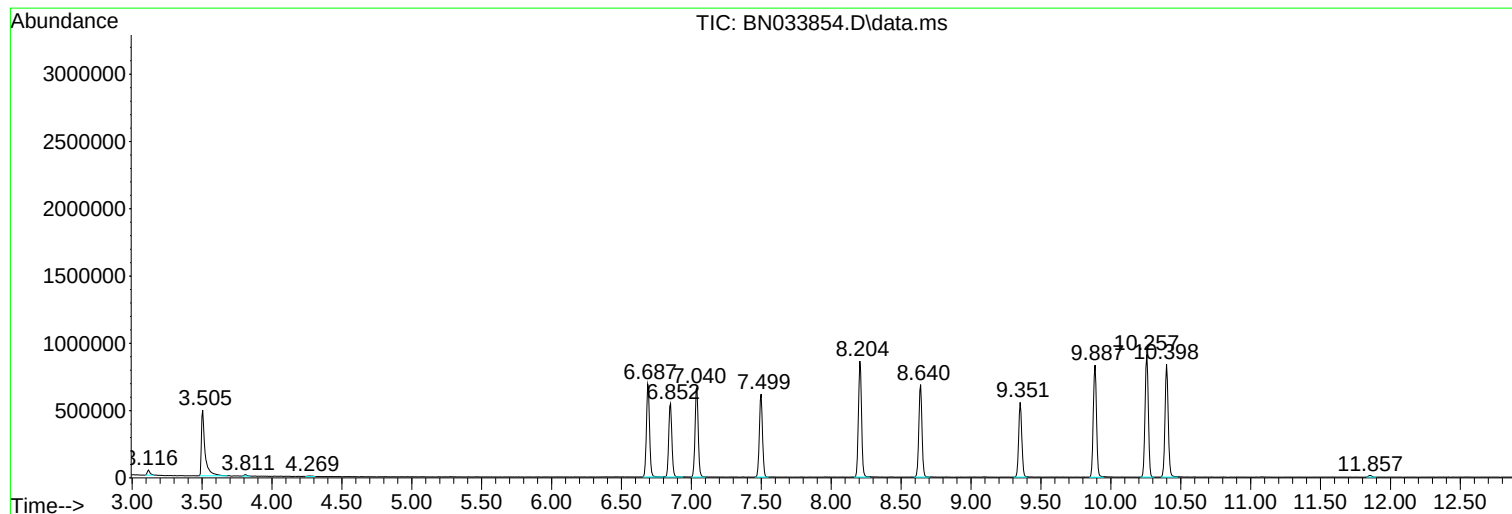

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091124\
Data File : BN033854.D
Acq On : 11 Sep 2024 09:28
Operator : JU/RC
Sample : PB163198BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK198

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091124\
Data File : BN033854.D
Acq On : 11 Sep 2024 09:28
Operator : JU/RC
Sample : PB163198BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK198

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc