

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091124\
 Data File : BN033859.D
 Acq On : 11 Sep 2024 13:08
 Operator : JU/RC
 Sample : PB163275BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK275

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN033859.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	18	22	33	rVB	36744	58079	1.23%	0.128%
2	3.499	83	87	111	rBV	465184	882662	18.74%	1.940%
3	3.810	136	140	146	rVB2	9888	14410	0.31%	0.032%
4	4.263	212	217	226	rVB5	4638	12100	0.26%	0.027%
5	6.687	622	629	643	rBV	678743	1084523	23.02%	2.383%
6	6.845	650	656	667	rVB	531884	845693	17.95%	1.858%
7	7.040	682	689	701	rBV	660516	1058291	22.46%	2.325%
8	7.498	759	767	775	rBV	621430	964849	20.48%	2.120%
9	8.204	880	887	901	rBV	857127	1345668	28.56%	2.957%
10	8.639	953	961	971	rBV	677873	1091742	23.17%	2.399%
11	9.351	1075	1082	1090	rBV	564809	868834	18.44%	1.909%
12	9.886	1165	1173	1186	rBV	834379	1336320	28.36%	2.936%
13	10.257	1228	1236	1245	rBV	902120	1461596	31.02%	3.212%
14	10.398	1252	1260	1272	rBV	816125	1358567	28.84%	2.985%
15	11.857	1501	1508	1518	rVB2	13255	22639	0.48%	0.050%
16	13.563	1791	1798	1805	rBV	1638322	2195575	46.60%	4.824%
17	13.827	1836	1843	1850	rBV	1722917	2457045	52.15%	5.399%
18	14.139	1889	1896	1906	rBV	1476868	2057463	43.67%	4.521%
19	14.357	1926	1933	1944	rBV	859863	1208561	25.65%	2.656%
20	15.139	2059	2066	2077	rBV	2244369	3111846	66.05%	6.838%
21	15.263	2082	2087	2098	rBV	752193	981734	20.84%	2.157%
22	15.380	2103	2107	2112	rVB4	10616	12129	0.26%	0.027%
23	15.927	2197	2200	2203	rVB3	6266	6888	0.15%	0.015%
24	16.680	2322	2328	2333	rBV2	3328	6364	0.14%	0.014%
25	16.892	2358	2364	2374	rVB	1820813	2498260	53.03%	5.490%
26	16.992	2374	2381	2397	rBV2	2534045	3492169	74.12%	7.673%
27	17.586	2478	2482	2489	rVB8	5738	10508	0.22%	0.023%
28	17.815	2517	2521	2529	rBV5	23791	39491	0.84%	0.087%
29	18.857	2694	2698	2705	rVB4	29939	42302	0.90%	0.093%
30	18.927	2706	2710	2715	rBV	27587	40008	0.85%	0.088%
31	19.115	2739	2742	2750	rVB7	13141	17241	0.37%	0.038%
32	19.298	2766	2773	2782	rBV	3126996	4093135	86.88%	8.994%
33	19.980	2884	2889	2892	rBV5	22804	50431	1.07%	0.111%
34	21.127	3079	3084	3091	rBV	2172458	2874408	61.01%	6.316%
35	23.721	3516	3525	3541	rVB2	2027208	4711244	100.00%	10.352%
36	23.909	3549	3557	3565	rBV	1446793	3196866	67.86%	7.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091124\
Data File : BN033859.D
Acq On : 11 Sep 2024 13:08
Operator : JU/RC
Sample : PB163275BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK275

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 45509641

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091124\
Data File : BN033859.D
Acq On : 11 Sep 2024 13:08
Operator : JU/RC
Sample : PB163275BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK275

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

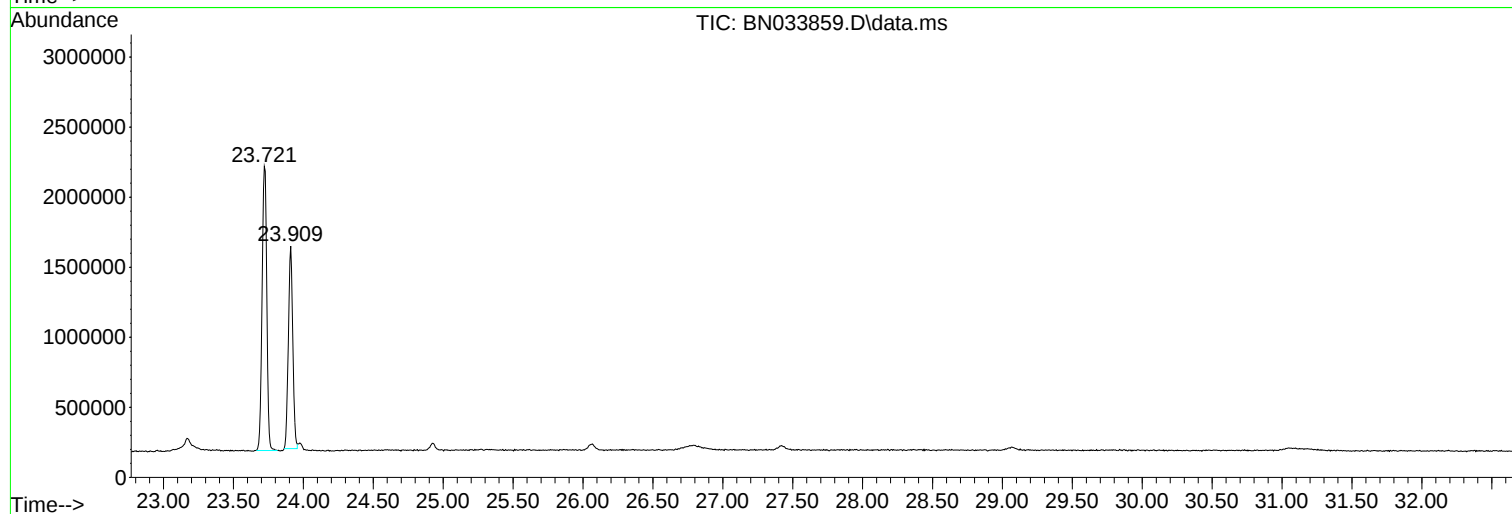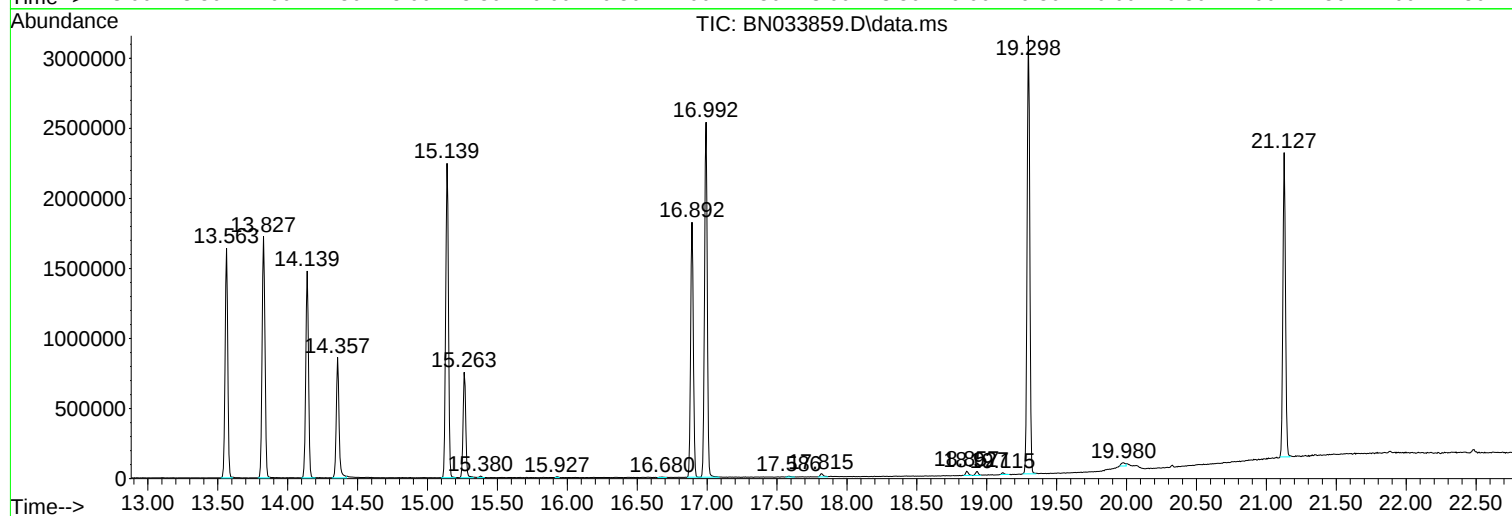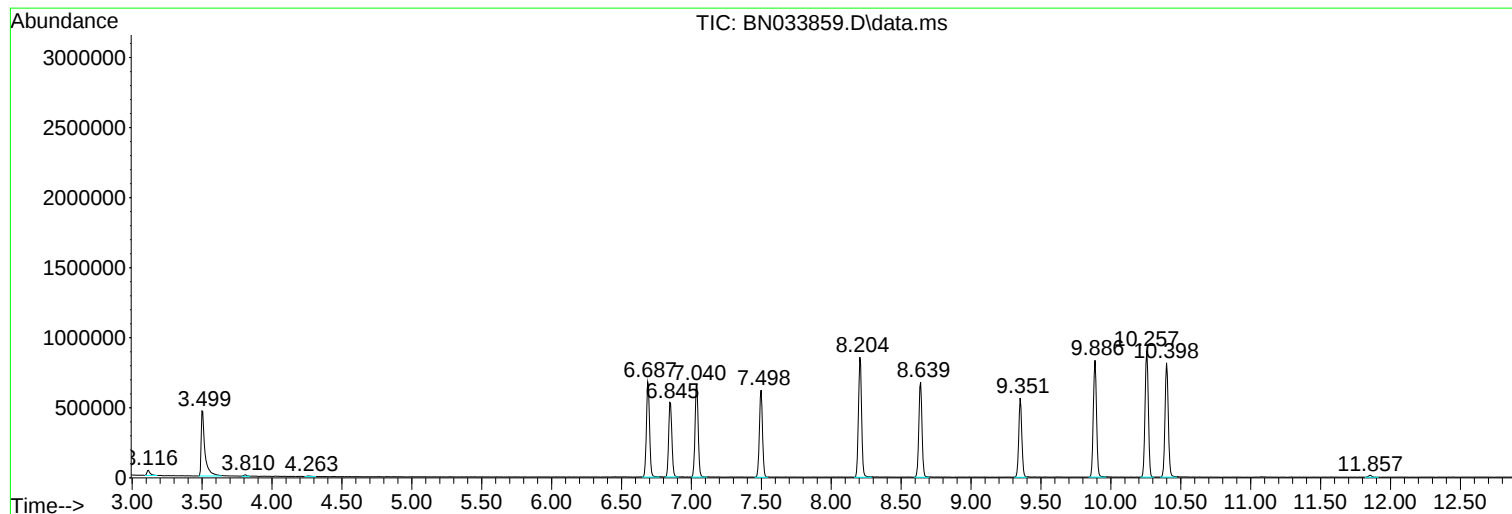

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091124\
Data File : BN033859.D
Acq On : 11 Sep 2024 13:08
Operator : JU/RC
Sample : PB163275BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK275

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091124\
Data File : BN033859.D
Acq On : 11 Sep 2024 13:08
Operator : JU/RC
Sample : PB163275BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK275

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc