

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091124\
 Data File : BN033861.D
 Acq On : 11 Sep 2024 14:58
 Operator : JU/RC
 Sample : PB163243BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK243

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN033861.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.111	17	21	30	rVB	34042	47697	1.03%	0.111%
2	3.499	83	87	108	rBV	435626	771635	16.66%	1.798%
3	3.805	135	139	145	rVB	8990	13240	0.29%	0.031%
4	4.252	212	215	223	rVB4	3717	9437	0.20%	0.022%
5	6.687	621	629	645	rVB	613023	954220	20.61%	2.223%
6	6.846	649	656	664	rBV	483464	734129	15.85%	1.711%
7	7.034	680	688	700	rBV	601344	926190	20.00%	2.158%
8	7.493	760	766	775	rVB	606826	938979	20.28%	2.188%
9	8.205	880	887	902	rBV	750615	1173331	25.34%	2.734%
10	8.634	953	960	970	rBV	595744	957748	20.68%	2.232%
11	9.352	1072	1082	1091	rBV	472585	753433	16.27%	1.756%
12	9.887	1164	1173	1187	rBV	719598	1170791	25.28%	2.728%
13	10.252	1229	1235	1243	rBV	878762	1437056	31.03%	3.349%
14	10.399	1252	1260	1271	rBV	717152	1199886	25.91%	2.796%
15	11.851	1500	1507	1515	rVB2	13003	21862	0.47%	0.051%
16	13.563	1791	1798	1807	rBV	1410353	1946358	42.03%	4.535%
17	13.828	1836	1843	1853	rBV	1535358	2181446	47.11%	5.083%
18	14.140	1889	1896	1903	rBV	1424303	2011444	43.44%	4.687%
19	14.357	1924	1933	1954	rBV	767771	1113871	24.05%	2.595%
20	15.139	2059	2066	2078	rBV	1947420	2765998	59.73%	6.445%
21	15.263	2081	2087	2100	rVV	632383	879630	19.00%	2.050%
22	15.381	2103	2107	2111	rVB4	8696	11987	0.26%	0.028%
23	15.928	2197	2200	2206	rVB3	5744	6842	0.15%	0.016%
24	16.681	2324	2328	2334	rVB5	4616	8264	0.18%	0.019%
25	16.892	2358	2364	2374	rBV	1885472	2499504	53.98%	5.824%
26	16.992	2374	2381	2392	rBV	2269050	3129871	67.59%	7.293%
27	17.586	2478	2482	2487	rBV7	4188	8348	0.18%	0.019%
28	17.816	2516	2521	2530	rBV2	28901	46386	1.00%	0.108%
29	18.857	2694	2698	2706	rBV3	24365	39252	0.85%	0.091%
30	18.933	2706	2711	2714	rBV	25257	34866	0.75%	0.081%
31	19.116	2738	2742	2749	rBV6	19107	29144	0.63%	0.068%
32	19.298	2767	2773	2780	rBV	2861244	3732838	80.61%	8.698%
33	21.127	3078	3084	3093	rBV2	2305189	3091975	66.77%	7.205%
34	23.721	3517	3525	3538	rVB2	2105076	4630597	100.00%	10.790%
35	23.910	3549	3557	3567	rBV	1597944	3637900	78.56%	8.477%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091124\
Data File : BN033861.D
Acq On : 11 Sep 2024 14:58
Operator : JU/RC
Sample : PB163243BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK243

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 42916155

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091124\
Data File : BN033861.D
Acq On : 11 Sep 2024 14:58
Operator : JU/RC
Sample : PB163243BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK243

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

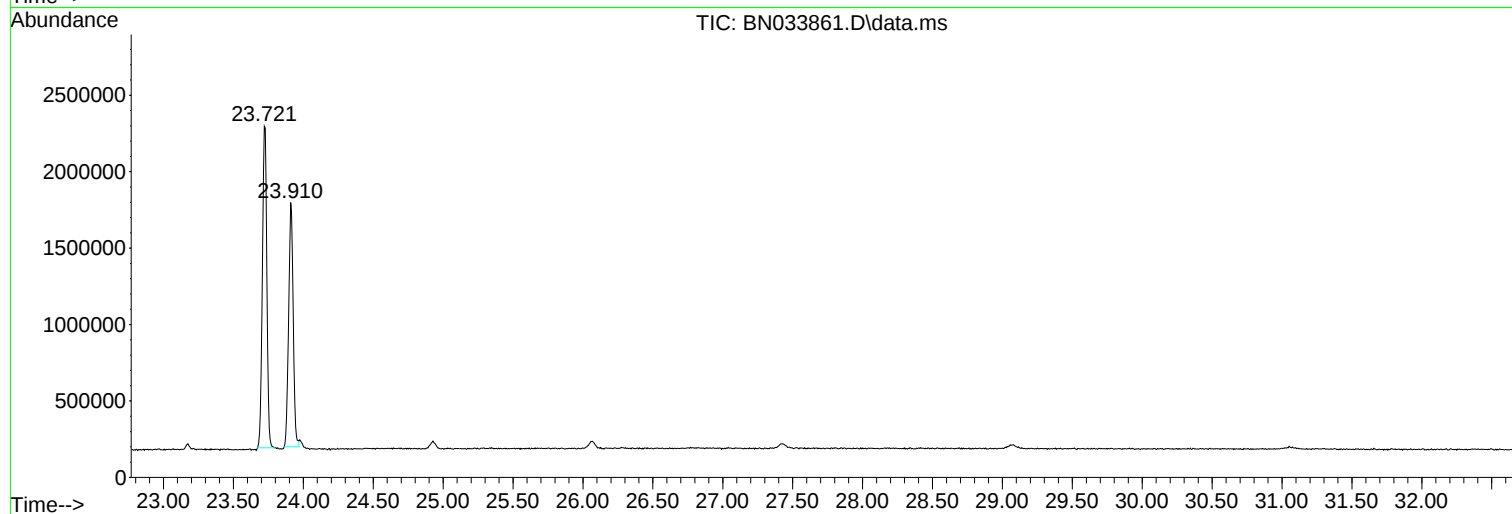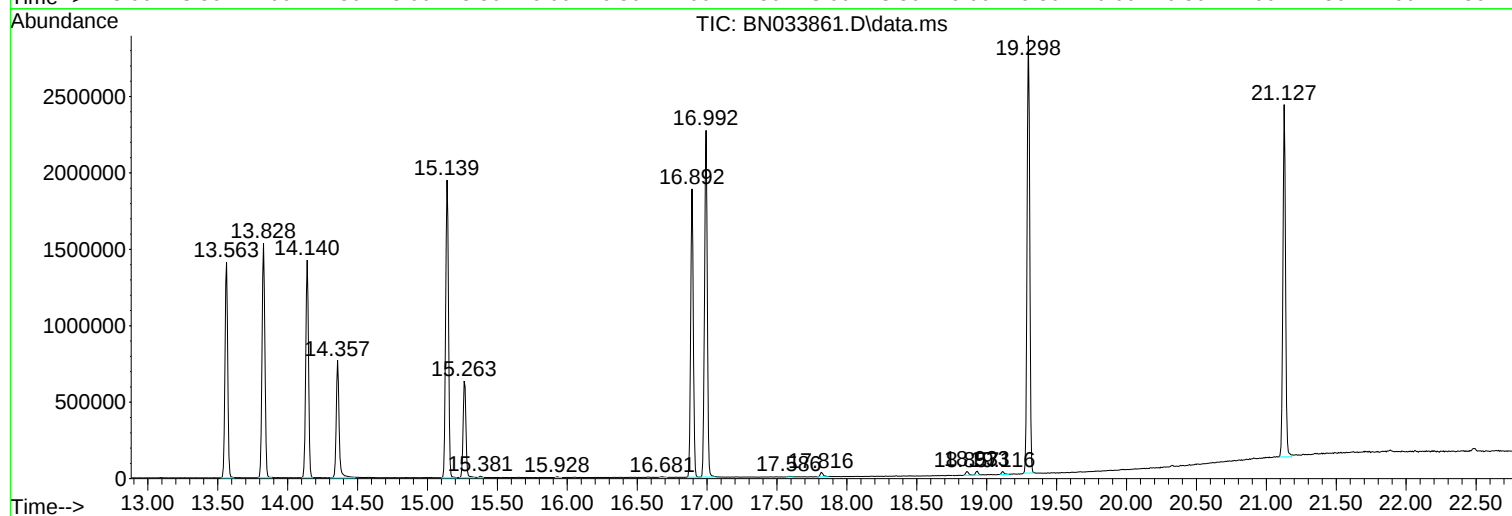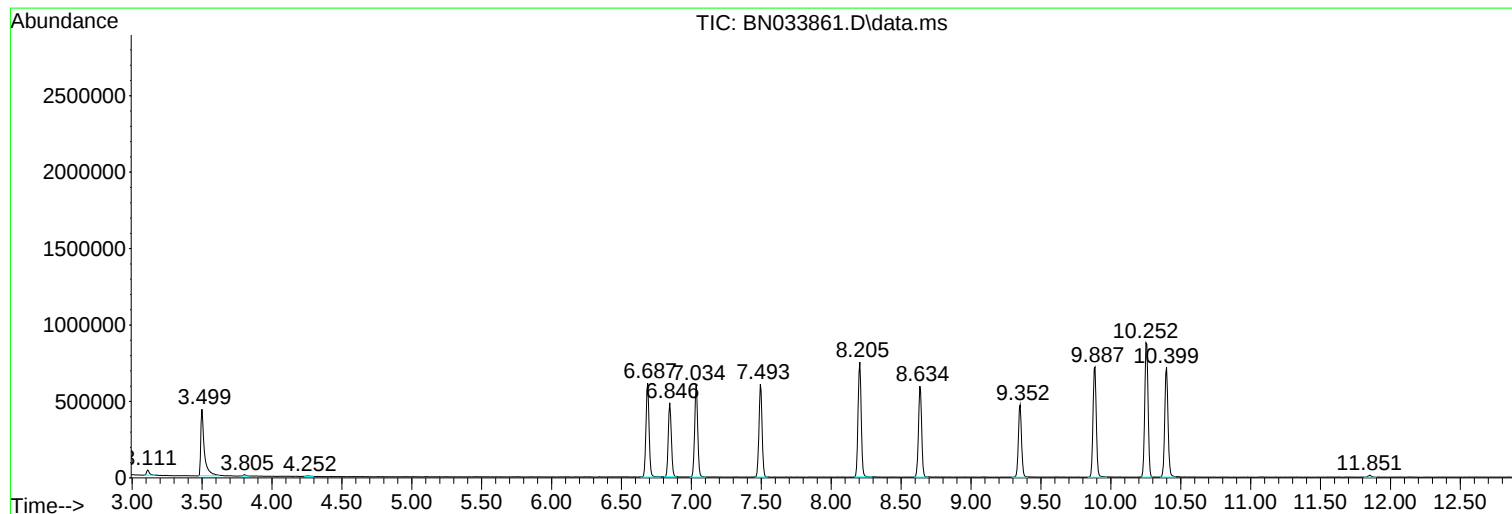

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091124\
Data File : BN033861.D
Acq On : 11 Sep 2024 14:58
Operator : JU/RC
Sample : PB163243BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK243

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091124\
Data File : BN033861.D
Acq On : 11 Sep 2024 14:58
Operator : JU/RC
Sample : PB163243BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK243

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------