

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091222\
 Data File : BN021716.D
 Acq On : 12 Sep 2022 11:23
 Operator : CG/JU
 Sample : PB147570BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB147570BL

Quant Time: Sep 13 02:33:49 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 13 02:32:27 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.062	152	6336	0.400	ng	0.00
7) Naphthalene-d8	10.888	136	19408	0.400	ng	0.00
13) Acenaphthene-d10	14.718	164	10489	0.400	ng	0.01
19) Phenanthrene-d10	17.470	188	20375	0.400	ng	0.01
29) Chrysene-d12	21.655	240	12947	0.400	ng	# 0.00
35) Perylene-d12	24.168	264	10859	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.592	112	6646	0.536	ng	0.00
5) Phenol-d6	7.217	99	7892	0.499	ng	0.00
8) Nitrobenzene-d5	9.233	82	5769	0.440	ng	0.00
11) 2-Methylnaphthalene-d10	12.478	152	19274	0.441	ng	0.00
14) 2,4,6-Tribromophenol	16.219	330	1138	0.330	ng	0.01
15) 2-Fluorobiphenyl	13.339	172	16338	0.356	ng	0.00
27) Fluoranthene-d10	19.497	212	19954	0.381	ng	0.00
31) Terphenyl-d14	20.088	244	12438	0.427	ng	0.00
Target Compounds						Qvalue
12) 2-Methylnaphthalene	12.180	142	1	0.127	ng	# 1
24) Pentachlorophenol	17.131	266	82	0.220	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091222\
Data File : BN021716.D
Acq On : 12 Sep 2022 11:23
Operator : CG/JU
Sample : PB147570BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB147570BL


Quant Time: Sep 13 02:33:49 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 13 02:32:27 2022
Response via : Initial Calibration

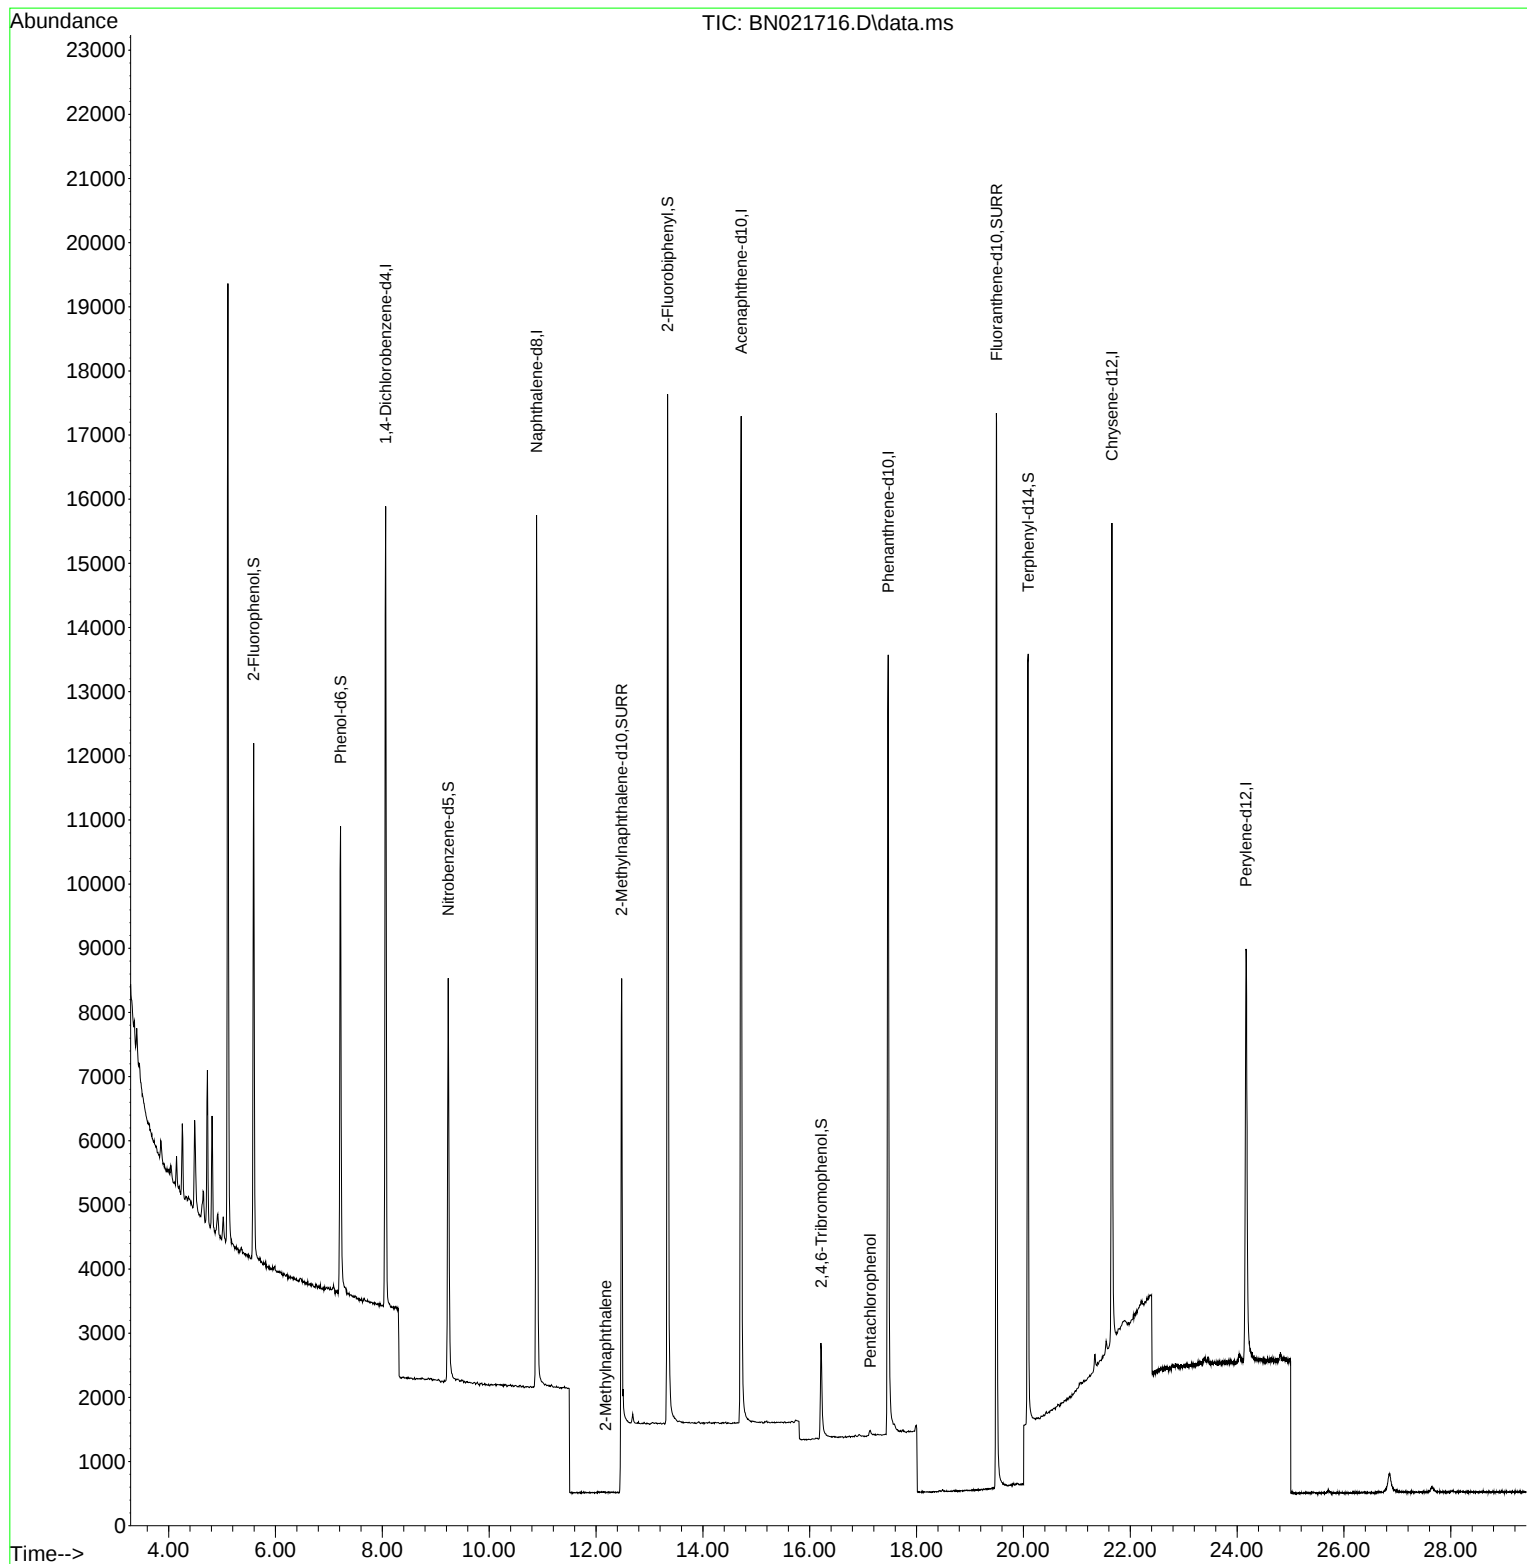






#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 8.062 min Scan# 60
Delta R.T. -0.000 min
Lab File: BN021716.D
Acq: 12 Sep 2022 11:23

Instrument :
BNA_N
ClientSampleId :
PB147570BL



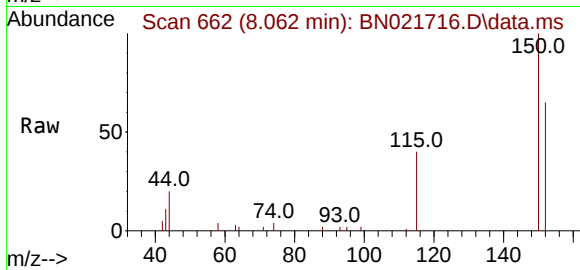


Tgt Ion:152 Resp: 6336
Ion Ratio Lower Upper
152 100
150 153.1 121.4 182.0
115 60.8 48.6 72.8

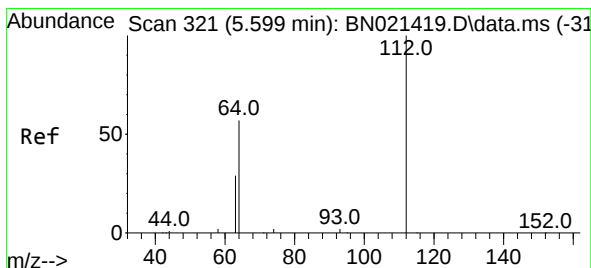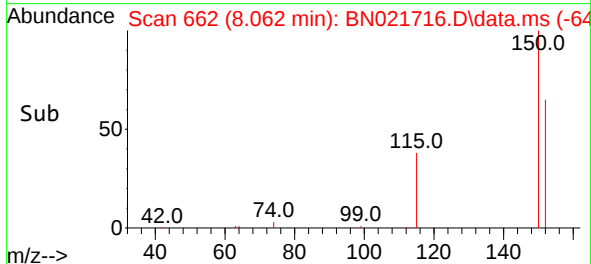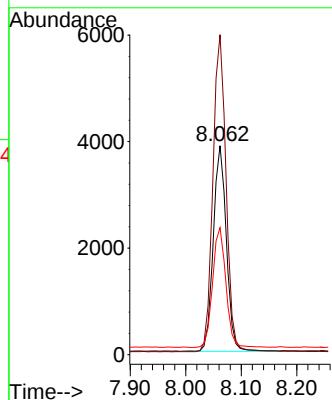

#4
2-Fluorophenol
Concen: 0.536 ng
RT: 5.592 min Scan# 320
Delta R.T. 0.007 min
Lab File: BN021716.D
Acq: 12 Sep 2022 11:23

Tgt Ion:112 Resp: 6646
Ion Ratio Lower Upper
112 100
64 56.5 43.5 65.3
63 29.1 22.6 34.0


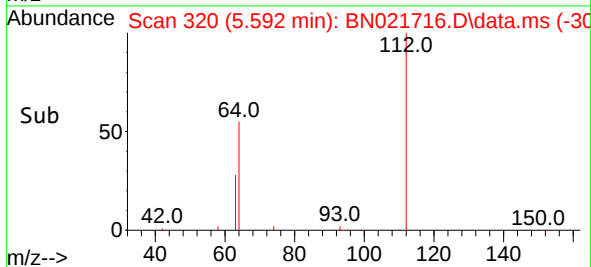
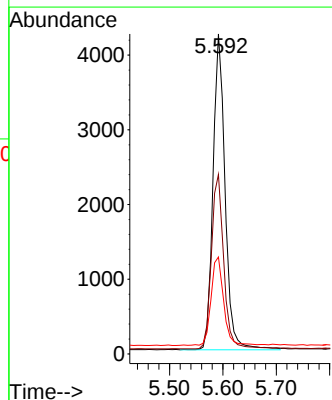
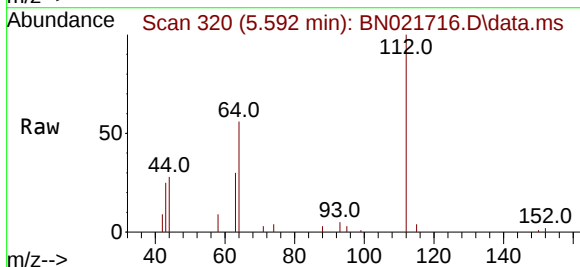




#5
Phenol-d6
Concen: 0.499 ng
RT: 7.217 min Scan# 54
Delta R.T. 0.007 min
Lab File: BN021716.D
Acq: 12 Sep 2022 11:23




Instrument :
BNA_N
ClientSampleId :
PB147570BL

Tgt Ion: 99 Resp: 7892
Ion Ratio Lower Upper
99 100
42 17.3 15.5 23.3
71 31.7 24.2 36.2

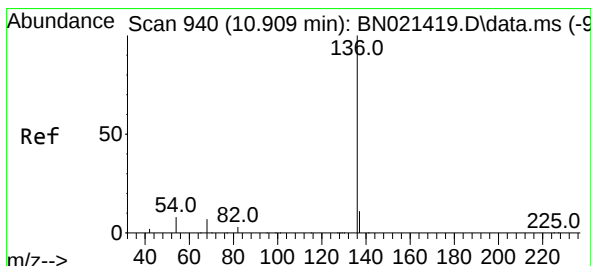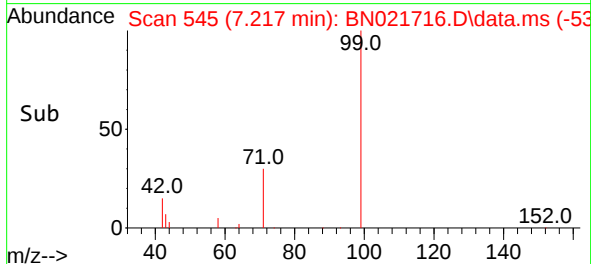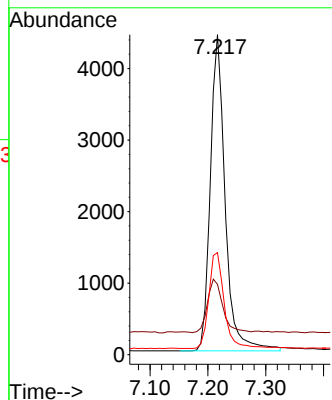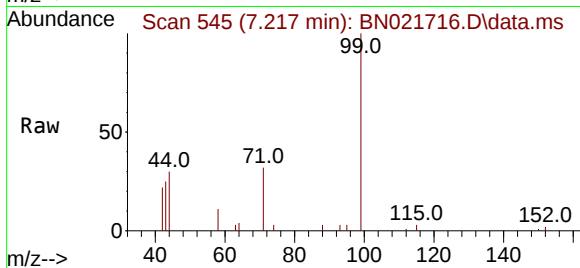

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.888 min Scan# 938
Delta R.T. 0.000 min
Lab File: BN021716.D
Acq: 12 Sep 2022 11:23

Tgt Ion: 136 Resp: 19408
Ion Ratio Lower Upper
136 100
137 11.2 9.3 13.9
54 9.2 6.9 10.3
68 7.9 6.1 9.1

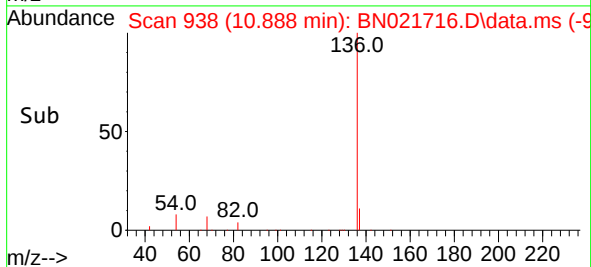
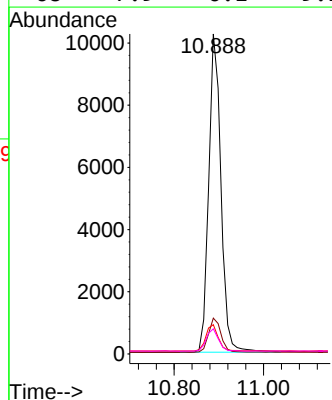
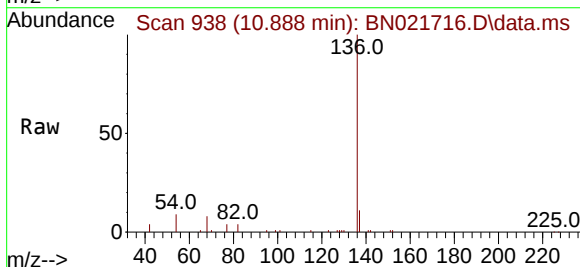




#8
 Nitrobenzene-d5
 Concen: 0.440 ng
 RT: 9.233 min Scan# 71
 Delta R.T. 0.000 min
 Lab File: BN021716.D
 Acq: 12 Sep 2022 11:23




Instrument :
 BNA_N
 ClientSampleId :
 PB147570BL


Tgt Ion: 82 Resp: 5769
 Ion Ratio Lower Upper
 82 100
 128 40.8 30.9 46.3
 54 49.6 42.7 64.1

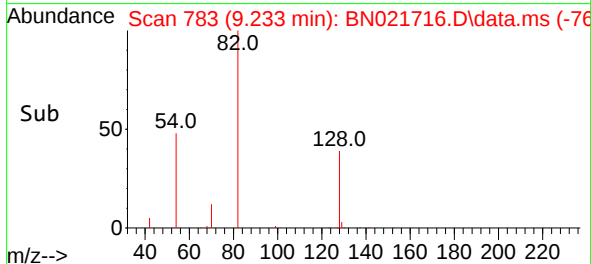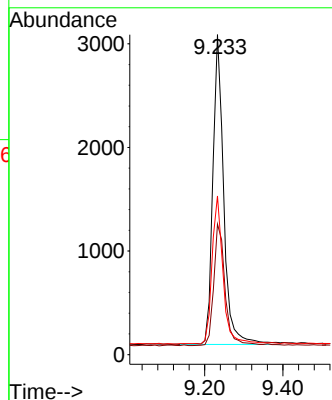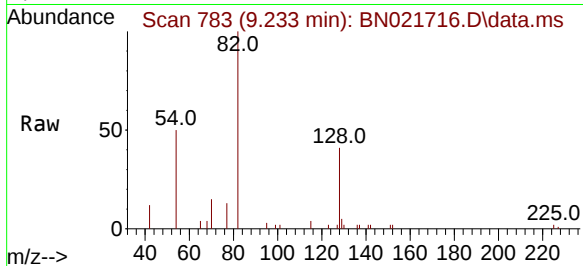

#11
 2-Methylnaphthalene-d10
 Concen: 0.441 ng
 RT: 12.478 min Scan# 1253
 Delta R.T. 0.004 min
 Lab File: BN021716.D
 Acq: 12 Sep 2022 11:23

Tgt Ion: 152 Resp: 19274
 Ion Ratio Lower Upper
 152 100
 151 20.2 14.5 21.7

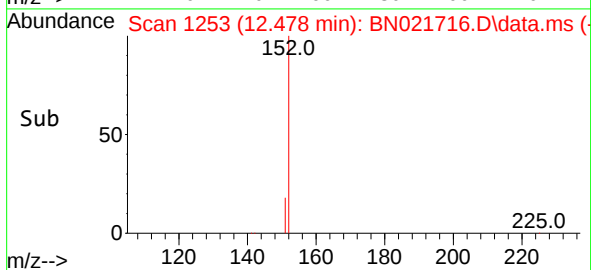
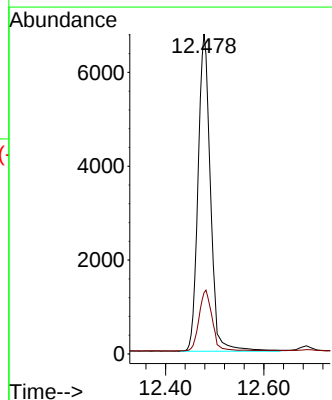
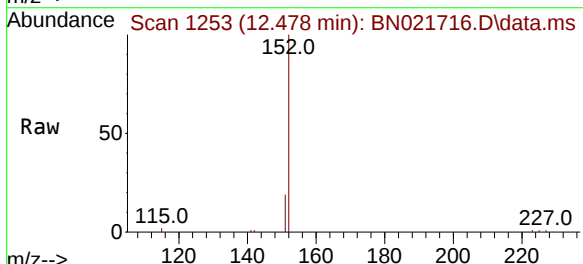


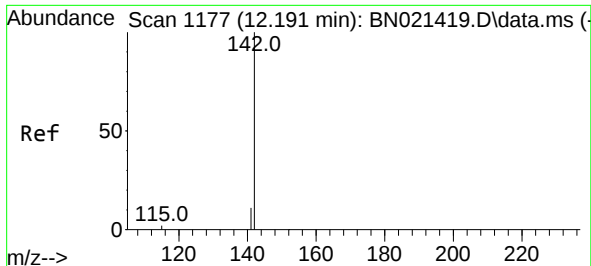

#12
2-Methylnaphthalene
Concen: 0.127 ng
RT: 12.180 min Scan# 1177
Delta R.T. 0.000 min
Lab File: BN021716.D
Acq: 12 Sep 2022 11:23




Instrument :
BNA_N
ClientSampleId :
PB147570BL


Tgt Ion:142 Resp: 1
Ion Ratio Lower Upper
142 100
141 110.0 12.2 18.2#
115 191.7 7.9 11.9#

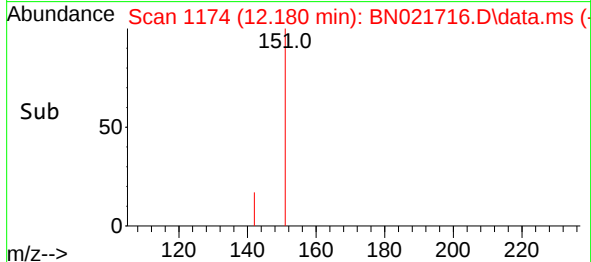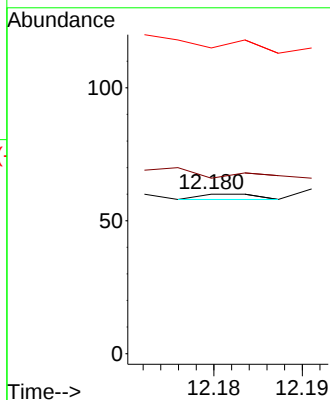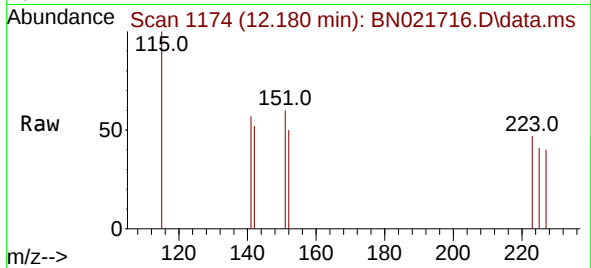

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.718 min Scan# 1467
Delta R.T. 0.011 min
Lab File: BN021716.D
Acq: 12 Sep 2022 11:23


Tgt Ion:164 Resp: 10489
Ion Ratio Lower Upper
164 100
162 103.0 82.2 123.4
160 48.5 39.5 59.3

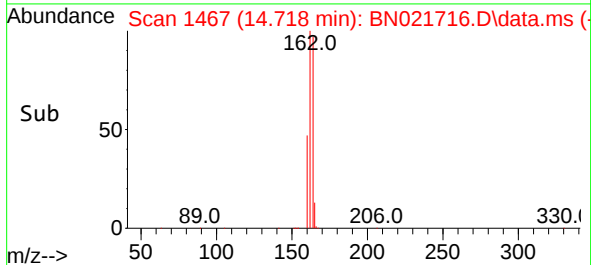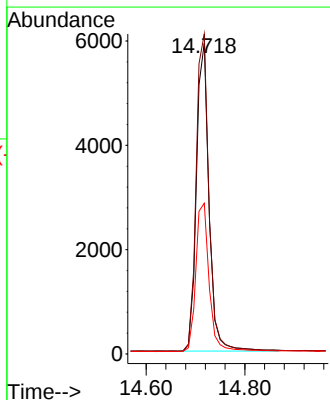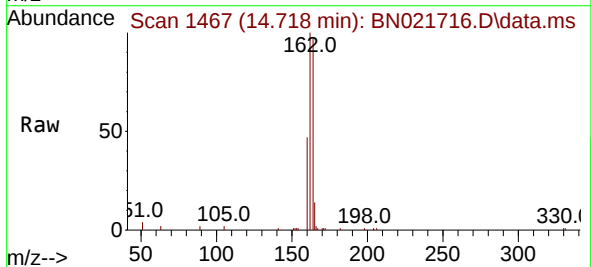



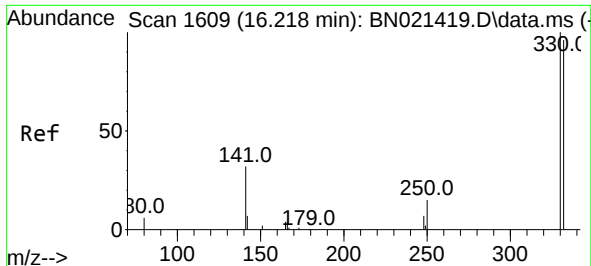


#14
 2,4,6-Tribromophenol
 Concen: 0.330 ng
 RT: 16.219 min Scan# 1
 Delta R.T. 0.010 min
 Lab File: BN021716.D
 Acq: 12 Sep 2022 11:23


Instrument :
 BNA_N
 ClientSampleId :
 PB147570BL

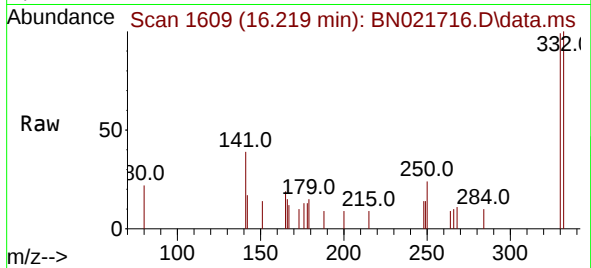



Tgt Ion:330 Resp: 1138
 Ion Ratio Lower Upper
 330 100
 332 96.2 79.3 118.9
 141 46.5 37.1 55.7

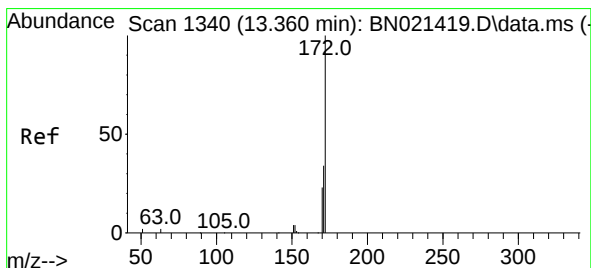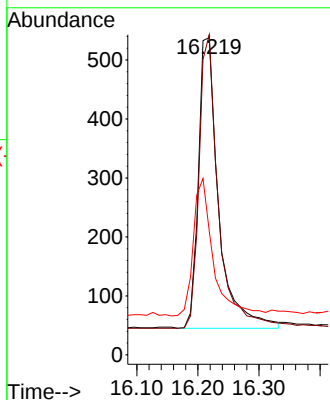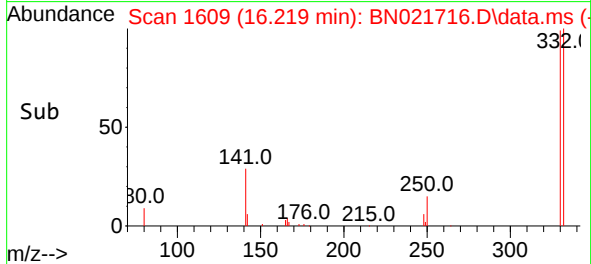


#15
 2-Fluorobiphenyl
 Concen: 0.356 ng
 RT: 13.339 min Scan# 1338
 Delta R.T. 0.000 min
 Lab File: BN021716.D
 Acq: 12 Sep 2022 11:23

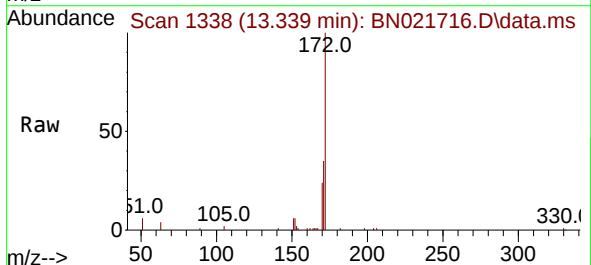

Tgt Ion:172 Resp: 16338
 Ion Ratio Lower Upper
 172 100
 171 34.6 27.8 41.6
 170 23.7 18.6 28.0

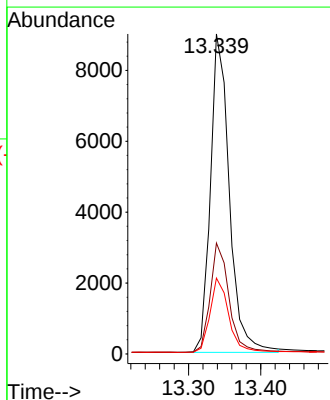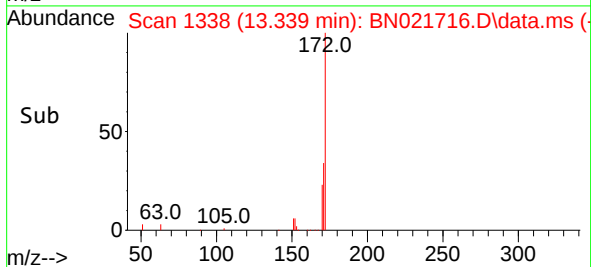

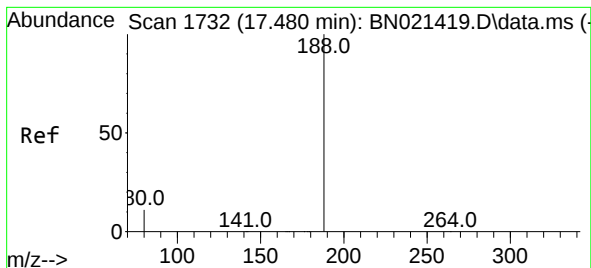

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.470 min Scan# 1731

Delta R.T. 0.010 min

Lab File: BN021716.D

Acq: 12 Sep 2022 11:23

Instrument :

BNA_N

ClientSampleId :

PB147570BL





Tgt Ion:188 Resp: 20375

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 10.9 9.5 14.3

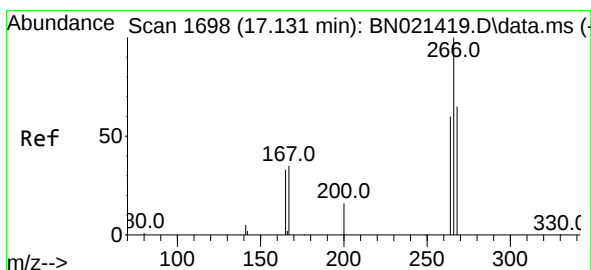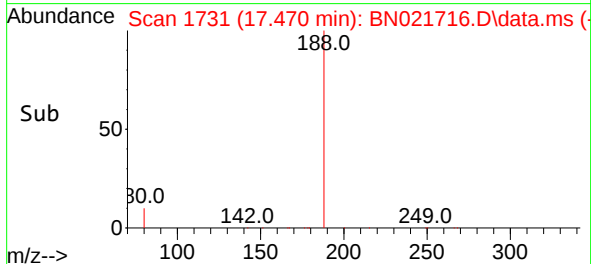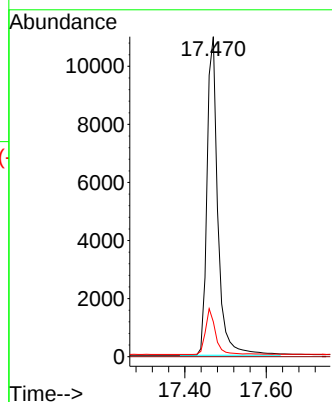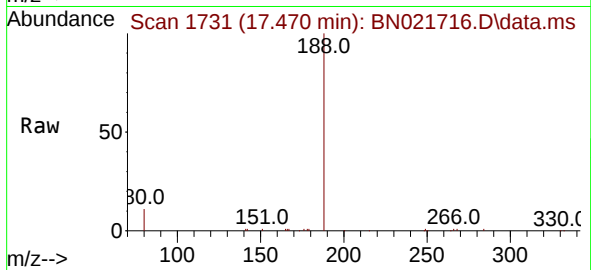

#24

Pentachlorophenol

Concen: 0.220 ng

RT: 17.131 min Scan# 1698

Delta R.T. 0.021 min

Lab File: BN021716.D

Acq: 12 Sep 2022 11:23




Tgt Ion:266 Resp: 82


Ion Ratio Lower Upper

266 100

264 58.5 49.0 73.6

268 61.0 50.9 76.3


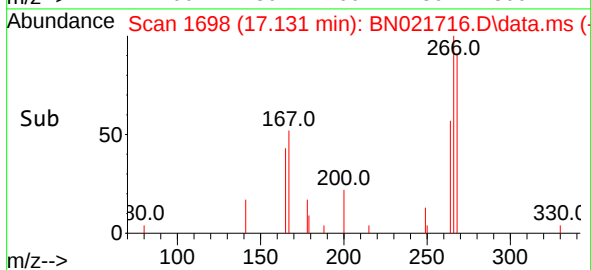
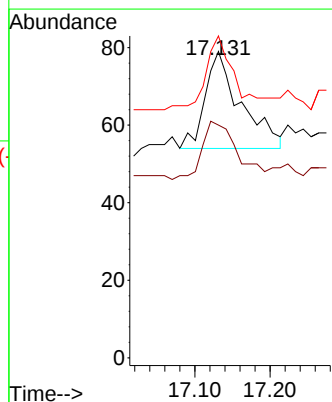
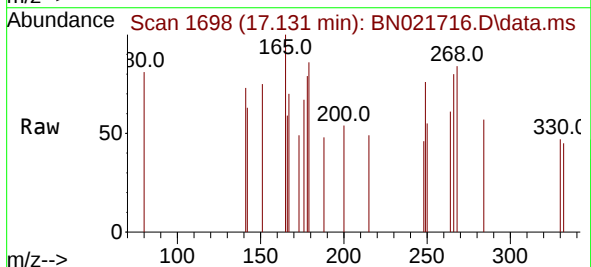


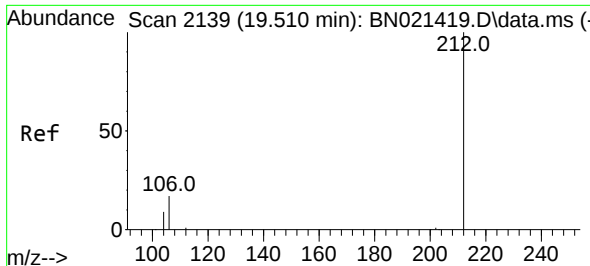

#27
Fluoranthene-d10
Concen: 0.381 ng
RT: 19.497 min Scan# 2136
Delta R.T. 0.004 min
Lab File: BN021716.D
Acq: 12 Sep 2022 11:23




Instrument :
BNA_N
ClientSampleId :
PB147570BL


Tgt Ion:212 Resp: 19954
Ion Ratio Lower Upper
212 100
106 17.9 14.2 21.2
104 9.9 7.8 11.6

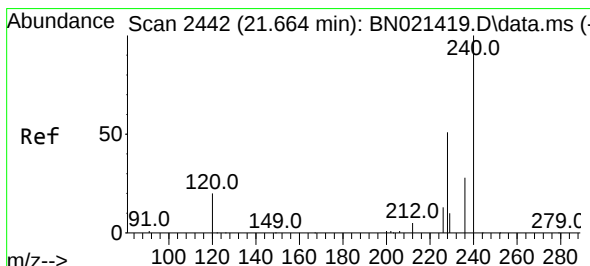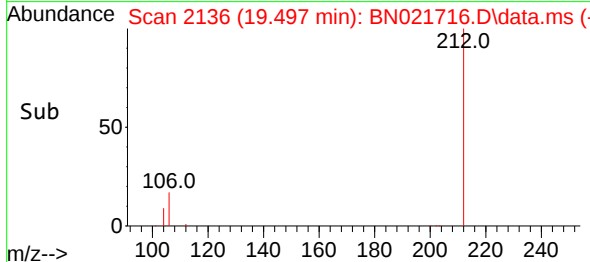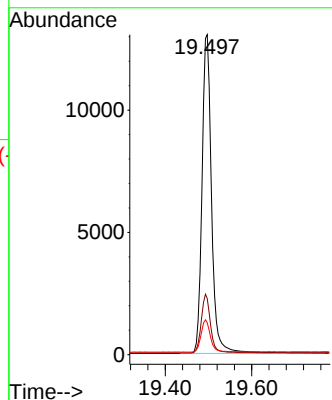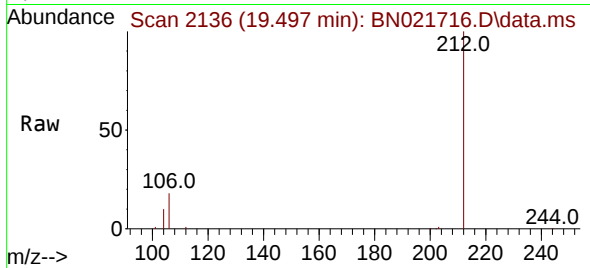

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.655 min Scan# 2441
Delta R.T. 0.000 min
Lab File: BN021716.D
Acq: 12 Sep 2022 11:23


Tgt Ion:240 Resp: 12947
Ion Ratio Lower Upper
240 100
120 16.2 10.2 15.4#
236 28.2 22.1 33.1

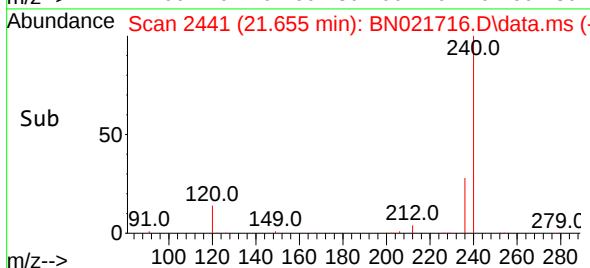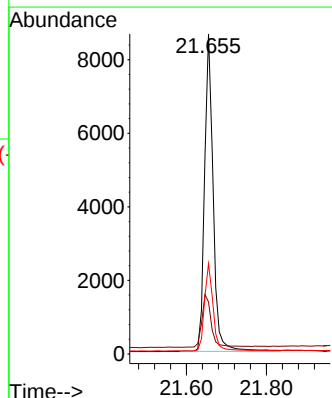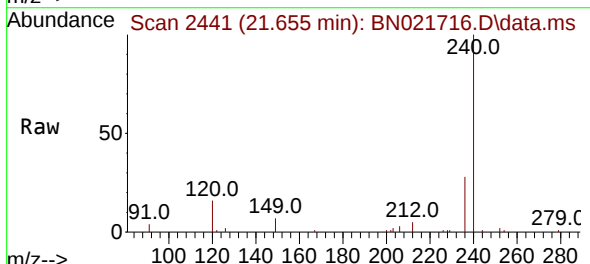



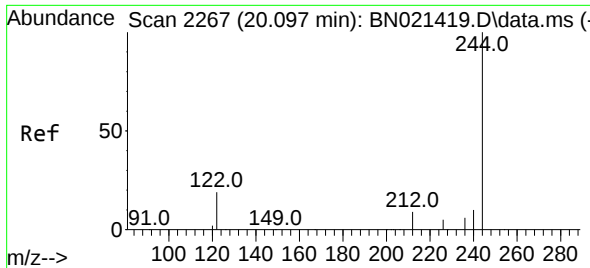


#31
 Terphenyl-d14
 Concen: 0.427 ng
 RT: 20.088 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BN021716.D
 Acq: 12 Sep 2022 11:23

Instrument :
 BNA_N
 ClientSampleId :
 PB147570BL

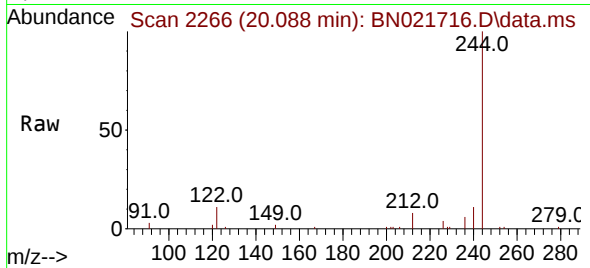

Tgt Ion:244 Resp: 12438
 Ion Ratio Lower Upper
 244 100
 212 7.7 6.5 9.7
 122 11.2 9.1 13.7

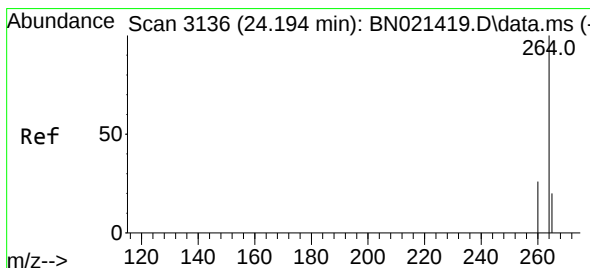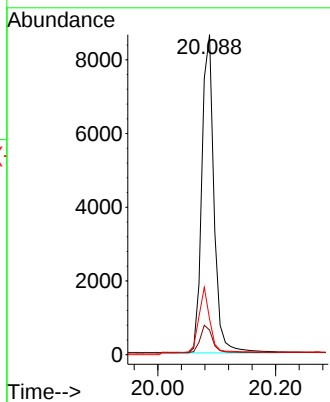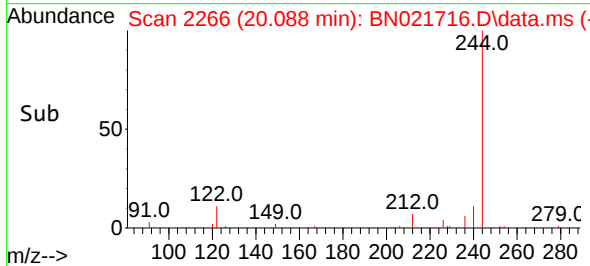

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.168 min Scan# 3127
 Delta R.T. 0.000 min
 Lab File: BN021716.D
 Acq: 12 Sep 2022 11:23

Tgt Ion:264 Resp: 10859
 Ion Ratio Lower Upper
 264 100
 260 26.0 21.0 31.6
 265 50.3 32.2 48.2#

