
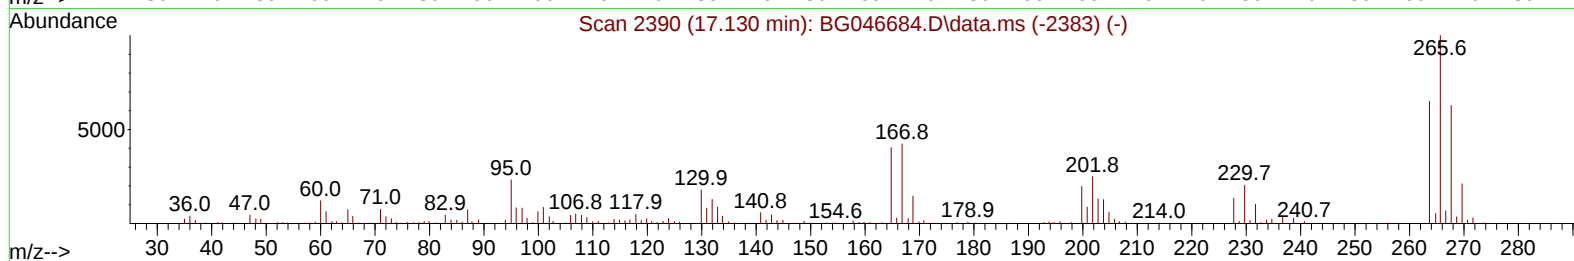
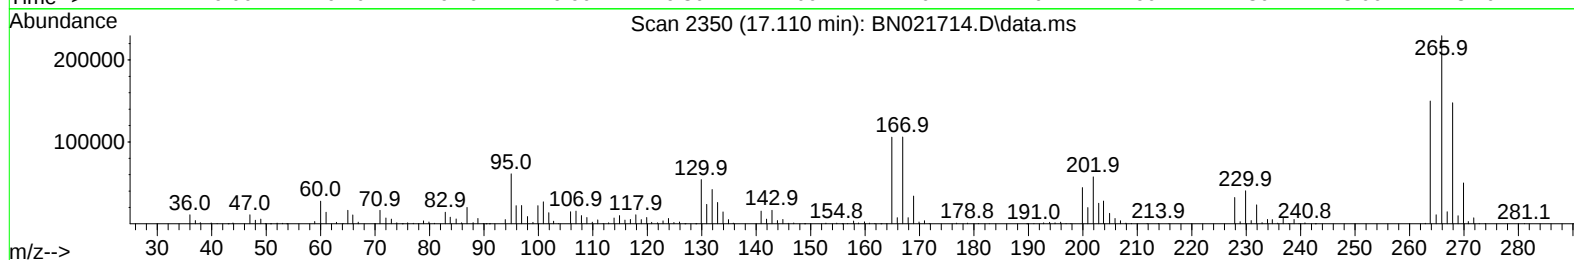


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091222\
 Data File : BN021714.D
 Acq On : 12 Sep 2022 10:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 13 05:51:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 13 05:51:30 2022
 Response via : Initial Calibration

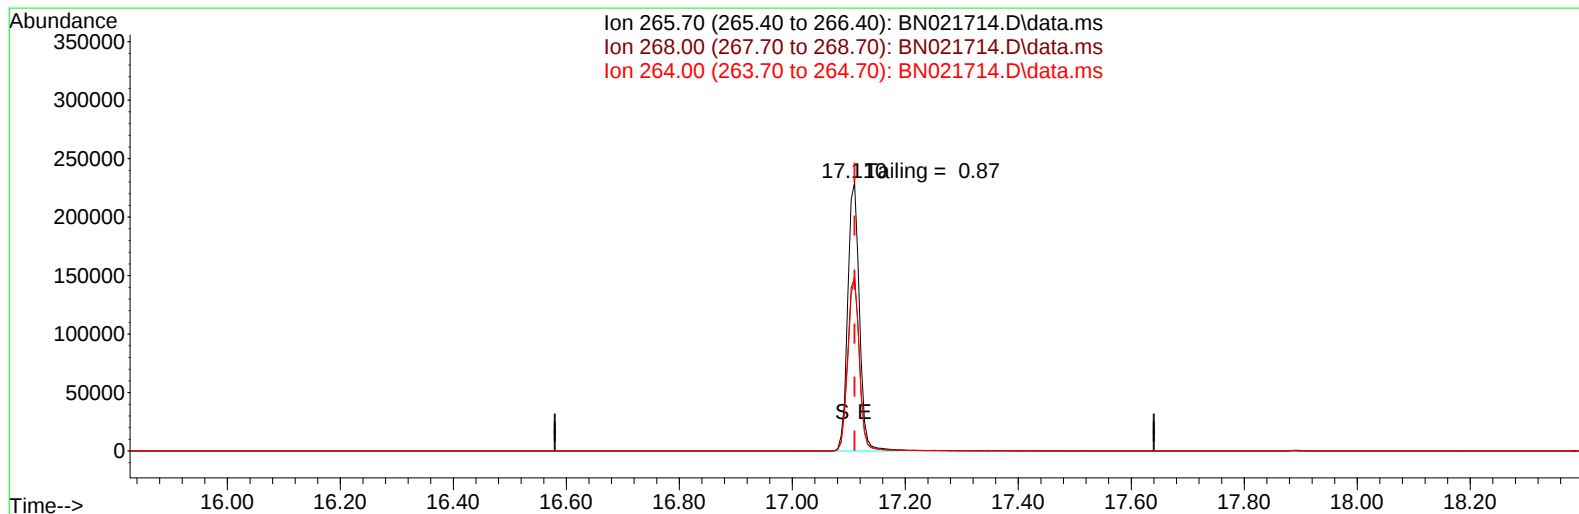

TIC: BN021714.D\data.ms

(70) Pentachlorophenol (C)




17.110min (0.000) 19427.55 ng

response 331606

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.39
264.00	61.60	65.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091222\
Data File : BN021714.D
Acq On : 12 Sep 2022 10:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 13 05:51:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 13 05:51:30 2022
Response via : Initial Calibration

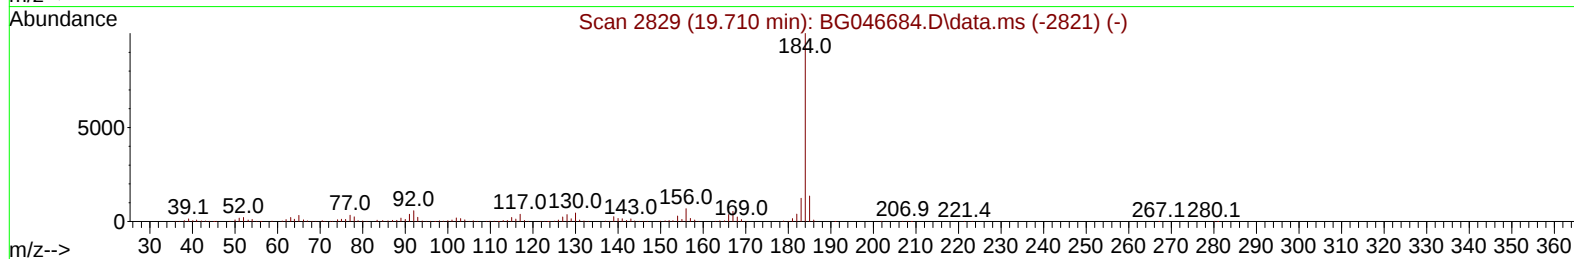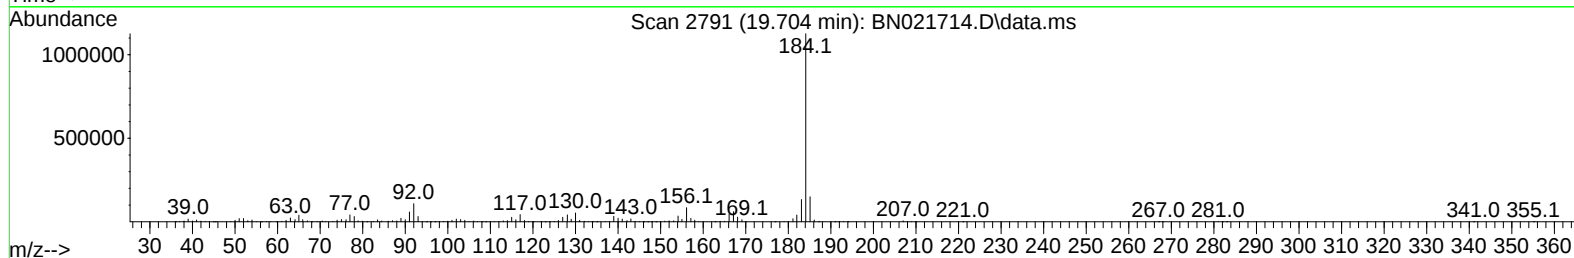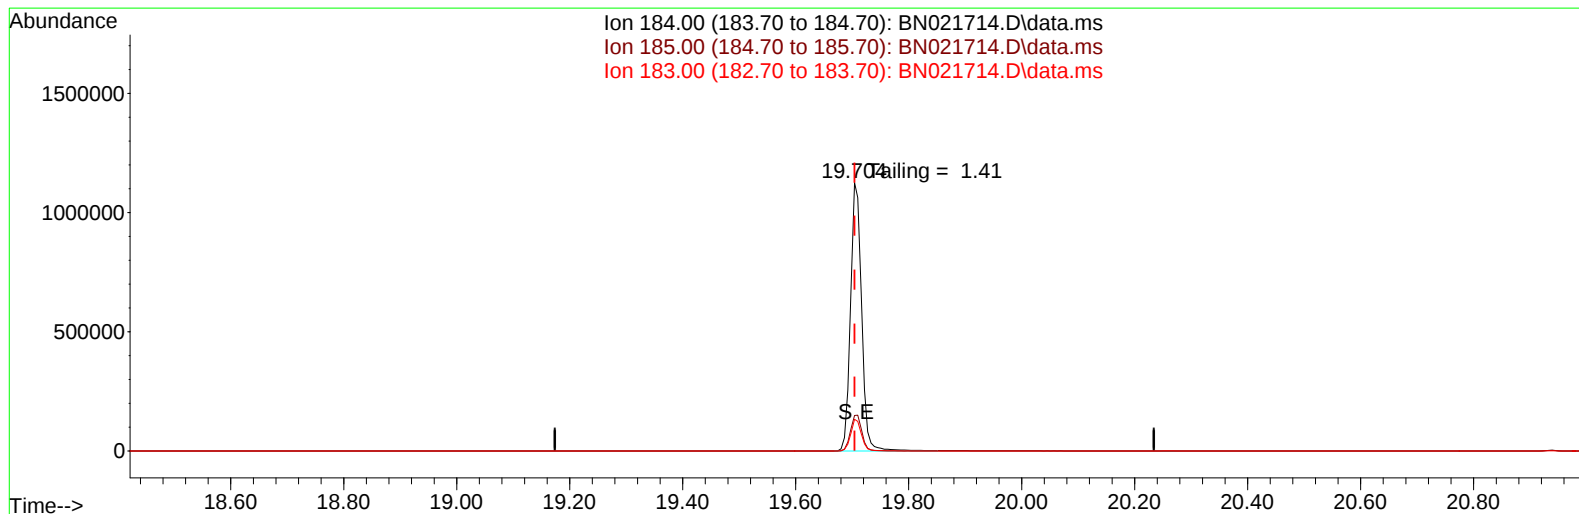

TIC: BN021714.D\data.ms

(77) Benzidine

19.704min (0.000) 0.00 ng

response 1548956

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.27
183.00	13.20	11.83
0.00	0.00	0.00