


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091222\
 Data File : BN021714.D
 Acq On : 12 Sep 2022 10:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 13 02:32:27 2022

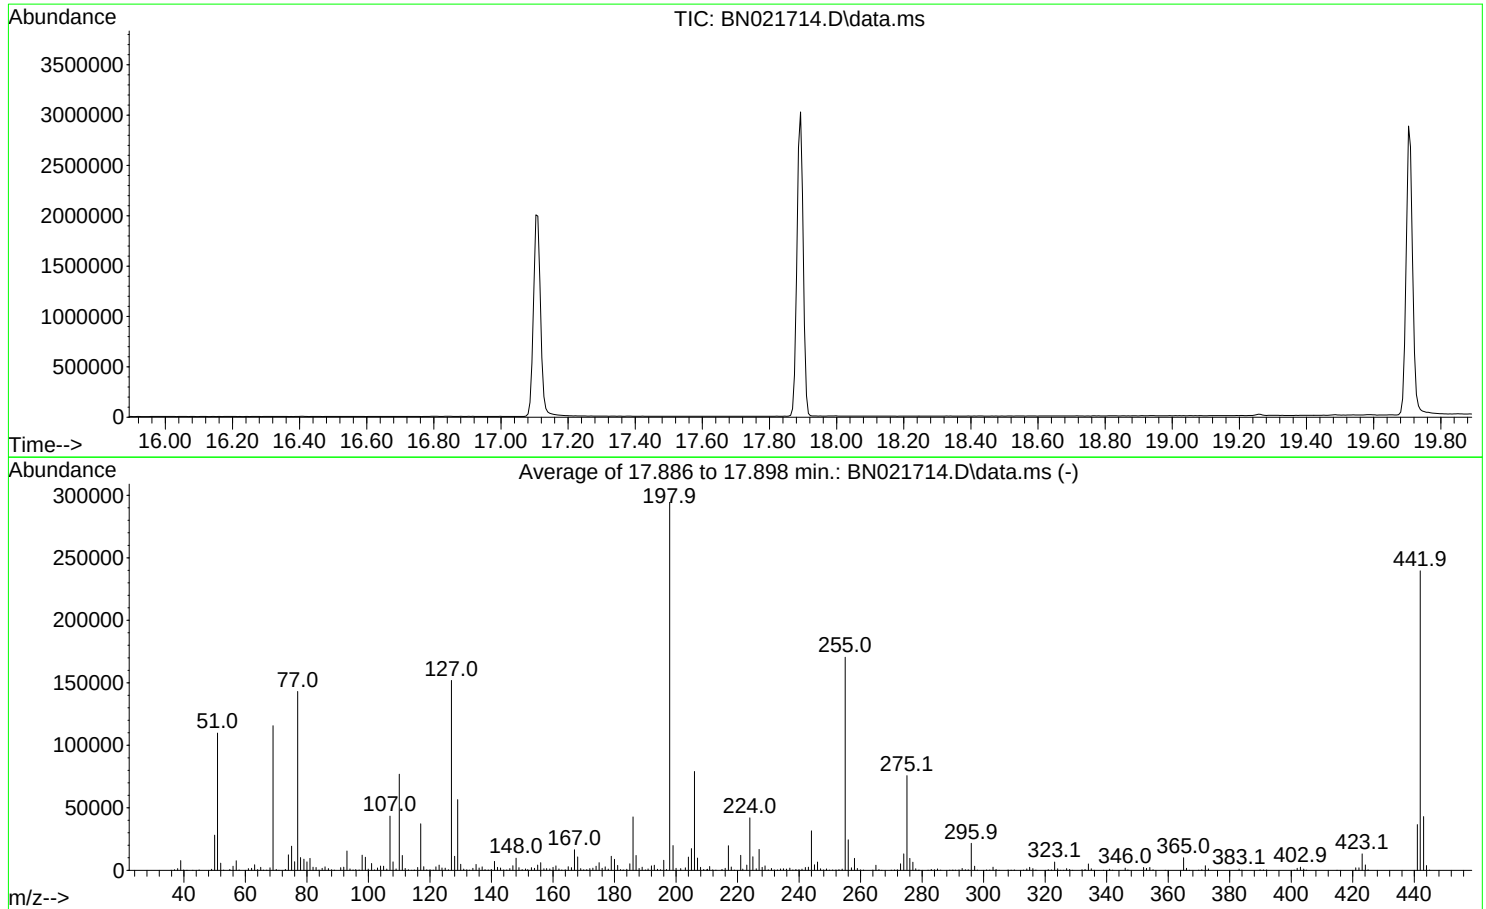




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	109808	PASS
68	69	0.00	2	1.8	2041	PASS
69	198	0.00	100	39.3	115728	PASS
70	69	0.00	2	0.6	692	PASS
127	198	10	80	51.6	151840	PASS
197	198	0.00	2	0.2	603	PASS
198	198	100	100	100.0	294336	PASS
199	198	5	9	6.7	19853	PASS
275	198	10	60	25.7	75709	PASS
365	198	1	100	3.4	10101	PASS
441	198	0.01	100	12.4	36507	PASS
442	442	50	100	100.0	239595	PASS
443	442	15	24	18.0	43016	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091222\
 Data File : BN021714.D
 Acq On : 12 Sep 2022 10:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 13 05:51:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 13 05:51:30 2022
 Response via : Initial Calibration

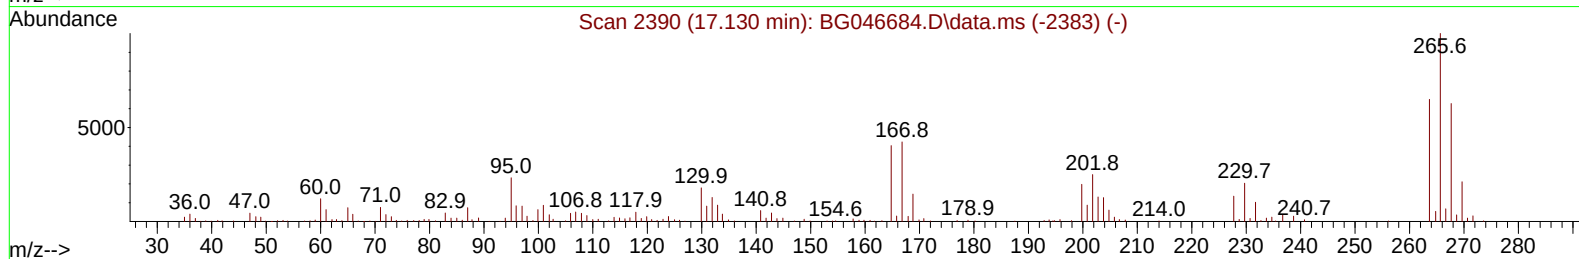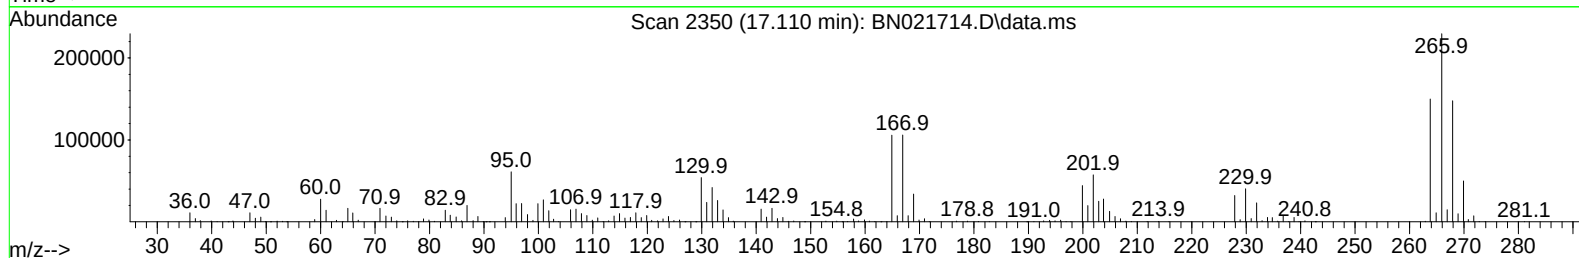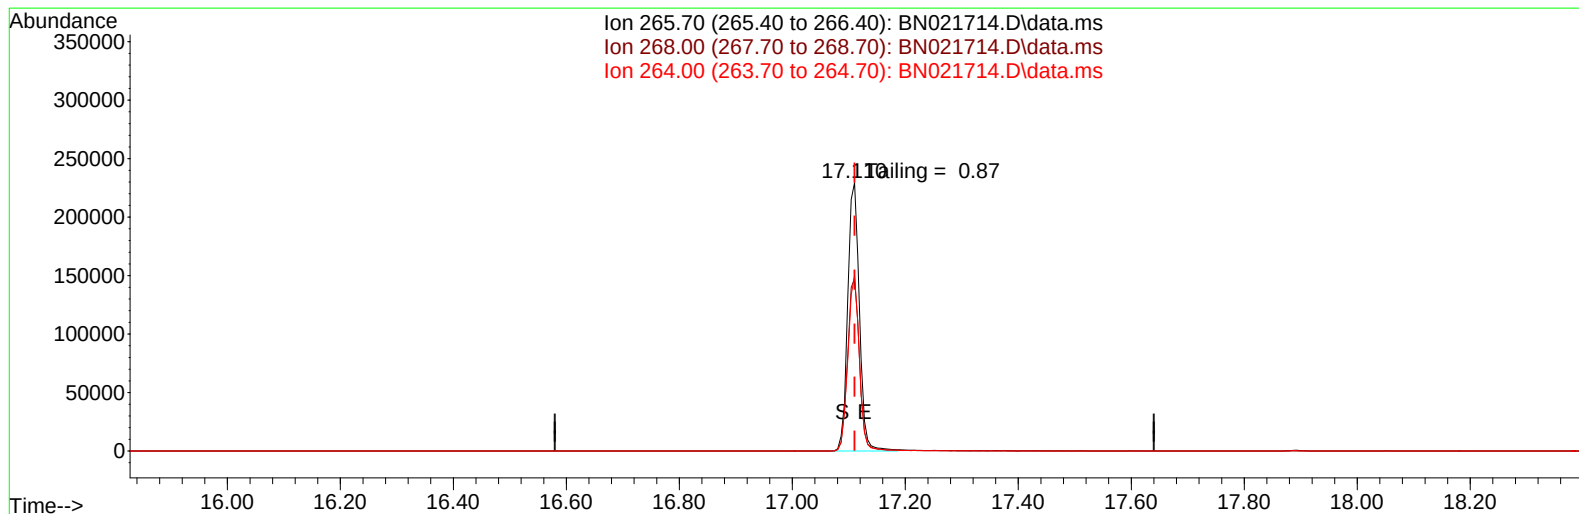

TIC: BN021714.D\data.ms

(70) Pentachlorophenol (C)

17.110min (0.000) 19427.55 ng




response 331606

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.39
264.00	61.60	65.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091222\
Data File : BN021714.D
Acq On : 12 Sep 2022 10:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 13 05:51:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 13 05:51:30 2022
Response via : Initial Calibration

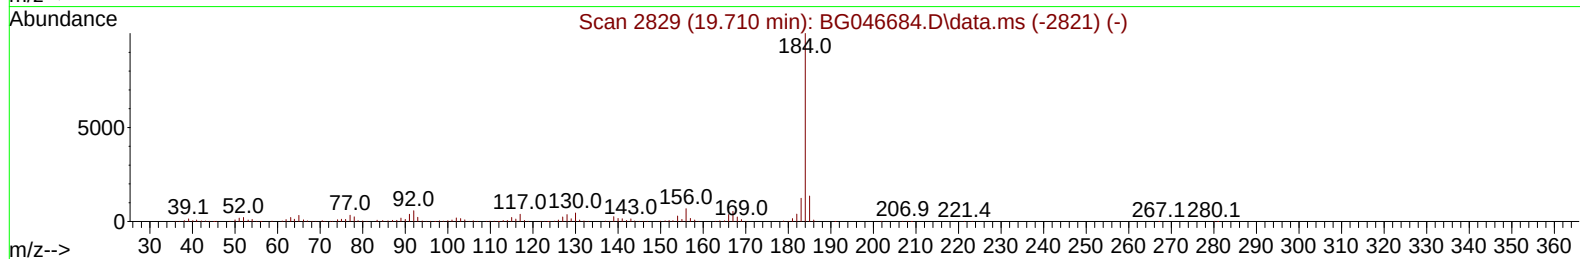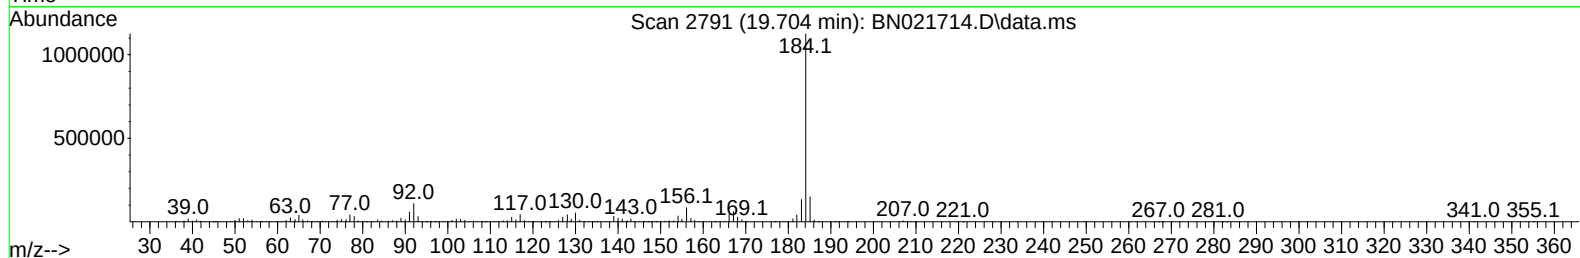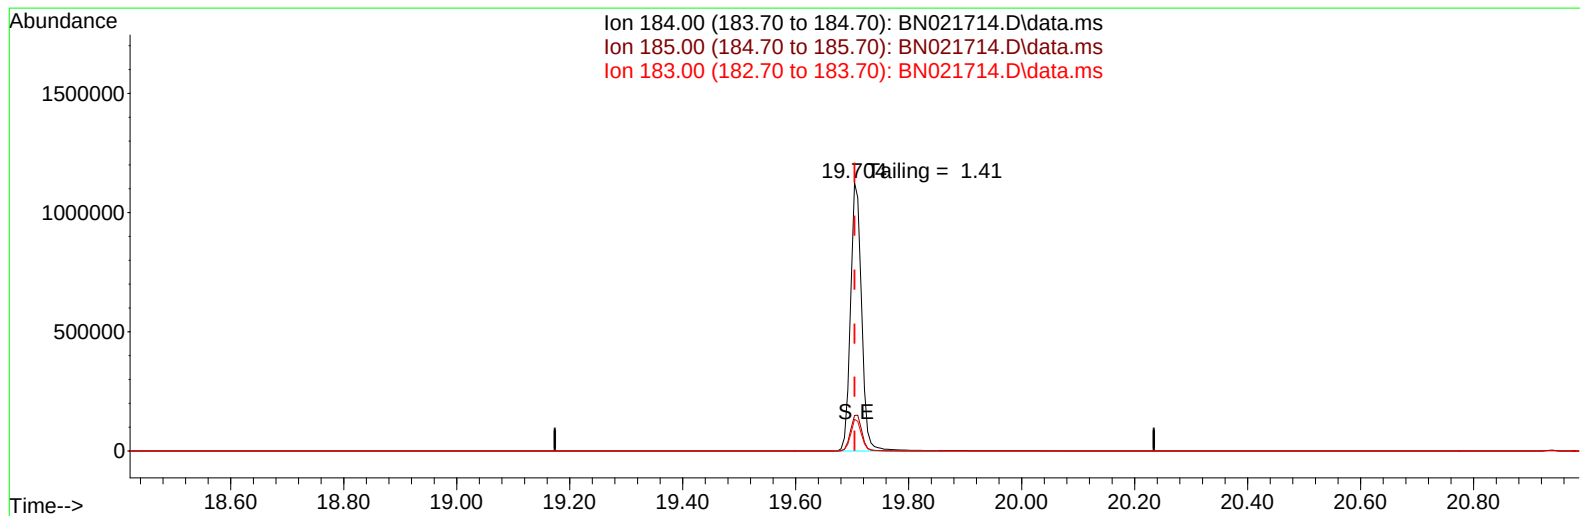

TIC: BN021714.D\data.ms

(77) Benzidine

19.704min (0.000) 0.00 ng

response 1548956

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.27
183.00	13.20	11.83
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/12/2022	BNA_N	<u>BN021714.D</u>
Compound Name	Response	Retention Time
DDT	875464	20.939
DDD	63379	20.498
DDE	4742	19.986
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
68121	943585	7.22

Instrument :
BNA_N
ClientSampleId :
DFTPP