


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091322\
 Data File : BN021723.D
 Acq On : 13 Sep 2022 11:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 13 02:32:27 2022

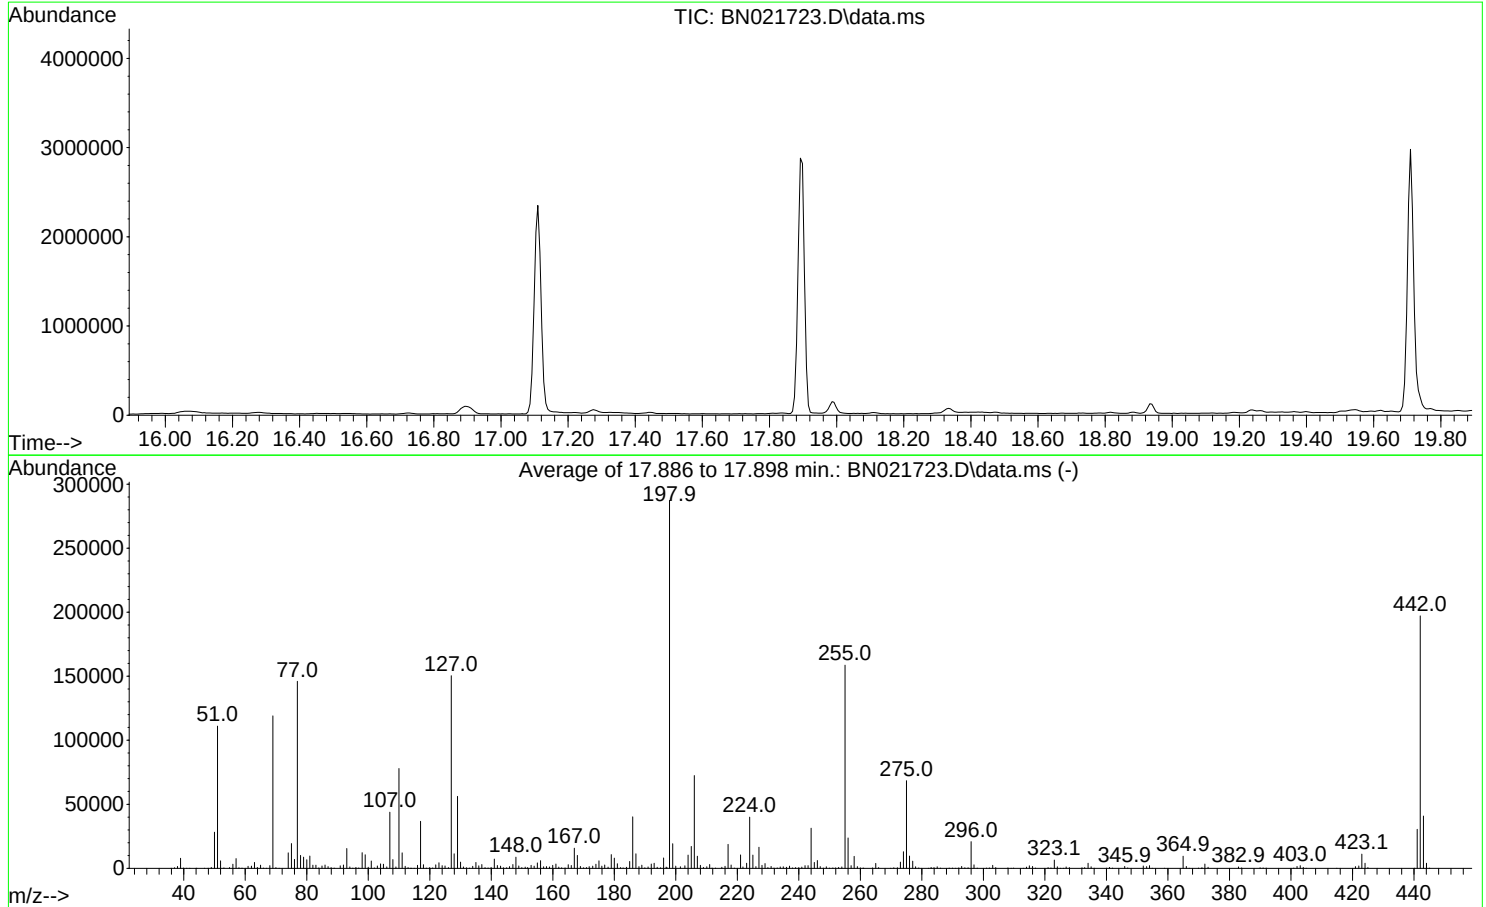




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	111109	PASS
68	69	0.00	2	1.7	2074	PASS
69	198	0.00	100	41.4	119044	PASS
70	69	0.00	2	0.5	554	PASS
127	198	10	80	52.4	150445	PASS
197	198	0.00	2	0.3	992	PASS
198	198	100	100	100.0	287360	PASS
199	198	5	9	6.7	19222	PASS
275	198	10	60	23.8	68419	PASS
365	198	1	100	3.3	9488	PASS
441	198	0.01	100	10.6	30439	PASS
442	442	50	100	100.0	197125	PASS
443	442	15	24	20.7	40763	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091322\
 Data File : BN021723.D
 Acq On : 13 Sep 2022 11:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 14 05:40:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 14 05:40:03 2022
 Response via : Initial Calibration

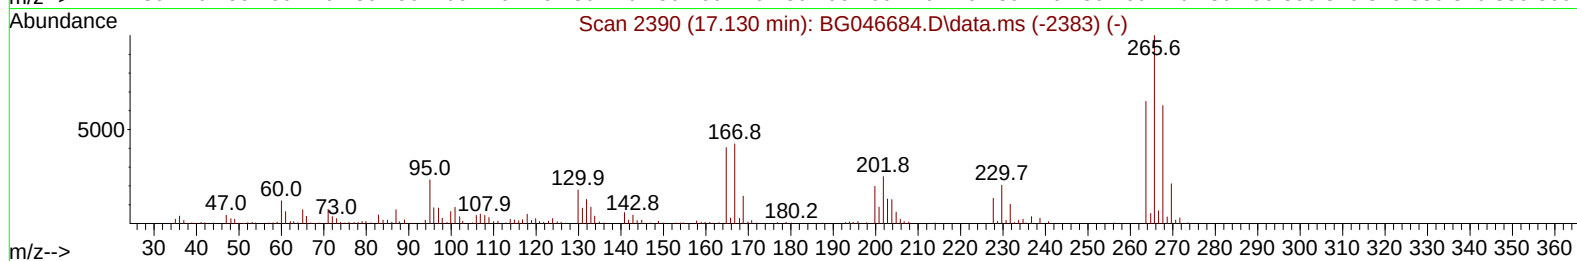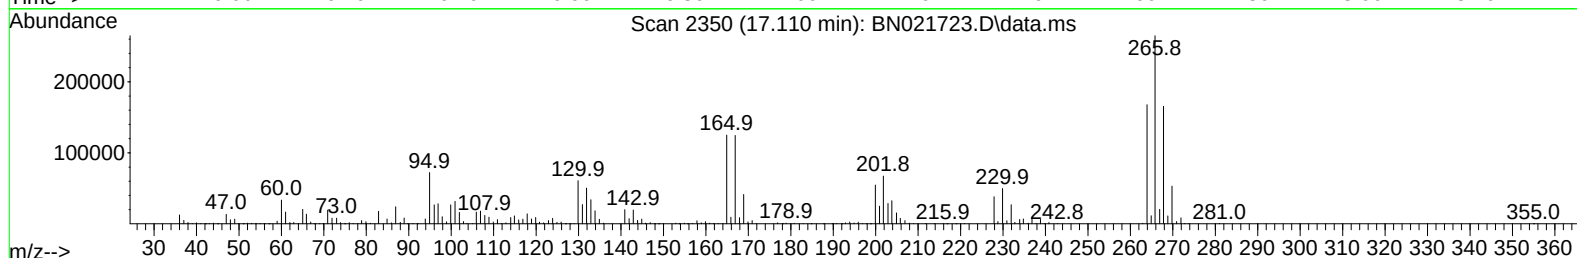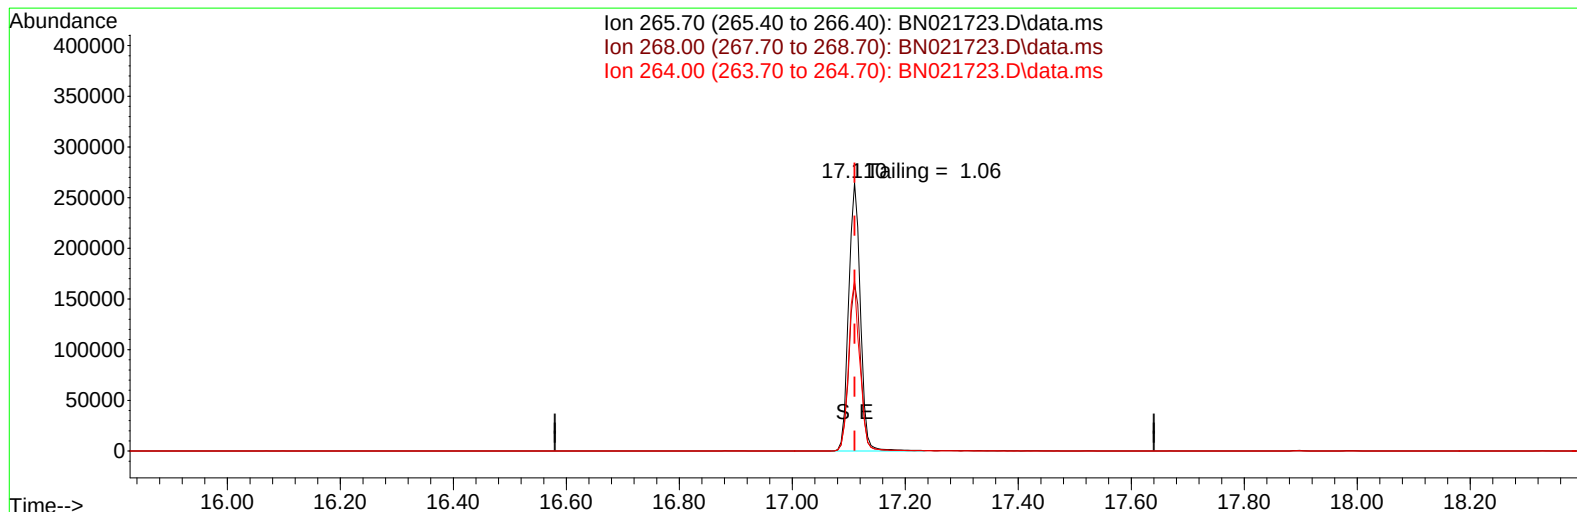

TIC: BN021723.D\data.ms

(70) Pentachlorophenol (C)

17.110min (0.000) 24126.24 ng




response 382460

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.52
264.00	61.60	63.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091322\
Data File : BN021723.D
Acq On : 13 Sep 2022 11:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 14 05:40:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 14 05:40:03 2022
Response via : Initial Calibration

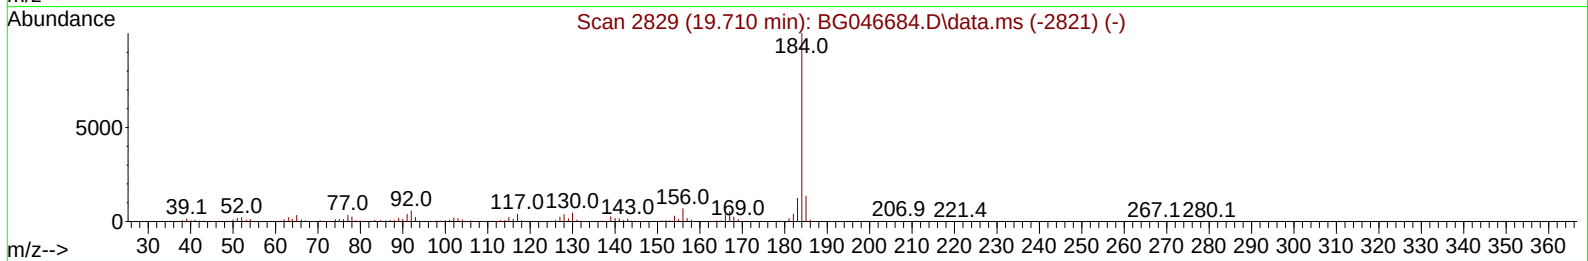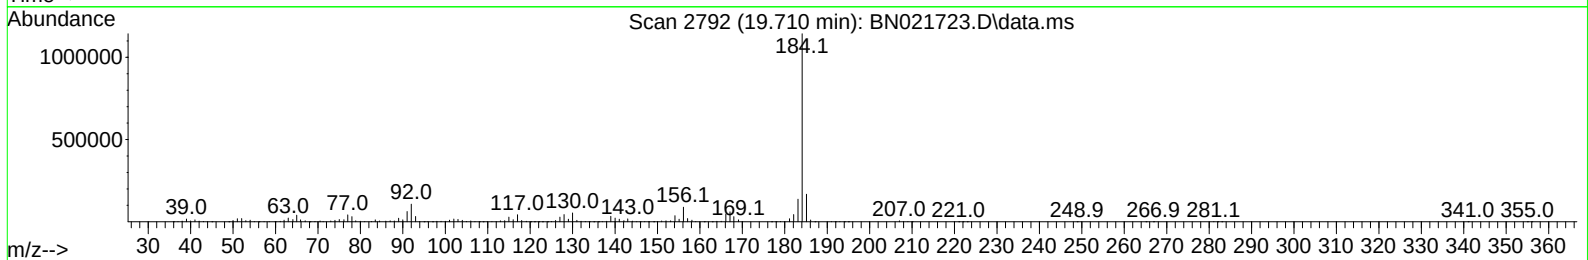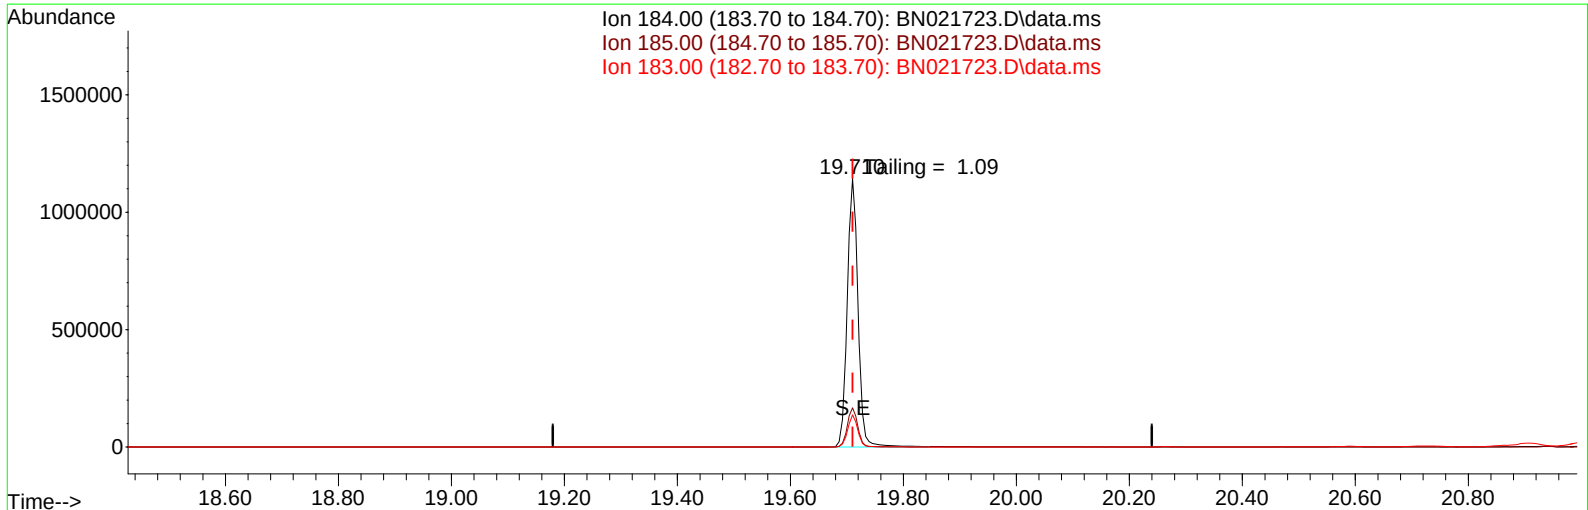

TIC: BN021723.D\data.ms

(77) Benzidine

19.710min (0.000) 44486.12 ng

response 1516659

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.62
183.00	13.20	12.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/13/2022	BNA_N	<u>BN021723.D</u>
Compound Name	Response	Retention Time
DDT	942251	20.939
DDD	70823	20.504
DDE	6856	19.992
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
77679	1019930	7.62

Instrument :
BNA_N
ClientSampleId :
DFTPP