

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091324\
 Data File : BN033900.D
 Acq On : 13 Sep 2024 17:06
 Operator : JU/RC
 Sample : P3898-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DDC15

Quant Time: Sep 13 17:59:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 11 01:58:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.493	152	174917	20.000	ng/u1	0.00
20) Naphthalene-d8	10.251	136	689748	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.134	164	398763	20.000	ng/u1	0.00
64) Phenanthrene-d10	16.892	188	809623	20.000	ng/u1	0.00
79) Chrysene-d12	21.127	240	863696	20.000	ng/u1	0.00
88) Perylene-d12	23.898	264	1059012	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.111	96	13042	3.043	ng/uL	0.00
4) Pyridine-d5	3.499	84	159375	12.509	ng/u1	0.00
7) Phenol-d5	6.681	99	218695	14.088	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	6.840	67	136990	14.223	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.028	132	178586	14.615	ng/u1	-0.01
15) 4-Methylphenol-d8	8.199	113	170752	13.368	ng/u1	-0.01
21) Nitrobenzene-d5	8.634	128	80476	14.638	ng/u1	0.00
24) 2-Nitrophenol-d4	9.346	143	79418	14.048	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	9.881	165	149178	14.011	ng/u1	0.00
31) 4-Chloroaniline-d4	10.393	131	220411	13.674	ng/u1	0.00
46) Dimethylphthalate-d6	13.557	166	461899	15.499	ng/u1	0.00
49) Acenaphthylene-d8	13.822	160	512623	15.291	ng/u1	0.00
54) 4-Nitrophenol-d4	14.357	143	65313	10.679	ng/u1	0.00
60) Fluorene-d10	15.134	176	389881	15.437	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.263	200	40652	8.421	ng/u1	0.00
73) Anthracene-d10	16.986	188	613802	16.126	ng/u1	0.00
81) Pyrene-d10	19.298	212	739852	15.374	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.710	264	876846	16.119	ng/u1	-0.01
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.545	266	12185	1.917	ng/u1	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091324\
Data File : BN033900.D
Acq On : 13 Sep 2024 17:06
Operator : JU/RC
Sample : P3898-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DDC15

Quant Time: Sep 13 17:59:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 11 01:58:59 2024
Response via : Initial Calibration

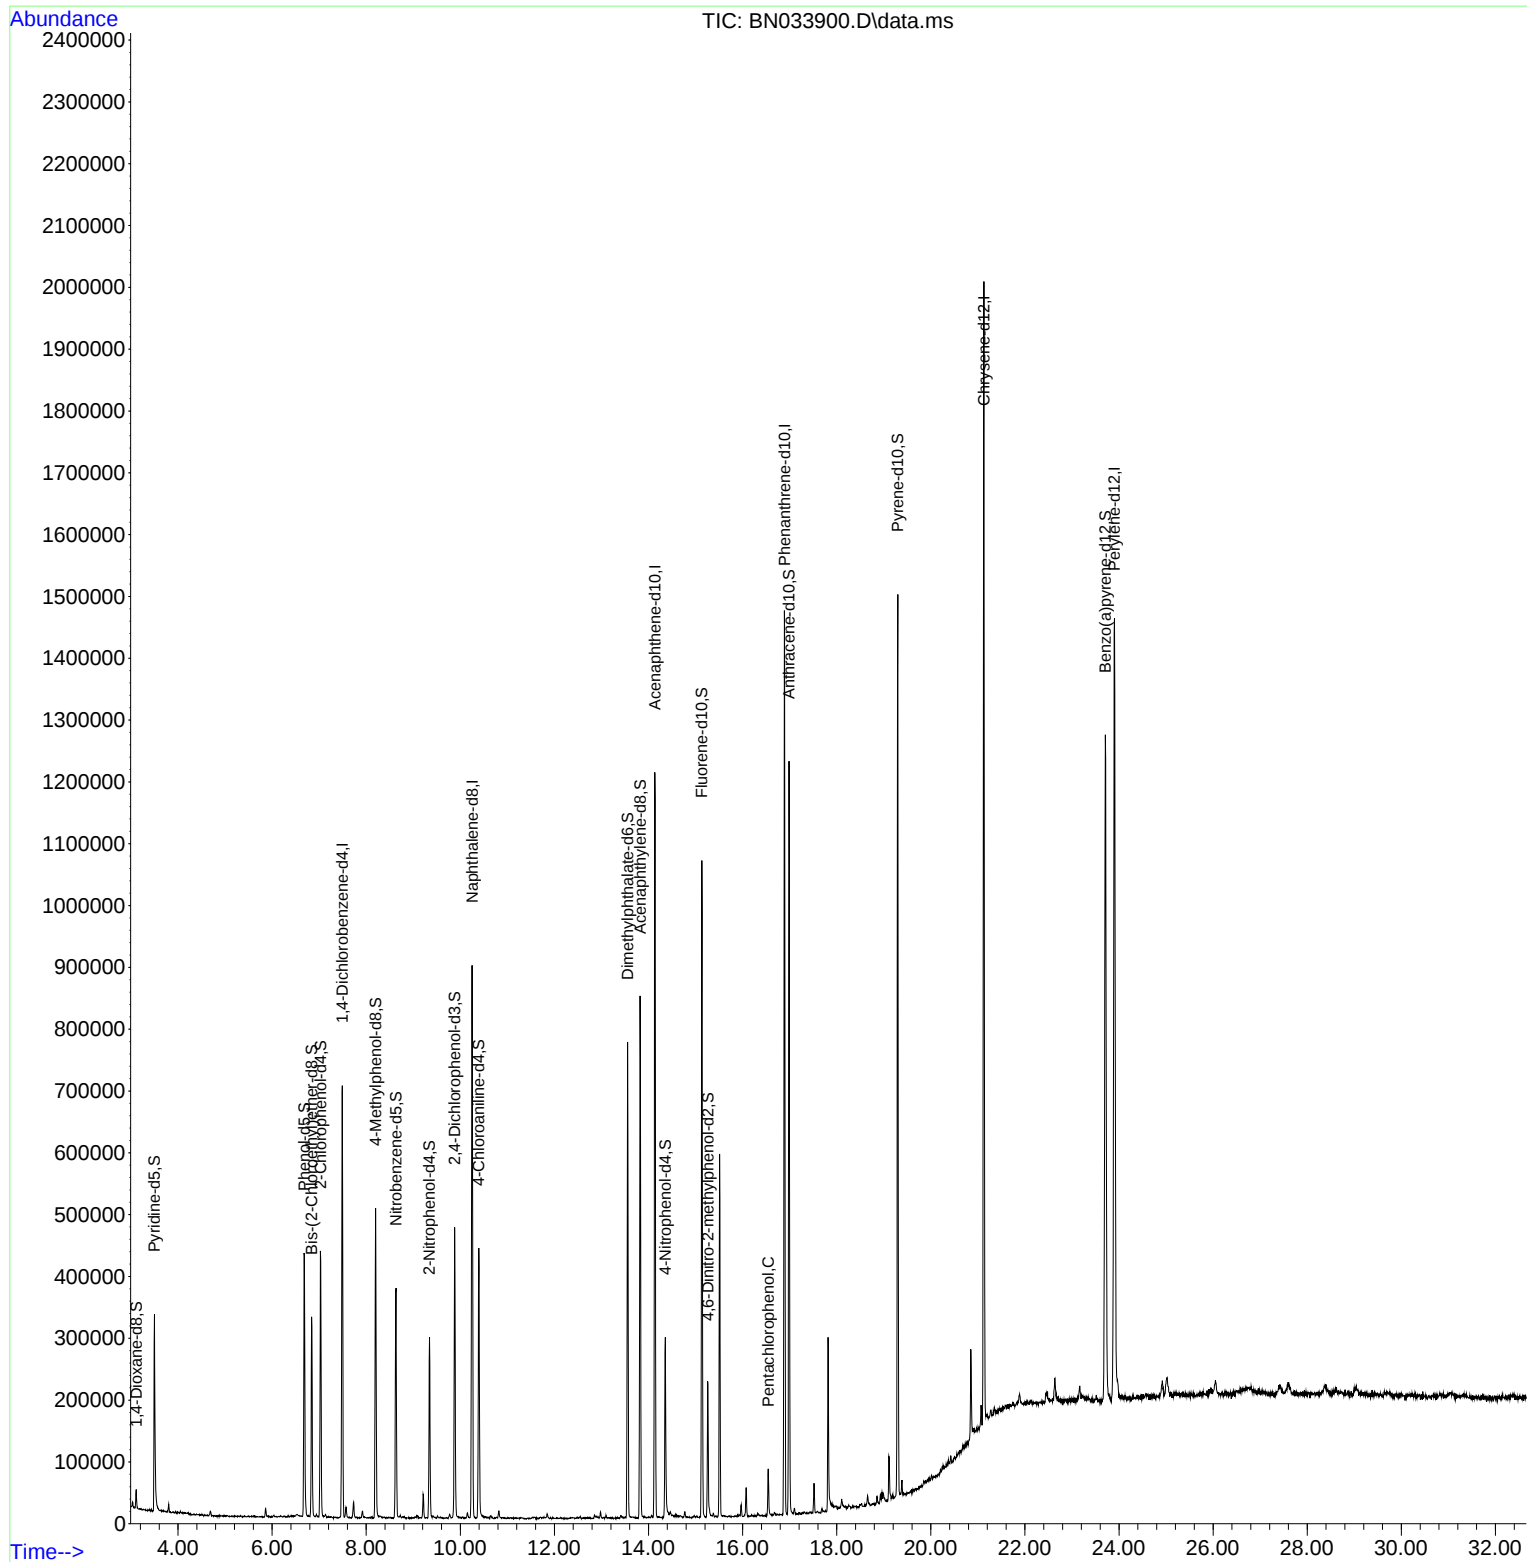

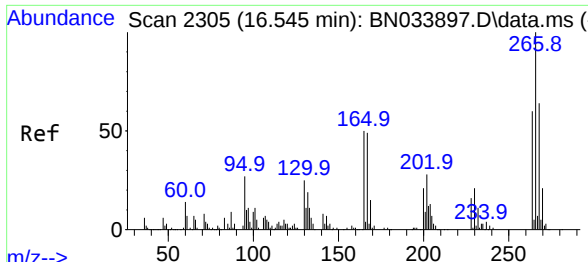

#71
Pentachlorophenol
Concen: 1.917 ng/ul
RT: 16.545 min Scan# 21
Delta R.T. -0.006 min
Lab File: BN033900.D
Acq: 13 Sep 2024 17:06

Instrument :
BNA_N
ClientSampleId :
DDC15

Tgt Ion:	266	Resp:	12185
Ion	Ratio	Lower	Upper
266	100		
264	59.0	51.1	76.7
268	58.9	52.8	79.2

