

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091324\
 Data File : BN033904.D
 Acq On : 13 Sep 2024 19:43
 Operator : JU/RC
 Sample : P3898-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DDC62

Quant Time: Sep 13 23:52:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 11 01:58:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.493	152	165089	20.000	ng/u1	0.00
20) Naphthalene-d8	10.251	136	652275	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.134	164	402096	20.000	ng/u1	0.00
64) Phenanthrene-d10	16.892	188	847970	20.000	ng/u1	0.00
79) Chrysene-d12	21.121	240	932644	20.000	ng/u1	0.00
88) Perylene-d12	23.904	264	1061916	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.111	96	12596	3.113	ng/uL	0.00
4) Pyridine-d5	3.499	84	149060	12.396	ng/u1	0.00
7) Phenol-d5	6.681	99	232654	15.879	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	6.840	67	144970	15.947	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.028	132	189396	16.422	ng/u1	-0.01
15) 4-Methylphenol-d8	8.199	113	192617	15.977	ng/u1	-0.01
21) Nitrobenzene-d5	8.628	128	88871	17.094	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.346	143	90943	17.011	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	9.881	165	168549	16.740	ng/u1	0.00
31) 4-Chloroaniline-d4	10.393	131	247849	16.260	ng/u1	0.00
46) Dimethylphthalate-d6	13.557	166	568956	18.934	ng/u1	0.00
49) Acenaphthylene-d8	13.822	160	632055	18.697	ng/u1	0.00
54) 4-Nitrophenol-d4	14.357	143	83066	13.469	ng/u1	0.00
60) Fluorene-d10	15.134	176	490339	19.254	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.263	200	58289	11.529	ng/u1	0.00
73) Anthracene-d10	16.986	188	824844	20.690	ng/u1	0.00
81) Pyrene-d10	19.292	212	1003134	19.304	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.710	264	1141686	20.930	ng/u1	-0.01
Target Compounds						
					Qvalue	
58) 2,3,4,6-Tetrachlorophenol	14.769	232	67255	9.588	ng/u1	98
71) Pentachlorophenol	16.551	266	840225	126.227	ng/u1	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091324\
Data File : BN033904.D
Acq On : 13 Sep 2024 19:43
Operator : JU/RC
Sample : P3898-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DDC62

Quant Time: Sep 13 23:52:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 11 01:58:59 2024
Response via : Initial Calibration

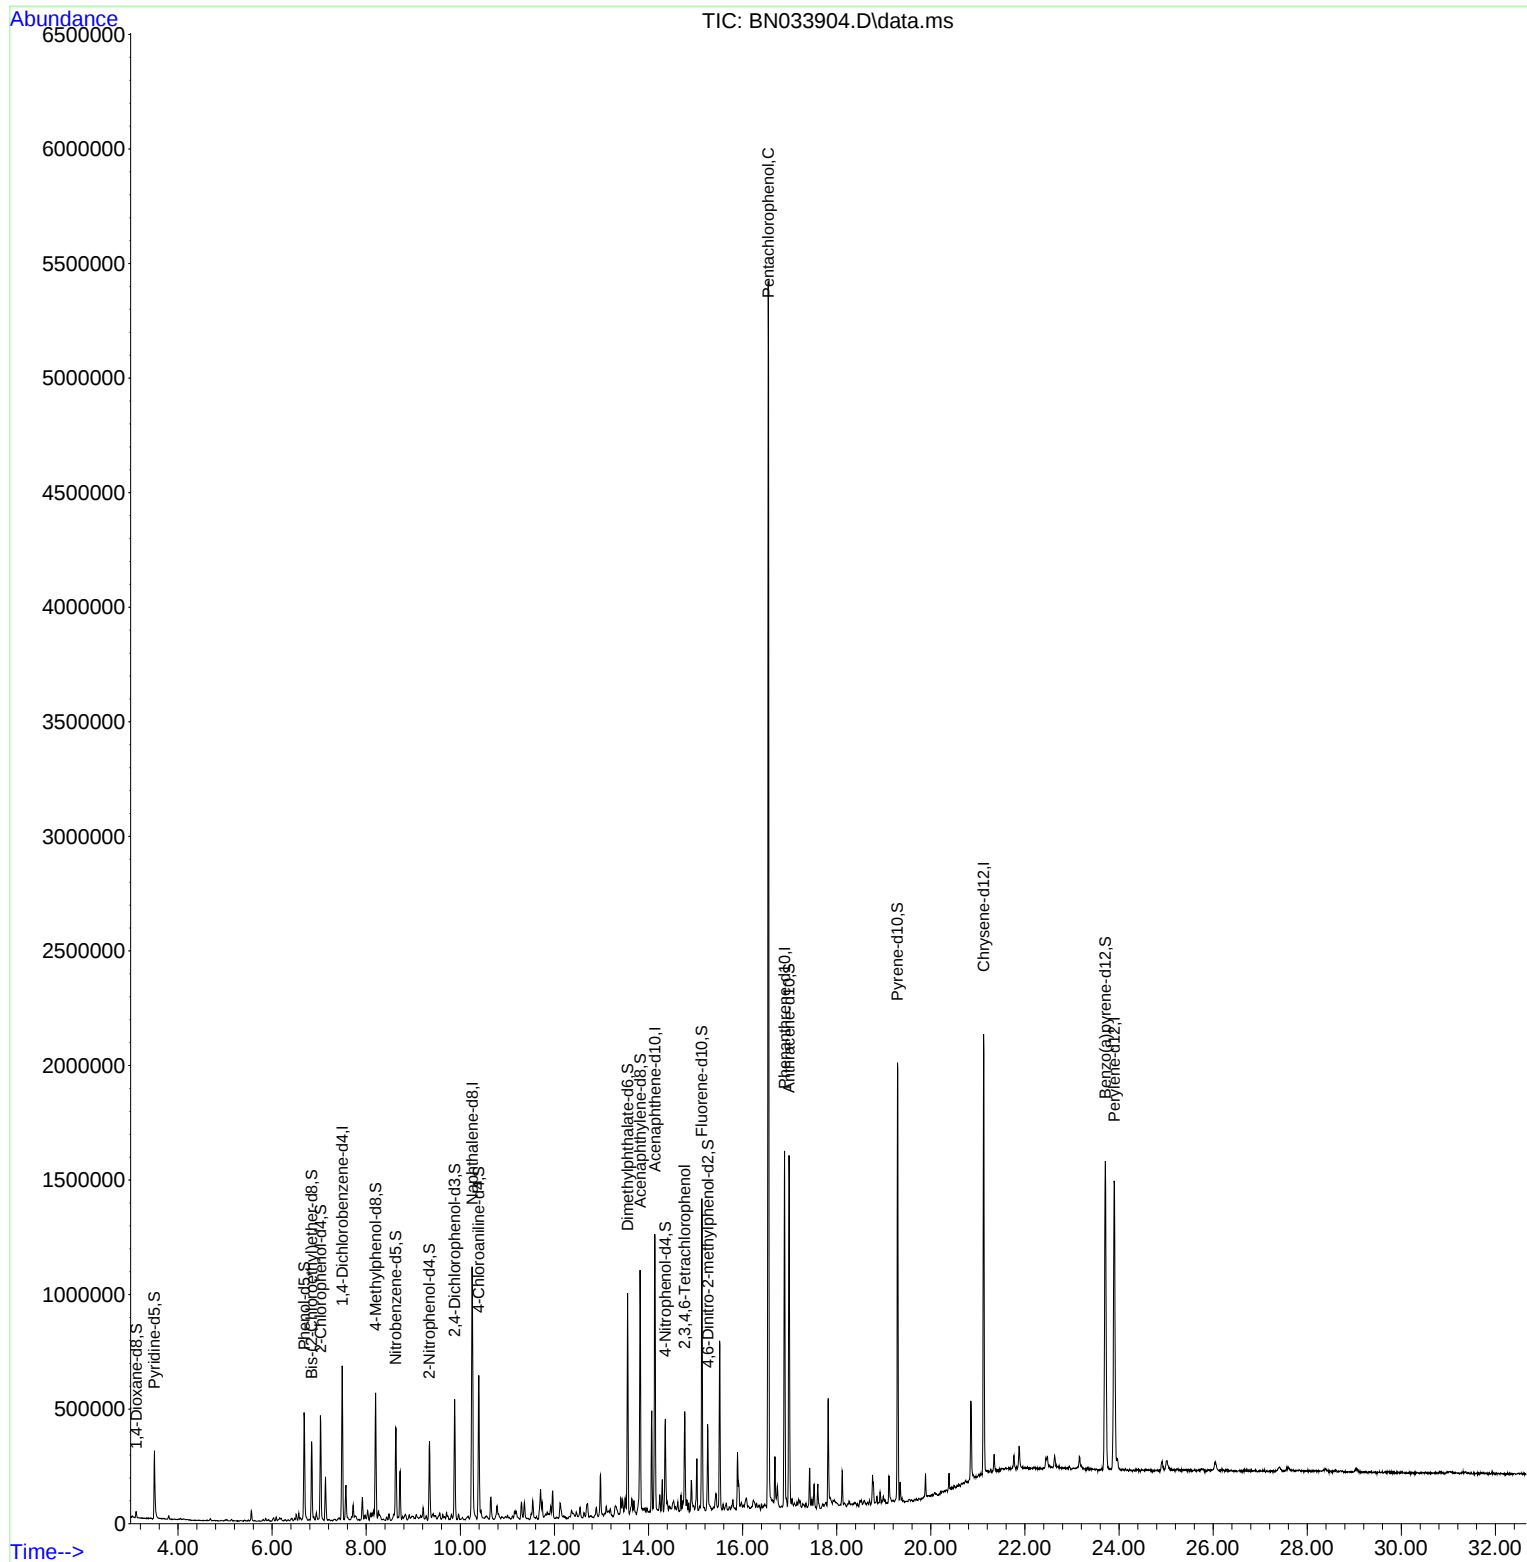




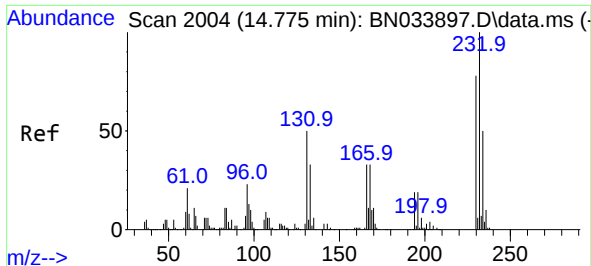


#58
2,3,4,6-Tetrachlorophenol
Concen: 9.588 ng/ul
RT: 14.769 min Scan# 2004
Delta R.T. -0.006 min
Lab File: BN033904.D
Acq: 13 Sep 2024 19:43

Instrument :
BNA_N
ClientSampleId :
DDC62

Tgt Ion:232 Resp: 67255

Ion	Ratio	Lower	Upper
232	100		
131	53.2	41.0	61.6
130	3.1	2.2	3.2
166	34.9	27.1	40.7

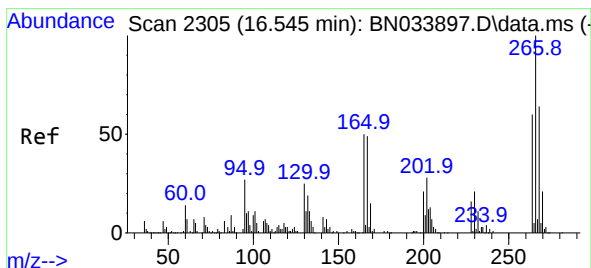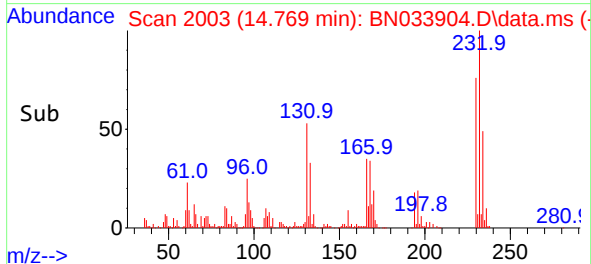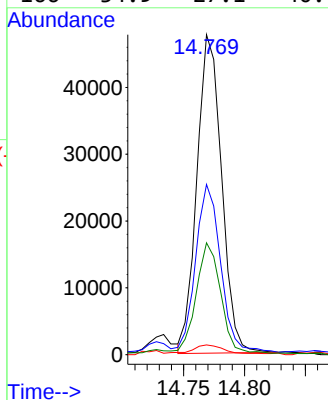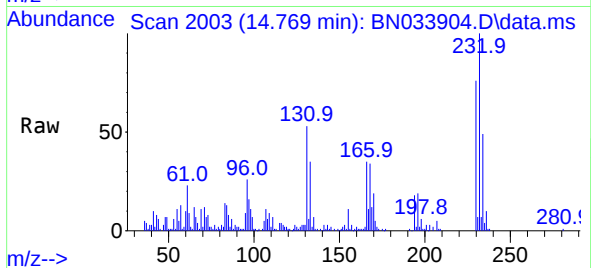

#71
Pentachlorophenol
Concen: 126.227 ng/ul
RT: 16.551 min Scan# 2306
Delta R.T. -0.000 min
Lab File: BN033904.D
Acq: 13 Sep 2024 19:43

Tgt Ion:266 Resp: 840225

Ion	Ratio	Lower	Upper
266	100		
264	62.1	51.1	76.7
268	63.7	52.8	79.2

