

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091324\
 Data File : BN033890.D
 Acq On : 13 Sep 2024 09:42
 Operator : JU/RC
 Sample : PB163351BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK351

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN033890.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.105	17	20	26	rVB	45487	55540	1.71%	0.173%
2	3.493	82	86	101	rBV	522961	764297	23.48%	2.388%
3	3.799	135	138	143	rBV	10023	13230	0.41%	0.041%
4	4.252	211	215	220	rBV	13434	23556	0.72%	0.074%
5	6.452	583	589	594	rVB5	3333	5914	0.18%	0.018%
6	6.681	622	628	636	rBV	626890	921369	28.30%	2.878%
7	6.840	649	655	664	rVB	467804	698639	21.46%	2.182%
8	7.028	679	687	701	rBV	598957	925263	28.42%	2.890%
9	7.493	759	766	773	rBV	519666	792079	24.33%	2.474%
10	8.199	878	886	897	rBV	697984	1065576	32.74%	3.329%
11	8.434	922	926	929	rVB5	3860	4776	0.15%	0.015%
12	8.634	950	960	969	rBV	538009	864290	26.55%	2.700%
13	9.093	1034	1038	1043	rVB4	7385	12245	0.38%	0.038%
14	9.346	1074	1081	1090	rBV	434199	679350	20.87%	2.122%
15	9.881	1164	1172	1184	rBV	660075	1042165	32.02%	3.256%
16	10.251	1227	1235	1244	rBV	674837	1083889	33.30%	3.386%
17	10.393	1250	1259	1270	rBV	605160	988094	30.35%	3.087%
18	10.475	1271	1273	1282	rVB8	5264	10836	0.33%	0.034%
19	11.093	1372	1378	1381	rVB8	2752	5553	0.17%	0.017%
20	11.575	1457	1460	1465	rVB7	3374	5875	0.18%	0.018%
21	11.851	1501	1507	1510	rBV4	8546	14607	0.45%	0.046%
22	12.534	1618	1623	1626	rBV3	3675	5861	0.18%	0.018%
23	13.557	1791	1797	1806	rBV	1019459	1429953	43.93%	4.467%
24	13.822	1835	1842	1854	rBV	1160279	1681356	51.65%	5.252%
25	14.134	1889	1895	1904	rBV	891838	1316241	40.44%	4.112%
26	14.357	1926	1933	1953	rBV	496756	792933	24.36%	2.477%
27	14.498	1955	1957	1964	rVB7	2584	4366	0.13%	0.014%
28	14.998	2038	2042	2044	rBV4	3400	4420	0.14%	0.014%
29	15.139	2059	2066	2073	rBV	1495057	2094021	64.33%	6.541%
30	15.263	2081	2087	2098	rBV	478801	649962	19.97%	2.030%
31	15.375	2103	2106	2110	rVB3	6039	8735	0.27%	0.027%
32	15.616	2145	2147	2150	rVB4	4442	3733	0.11%	0.012%
33	15.928	2197	2200	2204	rVB5	5360	6816	0.21%	0.021%
34	16.051	2217	2221	2225	rBV6	2695	3674	0.11%	0.011%
35	16.257	2252	2256	2260	rVV6	3871	5554	0.17%	0.017%
36	16.804	2346	2349	2353	rVB6	2965	3849	0.12%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091324\
 Data File : BN033890.D
 Acq On : 13 Sep 2024 09:42
 Operator : JU/RC
 Sample : PB163351BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK351

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Title : SVOA CALIBRATION

37	16.892	2358	2364	2373	rBV	1132896	1551126	47.65%	4.846%
38	16.986	2374	2380	2393	rBV	1622974	2342161	71.95%	7.317%
39	17.363	2441	2444	2447	rVB3	3120	4645	0.14%	0.015%
40	17.580	2479	2481	2483	rBV3	3044	3630	0.11%	0.011%
41	17.816	2517	2521	2527	rBV2	43544	68838	2.11%	0.215%
42	18.345	2609	2611	2616	rVB6	5306	6795	0.21%	0.021%
43	18.857	2695	2698	2705	rBV3	20669	30408	0.93%	0.095%
44	18.927	2707	2710	2715	rVB	15574	20565	0.63%	0.064%
45	19.116	2738	2742	2746	rBV4	25059	33472	1.03%	0.105%
46	19.298	2767	2773	2782	rBV	2155300	2796974	85.92%	8.737%
47	21.127	3079	3084	3094	rBV	1375985	1886127	57.94%	5.892%
48	23.715	3516	3524	3537	rVB2	1454043	3255149	100.00%	10.169%
49	23.904	3549	3556	3565	rBV2	882951	2023131	62.15%	6.320%


Sum of corrected areas: 32011638

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091324\
Data File : BN033890.D
Acq On : 13 Sep 2024 09:42
Operator : JU/RC
Sample : PB163351BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK351

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

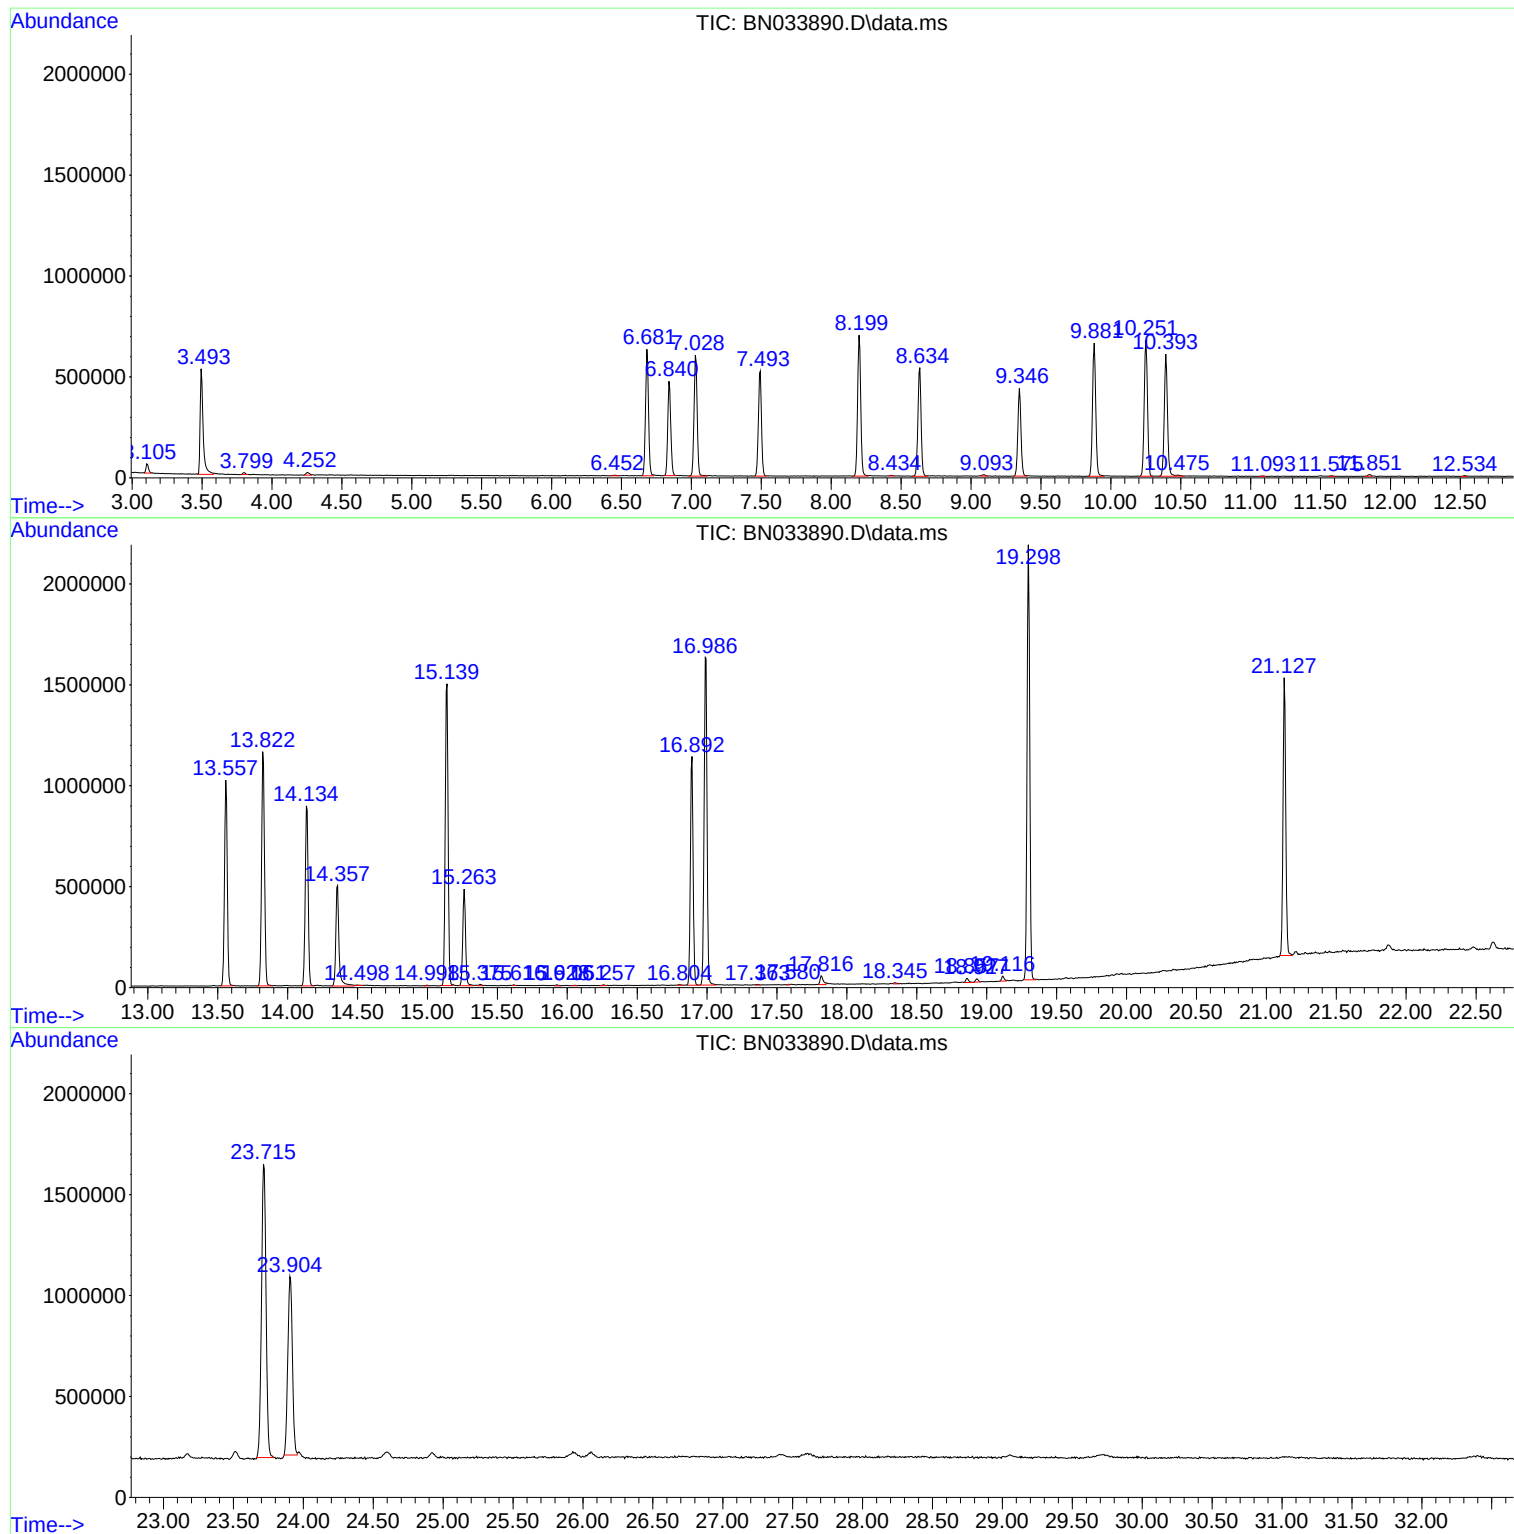

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091324\
Data File : BN033890.D
Acq On : 13 Sep 2024 09:42
Operator : JU/RC
Sample : PB163351BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK351

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091324\
Data File : BN033890.D
Acq On : 13 Sep 2024 09:42
Operator : JU/RC
Sample : PB163351BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK351

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc