

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091324\
 Data File : BN033898.D
 Acq On : 13 Sep 2024 15:47
 Operator : JU/RC
 Sample : PB163308BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK308

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN033898.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.111	17	21	27	rVB	55066	72934	1.90%	0.175%
2	3.493	82	86	100	rBV	627595	921817	23.97%	2.207%
3	3.805	133	139	143	rVB	17174	24366	0.63%	0.058%
4	4.246	210	214	220	rBV6	6792	14971	0.39%	0.036%
5	6.687	622	629	642	rBV	738057	1154848	30.03%	2.765%
6	6.840	649	655	666	rBV	584583	888323	23.10%	2.127%
7	7.028	681	687	696	rBV	756030	1168258	30.38%	2.797%
8	7.493	759	766	774	rVB	800772	1246195	32.41%	2.984%
9	8.199	880	886	902	rBV	860828	1357466	35.30%	3.250%
10	8.634	952	960	971	rBV	672253	1095746	28.50%	2.624%
11	9.081	1032	1036	1041	rVB5	3194	5930	0.15%	0.014%
12	9.346	1074	1081	1089	rVV	563413	872996	22.70%	2.090%
13	9.881	1164	1172	1186	rBV	834271	1336951	34.77%	3.201%
14	10.251	1227	1235	1245	rVB	1038174	1679118	43.67%	4.021%
15	10.393	1251	1259	1273	rBV	754570	1234082	32.09%	2.955%
16	10.710	1310	1313	1318	rVB6	2313	3965	0.10%	0.009%
17	11.845	1502	1506	1511	rBV2	13278	20958	0.55%	0.050%
18	13.557	1791	1797	1807	rBV	1277498	1773900	46.13%	4.248%
19	13.822	1835	1842	1854	rBV2	1471366	2101764	54.66%	5.033%
20	14.134	1887	1895	1904	rBV	1412758	2029627	52.78%	4.860%
21	14.210	1906	1908	1914	rVB6	3252	5714	0.15%	0.014%
22	14.357	1927	1933	1952	rBV	642465	970047	25.23%	2.323%
23	15.134	2059	2065	2077	rBV	1803310	2565624	66.72%	6.143%
24	15.263	2081	2087	2097	rBV	518537	710550	18.48%	1.701%
25	15.375	2103	2106	2111	rVB4	8287	12887	0.34%	0.031%
26	15.928	2196	2200	2203	rBV4	5469	7619	0.20%	0.018%
27	16.675	2321	2327	2332	rBV4	3821	7057	0.18%	0.017%
28	16.886	2357	2363	2372	rBV	1679174	2356435	61.28%	5.642%
29	16.986	2374	2380	2394	rVB	2105286	2822379	73.40%	6.758%
30	17.580	2477	2481	2486	rBV7	4896	8688	0.23%	0.021%
31	17.816	2517	2521	2530	rBV5	27832	46552	1.21%	0.111%
32	18.857	2694	2698	2704	rBV3	25143	35906	0.93%	0.086%
33	18.927	2706	2710	2716	rBV	23847	34688	0.90%	0.083%
34	19.110	2738	2741	2748	rBV4	20528	30570	0.79%	0.073%
35	19.298	2766	2773	2781	rBV	2524568	3338031	86.81%	7.993%
36	20.327	2945	2948	2952	rBV5	16106	21939	0.57%	0.053%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091324\
Data File : BN033898.D
Acq On : 13 Sep 2024 15:47
Operator : JU/RC
Sample : PB163308BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK308

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Title : SVOA CALIBRATION

37	21.127	3078	3084	3094	rBV	2100593	2846731	74.03%	6.816%
38	23.710	3515	3523	3537	rBV2	1696845	3845336	100.00%	9.208%
39	23.904	3548	3556	3564	rBV	1350235	3091837	80.40%	7.403%


Sum of corrected areas: 41762805

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091324\
Data File : BN033898.D
Acq On : 13 Sep 2024 15:47
Operator : JU/RC
Sample : PB163308BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK308

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

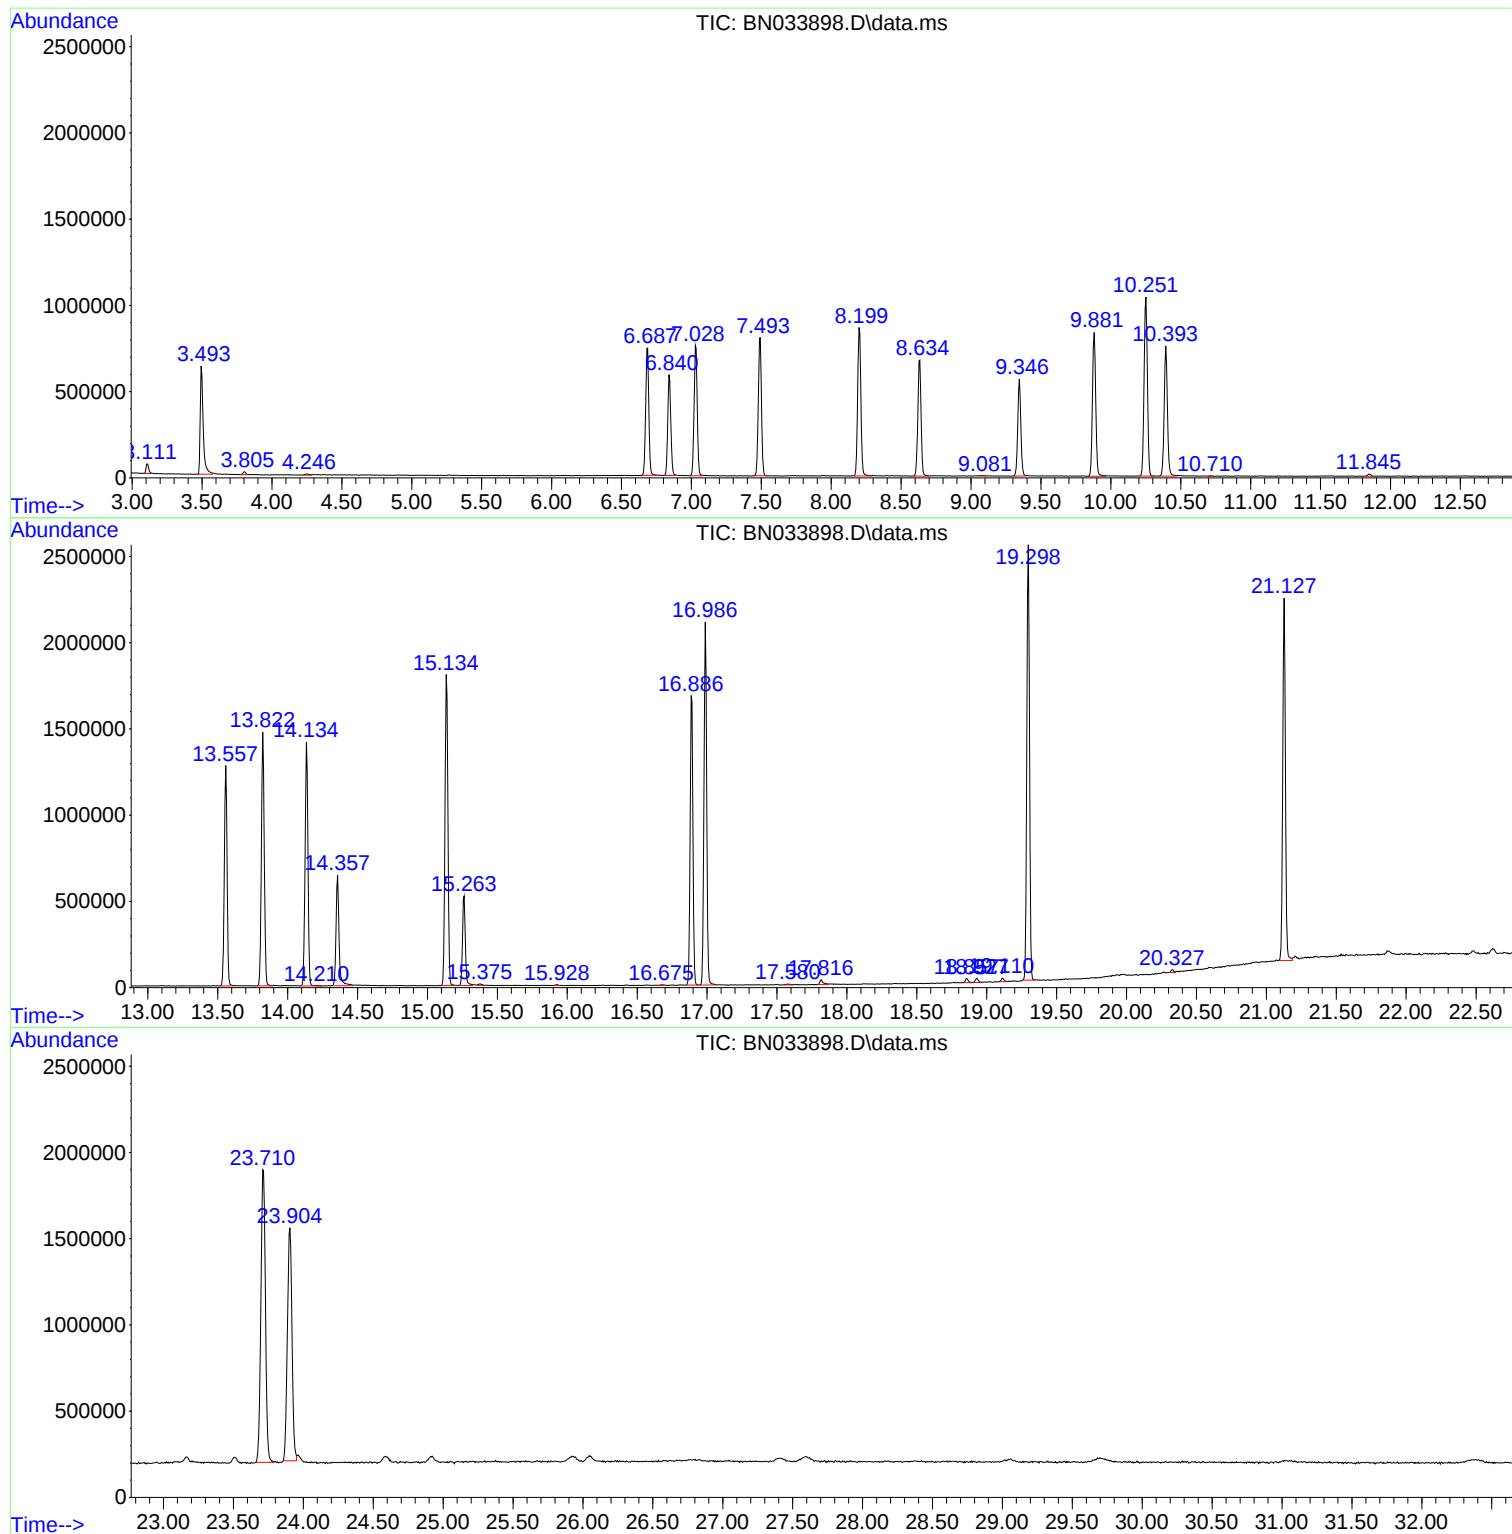

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091324\
Data File : BN033898.D
Acq On : 13 Sep 2024 15:47
Operator : JU/RC
Sample : PB163308BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK308

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091324\
Data File : BN033898.D
Acq On : 13 Sep 2024 15:47
Operator : JU/RC
Sample : PB163308BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK308

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc