

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091422\
 Data File : BN021729.D
 Acq On : 13 Sep 2022 17:29
 Operator : CG/JU
 Sample : SSTDICC0.1
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1

Quant Time: Sep 14 01:31:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 14 01:24:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.062	152	4829	0.400	ng	0.00
7) Naphthalene-d8	10.888	136	15298	0.400	ng	0.00
13) Acenaphthene-d10	14.707	164	9479	0.400	ng	0.00
19) Phenanthrene-d10	17.456	188	22024	0.400	ng	0.00
29) Chrysene-d12	21.656	240	16149	0.400	ng	0.00
35) Perylene-d12	24.168	264	13747	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.584	112	1284	0.136	ng	0.00
5) Phenol-d6	7.209	99	1554	0.129	ng	0.00
8) Nitrobenzene-d5	9.233	82	1195	0.116	ng	0.00
11) 2-Methylnaphthalene-d10	12.475	152	3041	0.088	ng	0.00
14) 2,4,6-Tribromophenol	16.209	330	387	0.124	ng	0.00
15) 2-Fluorobiphenyl	13.339	172	3642	0.088	ng	0.00
27) Fluoranthene-d10	19.494	212	5384	0.095	ng	0.00
31) Terphenyl-d14	20.080	244	3750	0.103	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.403	88	642	0.106	ng	# 90
3) n-Nitrosodimethylamine	3.736	42	599	0.110	ng	98
6) bis(2-Chloroethyl)ether	7.469	93	1541	0.102	ng	99
9) Naphthalene	10.941	128	4242	0.094	ng	95
10) Hexachlorobutadiene	11.219	225	724	0.092	ng	# 100
12) 2-Methylnaphthalene	12.180	142	783	0.136	ng	# 62
16) Acenaphthylene	14.429	152	3875	0.087	ng	100
17) Acenaphthene	14.771	154	2864	0.091	ng	99
18) Fluorene	15.758	166	3830	0.099	ng	99
21) 4-Bromophenyl-phenylether	16.647	248	1254	0.091	ng	98
22) Hexachlorobenzene	16.763	284	1390	0.082	ng	99
23) Atrazine	16.913	200	1010	0.126	ng	95
24) Pentachlorophenol	17.109	266	426	0.119	ng	97
25) Phenanthrene	17.502	178	6811	0.090	ng	100
26) Anthracene	17.594	178	5508	0.091	ng	99
28) Fluoranthene	19.523	202	7174	0.091	ng	100
30) Pyrene	19.886	202	7280	0.085	ng	95
32) Benzo(a)anthracene	21.638	228	5857	0.104	ng	98
33) Chrysene	21.692	228	6014	0.090	ng	98
34) Bis(2-ethylhexyl)phtha...	21.549	149	4679	0.206	ng	# 98
36) Indeno(1,2,3-cd)pyrene	26.811	276	5588	0.090	ng	97
37) Benzo(b)fluoranthene	23.394	252	5458	0.081	ng	# 77
38) Benzo(k)fluoranthene	23.443	252	5213	0.076	ng	# 77
39) Benzo(a)pyrene	24.054	252	4394	0.093	ng	# 71
40) Dibenzo(a,h)anthracene	26.835	278	4372	0.088	ng	# 86
41) Benzo(g,h,i)perylene	27.627	276	4747	0.087	ng	# 91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091422\
 Data File : BN021729.D
 Acq On : 13 Sep 2022 17:29
 Operator : CG/JU
 Sample : SSTDICC0.1
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1


Quant Time: Sep 14 01:31:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 14 01:24:46 2022
 Response via : Initial Calibration








#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 8.062 min Scan# 662
 Delta R.T. -0.000 min
 Lab File: BN021729.D
 Acq: 13 Sep 2022 17:29

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1



Tgt Ion: 152 Resp: 4829




Ion	Ratio	Lower	Upper
152	100		
150	149.0	121.8	182.8
115	59.6	48.3	72.5




#2
 1,4-Dioxane
 Concen: 0.106 ng
 RT: 3.403 min Scan# 17
 Delta R.T. -0.000 min
 Lab File: BN021729.D
 Acq: 13 Sep 2022 17:29

Tgt Ion: 88 Resp: 642

Ion	Ratio	Lower	Upper
88	100		
43	40.5	24.2	36.2
58	70.1	60.2	90.4







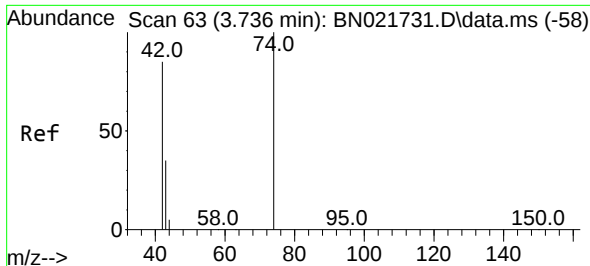

#3
n-Nitrosodimethylamine
Concen: 0.110 ng
RT: 3.736 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion: 42 Resp: 599
Ion Ratio Lower Upper
42 100
74 142.6 116.3 174.5
44 12.0 9.0 13.4

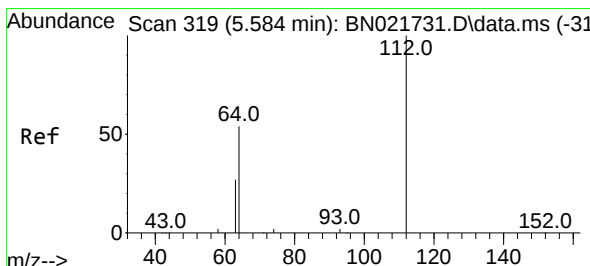

#4
2-Fluorophenol
Concen: 0.136 ng
RT: 5.584 min Scan# 319
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29

Tgt Ion: 112 Resp: 1284
Ion Ratio Lower Upper
112 100
64 56.5 45.4 68.2
63 29.5 23.3 34.9







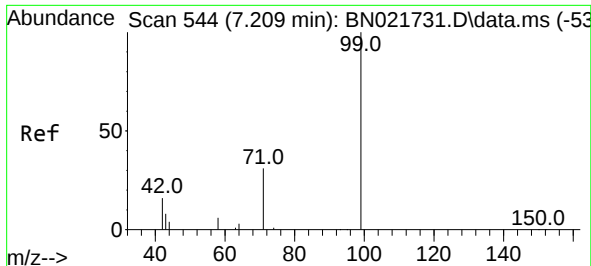

#5
Phenol-d6
Concen: 0.129 ng
RT: 7.209 min Scan# 544
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:	99	Resp:	1554
Ion	Ratio	Lower	Upper
99	100		
42	21.0	15.1	22.7
71	32.9	25.3	37.9

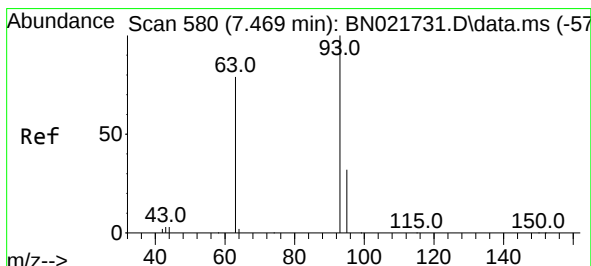

#6
bis(2-Chloroethyl)ether
Concen: 0.102 ng
RT: 7.469 min Scan# 580
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29

Tgt Ion:	93	Resp:	1541
Ion	Ratio	Lower	Upper
93	100		
63	74.4	60.0	90.0
95	31.7	26.2	39.4









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.888 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:	136	Resp:	15298
Ion Ratio	Lower	Upper	
136	100		
137	11.6	9.1	13.7
54	8.0	6.4	9.6
68	7.0	5.5	8.3



#8
Nitrobenzene-d5
Concen: 0.116 ng
RT: 9.233 min Scan# 783
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29

Tgt Ion:	82	Resp:	1195
Ion Ratio	Lower	Upper	
82	100		
128	47.9	35.6	53.4
54	53.0	37.8	56.8









#9
Naphthalene
Concen: 0.094 ng
RT: 10.941 min Scan# 943
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:	128	Resp:	4242
Ion	Ratio	Lower	Upper
128	100		
129	13.6	9.2	13.8
127	14.8	10.5	15.7



#10
Hexachlorobutadiene
Concen: 0.092 ng
RT: 11.219 min Scan# 969
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29

Tgt Ion:	225	Resp:	724
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.3	50.4	75.6







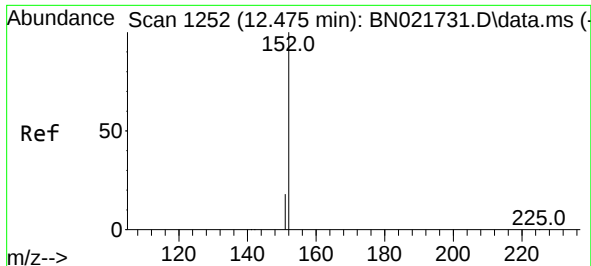

#11
2-Methylnaphthalene-d10
Concen: 0.088 ng
RT: 12.475 min Scan# 1173
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:152 Resp: 3041
Ion Ratio Lower Upper
152 100
151 22.2 15.6 23.4



#12
2-Methylnaphthalene
Concen: 0.136 ng
RT: 12.180 min Scan# 1174
Delta R.T. 0.004 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29

Tgt Ion:142 Resp: 783
Ion Ratio Lower Upper
142 100
141 24.6 10.6 16.0#
115 26.5 5.6 8.4#







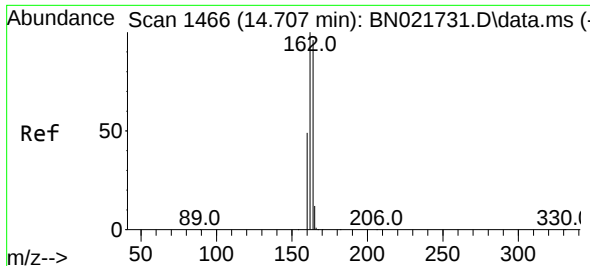

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.707 min Scan# 1466
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:164 Resp: 9479
Ion Ratio Lower Upper
164 100
162 104.4 83.2 124.8
160 50.7 40.9 61.3



#14
2,4,6-Tribromophenol
Concen: 0.124 ng
RT: 16.209 min Scan# 1603
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29

Tgt Ion:330 Resp: 387
Ion Ratio Lower Upper
330 100
332 96.6 76.8 115.2
141 47.8 37.2 55.8









#15
2-Fluorobiphenyl
Concen: 0.088 ng
RT: 13.339 min Scan# 1338
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:172 Resp: 3642
Ion Ratio Lower Upper
172 100
171 35.4 27.7 41.5
170 25.0 18.8 28.2



#16
Acenaphthylene
Concen: 0.087 ng
RT: 14.429 min Scan# 1440
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29

Tgt Ion:152 Resp: 3875
Ion Ratio Lower Upper
152 100
151 19.3 15.4 23.0
153 13.1 10.3 15.5









#17
Acenaphthene
Concen: 0.091 ng
RT: 14.771 min Scan# 1472
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:	154	Resp:	2864
Ion	Ratio	Lower	Upper
154	100		
153	114.2	91.0	136.4
152	58.6	46.0	69.0



#18
Fluorene
Concen: 0.099 ng
RT: 15.758 min Scan# 1564
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29

Tgt Ion:	166	Resp:	3830
Ion	Ratio	Lower	Upper
166	100		
165	100.2	79.4	119.0
167	14.0	10.6	15.8







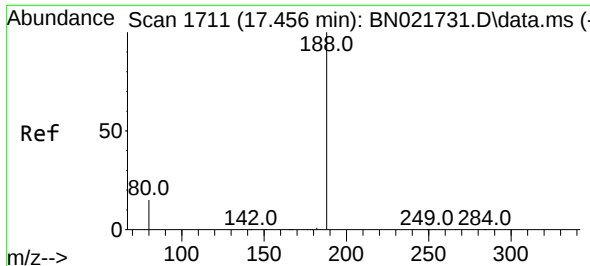

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.456 min Scan# 1711
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:188 Resp: 22024
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 15.5 12.6 19.0



#21
4-Bromophenyl-phenylether
Concen: 0.091 ng
RT: 16.647 min Scan# 1641
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29

Tgt Ion:248 Resp: 1254
Ion Ratio Lower Upper
248 100
250 97.0 77.8 116.8
141 65.6 49.0 73.4







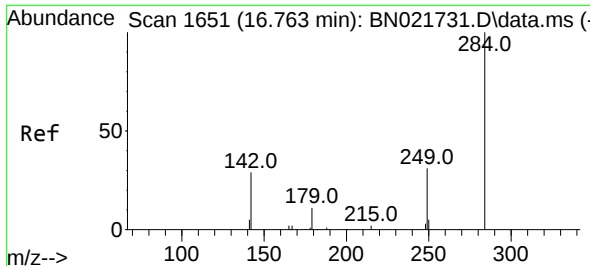

#22
Hexachlorobenzene
Concen: 0.082 ng
RT: 16.763 min Scan# 1651
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:284 Resp: 1390
Ion Ratio Lower Upper
284 100
142 42.6 33.4 50.2
249 32.1 25.1 37.7



#23
Atrazine
Concen: 0.126 ng
RT: 16.913 min Scan# 1664
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29

Tgt Ion:200 Resp: 1010
Ion Ratio Lower Upper
200 100
173 32.2 22.9 34.3
215 48.8 36.9 55.3





#24

Pentachlorophenol

Concen: 0.119 ng

RT: 17.109 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN021729.D

Acq: 13 Sep 2022 17:29

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:266 Resp: 426

Ion Ratio Lower Upper

266 100

264 61.3 50.0 75.0

268 65.5 50.2 75.2



#25

Phenanthrene

Concen: 0.090 ng

RT: 17.502 min Scan# 1715

Delta R.T. -0.000 min

Lab File: BN021729.D

Acq: 13 Sep 2022 17:29




Tgt Ion:178 Resp: 6811


Ion Ratio Lower Upper

178 100

176 19.1 15.3 22.9

179 15.3 12.2 18.4







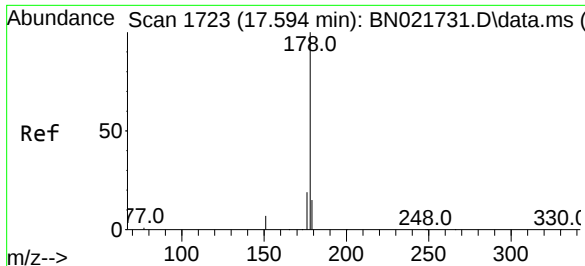

#26
 Anthracene
 Concen: 0.091 ng
 RT: 17.594 min Scan# 1723
 Delta R.T. -0.000 min
 Lab File: BN021729.D
 Acq: 13 Sep 2022 17:29




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1


Tgt Ion:178 Resp: 5508
 Ion Ratio Lower Upper
 178 100
 176 18.8 15.0 22.6
 179 15.8 12.2 18.2



#27
 Fluoranthene-d10
 Concen: 0.095 ng
 RT: 19.494 min Scan# 2111
 Delta R.T. -0.000 min
 Lab File: BN021729.D
 Acq: 13 Sep 2022 17:29

Tgt Ion:212 Resp: 5384
 Ion Ratio Lower Upper
 212 100
 106 18.0 14.3 21.5
 104 10.2 8.0 12.0









#28
Fluoranthene
Concen: 0.091 ng
RT: 19.523 min Scan# 2118
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:	202	Resp:	7174
Ion Ratio	Lower	Upper	
202	100		
101	13.7	11.0	16.4
203	17.2	13.7	20.5



#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.656 min Scan# 2417
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29

Tgt Ion:	240	Resp:	16149
Ion Ratio	Lower	Upper	
240	100		
120	11.8	9.8	14.8
236	27.7	22.2	33.4









#30
Pyrene
Concen: 0.085 ng
RT: 19.886 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:	202	Resp:	7280
Ion	Ratio	Lower	Upper
202	100		
200	21.0	15.0	22.4
203	17.9	12.8	19.2



#31
Terphenyl-d14
Concen: 0.103 ng
RT: 20.080 min Scan# 2241
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29

Tgt Ion:	244	Resp:	3750
Ion	Ratio	Lower	Upper
244	100		
212	10.8	7.9	11.9
122	20.4	15.8	23.8









#32
Benzo(a)anthracene
Concen: 0.104 ng
RT: 21.638 min Scan# 2415
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:228 Resp: 5857
Ion Ratio Lower Upper
228 100
226 27.8 21.5 32.3
229 20.5 15.8 23.8



#33
Chrysene
Concen: 0.090 ng
RT: 21.692 min Scan# 2421
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29

Tgt Ion:228 Resp: 6014
Ion Ratio Lower Upper
228 100
226 31.2 24.5 36.7
229 21.2 16.0 24.0









#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.206 ng
 RT: 21.549 min Scan# 2405
 Delta R.T. -0.000 min
 Lab File: BN021729.D
 Acq: 13 Sep 2022 17:29




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1


Tgt Ion:149 Resp: 4679
 Ion Ratio Lower Upper
 149 100
 167 26.8 20.8 31.2
 279 3.5 2.1 3.1#



#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.168 min Scan# 3103
 Delta R.T. -0.000 min
 Lab File: BN021729.D
 Acq: 13 Sep 2022 17:29

Tgt Ion:264 Resp: 13747
 Ion Ratio Lower Upper
 264 100
 260 26.0 20.6 31.0
 265 44.4 34.4 51.6







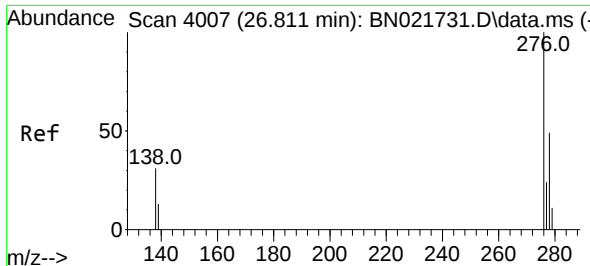

#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.090 ng
 RT: 26.811 min Scan# 4007
 Delta R.T. -0.000 min
 Lab File: BN021729.D
 Acq: 13 Sep 2022 17:29




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1


Tgt Ion:276 Resp: 5588
 Ion Ratio Lower Upper
 276 100
 138 32.1 27.4 41.0
 277 25.6 19.8 29.6



#37
 Benzo(b)fluoranthene
 Concen: 0.081 ng
 RT: 23.394 min Scan# 2838
 Delta R.T. -0.000 min
 Lab File: BN021729.D
 Acq: 13 Sep 2022 17:29


Tgt Ion:252 Resp: 5458
 Ion Ratio Lower Upper
 252 100
 253 35.4 19.6 29.4#
 125 26.5 13.0 19.4#





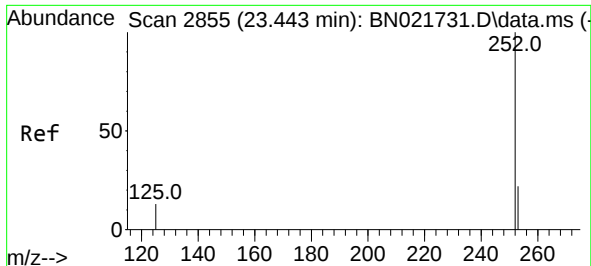


#38
Benzo(k)fluoranthene
Concen: 0.076 ng
RT: 23.443 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1







Tgt Ion:252 Resp: 5213
Ion Ratio Lower Upper
252 100
253 35.1 19.4 29.2#
125 26.1 12.6 18.8#



#39
Benzo(a)pyrene
Concen: 0.093 ng
RT: 24.054 min Scan# 3064
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29

Tgt Ion:252 Resp: 4394
Ion Ratio Lower Upper
252 100
253 40.1 20.8 31.2#
125 35.8 17.4 26.0#







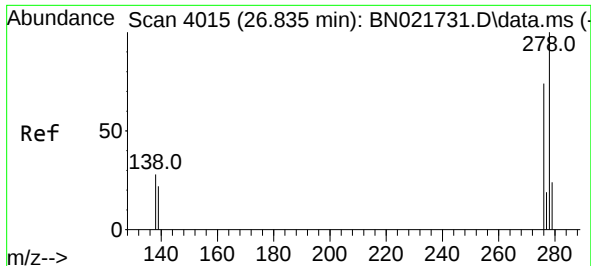

#40
Dibenzo(a,h)anthracene
Concen: 0.088 ng
RT: 26.835 min Scan# 4015
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Tgt Ion:278 Resp: 4372
Ion Ratio Lower Upper
278 100
139 30.8 19.2 28.8#
279 32.9 20.5 30.7#



#41
Benzo(g,h,i)perylene
Concen: 0.087 ng
RT: 27.627 min Scan# 4286
Delta R.T. -0.000 min
Lab File: BN021729.D
Acq: 13 Sep 2022 17:29

Tgt Ion:276 Resp: 4747
Ion Ratio Lower Upper
276 100
277 27.4 19.2 28.8
138 36.3 24.2 36.2#

