
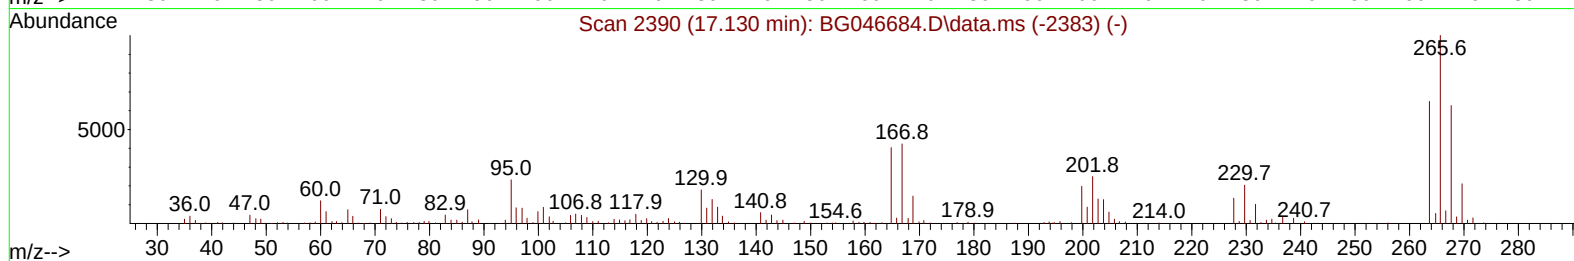
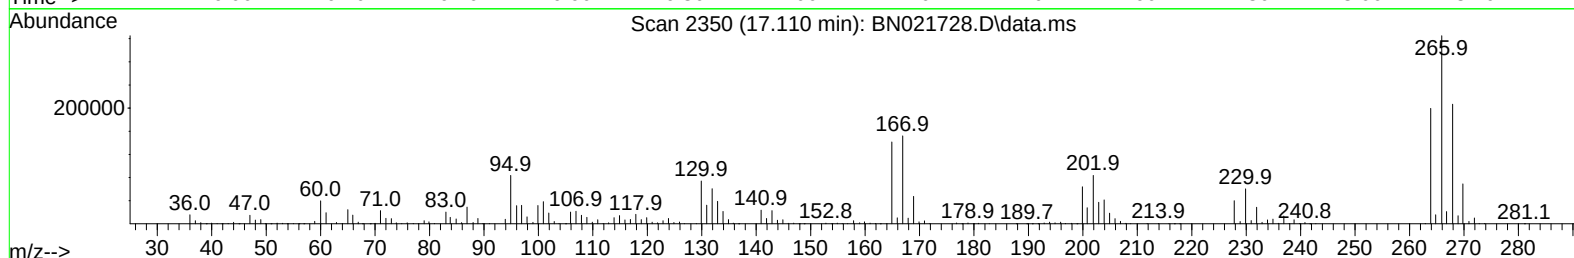


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091422\
Data File : BN021728.D
Acq On : 13 Sep 2022 16:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 05:48:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 14 05:48:40 2022
Response via : Initial Calibration

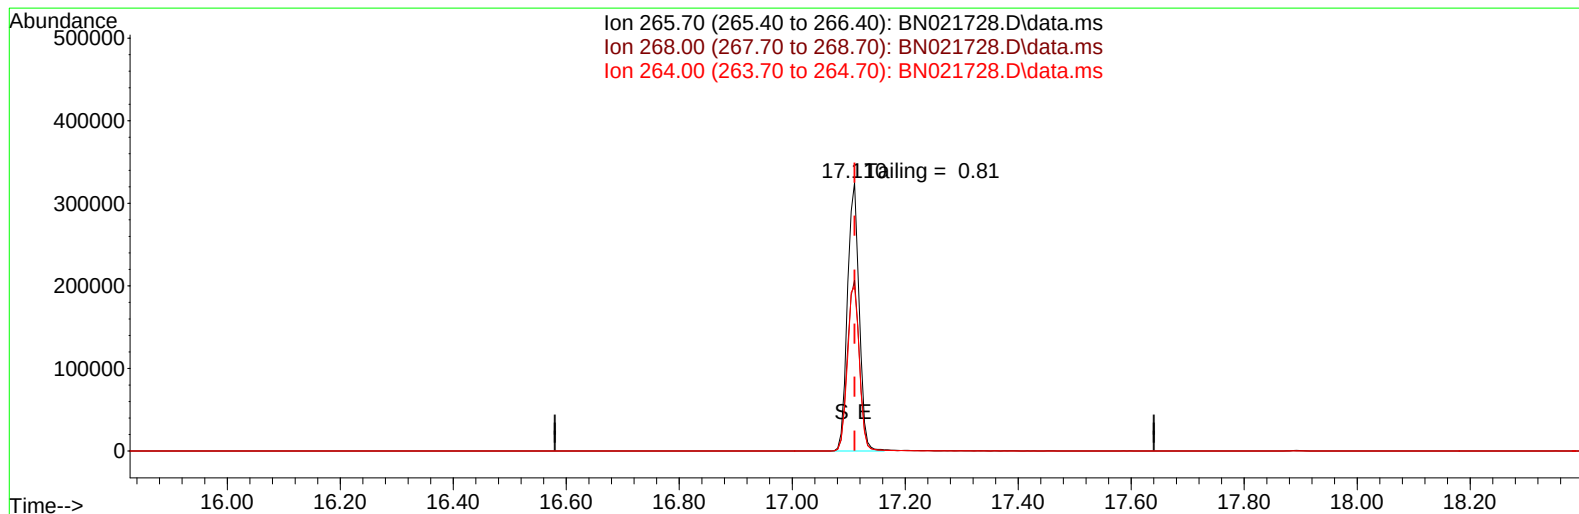

TIC: BN021728.D\data.ms

(70) Pentachlorophenol (C)




17.110min (0.000) 24827.93 ng

response 468793

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.58
264.00	61.60	61.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091422\
Data File : BN021728.D
Acq On : 13 Sep 2022 16:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 05:48:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 14 05:48:40 2022
Response via : Initial Calibration

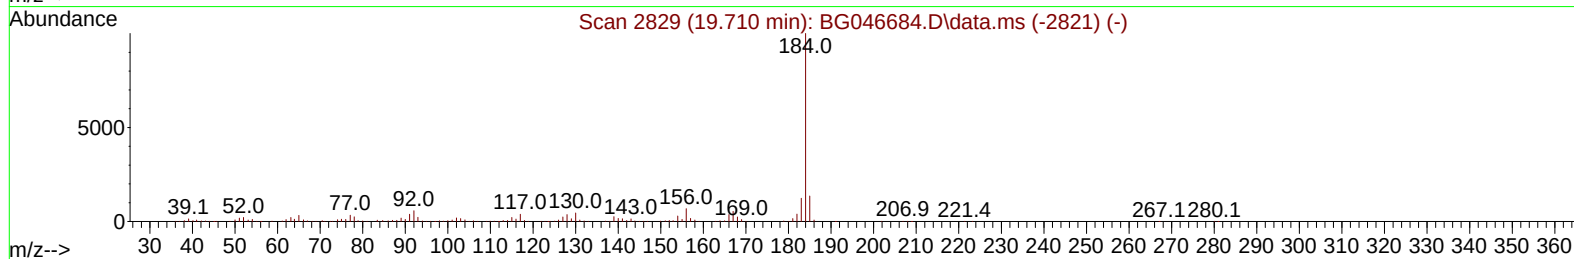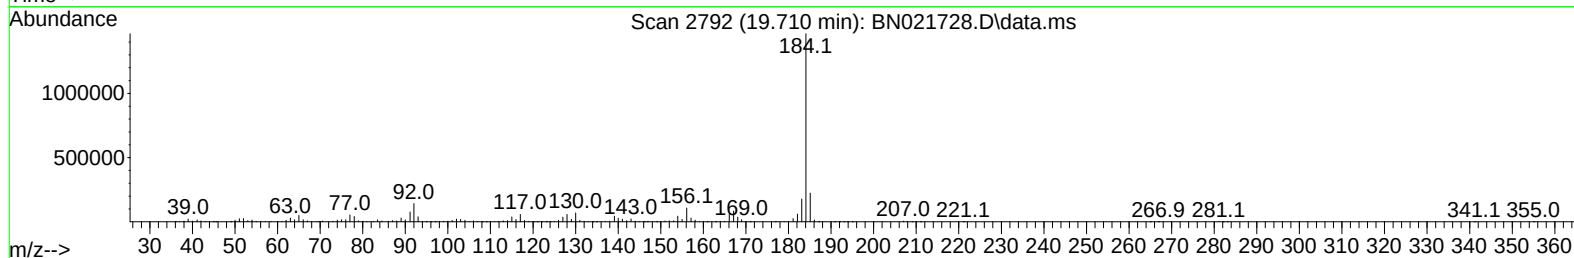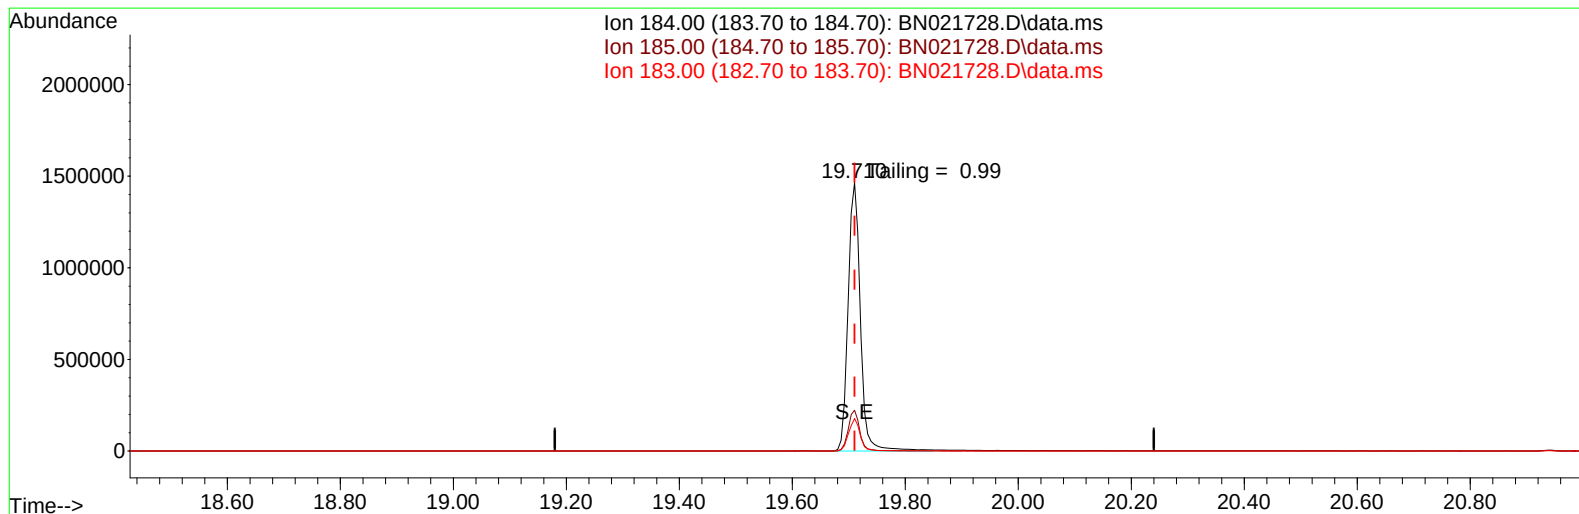

TIC: BN021728.D\data.ms

(77) Benzidine**19.710min (0.000) 1135186.03 ng****response 2239522**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.24
183.00	13.20	12.12
0.00	0.00	0.00