
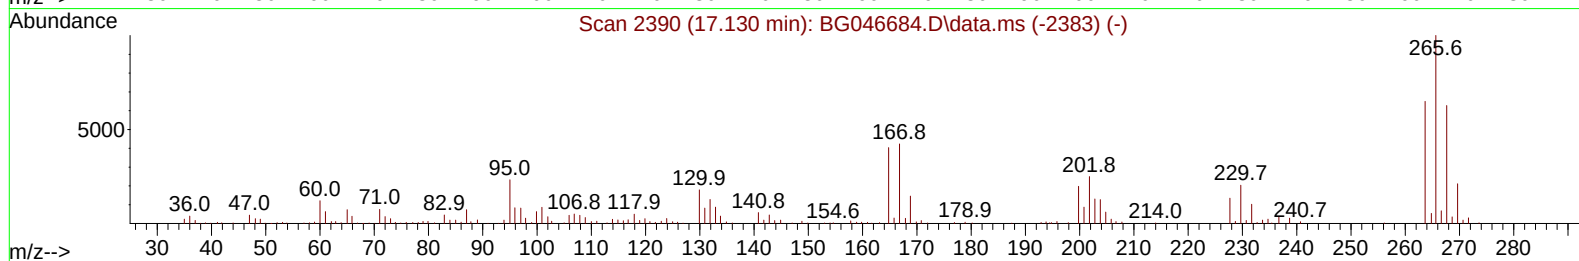
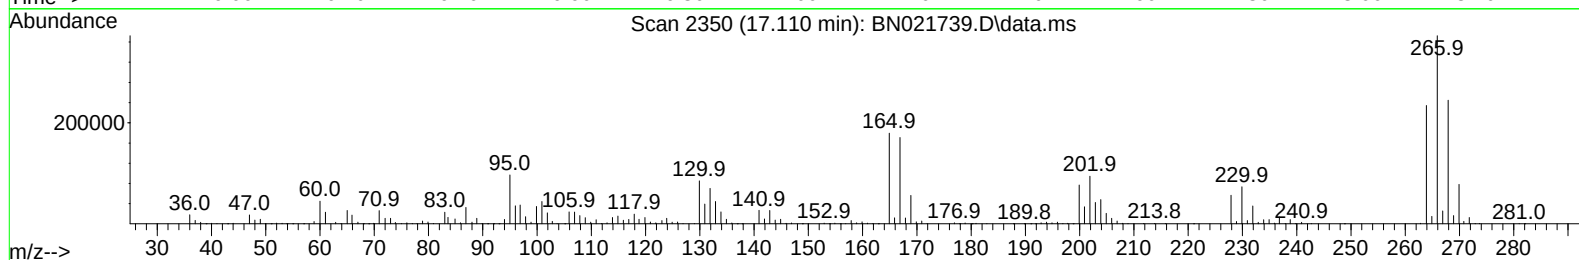


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091422\
Data File : BN021739.D
Acq On : 14 Sep 2022 09:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 06:19:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 15 06:19:42 2022
Response via : Initial Calibration

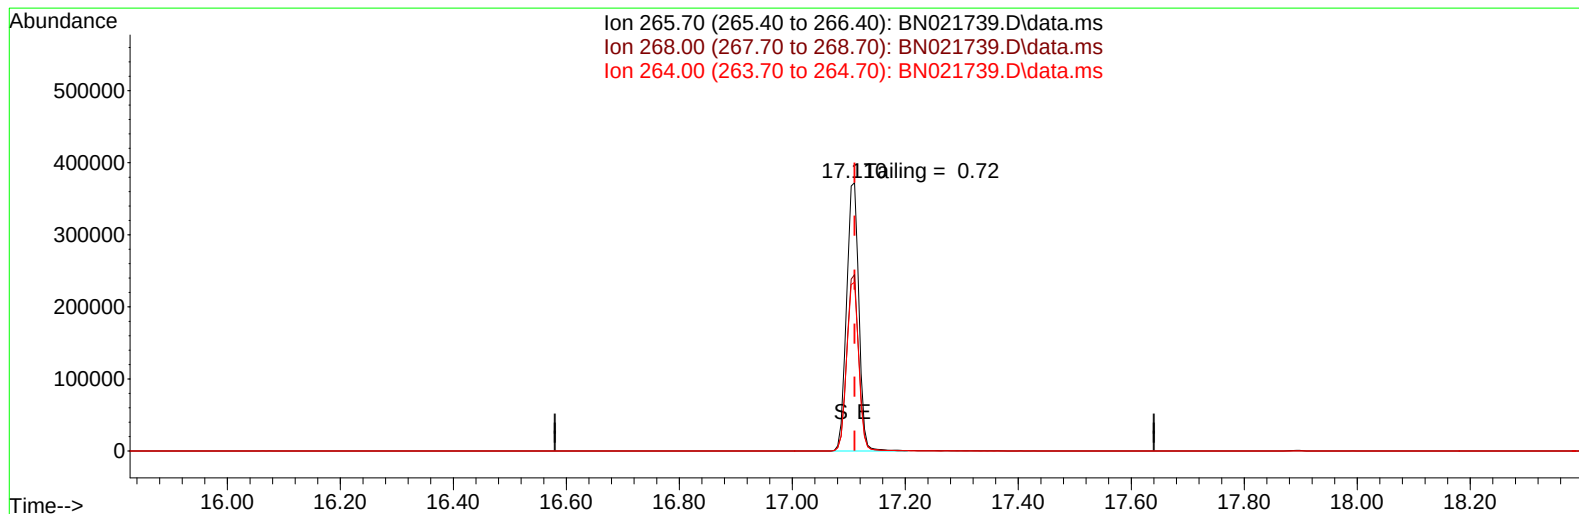

TIC: BN021739.D\data.ms

(70) Pentachlorophenol (C)




17.110min (0.000) 608469.91 ng

response 563464

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.68
264.00	61.60	62.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091422\
Data File : BN021739.D
Acq On : 14 Sep 2022 09:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 06:19:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 15 06:19:42 2022
Response via : Initial Calibration

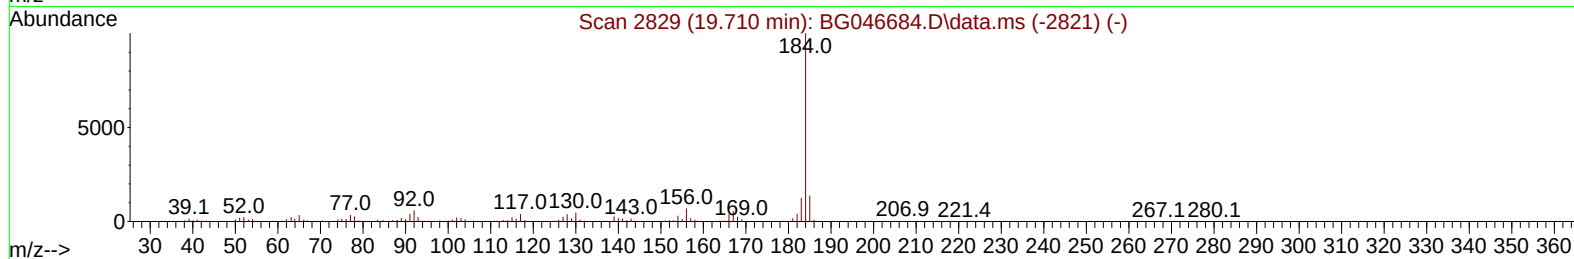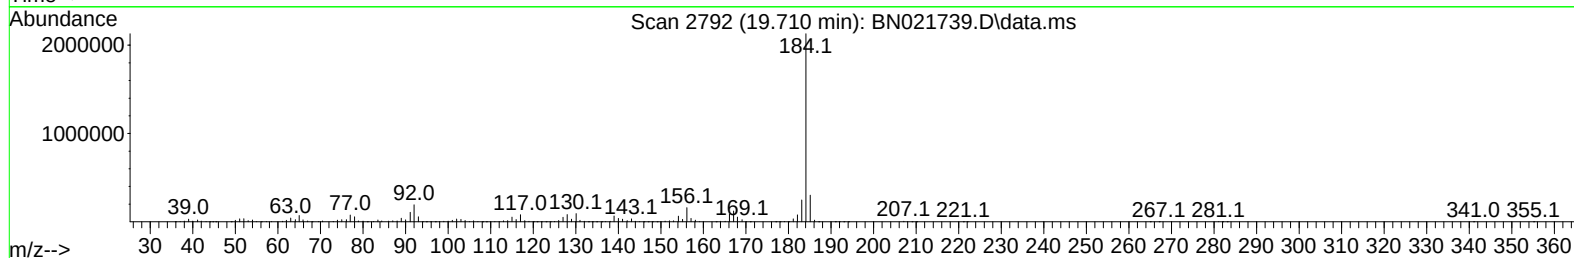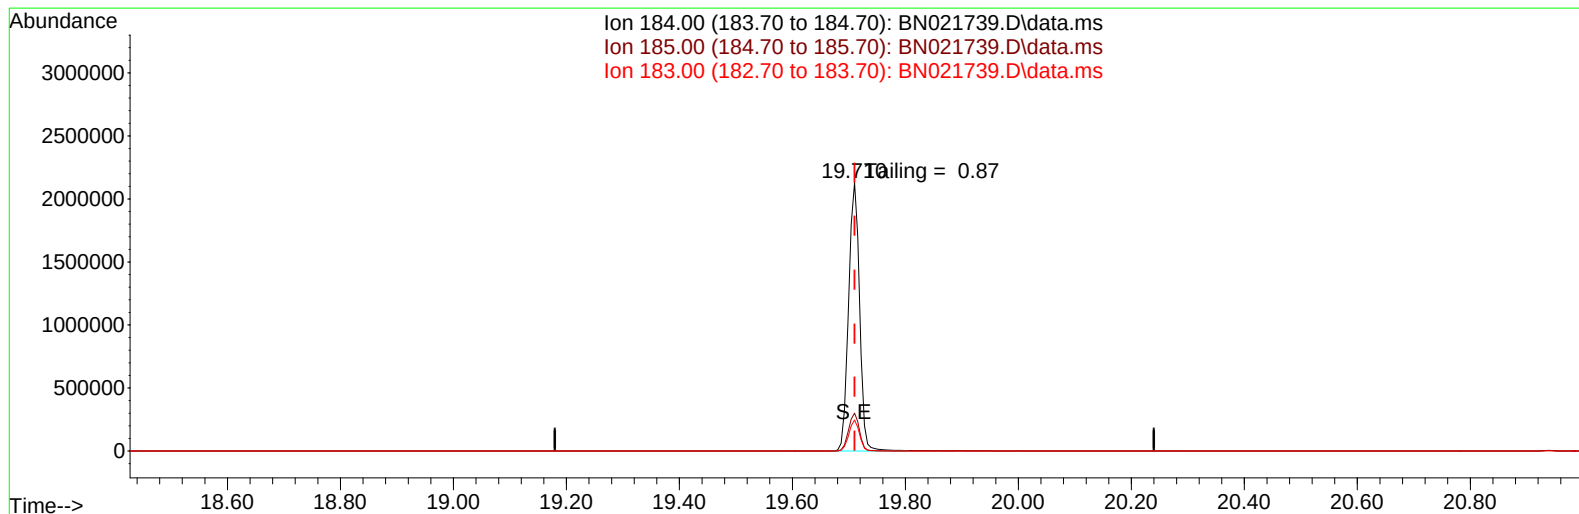

TIC: BN021739.D\data.ms

(77) Benzidine

19.710min (0.000) 203935.83 ng

response 2891743

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.17
183.00	13.20	11.59
0.00	0.00	0.00