
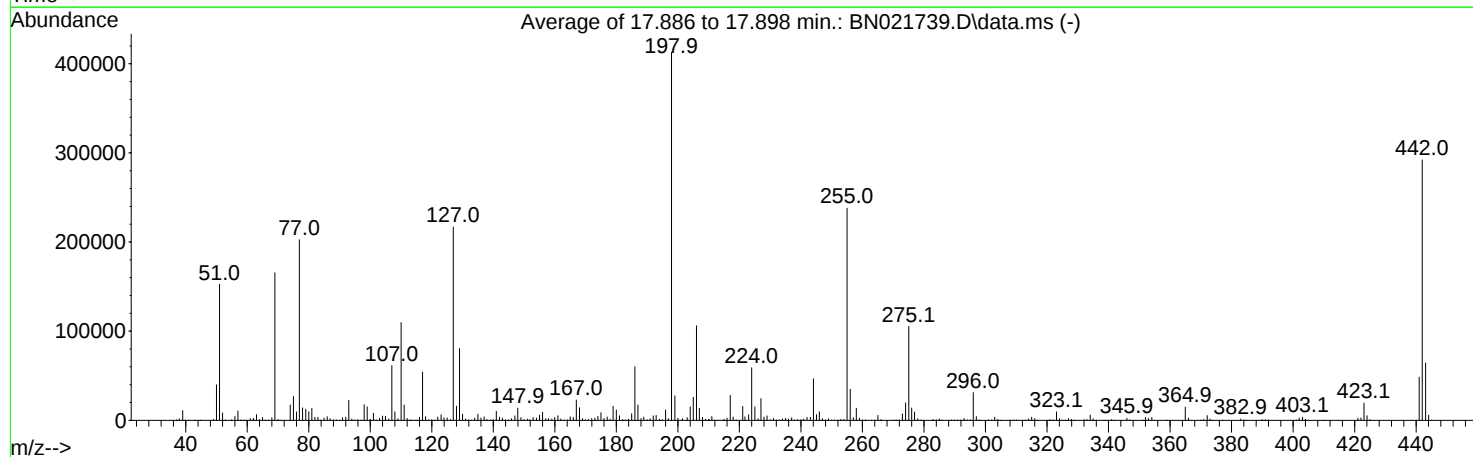


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091422\
 Data File : BN021739.D
 Acq On : 14 Sep 2022 09:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 14 01:55:04 2022

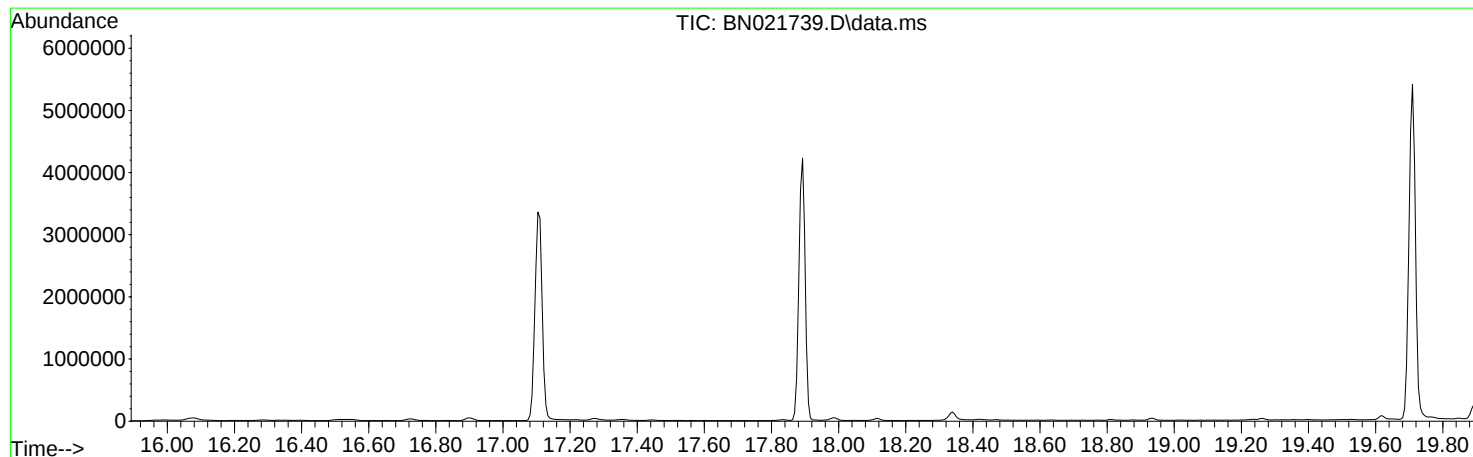




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	152571	PASS
68	69	0.00	2	1.6	2714	PASS
69	198	0.00	100	40.1	165437	PASS
70	69	0.00	2	0.5	879	PASS
127	198	10	80	52.5	216768	PASS
197	198	0.00	2	0.4	1831	PASS
198	198	100	100	100.0	412736	PASS
199	198	5	9	6.6	27304	PASS
275	198	10	60	25.5	105379	PASS
365	198	1	100	3.6	14855	PASS
441	198	0.01	100	11.7	48304	PASS
442	442	50	100	100.0	292096	PASS
443	442	15	24	22.0	64309	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091422\
Data File : BN021739.D
Acq On : 14 Sep 2022 09:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 15 06:19:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 15 06:19:42 2022
Response via : Initial Calibration

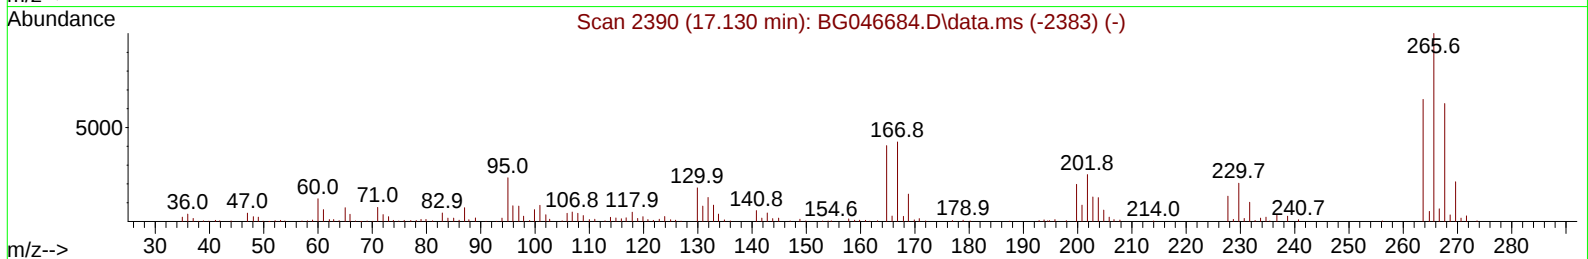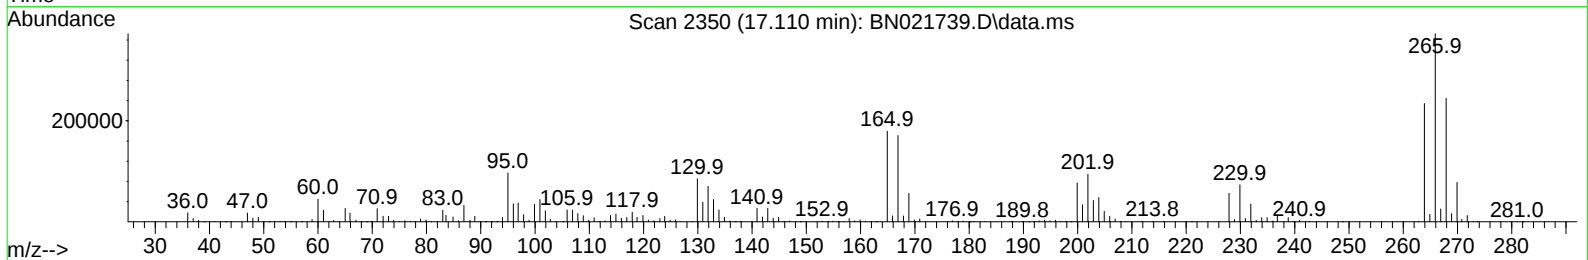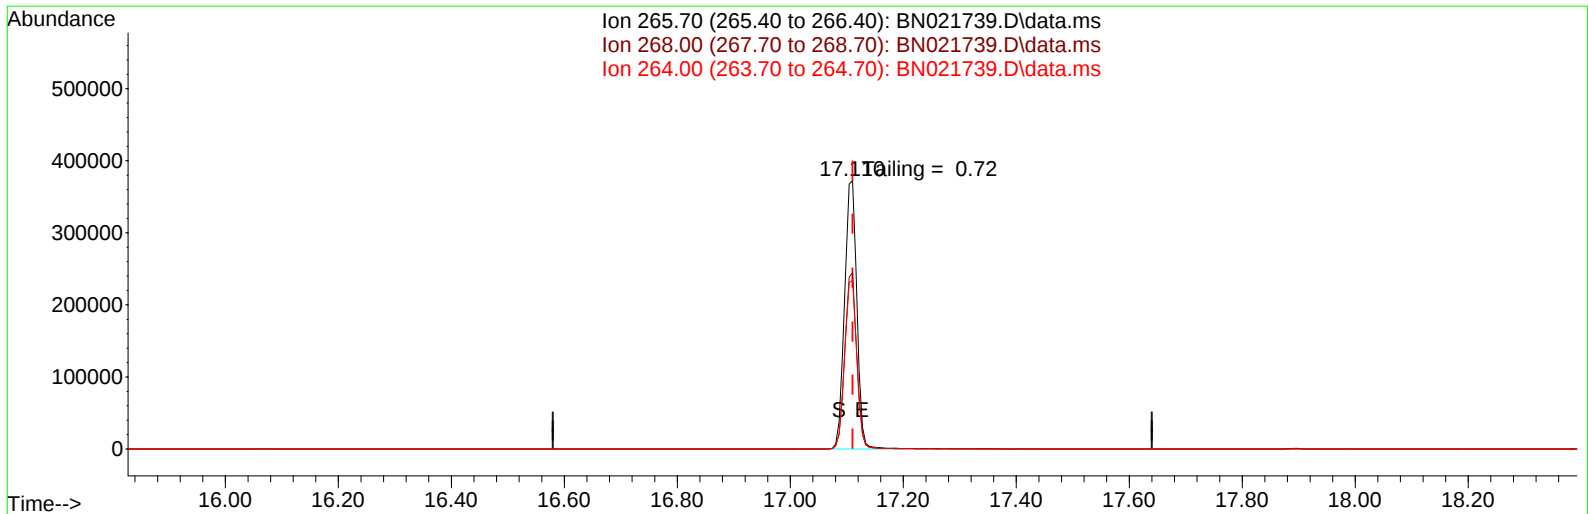

TIC: BN021739.D\data.ms

(70) Pentachlorophenol (C)

17.110min (0.000) 608469.91 ng




response 563464

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.68
264.00	61.60	62.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091422\
 Data File : BN021739.D
 Acq On : 14 Sep 2022 09:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 15 06:19:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 15 06:19:42 2022
 Response via : Initial Calibration

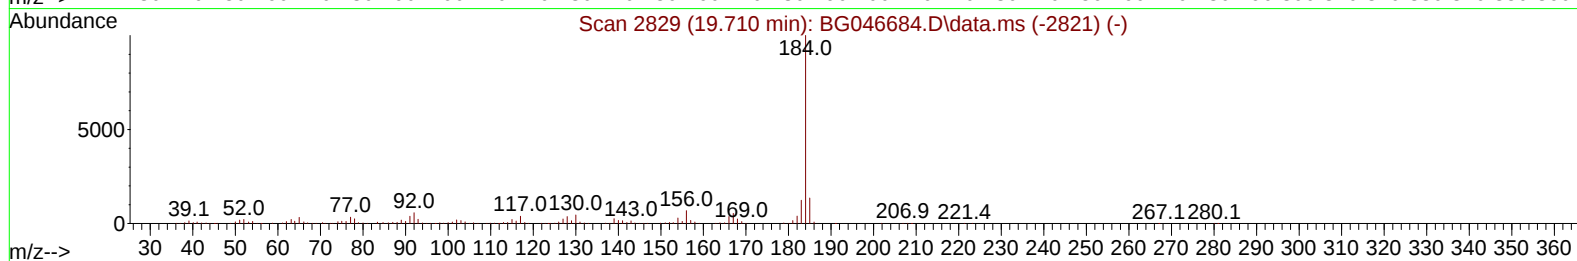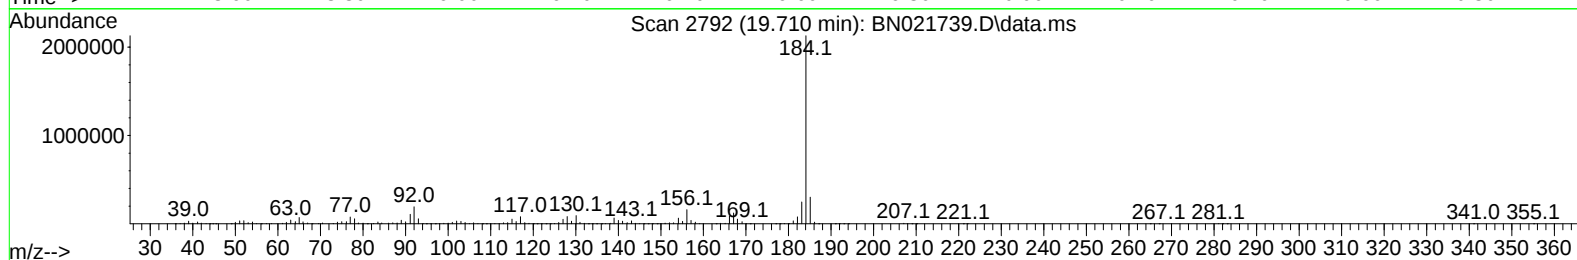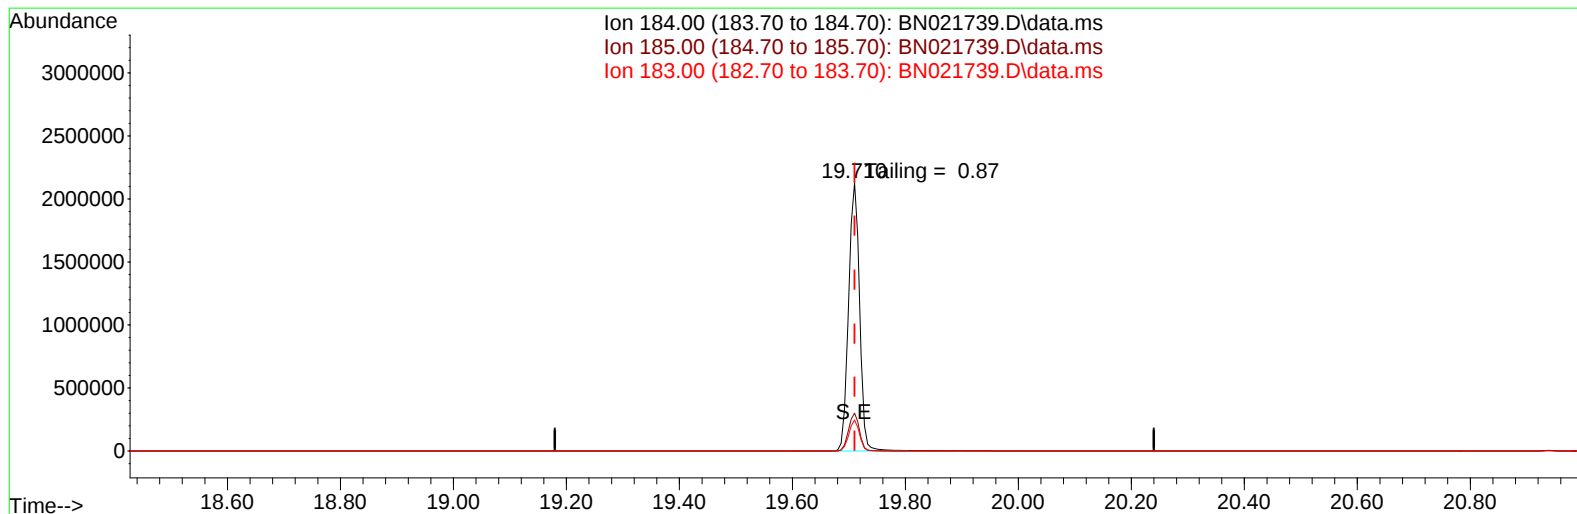

TIC: BN021739.D\data.ms

(77) Benzidine

19.710min (0.000) 203935.83 ng

response 2891743

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.17
183.00	13.20	11.59
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/14/2022	BNA_N	<u>BN021739.D</u>
Compound Name	Response	Retention Time
DDT	1363194	20.939
DDD	25852	20.498
DDE	2228	19.986
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28080	1391274	2.02

Instrument :
BNA_N
ClientSampleId :
DFTPP