


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091422\
 Data File : BN021757.D
 Acq On : 14 Sep 2022 21:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 14 01:55:04 2022

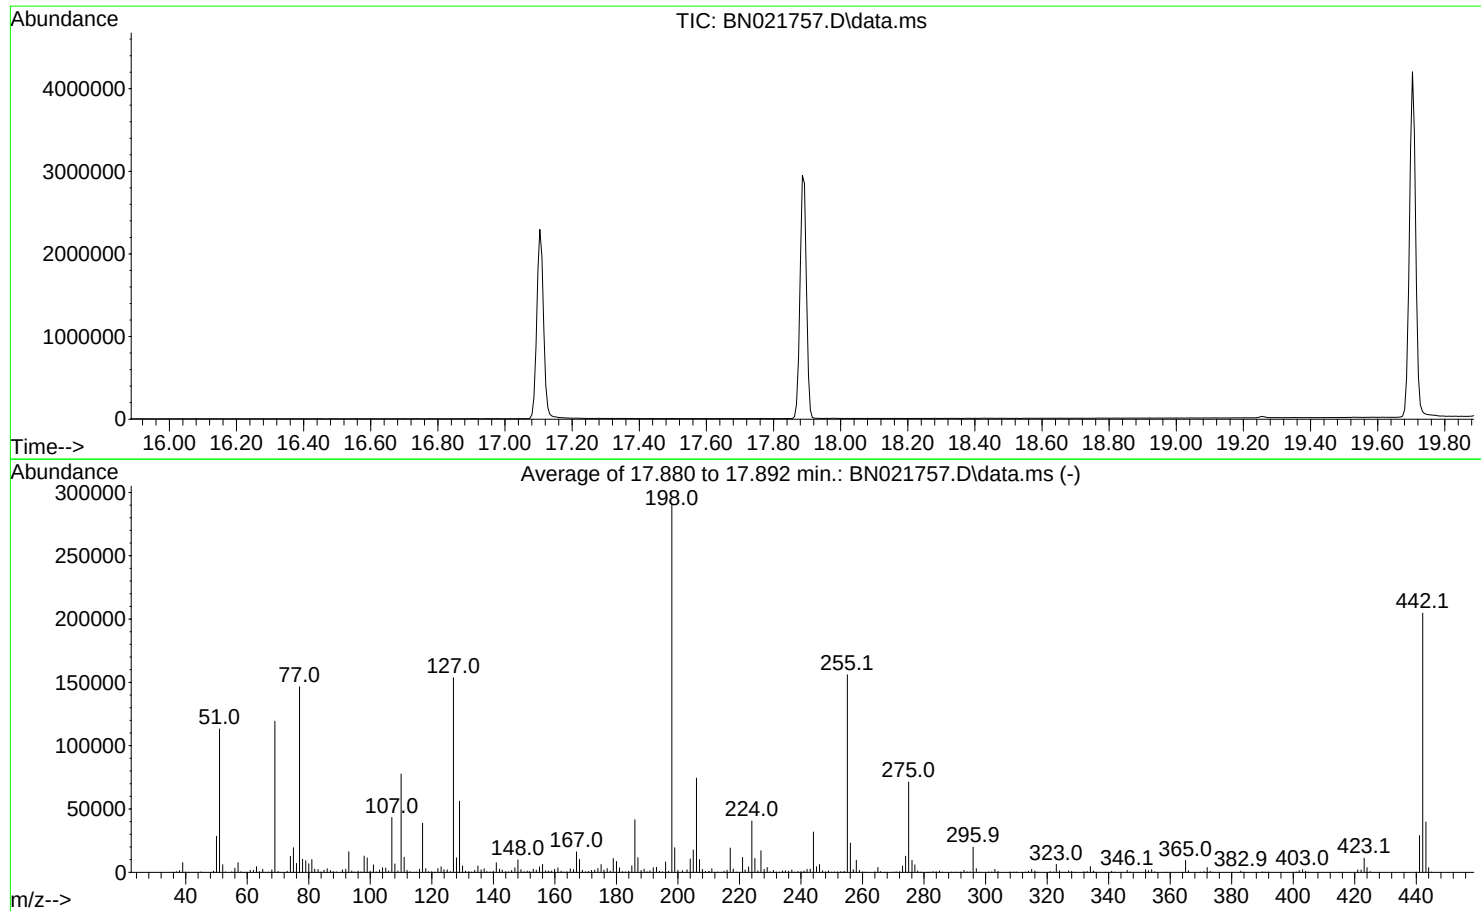




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	113216	PASS
68	69	0.00	2	1.7	1981	PASS
69	198	0.00	100	41.1	119405	PASS
70	69	0.00	2	0.6	661	PASS
127	198	10	80	52.9	153765	PASS
197	198	0.00	2	0.3	847	PASS
198	198	100	100	100.0	290539	PASS
199	198	5	9	6.7	19400	PASS
275	198	10	60	24.5	71237	PASS
365	198	1	100	3.2	9394	PASS
441	198	0.01	100	10.0	29051	PASS
442	442	50	100	100.0	204701	PASS
443	442	15	24	19.4	39709	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091422\
 Data File : BN021757.D
 Acq On : 14 Sep 2022 21:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 15 06:21:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 15 06:19:42 2022
 Response via : Initial Calibration

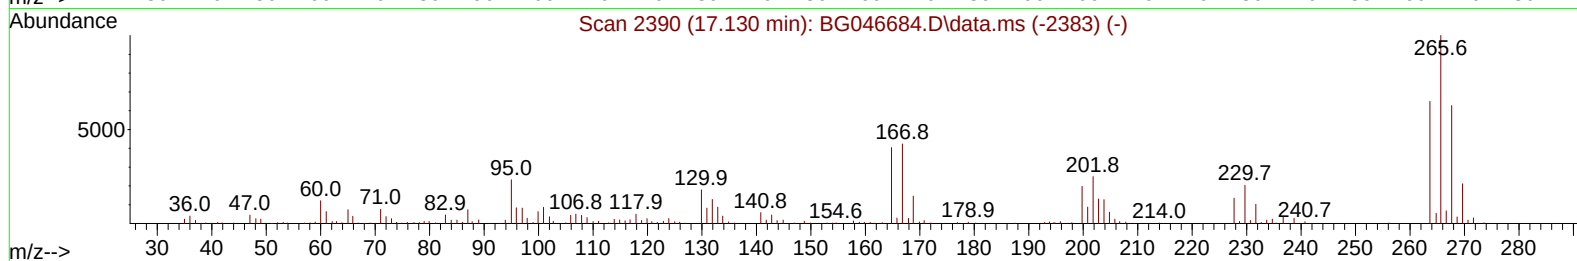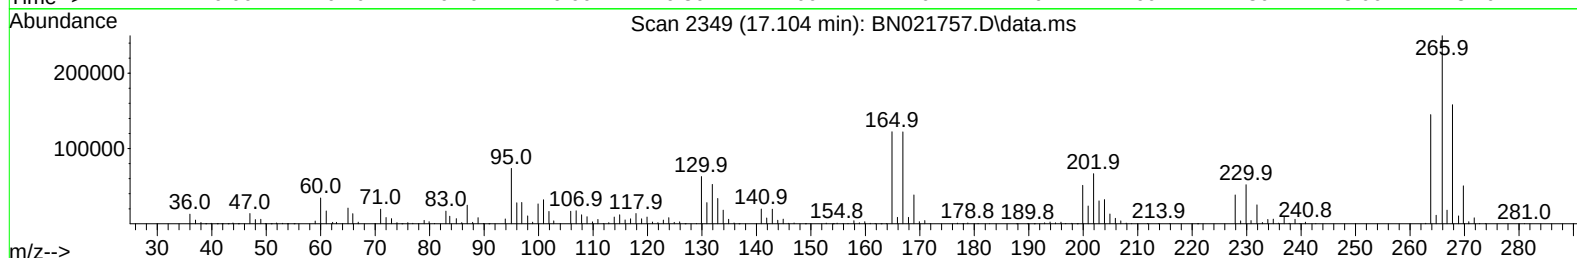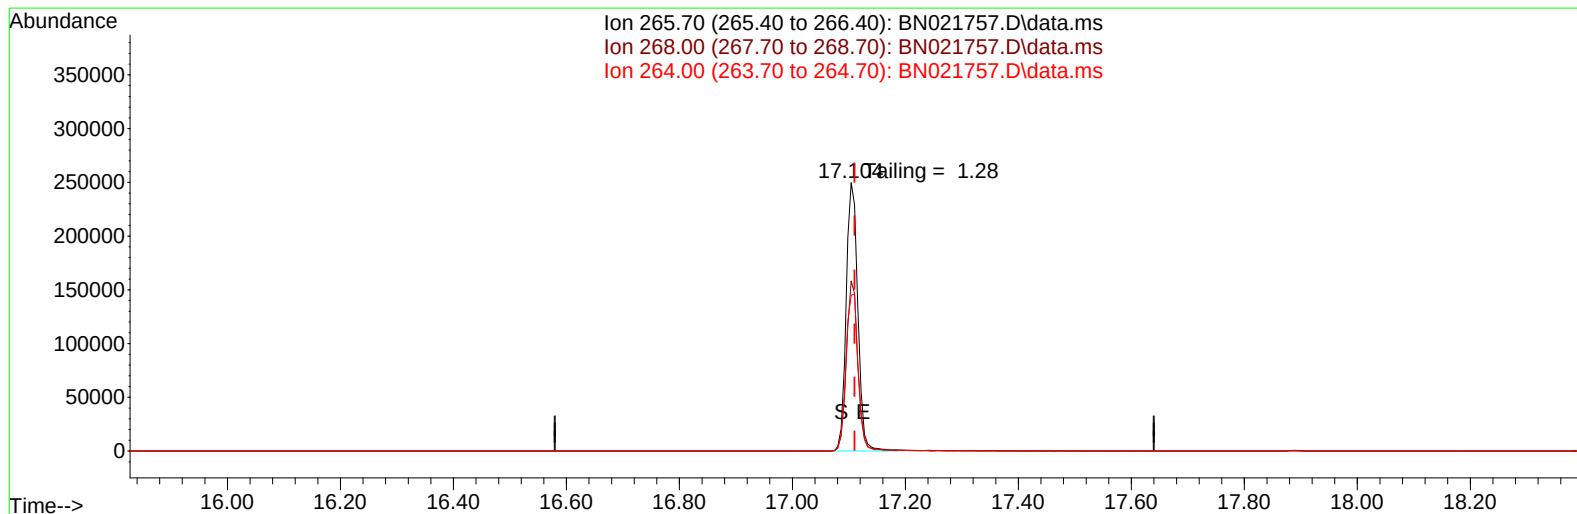

TIC: BN021757.D\data.ms

(70) Pentachlorophenol (C)

17.104min (-0.006) 20981.75 ng




response 358793

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.33
264.00	61.60	58.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091422\
 Data File : BN021757.D
 Acq On : 14 Sep 2022 21:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 15 06:21:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 15 06:19:42 2022
 Response via : Initial Calibration

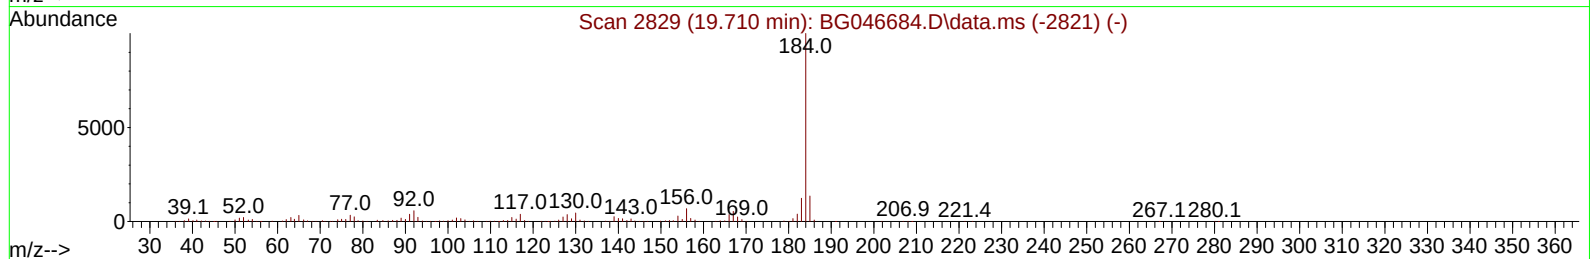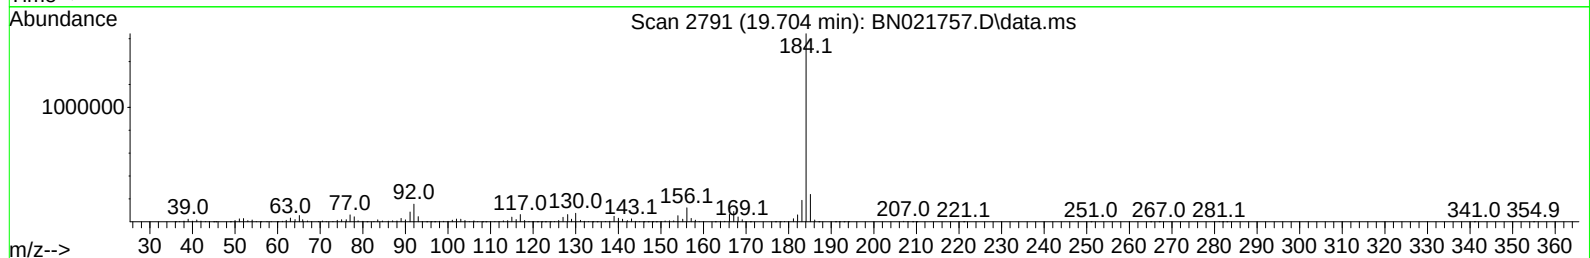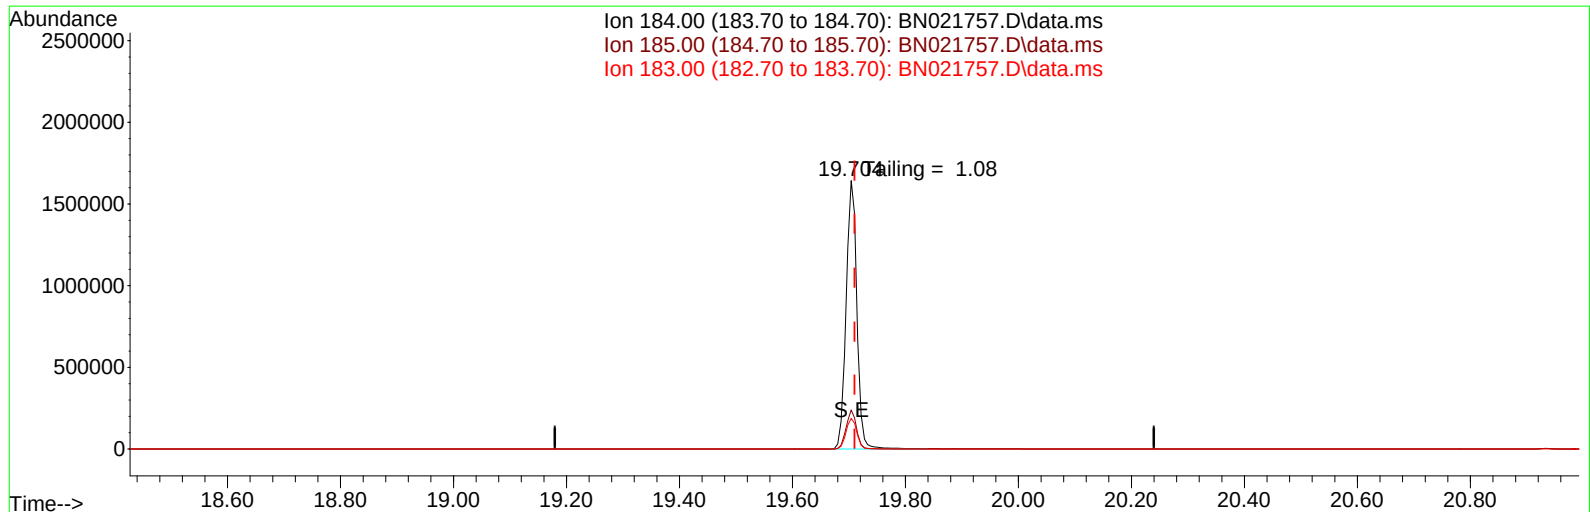

TIC: BN021757.D\data.ms

(77) Benzidine

19.704min (-0.006) 0.00 ng

response 2175915

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.53
183.00	13.20	11.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/14/2022	BNA_N	<u>BN021757.D</u>
Compound Name	Response	Retention Time
DDT	1071570	20.933
DDD	26375	20.492
DDE	1390	19.986
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27765	1099335	2.53

Instrument :
BNA_N
ClientSampleId :
DFTPP