
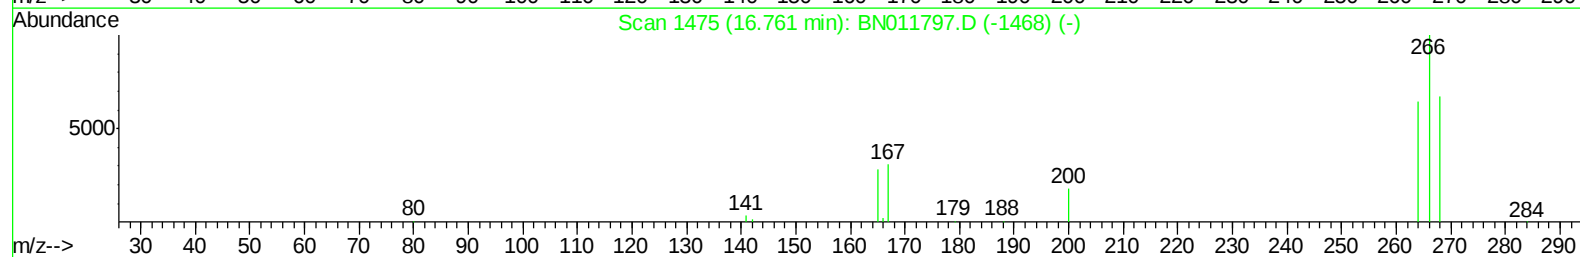
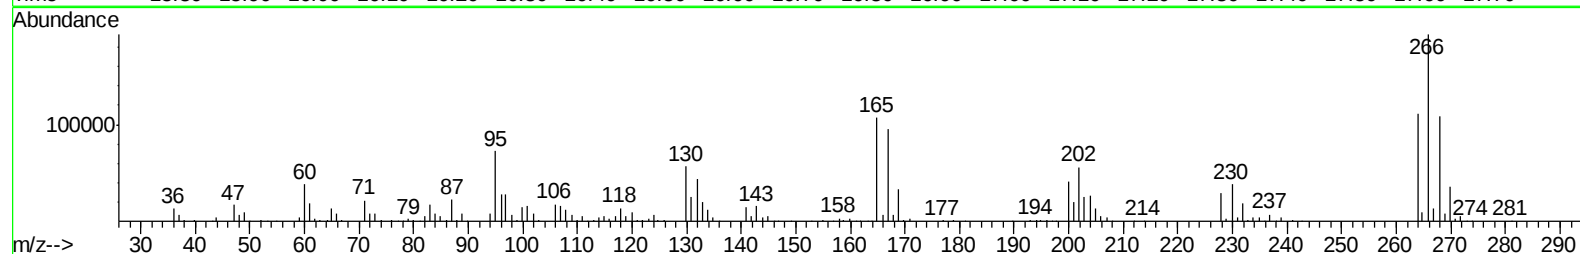


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN091520\
 Data File : BN011794.D
 Acq On : 15 Sep 2020 10:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 07:33:56 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN091520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 15 14:55:25 2020
 Response via : Initial Calibration

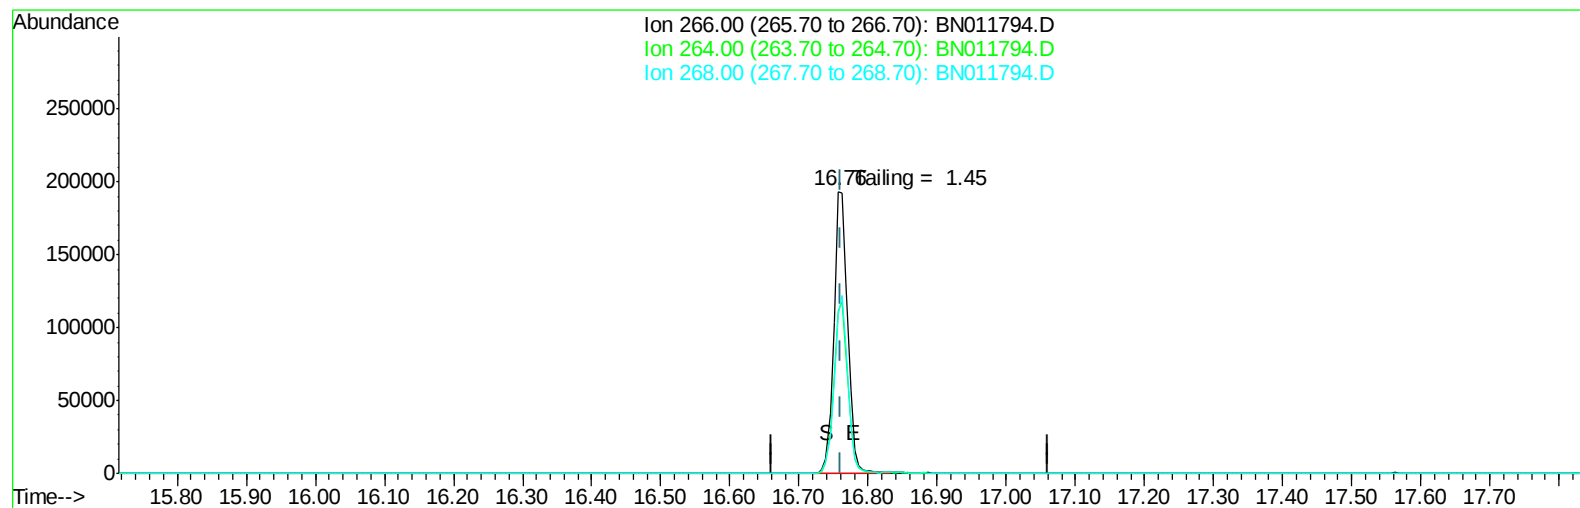

TIC: BN011794.D

(24) Pentachlorophenol

16.757min (-0.005) 0.00ng

response 269002

Ion	Exp%	Act%
266.00	100	100
264.00	64.00	61.37
268.00	65.50	62.09
0.00	0.00	0.00