


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091520\
 Data File : BN011794.D
 Acq On : 15 Sep 2020 10:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 16 12:37:34 2020

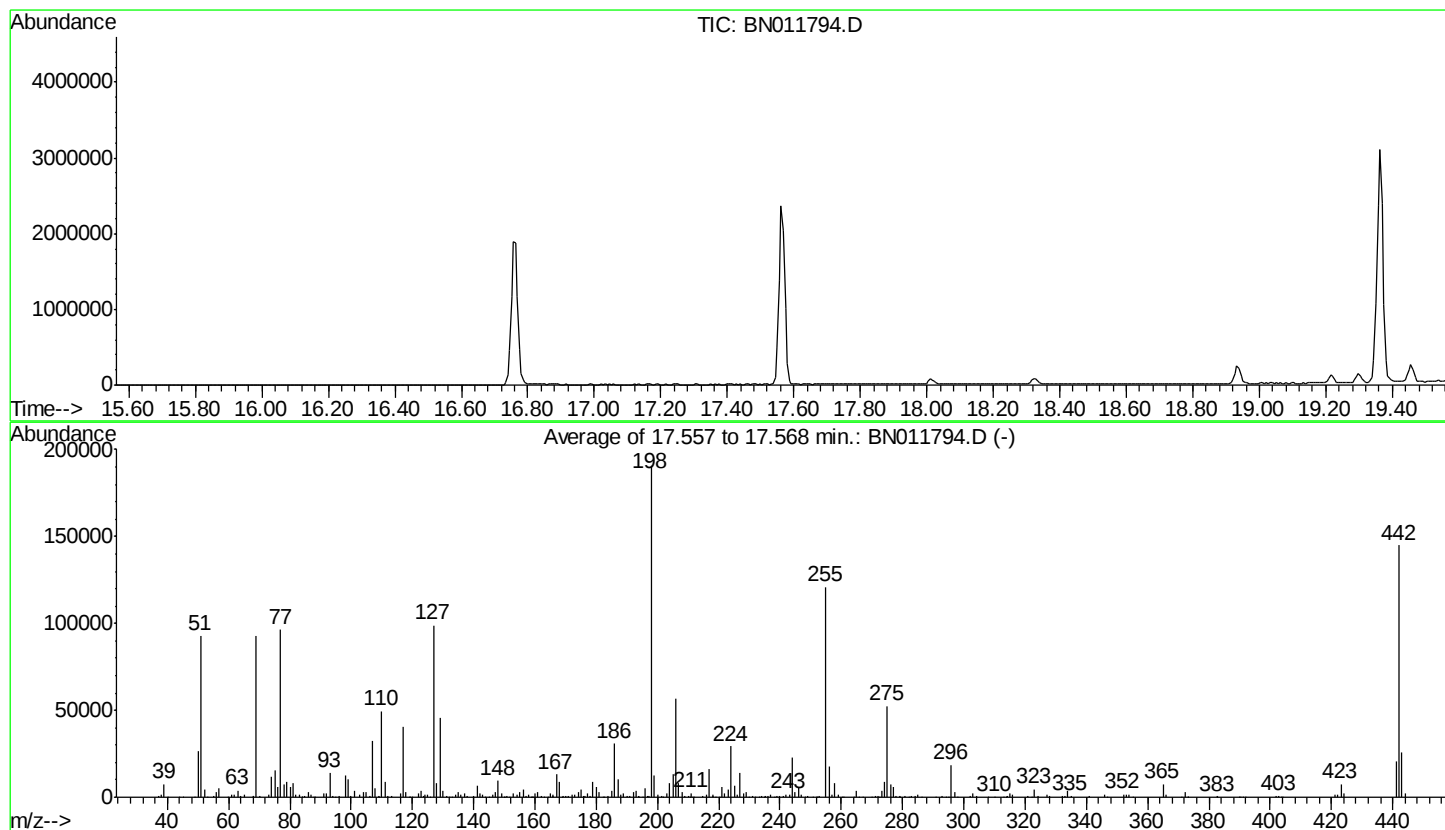

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.8	93035	PASS
68	69	0.00	2	1.1	1058	PASS
69	198	0.00	100	48.6	92770	PASS
70	69	0.00	2	0.7	604	PASS
127	198	10	80	51.9	98973	PASS
197	198	0.00	2	0.5	865	PASS
198	198	100	100	100.0	190805	PASS
199	198	5	9	6.5	12426	PASS
275	198	10	60	27.4	52341	PASS
365	198	1	100	4.1	7740	PASS
441	198	0.01	100	11.0	20903	PASS
442	198	50	100	76.0	145037	PASS
443	442	15	24	18.0	26040	PASS