

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091522\
 Data File : BN021780.D
 Acq On : 15 Sep 2022 23:34
 Operator : CG/JU
 Sample : PB147657BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB147657BL

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 09/16/2022
 Supervised By :Jagrut Upadhyay 09/16/2022

Quant Time: Sep 16 06:27:52 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 14 01:55:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.054	152	4868	0.400	ng	0.00
7) Naphthalene-d8	10.888	136	14185	0.400	ng	0.00
13) Acenaphthene-d10	14.707	164	7494	0.400	ng	0.00
19) Phenanthrene-d10	17.456	188	16124	0.400	ng	0.00
29) Chrysene-d12	21.647	240	10663	0.400	ng	# 0.00
35) Perylene-d12	24.154	264	8482	0.400	ng	#-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.584	112	4887	0.384	ng	0.00
5) Phenol-d6	7.209	99	5731	0.355	ng	0.00
8) Nitrobenzene-d5	9.233	82	4068m	0.347	ng	0.00
11) 2-Methylnaphthalene-d10	12.475	152	12631	0.353	ng	0.00
14) 2,4,6-Tribromophenol	16.209	330	709	0.207	ng	0.00
15) 2-Fluorobiphenyl	13.339	172	11423	0.373	ng	0.00
27) Fluoranthene-d10	19.490	212	16192	0.373	ng	0.00
31) Terphenyl-d14	20.080	244	10355	0.425	ng	0.00

Target Compounds Qvalue

 (#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091522\
Data File : BN021780.D
Acq On : 15 Sep 2022 23:34
Operator : CG/JU
Sample : PB147657BL
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
PB147657BL

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 09/16/2022
Supervised By :Jagrut Upadhyay 09/16/2022


Quant Time: Sep 16 06:27:52 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 14 01:55:04 2022
Response via : Initial Calibration

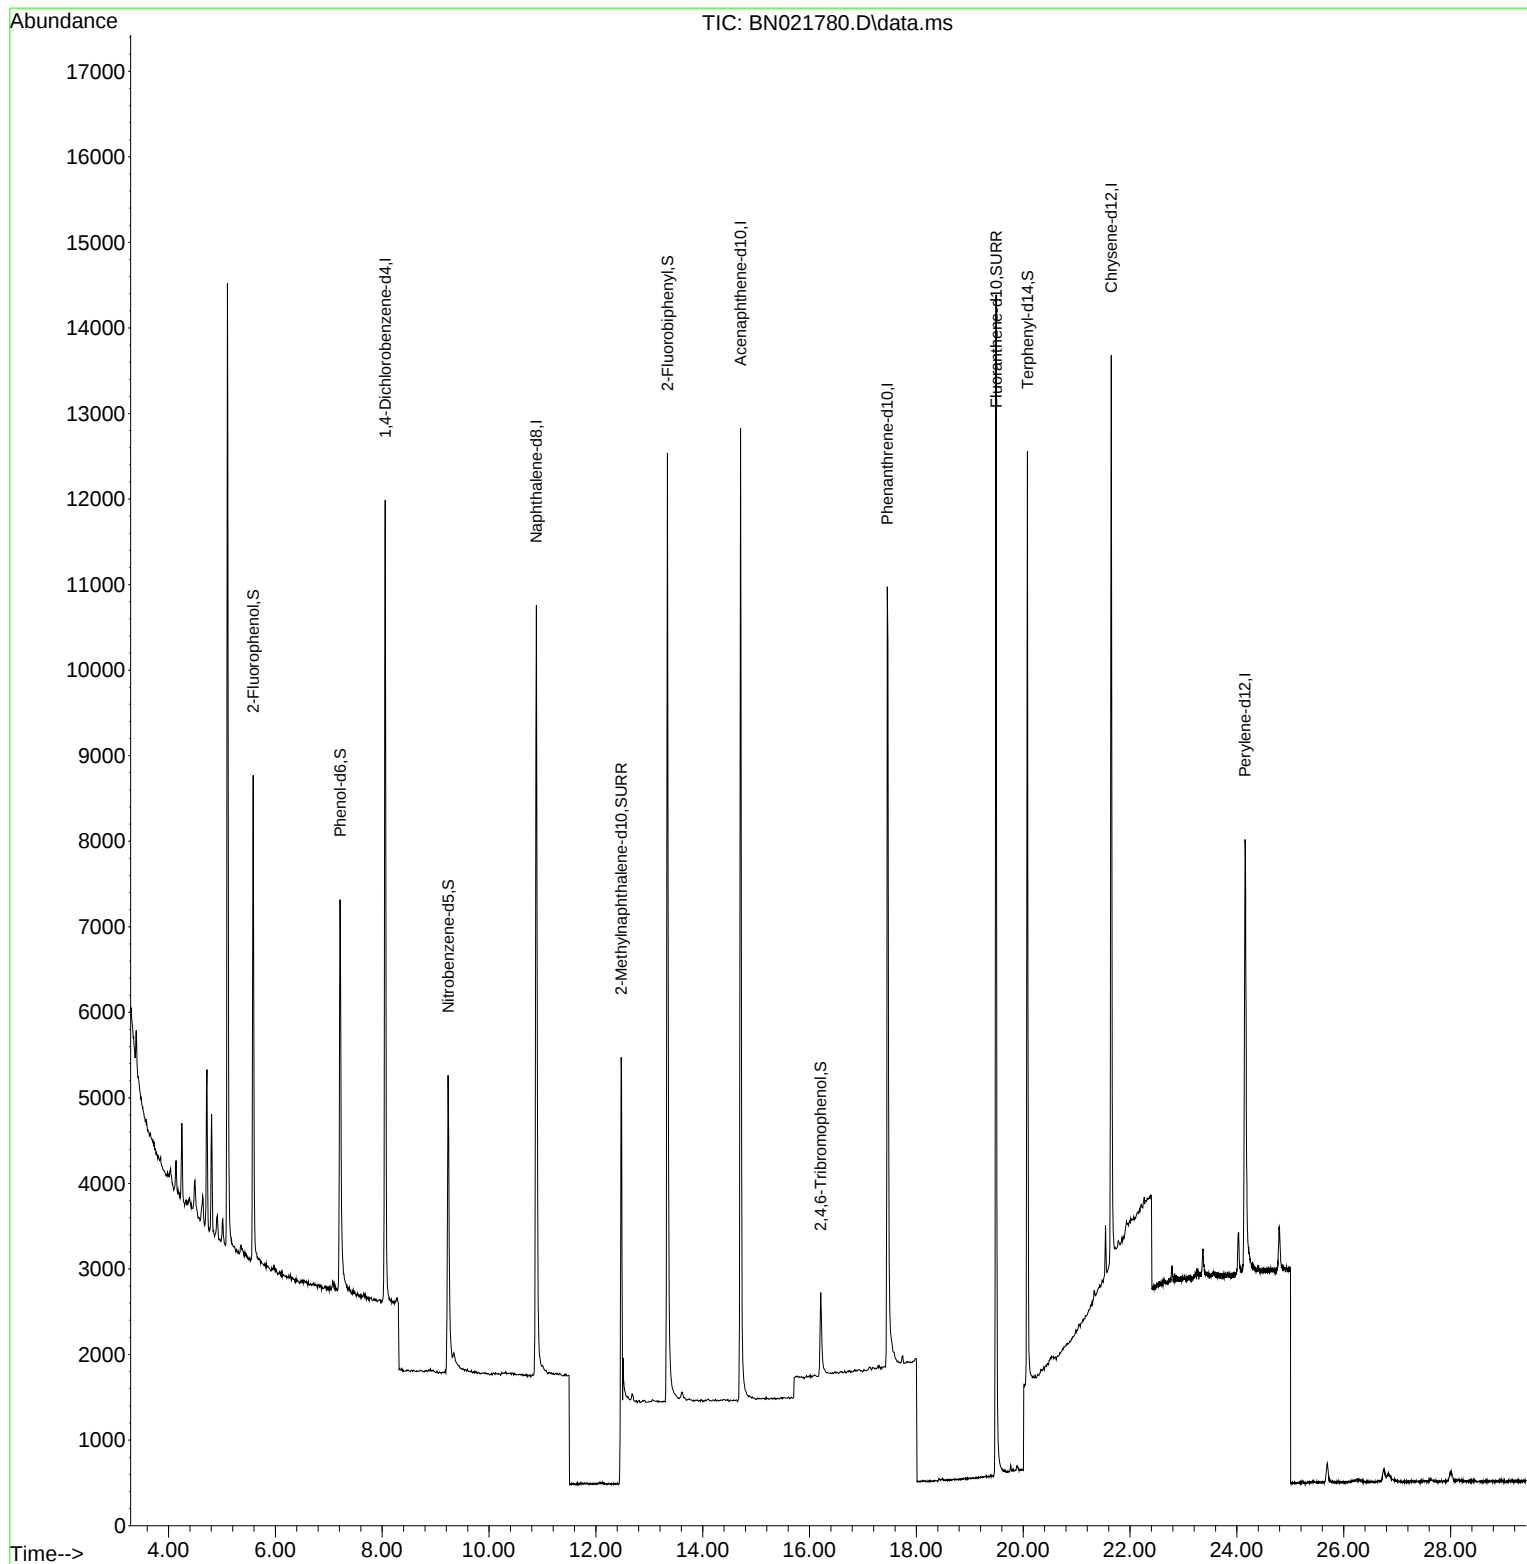

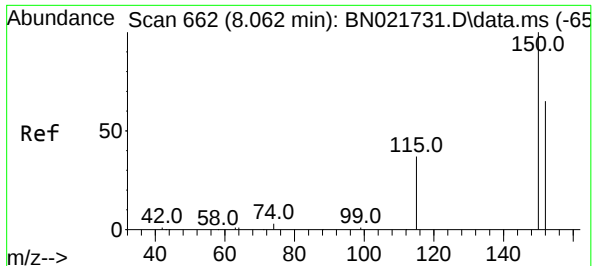

#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 8.054 min Scan# 662
Delta R.T. -0.008 min
Lab File: BN021780.D
Acq: 15 Sep 2022 23:34




Instrument :
BNA_N
ClientSampleId :
PB147657BL

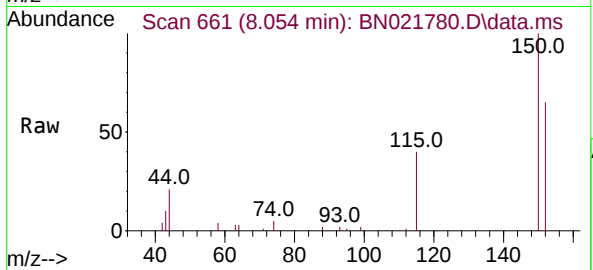

Tgt Ion:152 Resp: 4868
Ion Ratio Lower Upper
152 100
150 155.0 121.8 182.8
115 61.6 48.3 72.5




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 09/16/2022
Supervised By :Jagrut Upadhyay 09/16/2022

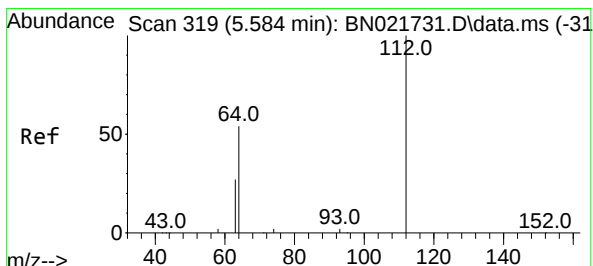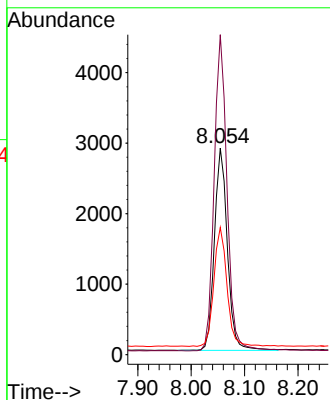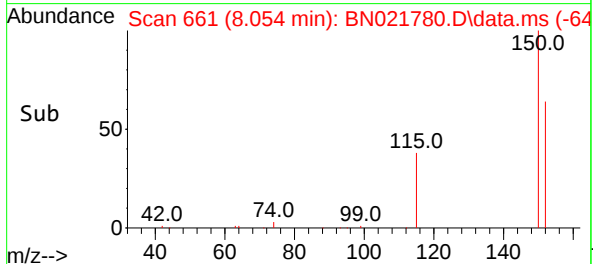

#4
2-Fluorophenol
Concen: 0.384 ng
RT: 5.584 min Scan# 319
Delta R.T. -0.000 min
Lab File: BN021780.D
Acq: 15 Sep 2022 23:34


Tgt Ion:112 Resp: 4887
Ion Ratio Lower Upper
112 100
64 57.1 45.4 68.2
63 29.5 23.3 34.9

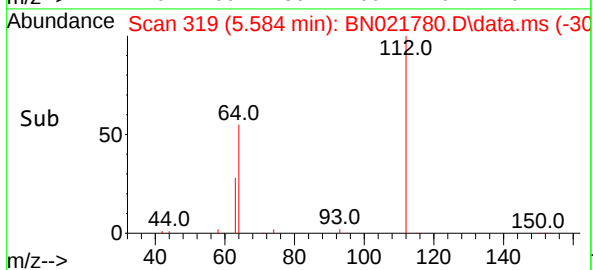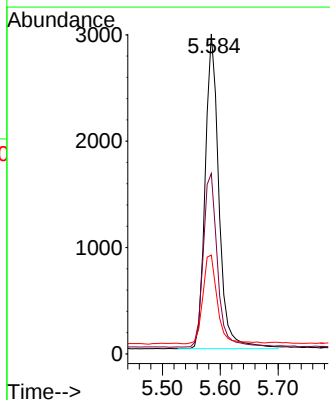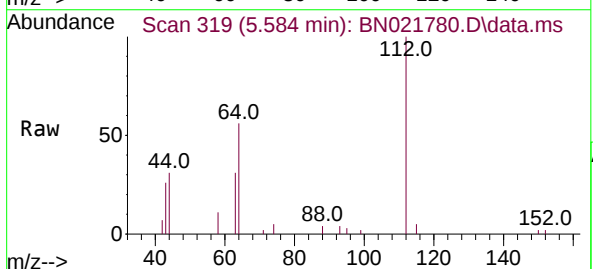

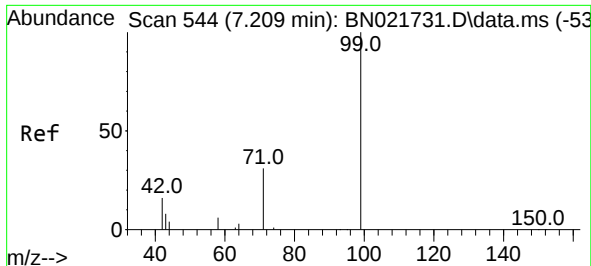

#5
Phenol-d6
Concen: 0.355 ng
RT: 7.209 min Scan# 544
Delta R.T. -0.000 min
Lab File: BN021780.D
Acq: 15 Sep 2022 23:34




Instrument :
BNA_N
ClientSampleId :
PB147657BL

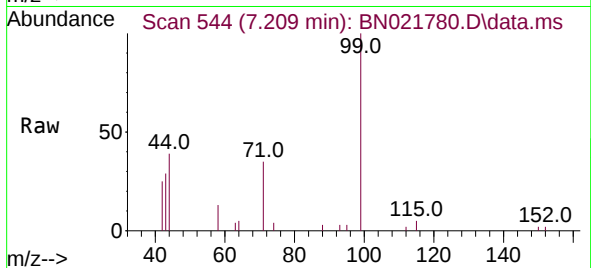


Tgt Ion: 99 Resp: 5731
Ion Ratio Lower Upper
99 100
42 18.6 15.1 22.7
71 31.8 25.3 37.9

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 09/16/2022
Supervised By :Jagrut Upadhyay 09/16/2022

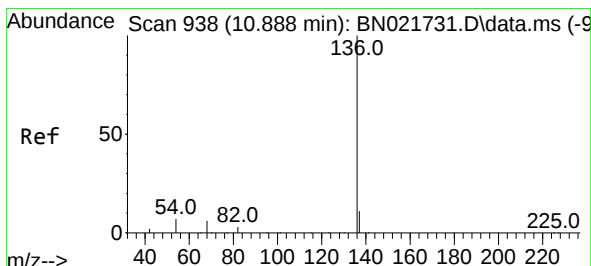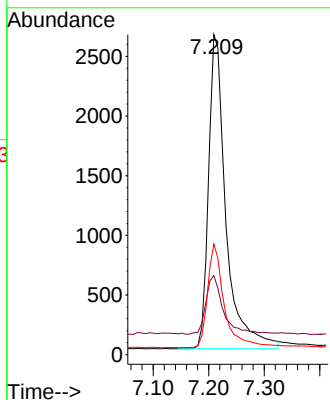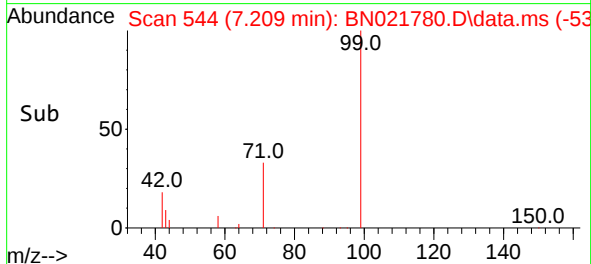


#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.888 min Scan# 938
Delta R.T. -0.000 min
Lab File: BN021780.D
Acq: 15 Sep 2022 23:34

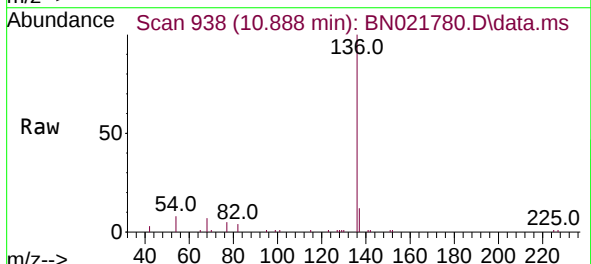


Tgt Ion:136 Resp: 14185
Ion Ratio Lower Upper
136 100
137 11.5 9.1 13.7
54 7.7 6.4 9.6
68 6.5 5.5 8.3

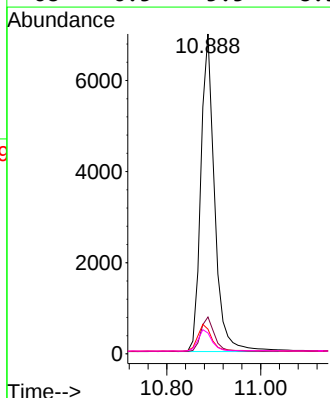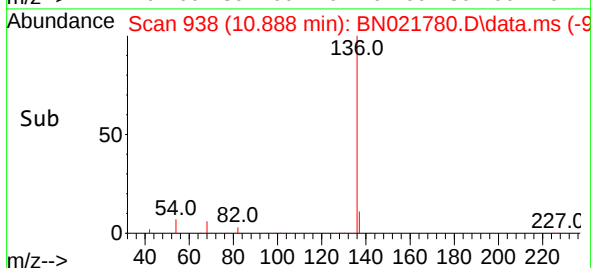

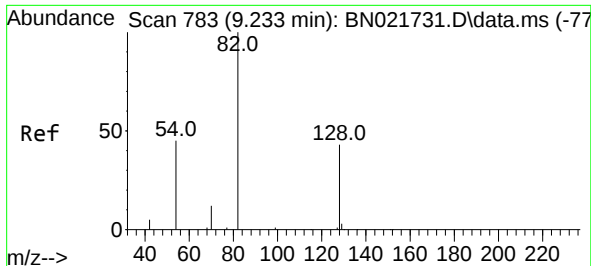

#8
Nitrobenzene-d5
Concen: 0.347 ng m
RT: 9.233 min Scan# 783
Delta R.T. -0.000 min
Lab File: BN021780.D
Acq: 15 Sep 2022 23:34




Instrument :
BNA_N
ClientSampleId :
PB147657BL

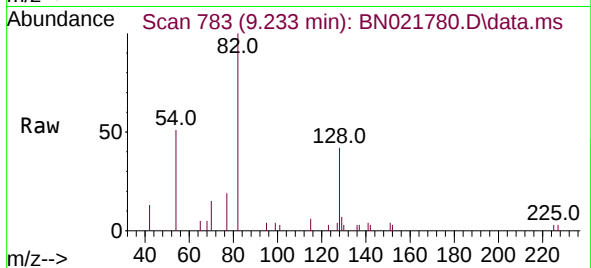

Tgt Ion: 82 Resp: 4068
Ion Ratio Lower Upper
82 100
128 41.6 35.6 53.4
54 50.6 37.8 56.8




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 09/16/2022
Supervised By :Jagrut Upadhyay 09/16/2022

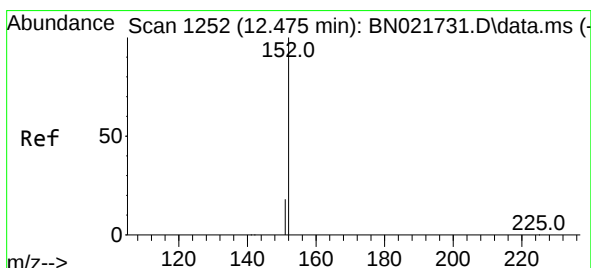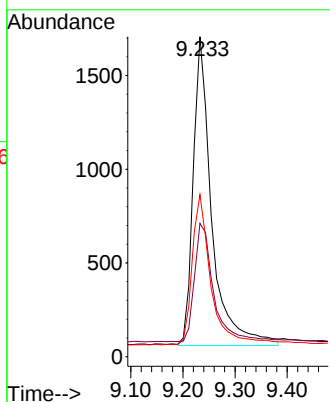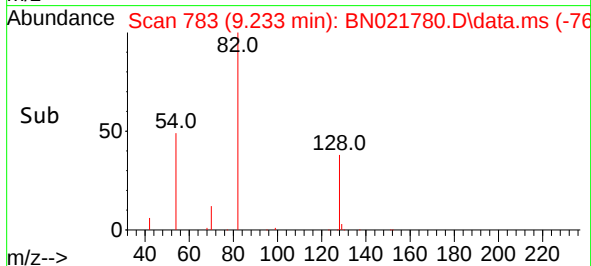

#11
2-Methylnaphthalene-d10
Concen: 0.353 ng
RT: 12.475 min Scan# 1252
Delta R.T. -0.000 min
Lab File: BN021780.D
Acq: 15 Sep 2022 23:34


Tgt Ion:152 Resp: 12631
Ion Ratio Lower Upper
152 100
151 21.5 15.6 23.4

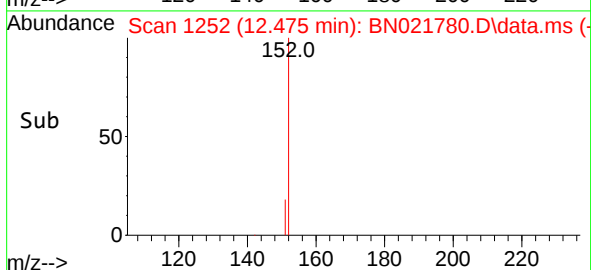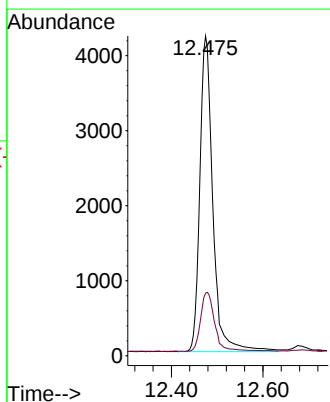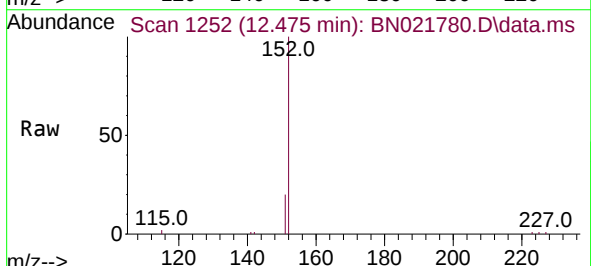

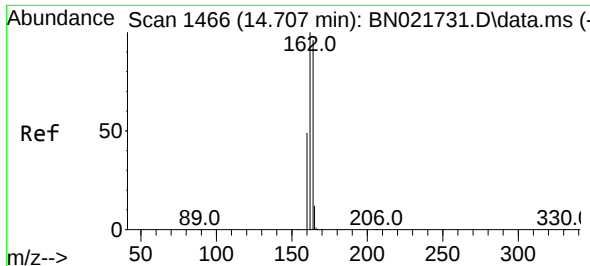

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.707 min Scan# 1466
Delta R.T. -0.000 min
Lab File: BN021780.D
Acq: 15 Sep 2022 23:34




Instrument :
BNA_N
ClientSampleId :
PB147657BL




Tgt Ion:164 Resp: 7494
Ion Ratio Lower Upper
164 100
162 103.8 83.2 124.8
160 51.5 40.9 61.3

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 09/16/2022
Supervised By :Jagrut Upadhyay 09/16/2022

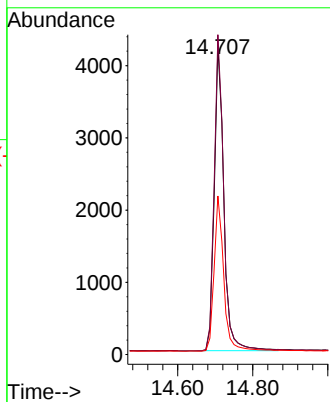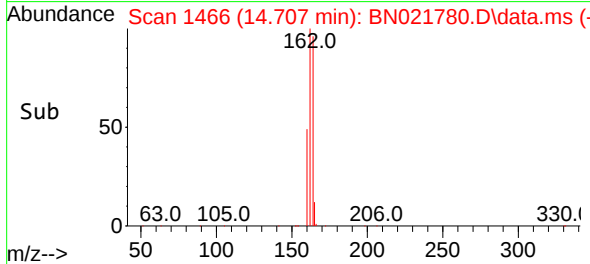


#14
2,4,6-Tribromophenol
Concen: 0.207 ng
RT: 16.209 min Scan# 1603
Delta R.T. -0.000 min
Lab File: BN021780.D
Acq: 15 Sep 2022 23:34

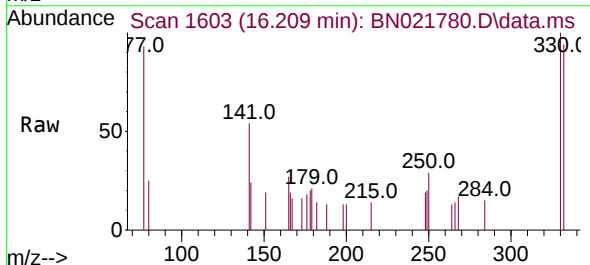


Tgt Ion:330 Resp: 709
Ion Ratio Lower Upper
330 100
332 95.9 76.8 115.2
141 49.8 37.2 55.8

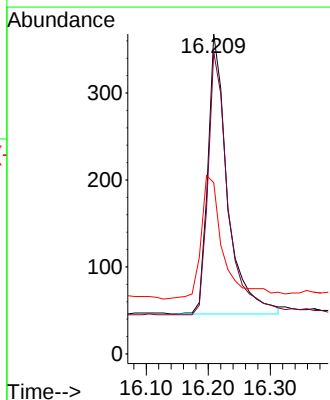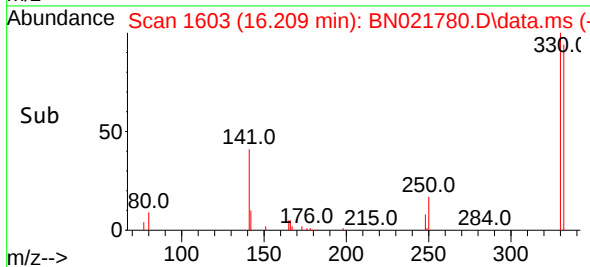



#15
2-Fluorobiphenyl
Concen: 0.373 ng
RT: 13.339 min Scan# 1338
Delta R.T. -0.000 min
Lab File: BN021780.D
Acq: 15 Sep 2022 23:34




Instrument :
BNA_N
ClientSampleId :
PB147657BL




Tgt Ion:172 Resp: 11423
Ion Ratio Lower Upper
172 100
171 35.4 27.7 41.5
170 24.3 18.8 28.2

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 09/16/2022
Supervised By :Jagrut Upadhyay 09/16/2022

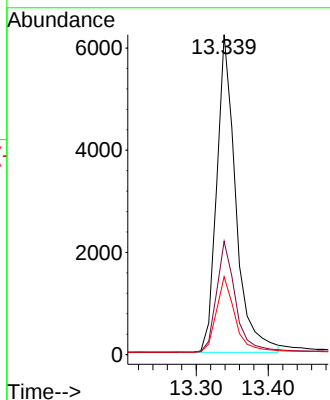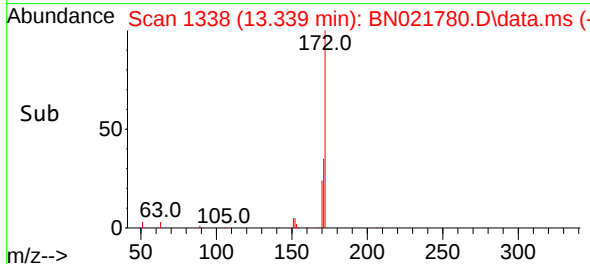


#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.456 min Scan# 1711
Delta R.T. -0.000 min
Lab File: BN021780.D
Acq: 15 Sep 2022 23:34

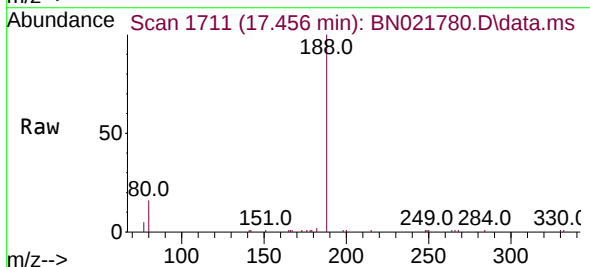


Tgt Ion:188 Resp: 16124
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 16.4 12.6 19.0

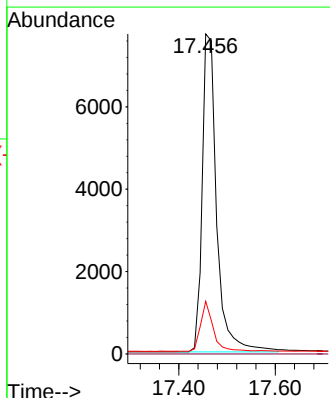



#27
Fluoranthene-d10
Concen: 0.373 ng
RT: 19.490 min Scan# 2111
Delta R.T. -0.004 min
Lab File: BN021780.D
Acq: 15 Sep 2022 23:34




Instrument :
BNA_N
ClientSampleId :
PB147657BL



Tgt Ion:212 Resp: 16192
Ion Ratio Lower Upper
212 100
106 18.1 14.3 21.5
104 10.3 8.0 12.0




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 09/16/2022
Supervised By :Jagrut Upadhyay 09/16/2022

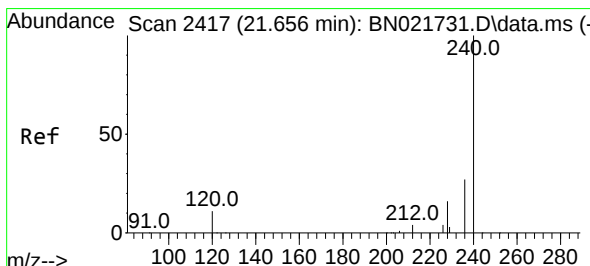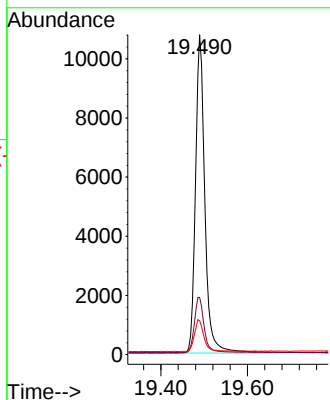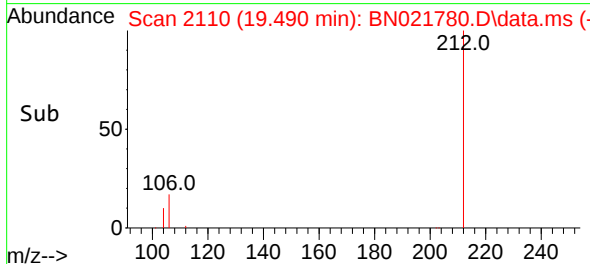

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.647 min Scan# 2416
Delta R.T. -0.009 min
Lab File: BN021780.D
Acq: 15 Sep 2022 23:34

Tgt Ion:240 Resp: 10663
Ion Ratio Lower Upper
240 100
120 17.6 9.8 14.8#
236 28.3 22.2 33.4

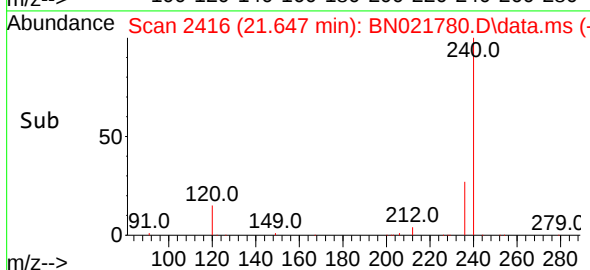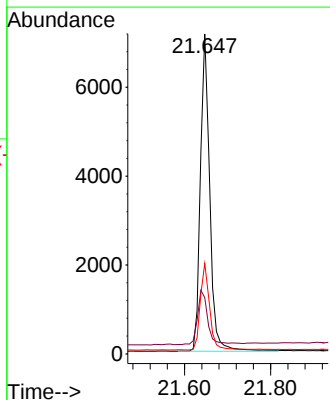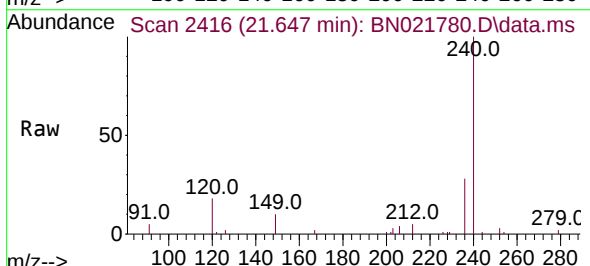




#31
 Terphenyl-d14
 Concen: 0.425 ng
 RT: 20.080 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN021780.D
 Acq: 15 Sep 2022 23:34

Instrument :

BNA_N

ClientSampleId :

PB147657BL






Tgt Ion:244 Resp: 1035
 Ion Ratio Lower Upper
 244 100
 212 8.5 7.9 11.9
 122 13.7 15.8 23.8


Manual Integrations

APPROVED

Reviewed By :Christian Giraldo 09/16/2022
 Supervised By :Jagrut Upadhyay 09/16/2022

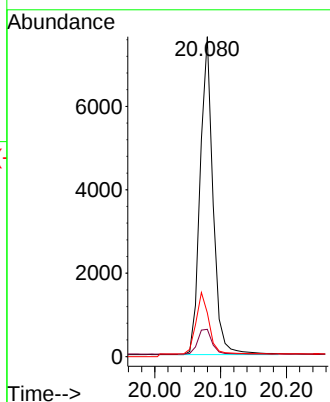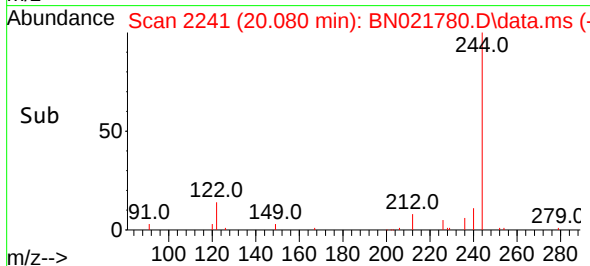

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.154 min Scan# 3098
 Delta R.T. -0.015 min
 Lab File: BN021780.D
 Acq: 15 Sep 2022 23:34

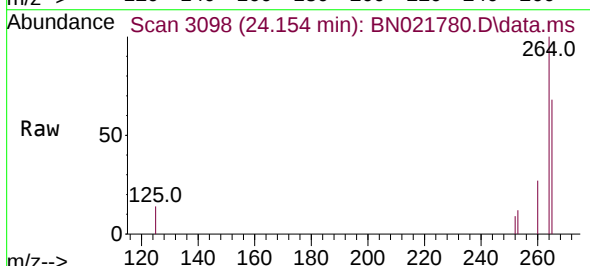

Tgt Ion:264 Resp: 8482
 Ion Ratio Lower Upper
 264 100
 260 26.8 20.6 31.0
 265 67.7 34.4 51.6

