


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091522\
 Data File : BN021778.D
 Acq On : 15 Sep 2022 21:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 14 01:55:04 2022

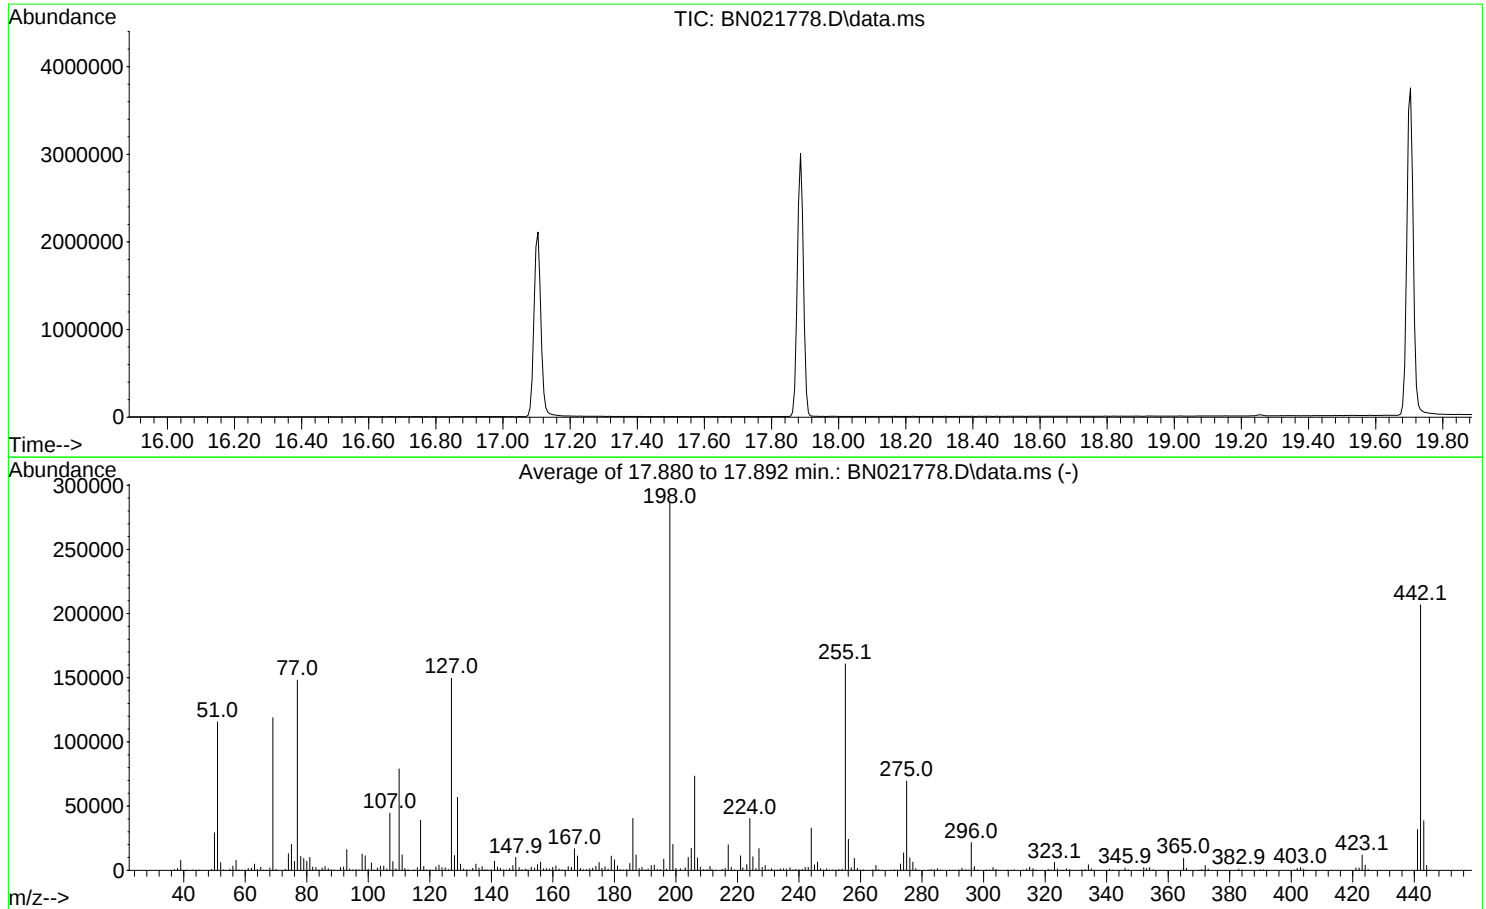




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	115584	PASS
68	69	0.00	2	1.6	1886	PASS
69	198	0.00	100	41.5	118933	PASS
70	69	0.00	2	0.6	695	PASS
127	198	10	80	52.2	149725	PASS
197	198	0.00	2	0.3	942	PASS
198	198	100	100	100.0	286613	PASS
199	198	5	9	7.0	20189	PASS
275	198	10	60	24.2	69499	PASS
365	198	1	100	3.3	9380	PASS
441	198	0.01	100	11.1	31781	PASS
442	442	50	100	100.0	206869	PASS
443	442	15	24	18.7	38587	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091522\
 Data File : BN021778.D
 Acq On : 15 Sep 2022 21:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 16 07:53:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 16 07:52:15 2022
 Response via : Initial Calibration

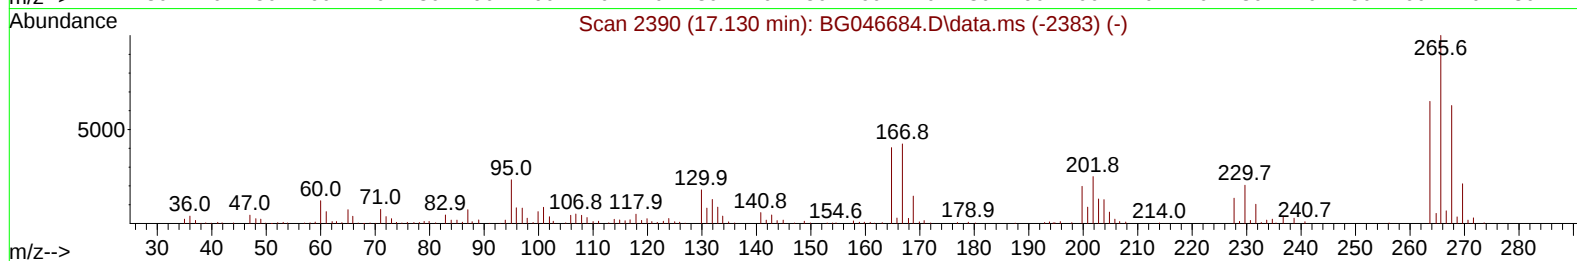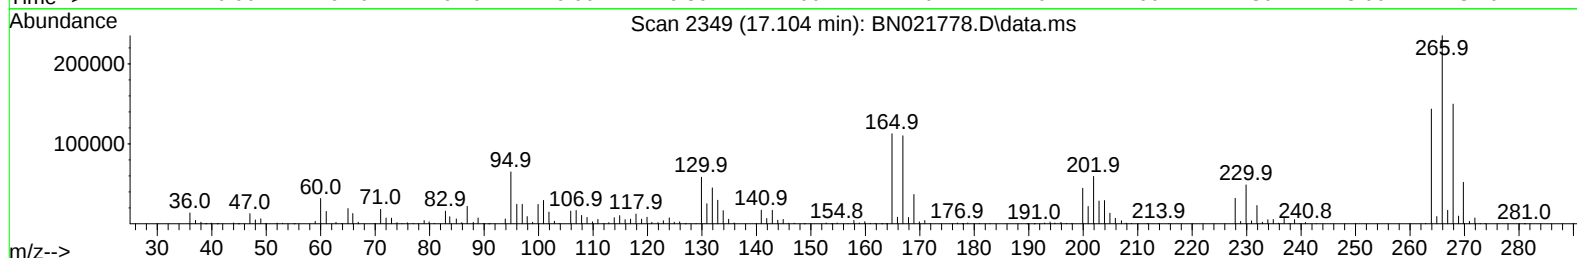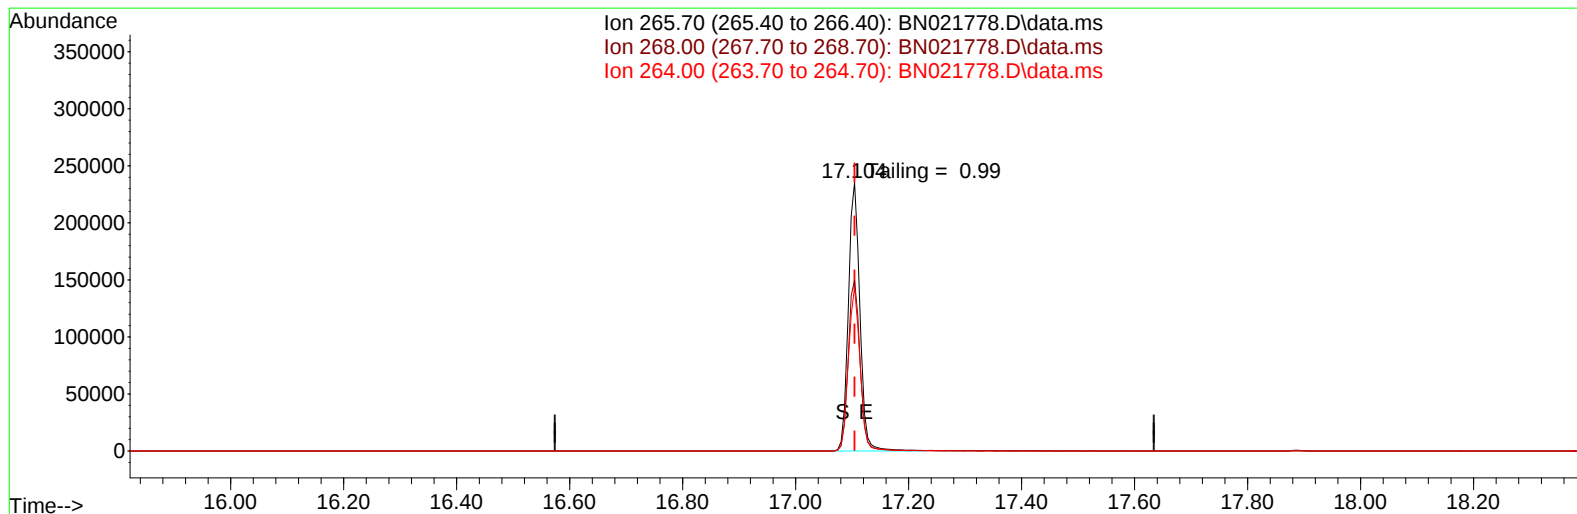

TIC: BN021778.D\data.ms

(70) Pentachlorophenol (C)

17.104min (-0.000) 20199.75 ng




response 334007

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.66
264.00	61.60	61.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091522\
Data File : BN021778.D
Acq On : 15 Sep 2022 21:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 16 07:53:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 16 07:52:15 2022
Response via : Initial Calibration

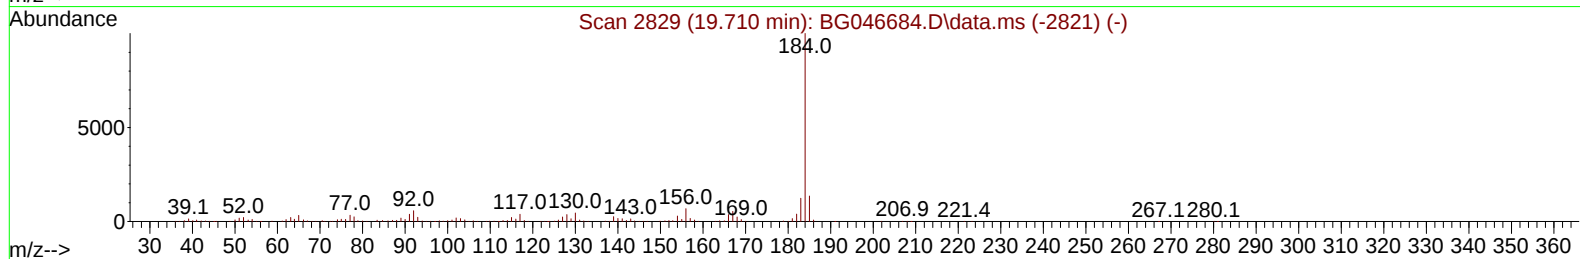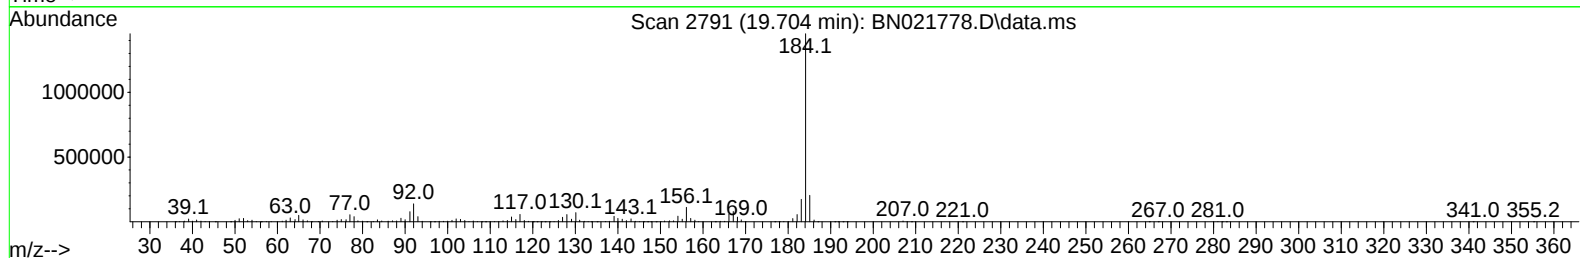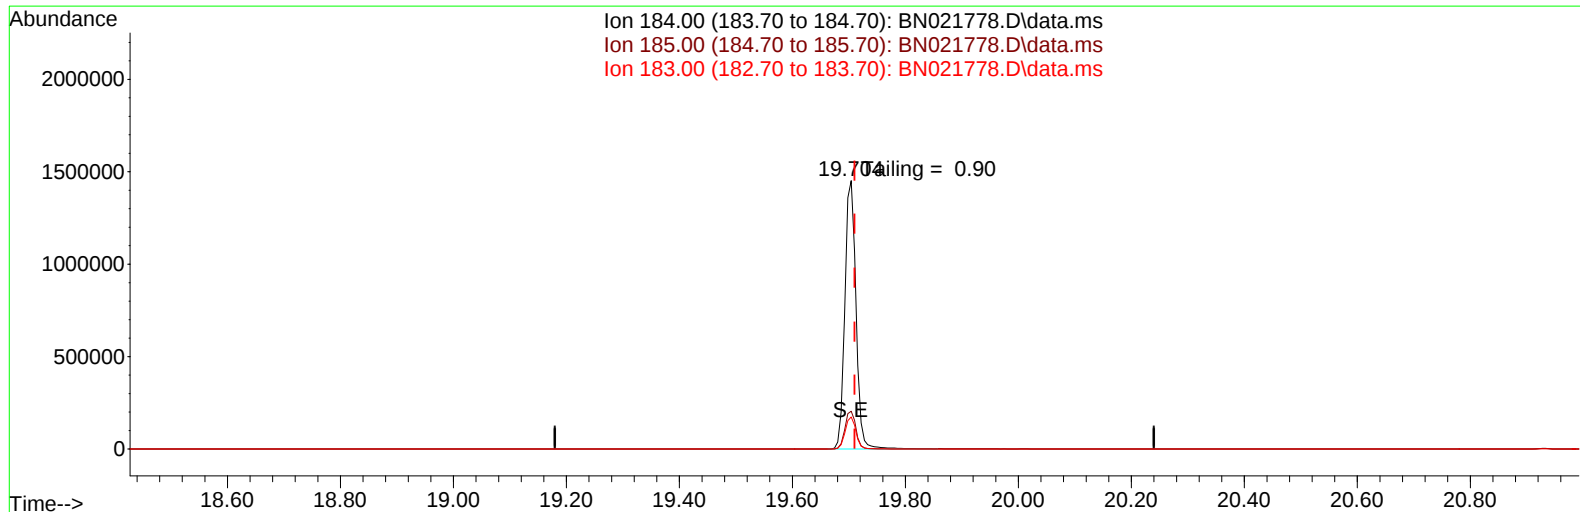

TIC: BN021778.D\data.ms

(77) Benzidine

19.704min (-0.006) 0.00 ng

response 1976164

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.09
183.00	13.20	11.93
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/15/2022	BNA_N	<u>BN021778.D</u>
Compound Name	Response	Retention Time
DDT	1003531	20.933
DDD	22750	20.492
DDE	1919	19.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24669	1028200	2.40

Instrument :
BNA_N
ClientSampleId :
DFTPP