

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091622\
 Data File : BN021785.D
 Acq On : 16 Sep 2022 12:50
 Operator : CG/JU
 Sample : PB147637BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK637

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
 Title : SVOA CALIBRATION

Signal : TIC: BN021785.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	7	12	20	rVB	46139	67877	1.54%	0.148%
2	3.787	82	85	113	rBV	516793	864511	19.60%	1.882%
3	4.134	140	144	151	rVB	17730	27599	0.63%	0.060%
4	7.199	658	665	679	rVB	721815	1149285	26.06%	2.502%
5	7.369	685	694	708	rVB	613300	980340	22.23%	2.134%
6	7.569	721	728	742	rBV	720902	1150772	26.09%	2.505%
7	8.046	802	809	820	rVB	588331	937581	21.26%	2.041%
8	8.763	924	931	941	rBV	895395	1471534	33.36%	3.203%
9	9.222	1002	1009	1018	rBV	703017	1160413	26.31%	2.526%
10	9.952	1126	1133	1147	rBV	559497	931059	21.11%	2.027%
11	10.493	1216	1225	1236	rBV	881807	1487399	33.72%	3.238%
12	10.875	1282	1290	1301	rBV	893107	1500728	34.02%	3.267%
13	11.016	1306	1314	1328	rBV	937595	1617502	36.67%	3.521%
14	12.463	1555	1560	1570	rVB	15772	26749	0.61%	0.058%
15	14.110	1834	1840	1851	rVB	1706806	2385230	54.08%	5.192%
16	14.398	1882	1889	1900	rBV	1875909	2794922	63.37%	6.083%
17	14.704	1934	1941	1949	rBV	1382889	2115987	47.97%	4.606%
18	14.898	1968	1974	1997	rBV	719278	1108581	25.13%	2.413%
19	15.698	2103	2110	2120	rVB	2391784	3554700	80.59%	7.737%
20	15.810	2123	2129	2144	rBV	606774	825203	18.71%	1.796%
21	15.934	2146	2150	2156	rBV	20632	29998	0.68%	0.065%
22	16.481	2239	2243	2246	rBV2	5930	7223	0.16%	0.016%
23	17.239	2366	2372	2376	rBV5	2749	5861	0.13%	0.013%
24	17.457	2402	2409	2419	rBV	1760829	2521283	57.16%	5.488%
25	17.557	2419	2426	2445	rVV	2659144	3899977	88.42%	8.489%
26	19.410	2737	2741	2748	rBV2	29878	43694	0.99%	0.095%
27	19.481	2749	2753	2759	rBV	29526	41027	0.93%	0.089%
28	19.851	2809	2816	2826	rBV	3134896	4410673	100.00%	9.600%
29	21.645	3116	3121	3129	rBV	1876070	2516548	57.06%	5.478%
30	23.992	3512	3520	3532	rBV2	1873767	4039797	91.59%	8.793%
31	24.151	3540	3547	3562	rVB2	1026812	2268693	51.44%	4.938%




Sum of corrected areas: 45942746

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091622\
Data File : BN021785.D
Acq On : 16 Sep 2022 12:50
Operator : CG/JU
Sample : PB147637BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK637

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

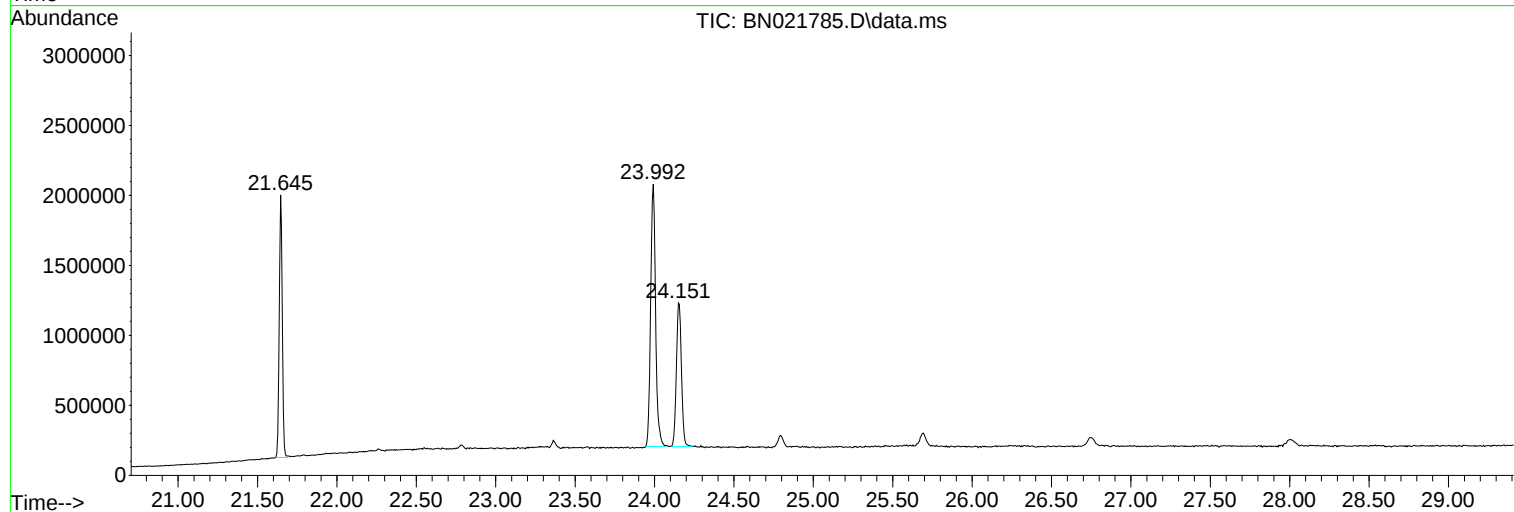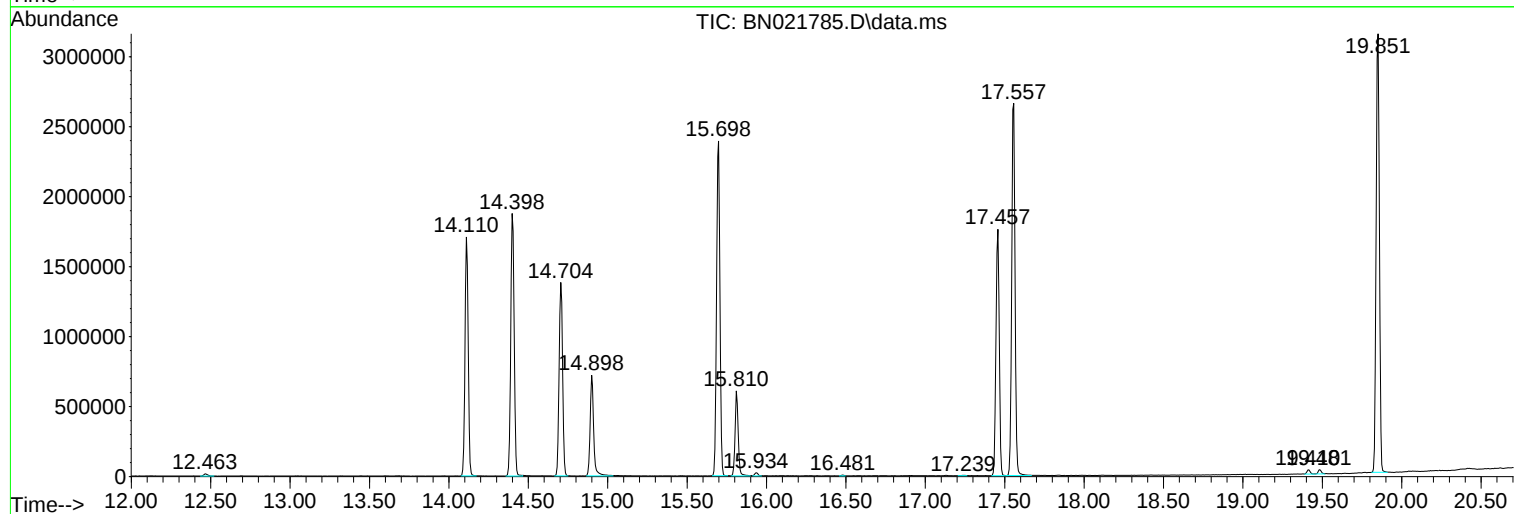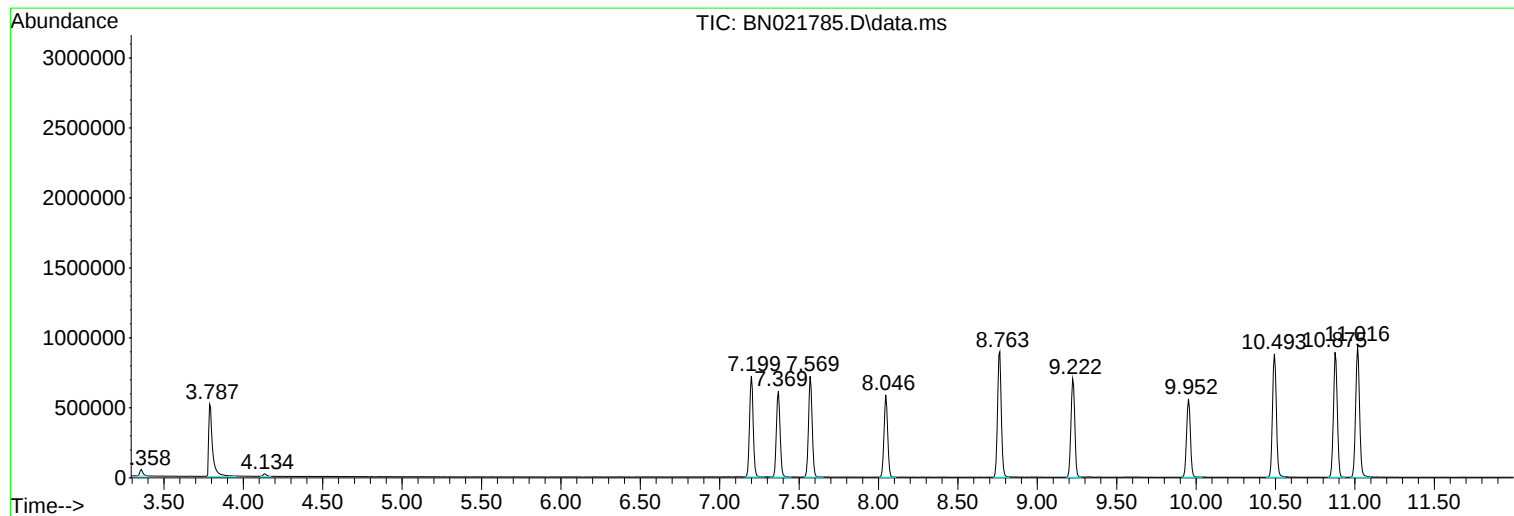

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091622\
Data File : BN021785.D
Acq On : 16 Sep 2022 12:50
Operator : CG/JU
Sample : PB147637BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK637

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091622\
Data File : BN021785.D
Acq On : 16 Sep 2022 12:50
Operator : CG/JU
Sample : PB147637BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK637

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc