

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
 Data File : BN033998.D
 Acq On : 16 Sep 2024 21:14
 Operator : JU/RC
 Sample : SP96631
 Misc : SFAM SURROGATE
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Sep 17 00:42:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.477	152	4888	0.400	ng/ul	0.00
4) Naphthalene-d8	10.233	136	13737	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.119	164	7604	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.978	188	2356386	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.10
23) Perylene-d12	23.237	264	19291	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	86416	17.197	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.834	152	15180	0.770	ng/ul	-0.01
18) Fluoranthene-d10	18.915	212	39357	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.127	166	4531	0.163	ng/ul#	12
26) Benzo(a)pyrene	23.105	252	9820	0.163	ng/ul#	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN033998.D
Acq On : 16 Sep 2024 21:14
Operator : JU/RC
Sample : SP96631
Misc : SFAM SURROGATE
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Sep 17 00:42:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration




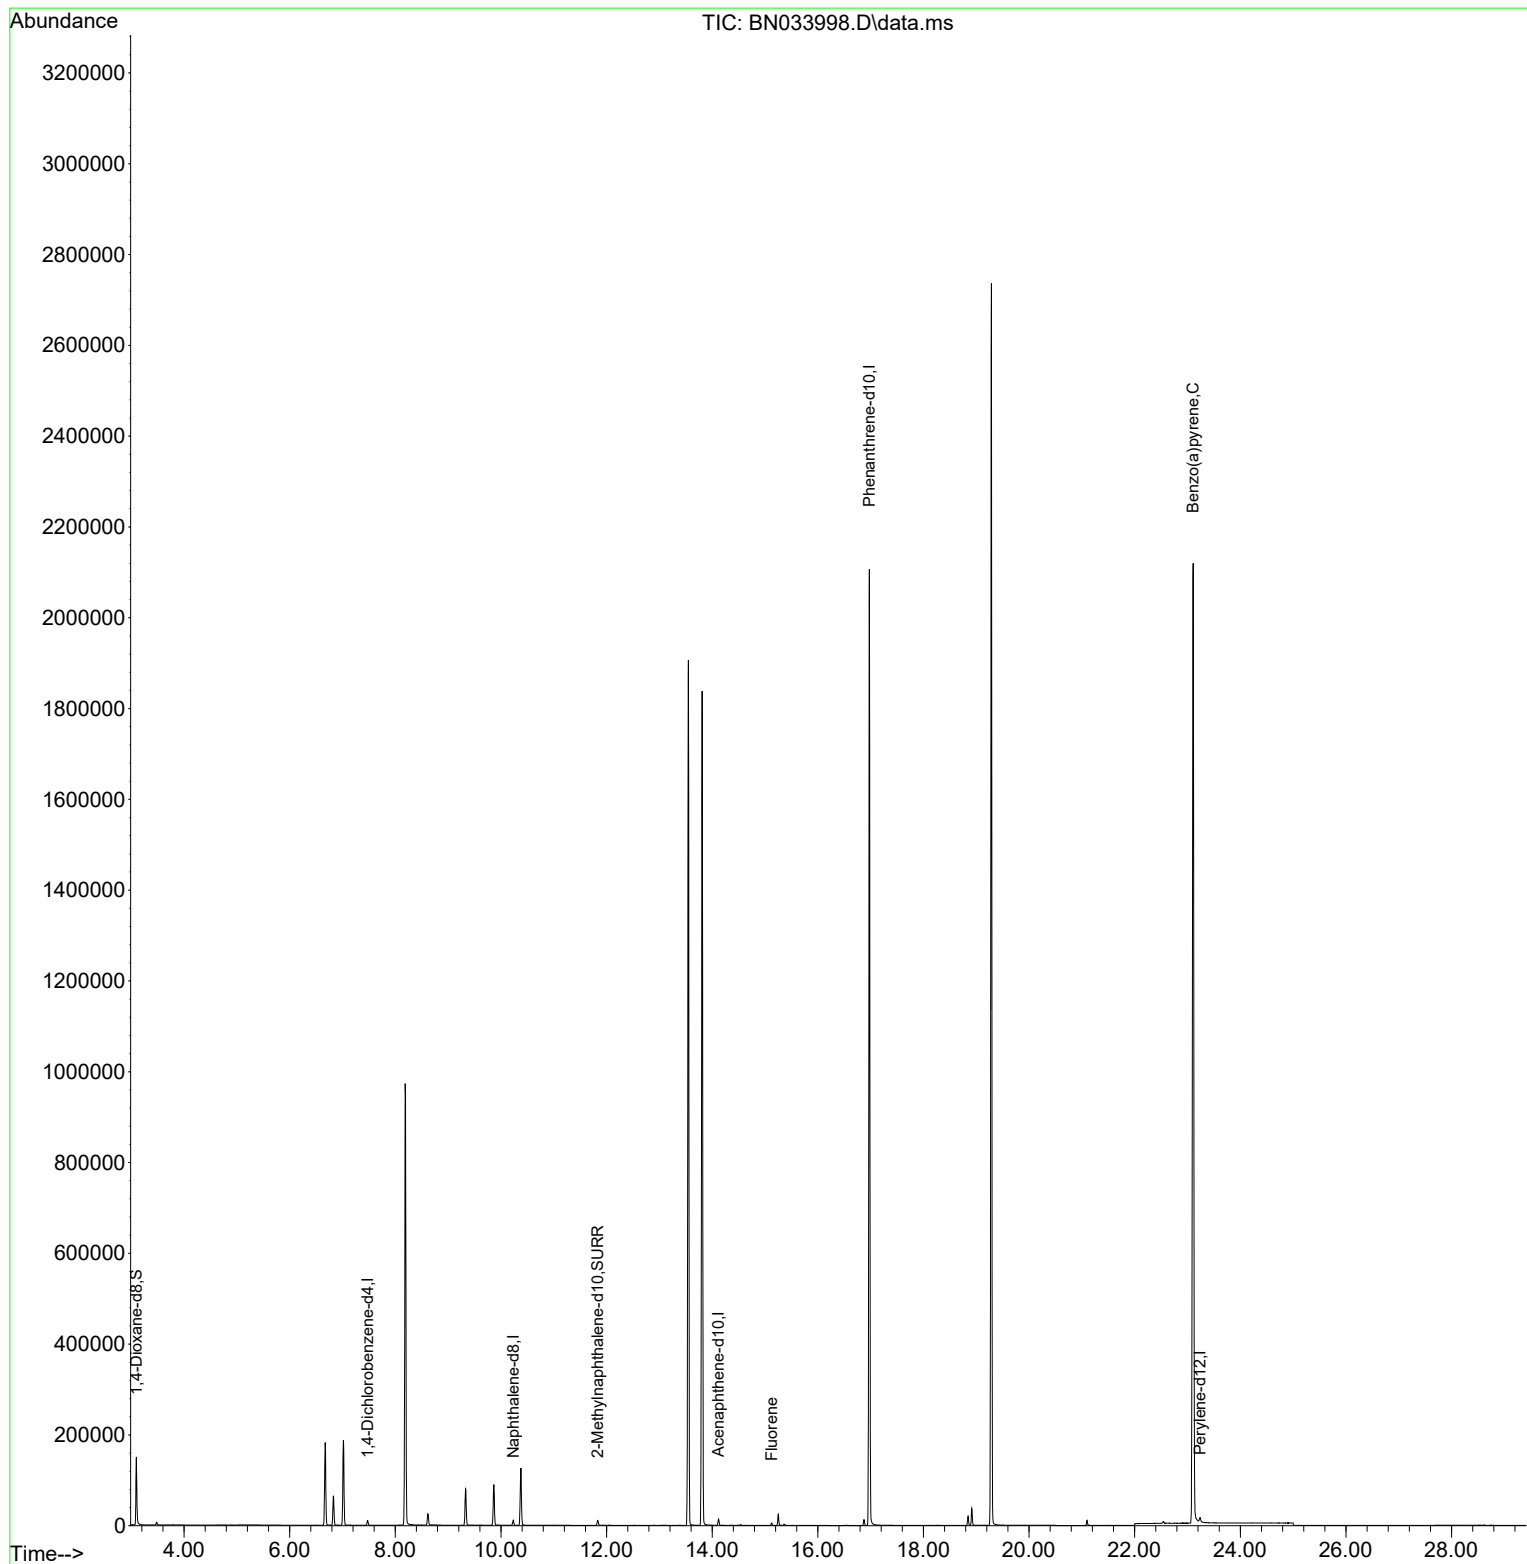


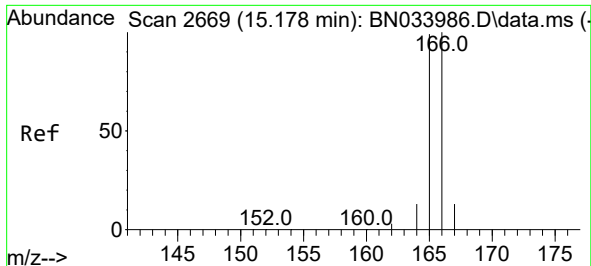

#12
Fluorene
Concen: 0.163 ng/ul
RT: 15.127 min Scan# 2658
Delta R.T. -0.060 min
Lab File: BN033998.D
Acq: 16 Sep 2024 21:14

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:166 Resp: 4531
Ion Ratio Lower Upper
166 100
165 5.8 79.1 118.7#
167 34.5 11.4 17.0#

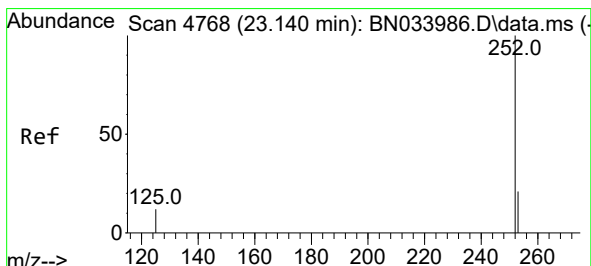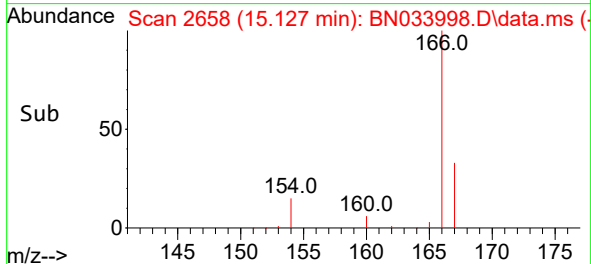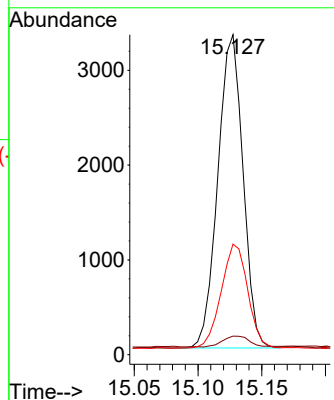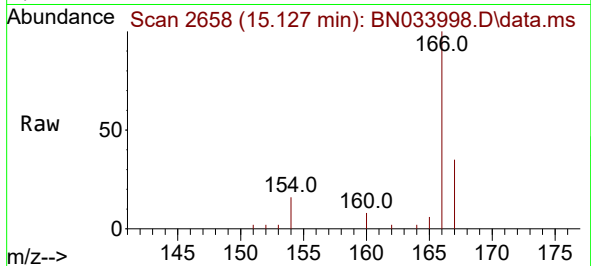

#26
Benzo(a)pyrene
Concen: 0.163 ng/ul
RT: 23.105 min Scan# 4756
Delta R.T. -0.047 min
Lab File: BN033998.D
Acq: 16 Sep 2024 21:14

Tgt Ion:252 Resp: 9820
Ion Ratio Lower Upper
252 100
253 34.0 22.8 34.2
125 31.6 18.0 27.0#

