

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
 Data File : BN034002.D
 Acq On : 17 Sep 2024 00:14
 Operator : JU/RC
 Sample : P3994-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Sep 17 00:43:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.477	152	7110	0.400	ng/ul	0.00
4) Naphthalene-d8	10.233	136	19744	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.119	164	10556	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.974	188	1802527	0.400	ng/ul	# 0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.10
23) Perylene-d12	23.234	264	18520	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	28477	3.896	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.834	152	8460	0.299	ng/ul	-0.01
18) Fluoranthene-d10	18.915	212	22864	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
11) Acenaphthene	14.221	153	5098	0.147	ng/ul#	23
26) Benzo(a)pyrene	23.102	252	5704	0.099	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034002.D
Acq On : 17 Sep 2024 00:14
Operator : JU/RC
Sample : P3994-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Sep 17 00:43:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

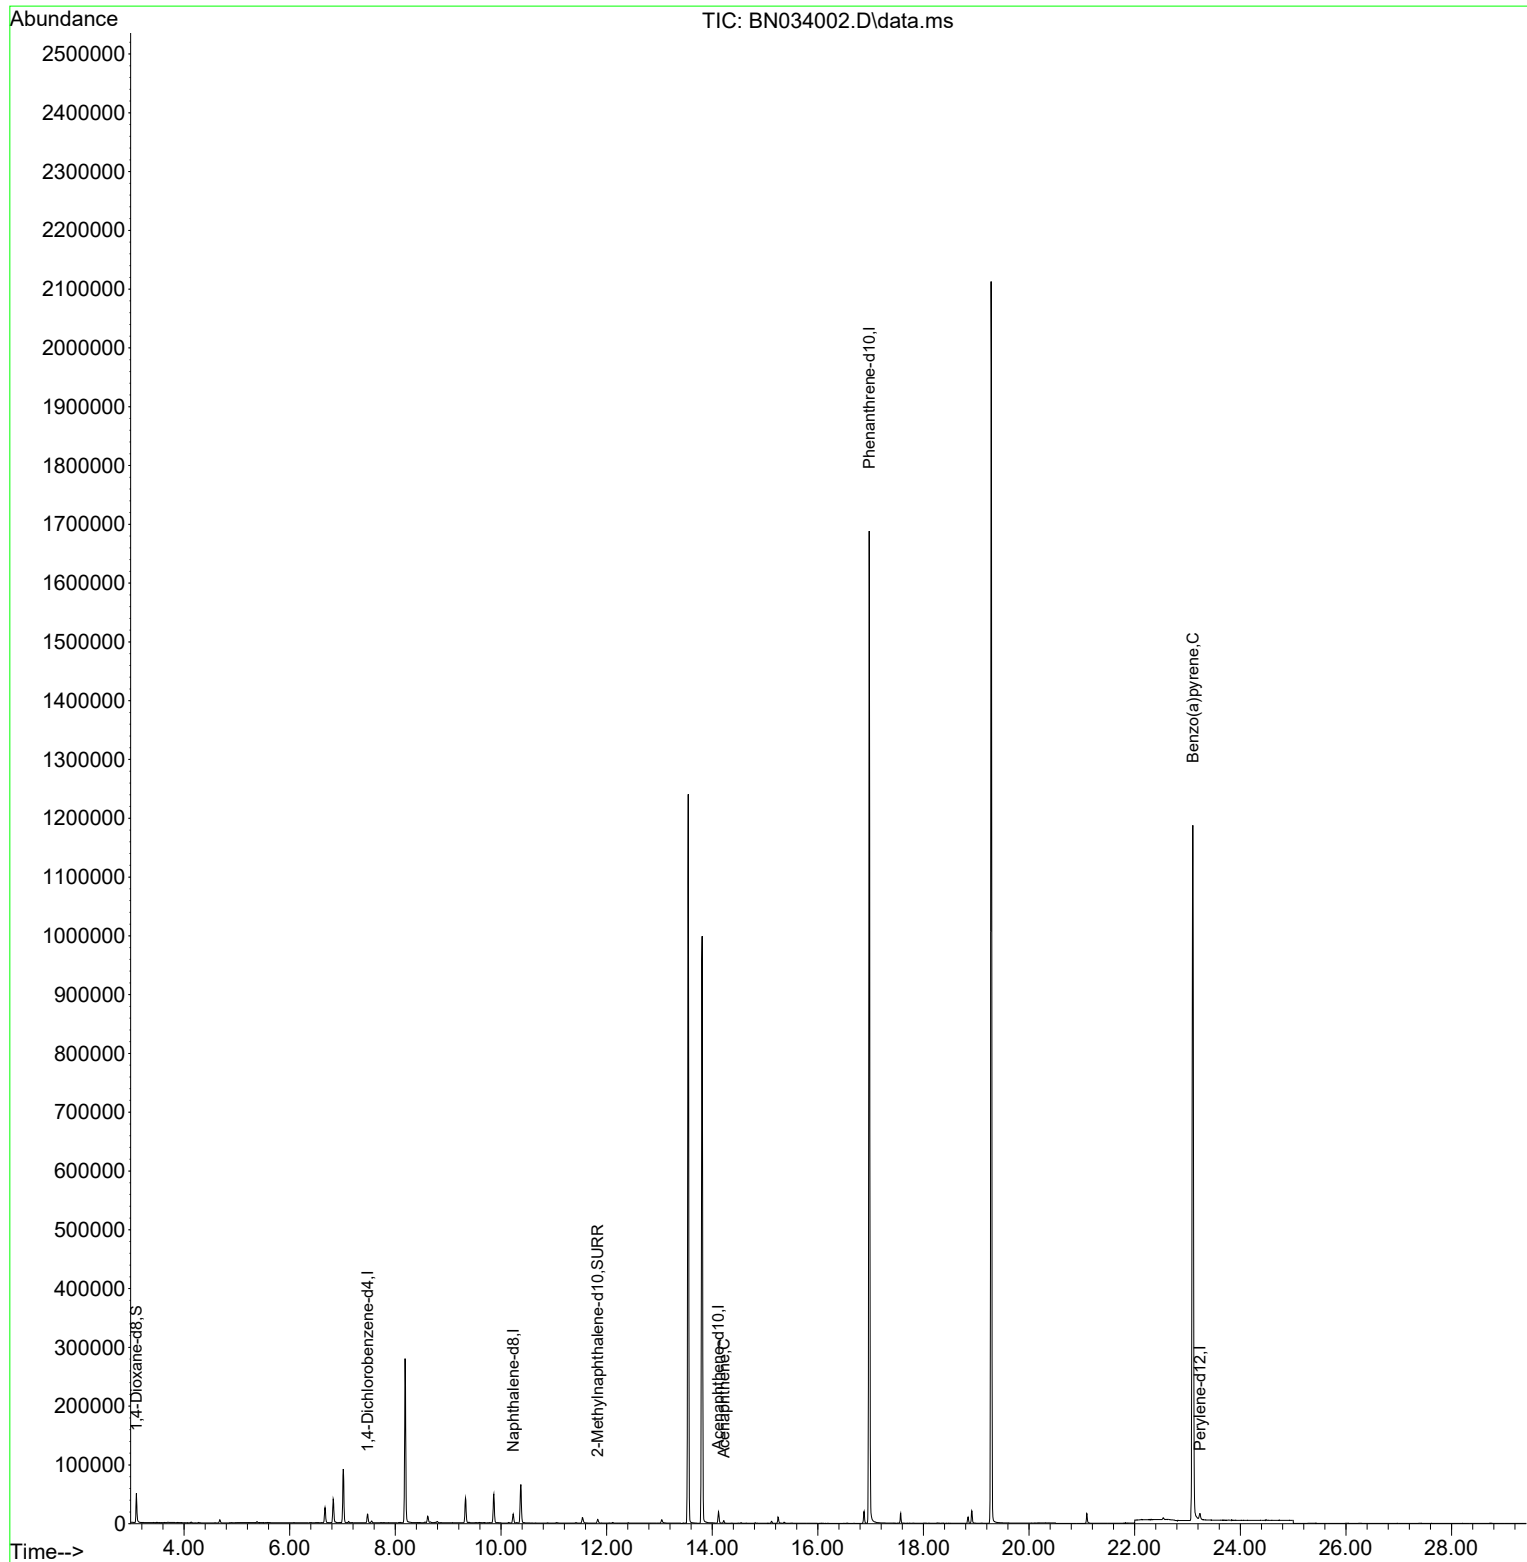

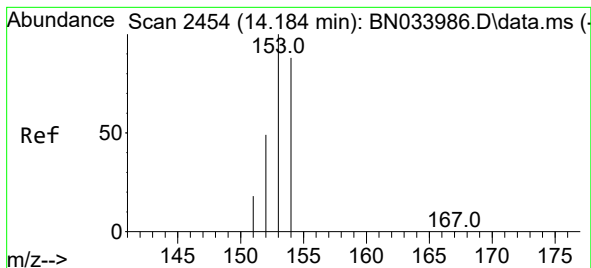

#11

Acenaphthene

Concen: 0.147 ng/ul

RT: 14.221 min Scan# 24

Delta R.T. 0.028 min

Lab File: BN034002.D

Acq: 17 Sep 2024 00:14

Instrument :

BNA_N

ClientSampleId :





Tgt Ion:153 Resp: 5098

Ion Ratio Lower Upper

153 100

152 2.7 39.8 59.8#

154 10.2 69.0 103.6#

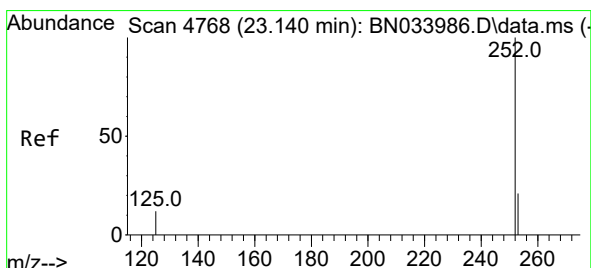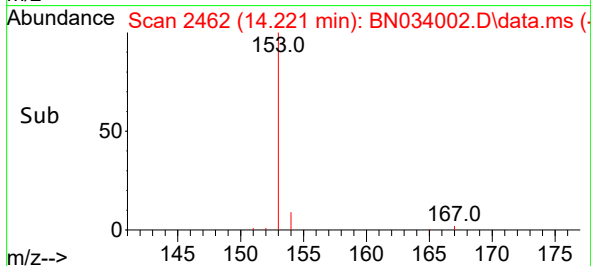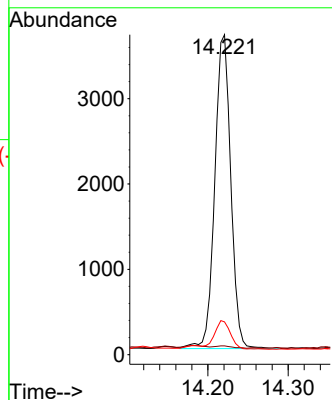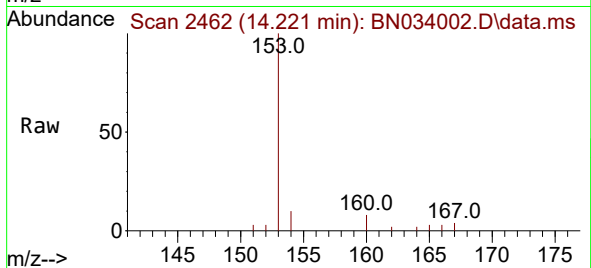

#26

Benzo(a)pyrene

Concen: 0.099 ng/ul

RT: 23.102 min Scan# 4755

Delta R.T. -0.050 min

Lab File: BN034002.D

Acq: 17 Sep 2024 00:14

Tgt Ion:252 Resp: 5704

Ion Ratio Lower Upper

252 100

253 40.5 22.8 34.2#

125 38.8 18.0 27.0#

