




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN033987.D
Acq On : 16 Sep 2024 14:31
Operator : JU/RC
Sample : PB163314BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK314

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/17/2024
Supervised By :mohammad ahmed 09/17/2024

Quant Time: Sep 16 15:31:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

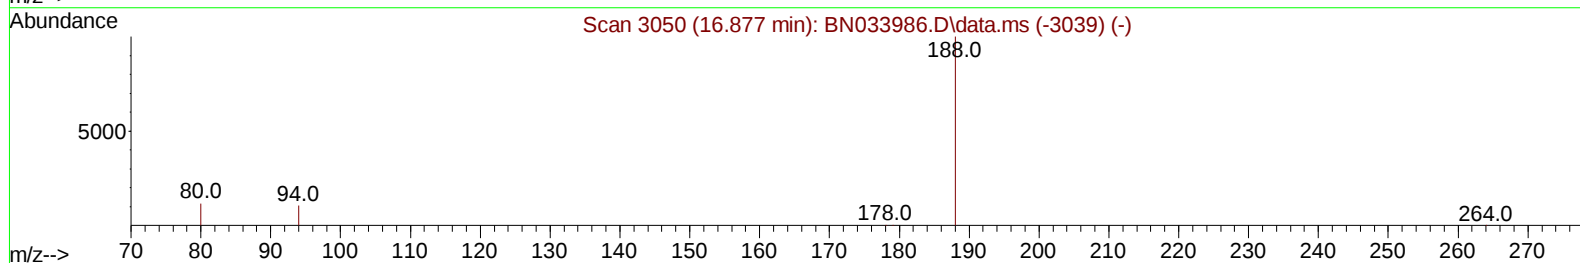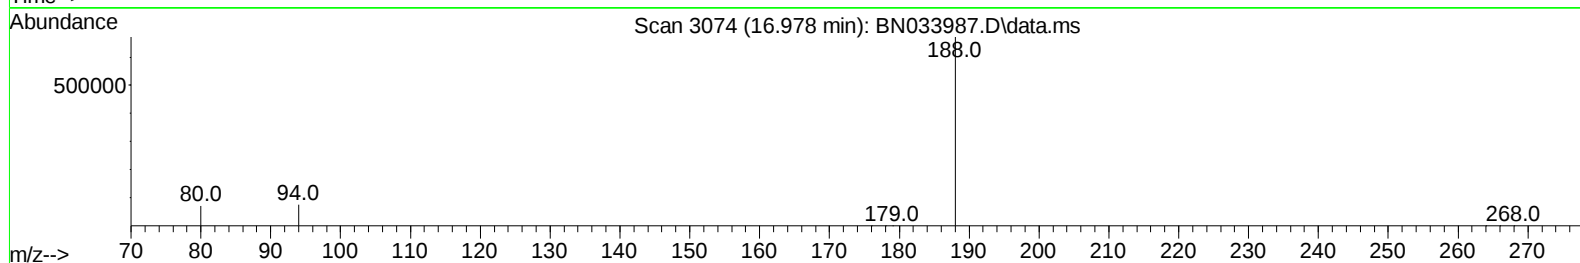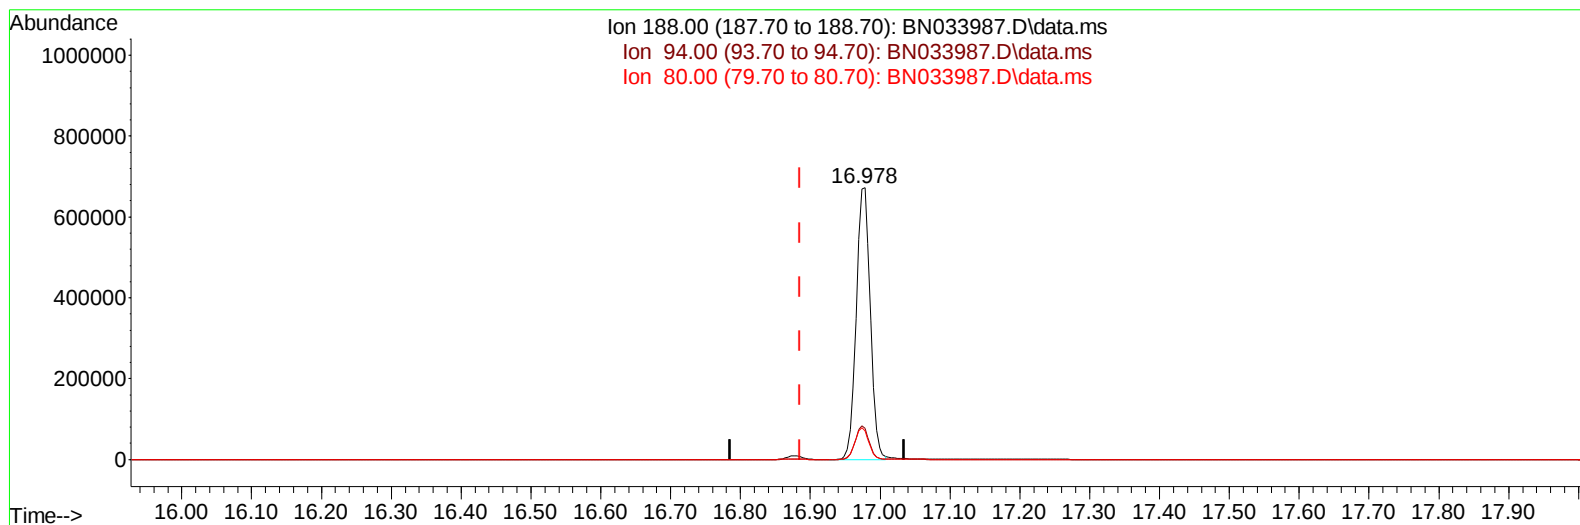

TIC: BN033987.D\data.ms

(13) Phenanthrene-d10 (I)**16.978min (+ 0.093) 0.40 ng/u1****response 935623**

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.30	11.37
80.00	11.50	10.44
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN033987.D
Acq On : 16 Sep 2024 14:31
Operator : JU/RC
Sample : PB163314BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK314

Manual IntegrationsAPPROVED

Quant Time: Sep 16 15:31:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/17/2024
Supervised By :mohammad ahmed 09/17/2024

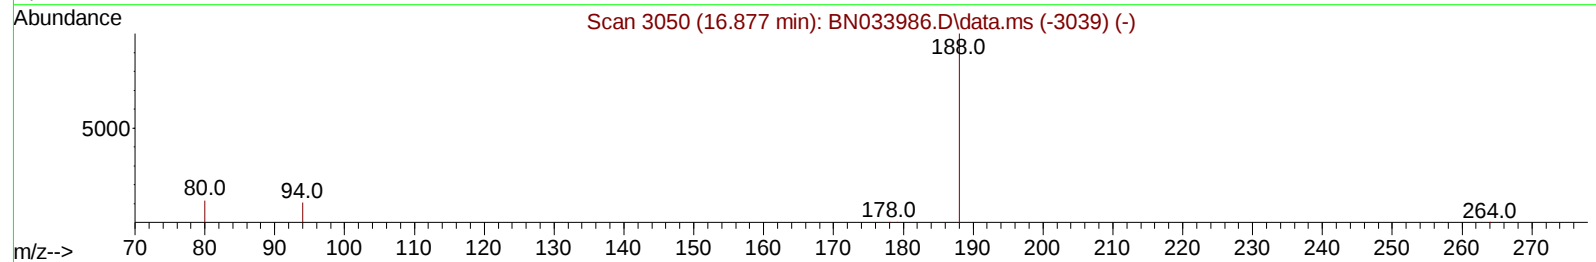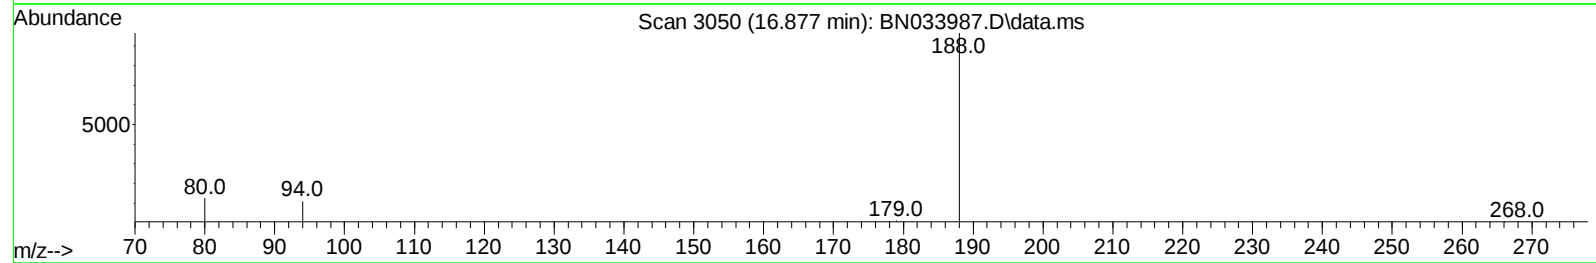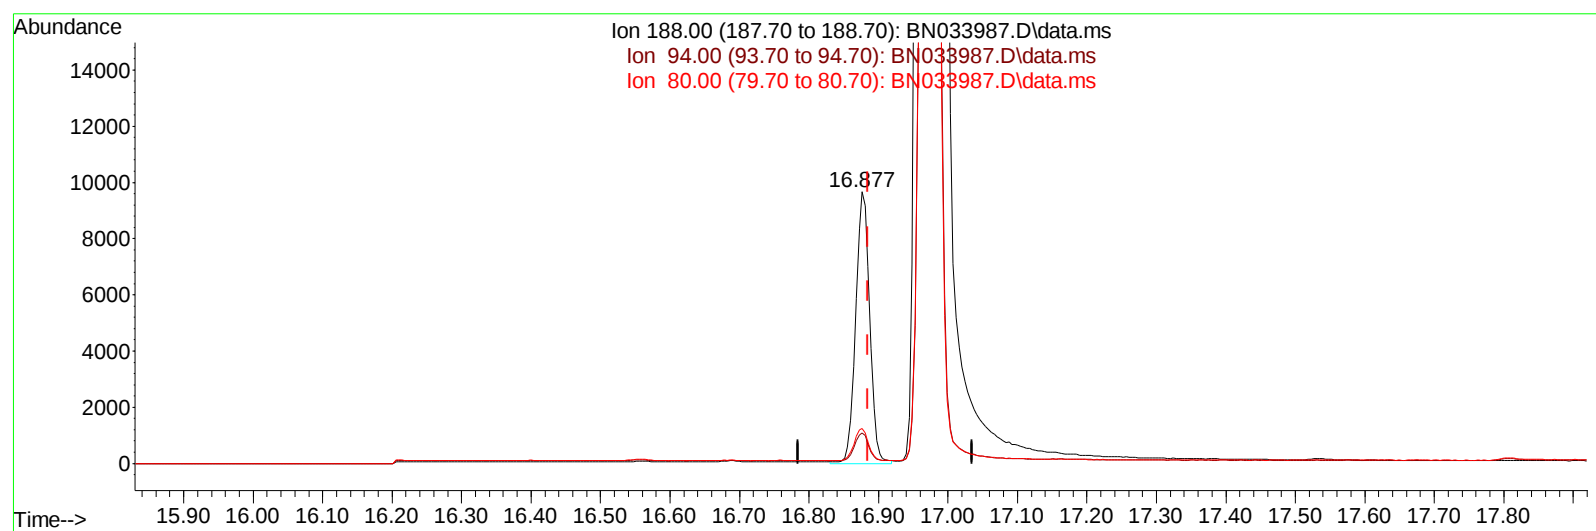

TIC: BN033987.D\data.ms

(13) Phenanthrene-d10 (I)

16.877min (-0.009) 0.40 ng/u1 m

response 13636

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.30	11.29
80.00	11.50	12.89
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN033987.D
Acq On : 16 Sep 2024 14:31
Operator : JU/RC
Sample : PB163314BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK314

Manual IntegrationsAPPROVED

Quant Time: Sep 16 15:31:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/17/2024
Supervised By :mohammad ahmed 09/17/2024

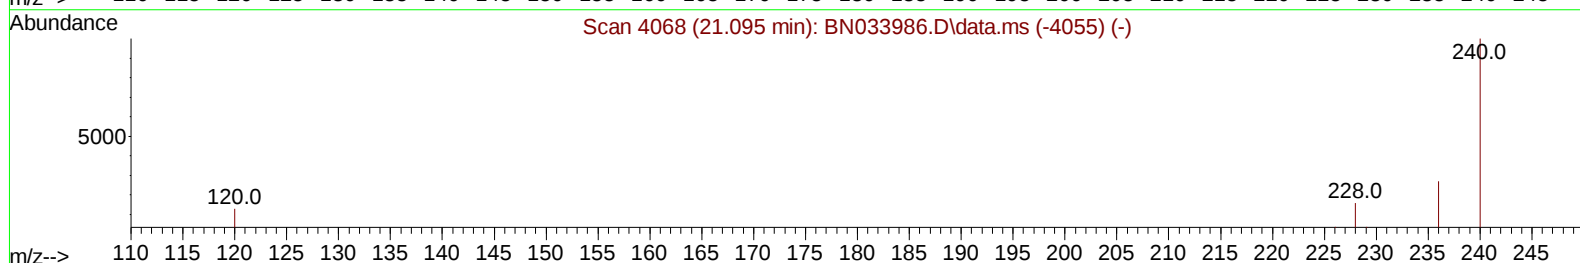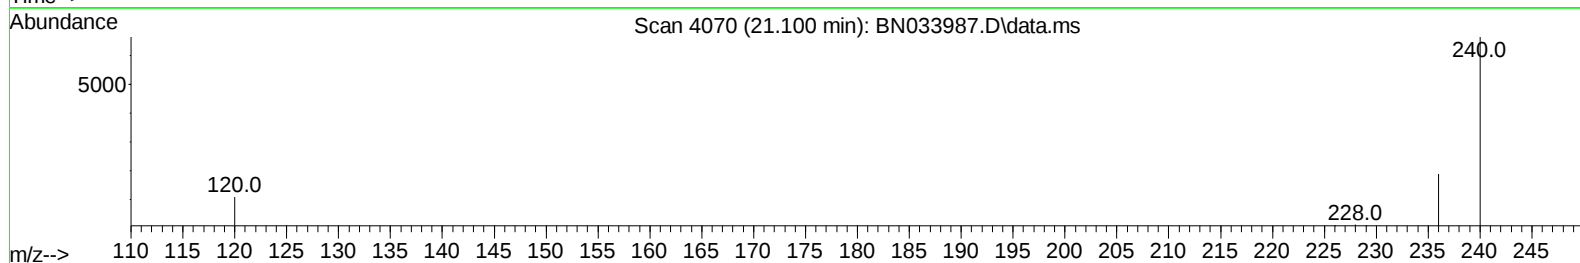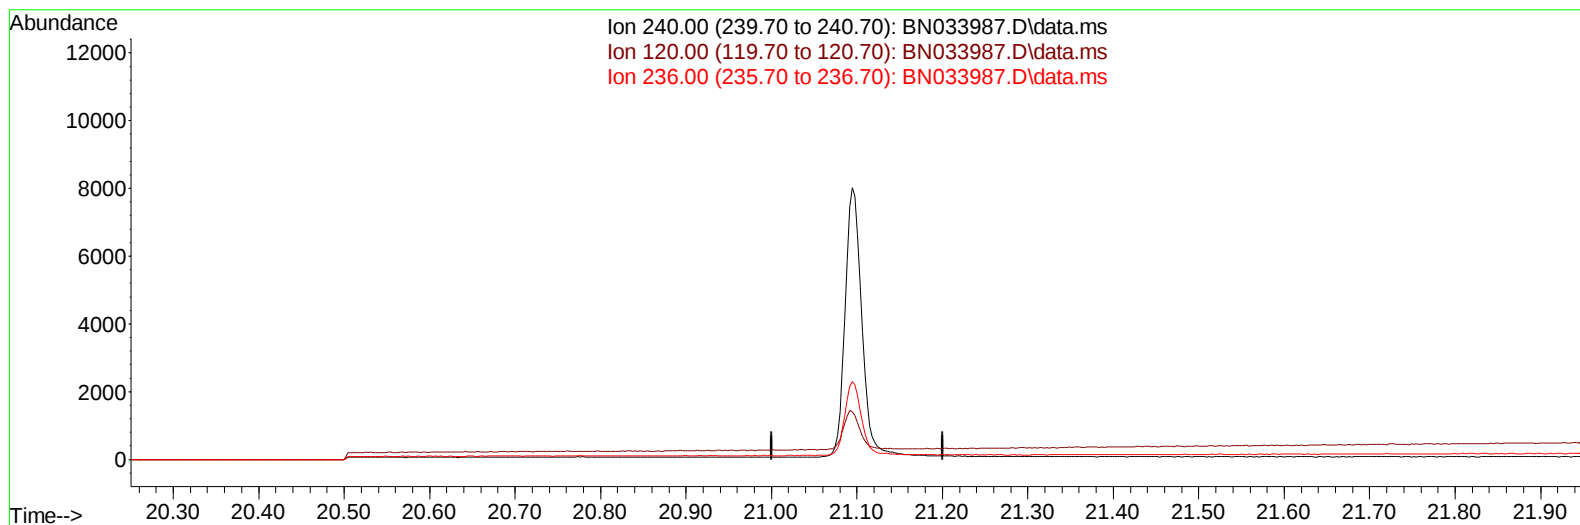

TIC: BN033987.D\data.ms

(17) Chrysene-d12

21.101min (-21.101) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	16.40	0.00#
236.00	28.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN033987.D
Acq On : 16 Sep 2024 14:31
Operator : JU/RC
Sample : PB163314BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK314

Manual IntegrationsAPPROVED

Quant Time: Sep 16 15:31:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/17/2024
Supervised By :mohammad ahmed 09/17/2024

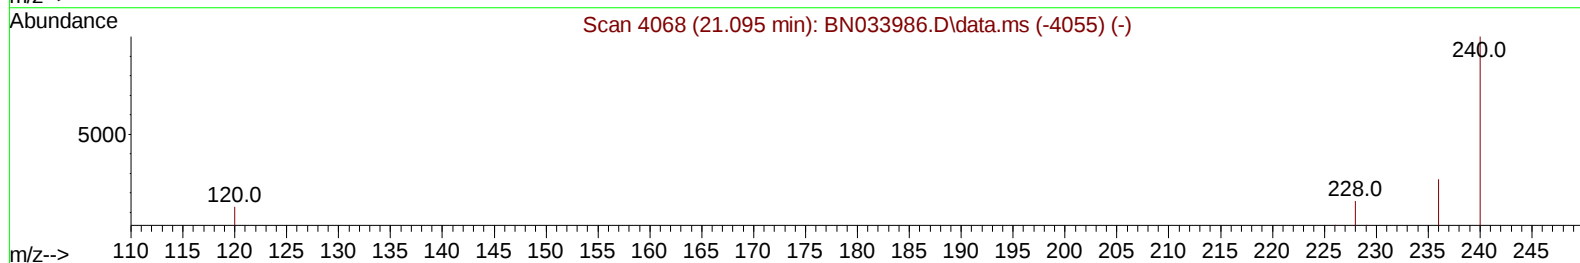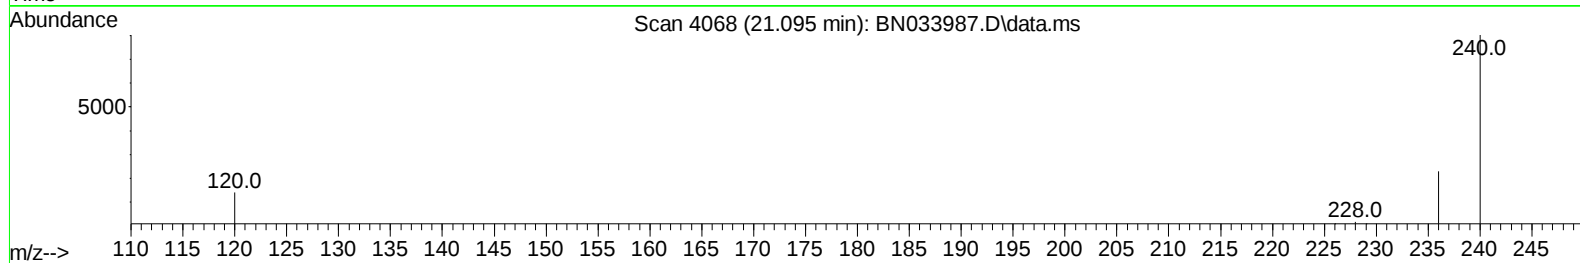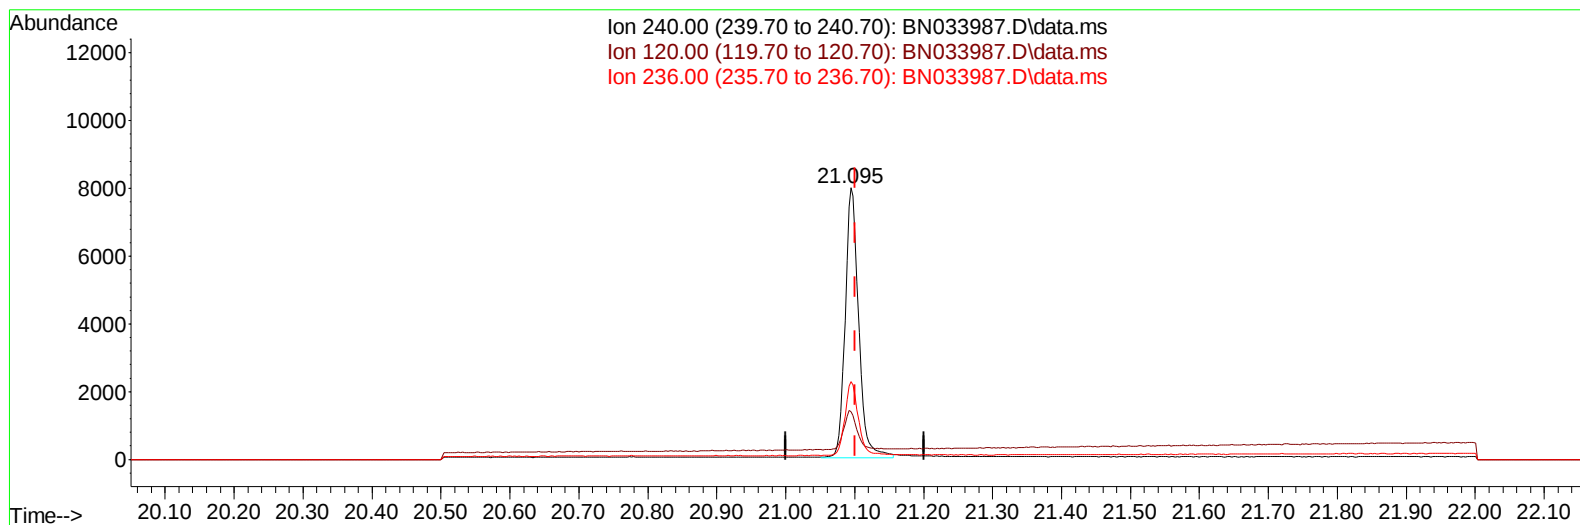

TIC: BN033987.D\data.ms

(17) Chrysene-d12

21.095min (-0.006) 0.40 ng/ul m

response 10831

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.40	17.57
236.00	28.30	28.75
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN033987.D
Acq On : 16 Sep 2024 14:31
Operator : JU/RC
Sample : PB163314BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK314

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/17/2024
Supervised By :mohammad ahmed 09/17/2024

Quant Time: Sep 16 15:31:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

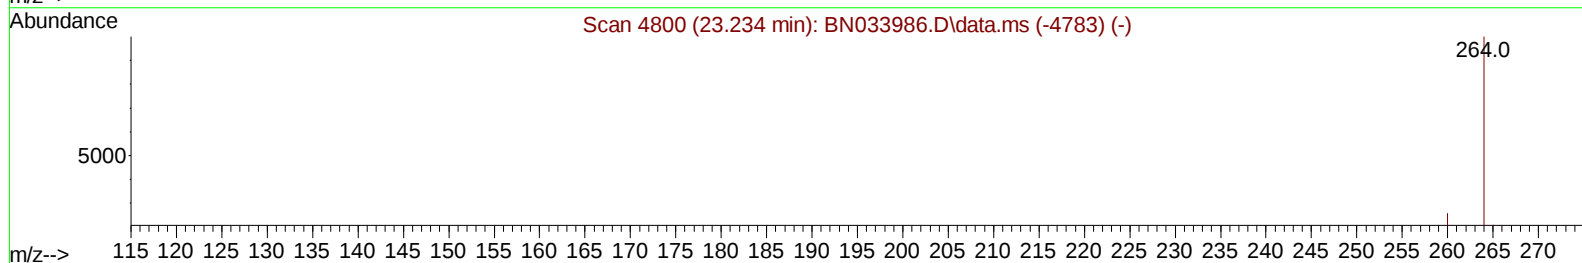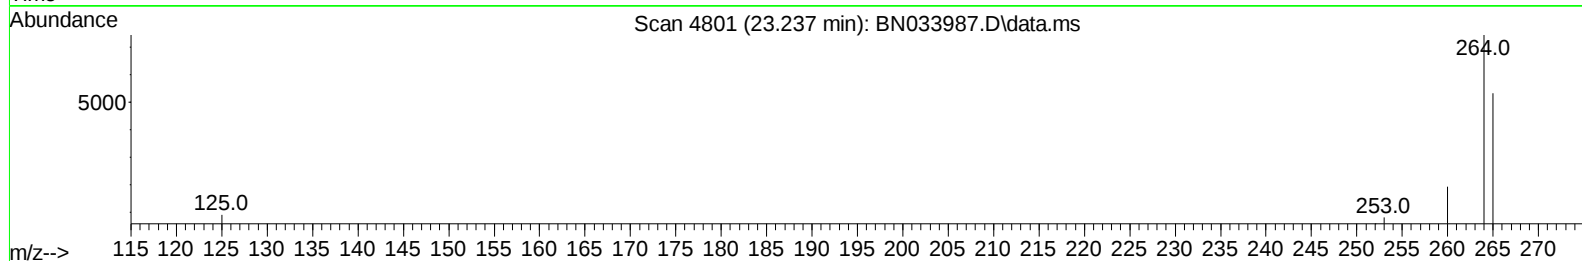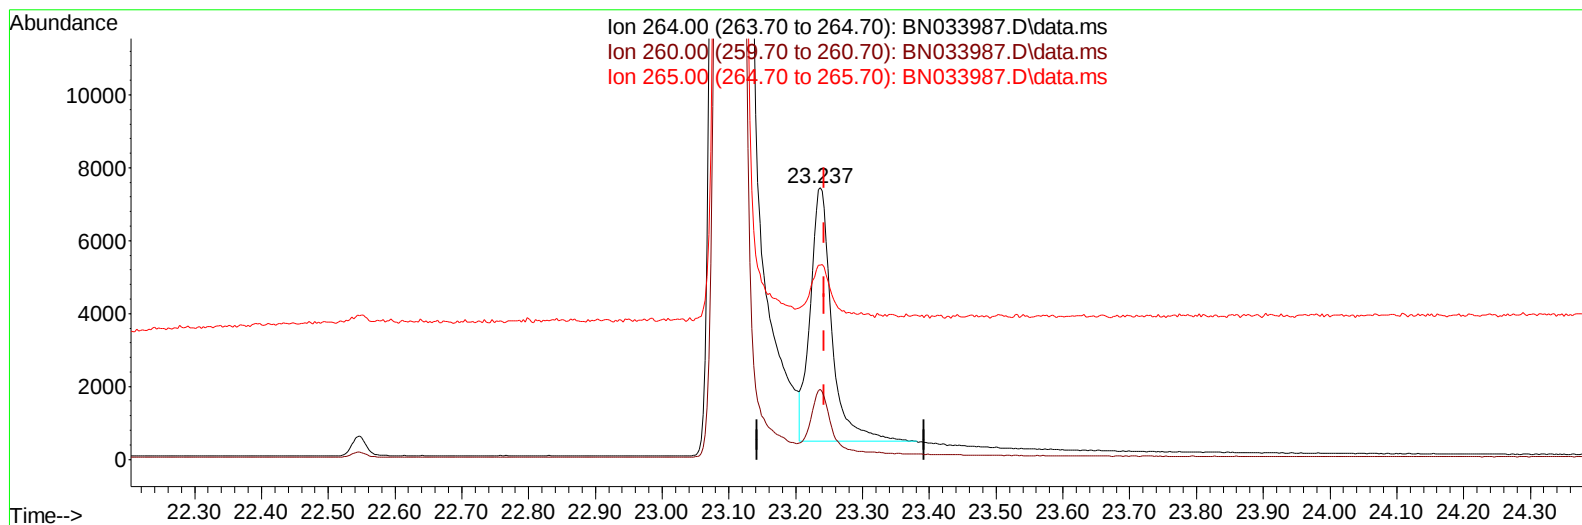

TIC: BN033987.D\data.ms

(23) Perylene-d12 (I)

23.237min (-0.006) 0.40 ng/u1

response 15853

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	25.87
265.00	73.30	71.47
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN033987.D
Acq On : 16 Sep 2024 14:31
Operator : JU/RC
Sample : PB163314BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK314

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/17/2024
Supervised By :mohammad ahmed 09/17/2024

Quant Time: Sep 16 15:31:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

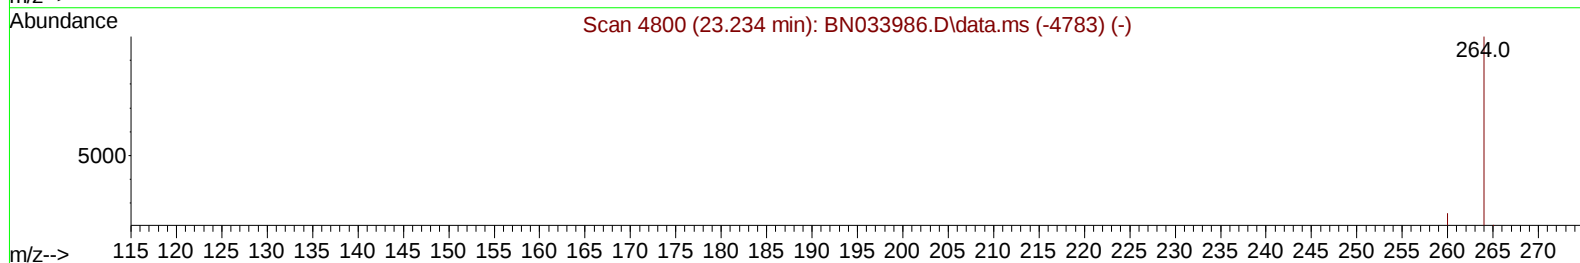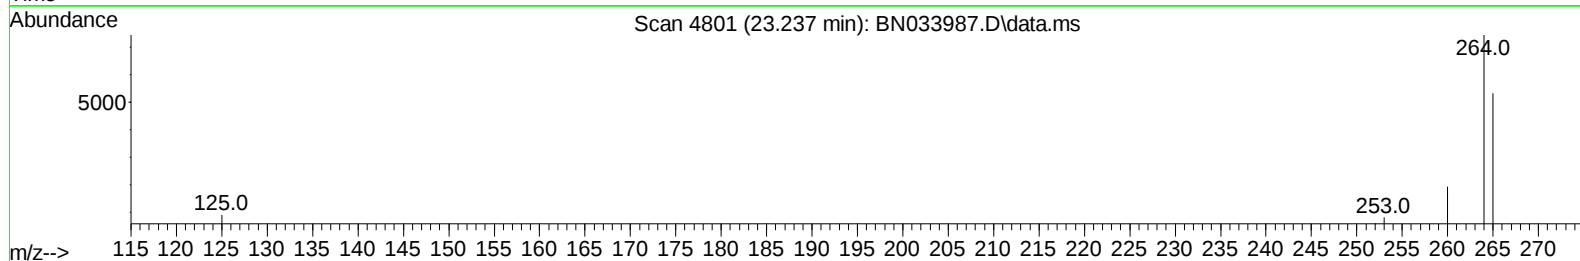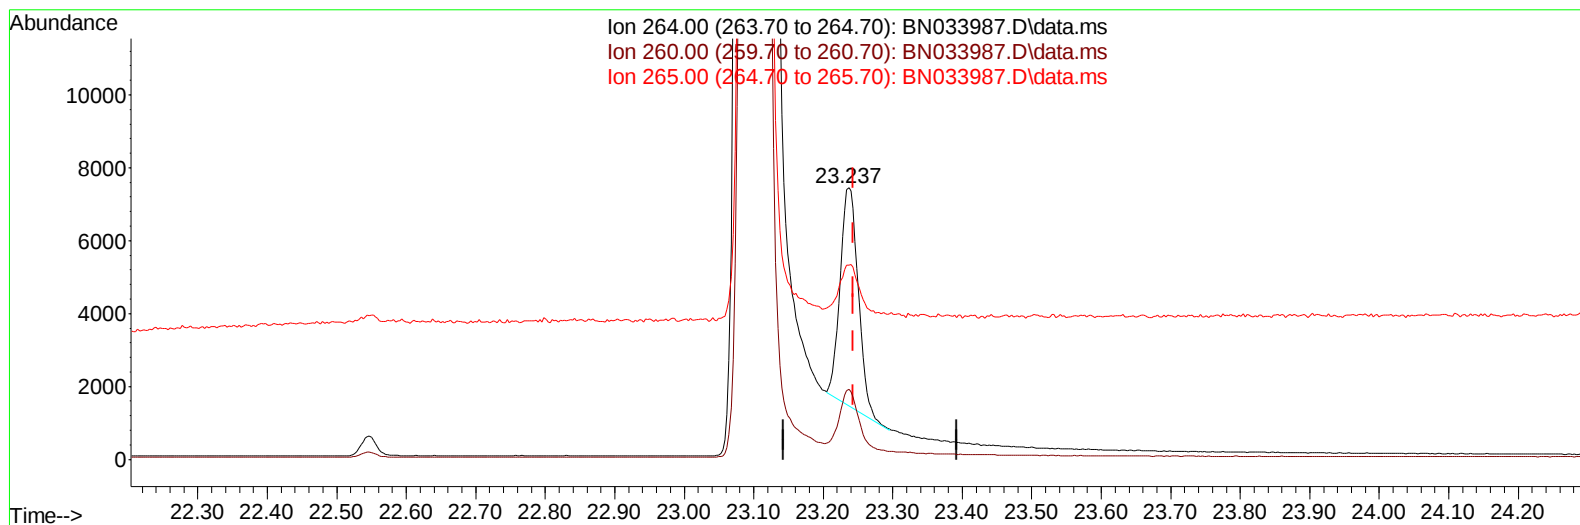

TIC: BN033987.D\data.ms

(23) Perylene-d12 (I)

23.237min (-0.006) 0.40 ng/ul m

response 10805

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	25.87
265.00	73.30	71.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
 Data File : BN033987.D
 Acq On : 16 Sep 2024 14:31
 Operator : JU/RC
 Sample : PB163314BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK314

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/17/2024
 Supervised By :mohammad ahmed 09/17/2024

Quant Time: Sep 16 15:31:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.477	152	4544	0.400	ng/ul	0.00
4) Naphthalene-d8	10.233	136	12634	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.124	164	6639	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.877	188	13636m	0.400	ng/ul	0.00
17) Chrysene-d12	21.095	240	10831m	0.400	ng/ul	0.00
23) Perylene-d12	23.237	264	10805m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	31283	6.696	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.834	152	5662	0.312	ng/ul	-0.01
18) Fluoranthene-d10	18.915	212	11003	0.341	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN033987.D
Acq On : 16 Sep 2024 14:31
Operator : JU/RC
Sample : PB163314BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK314

Manual IntegrationsAPPROVED

Quant Time: Sep 16 15:31:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/17/2024
Supervised By :mohammad ahmed 09/17/2024

